

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030586.D
 Acq On : 12 Aug 2022 11:58
 Operator : JC/MD
 Sample : N4144-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EY150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	16	rVB2	5593	6788	0.68%	0.085%
2	1.368	42	46	53	rVB	109754	116599	11.71%	1.467%
3	1.666	91	95	105	rVB	87575	114131	11.46%	1.436%
4	2.306	194	200	209	rVB	203414	306633	30.79%	3.859%
5	2.398	210	215	229	rVB	14279	31048	3.12%	0.391%
6	2.672	258	260	261	rVB	725	373	0.04%	0.005%
7	2.709	265	266	269	rVB2	610	348	0.03%	0.004%
8	2.758	272	274	275	rBV	354	374	0.04%	0.005%
9	2.788	277	279	284	rVB4	1213	1239	0.12%	0.016%
10	2.825	284	285	288	rVB2	465	407	0.04%	0.005%
11	2.861	288	291	294	rBV3	423	501	0.05%	0.006%
12	2.940	297	304	305	rBV2	1522	2055	0.21%	0.026%
13	3.099	327	330	331	rBV2	501	502	0.05%	0.006%
14	3.154	338	339	342	rBV2	726	568	0.06%	0.007%
15	3.349	368	371	374	rVB3	576	511	0.05%	0.006%
16	3.532	398	401	402	rVB2	460	372	0.04%	0.005%
17	3.611	406	414	423	rVV	15258	36063	3.62%	0.454%
18	3.776	438	441	442	rBV2	280	340	0.03%	0.004%
19	3.959	470	471	475	rBV	448	519	0.05%	0.007%
20	4.001	475	478	480	rBV3	928	942	0.09%	0.012%
21	4.349	533	535	537	rVV2	473	363	0.04%	0.005%
22	4.477	546	556	569	rVV	93505	295512	29.67%	3.719%
23	4.788	606	607	610	rVB2	713	449	0.05%	0.006%
24	4.818	610	612	615	rBV3	437	656	0.07%	0.008%
25	4.891	623	624	629	rBV2	407	420	0.04%	0.005%
26	5.062	638	652	669	rBV2	129829	416754	41.84%	5.244%
27	5.178	669	671	674	rVV3	585	552	0.06%	0.007%
28	5.391	697	706	715	rVB3	9971	27172	2.73%	0.342%
29	5.556	728	733	742	rVB3	1448	3478	0.35%	0.044%
30	5.666	749	751	753	rVB	399	350	0.04%	0.004%
31	5.690	753	755	756	rBV	382	351	0.04%	0.004%
32	5.751	764	765	767	rBV2	507	390	0.04%	0.005%
33	5.824	775	777	780	rVB	449	403	0.04%	0.005%
34	5.970	789	801	816	rBV2	334926	996032	100.00%	12.534%
35	6.214	838	841	844	rVB	392	411	0.04%	0.005%
36	6.635	909	910	912	rBV2	471	421	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030586.D
 Acq On : 12 Aug 2022 11:58
 Operator : JC/MD
 Sample : N4144-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EY150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.763	921	931	947	rBV	282513	666864	66.95%	8.392%
38	7.117	982	989	999	rVB7	8480	20800	2.09%	0.262%
39	7.190	999	1001	1003	rBV2	440	464	0.05%	0.006%
40	7.238	1006	1009	1010	rVB2	533	450	0.05%	0.006%
41	7.312	1012	1021	1035	rBV	208797	466612	46.85%	5.872%
42	7.476	1044	1048	1051	rBV3	1095	1459	0.15%	0.018%
43	7.751	1091	1093	1095	rVB2	487	407	0.04%	0.005%
44	7.775	1095	1097	1100	rBV2	454	553	0.06%	0.007%
45	7.927	1118	1122	1124	rBV3	1377	1971	0.20%	0.025%
46	8.226	1168	1171	1172	rBV	696	570	0.06%	0.007%
47	8.324	1181	1187	1199	rBV	141351	238214	23.92%	2.998%
48	8.488	1209	1214	1220	rBV6	1161	2305	0.23%	0.029%
49	8.653	1234	1241	1249	rBV	466757	744093	74.71%	9.364%
50	8.952	1284	1290	1301	rBV	110826	160153	16.08%	2.015%
51	9.281	1338	1344	1349	rBV3	3675	5985	0.60%	0.075%
52	9.384	1356	1361	1377	rBV	399220	578512	58.08%	7.280%
53	9.707	1412	1414	1416	rBV2	355	356	0.04%	0.004%
54	9.823	1431	1433	1436	rVB	604	478	0.05%	0.006%
55	10.006	1458	1463	1465	rBV3	571	645	0.06%	0.008%
56	10.055	1465	1471	1480	rBV	590155	785955	78.91%	9.890%
57	10.384	1522	1525	1527	rBV2	409	531	0.05%	0.007%
58	10.433	1531	1533	1534	rBV	482	475	0.05%	0.006%
59	10.762	1581	1587	1588	rBV2	422	677	0.07%	0.009%
60	10.780	1588	1590	1593	rVB3	726	722	0.07%	0.009%
61	11.024	1626	1630	1631	rVB3	535	611	0.06%	0.008%
62	11.195	1652	1658	1666	rBV	389437	493525	49.55%	6.210%
63	11.286	1672	1673	1675	rBV	557	393	0.04%	0.005%
64	11.421	1694	1695	1697	rBV	719	587	0.06%	0.007%
65	11.445	1697	1699	1702	rVB3	387	398	0.04%	0.005%
66	11.707	1738	1742	1745	rVB2	595	938	0.09%	0.012%
67	11.872	1767	1769	1774	rVB4	1326	1525	0.15%	0.019%
68	11.963	1782	1784	1786	rBV3	478	535	0.05%	0.007%
69	12.024	1789	1794	1805	rVB	593467	716270	71.91%	9.014%
70	12.225	1822	1827	1833	rBV	12246	20027	2.01%	0.252%
71	12.323	1837	1843	1849	rBV	520692	653134	65.57%	8.219%
72	12.457	1864	1865	1868	rVB	666	377	0.04%	0.005%
73	12.561	1880	1882	1883	rVB2	753	418	0.04%	0.005%
74	12.664	1897	1899	1903	rBV2	464	619	0.06%	0.008%
75	12.768	1913	1916	1917	rVV2	667	539	0.05%	0.007%
76	12.896	1935	1937	1938	rBV	660	392	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030586.D
 Acq On : 12 Aug 2022 11:58
 Operator : JC/MD
 Sample : N4144-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EY150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.317	2005	2006	2010	rBV2	506	415	0.04%	0.005%
78	13.359	2010	2013	2015	rBV2	404	403	0.04%	0.005%
79	13.390	2015	2018	2020	rVV2	398	462	0.05%	0.006%
80	13.469	2029	2031	2033	rBV2	585	683	0.07%	0.009%
81	13.518	2036	2039	2041	rVB2	684	728	0.07%	0.009%
82	13.548	2041	2044	2045	rBV2	328	379	0.04%	0.005%
83	13.640	2057	2059	2060	rBV	576	380	0.04%	0.005%
84	13.731	2072	2074	2076	rBV	734	706	0.07%	0.009%
85	13.756	2076	2078	2079	rVV	618	529	0.05%	0.007%
86	13.780	2080	2082	2083	rVV2	1037	686	0.07%	0.009%
87	13.810	2085	2087	2090	rVB3	1118	1228	0.12%	0.015%
88	13.847	2090	2093	2094	rBV2	633	579	0.06%	0.007%
89	13.969	2111	2113	2117	rBV	461	558	0.06%	0.007%
90	14.176	2144	2147	2149	rBV	572	527	0.05%	0.007%
91	14.255	2158	2160	2163	rVB2	631	393	0.04%	0.005%
92	14.280	2163	2164	2168	rBV2	615	577	0.06%	0.007%
93	14.316	2168	2170	2172	rVB2	542	383	0.04%	0.005%
94	14.451	2189	2192	2194	rBV3	568	774	0.08%	0.010%
95	14.542	2206	2207	2210	rBV2	354	372	0.04%	0.005%
96	15.133	2303	2304	2305	rBV	785	372	0.04%	0.005%
97	15.694	2394	2396	2399	rBV2	702	532	0.05%	0.007%
98	16.030	2449	2451	2452	rVV	688	392	0.04%	0.005%
99	16.151	2469	2471	2474	rVB2	596	442	0.04%	0.006%
100	16.292	2492	2494	2496	rBV2	724	569	0.06%	0.007%




Sum of corrected areas: 7946635

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030586.D
Acq On : 12 Aug 2022 11:58
Operator : JC/MD
Sample : N4144-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EY150

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

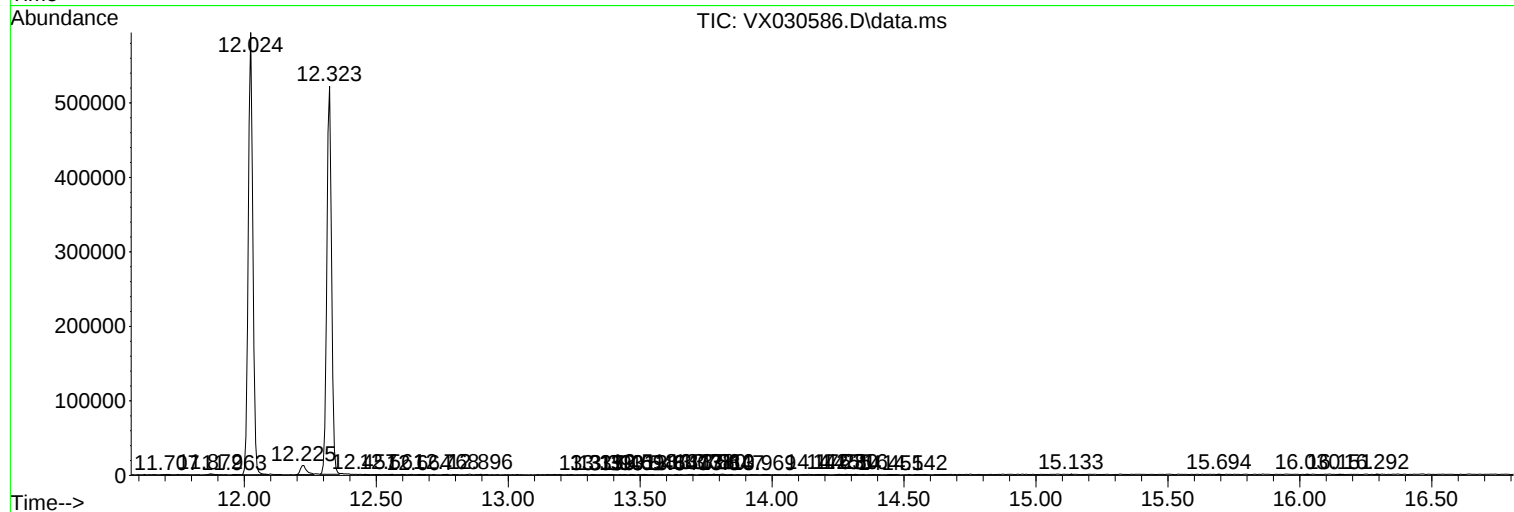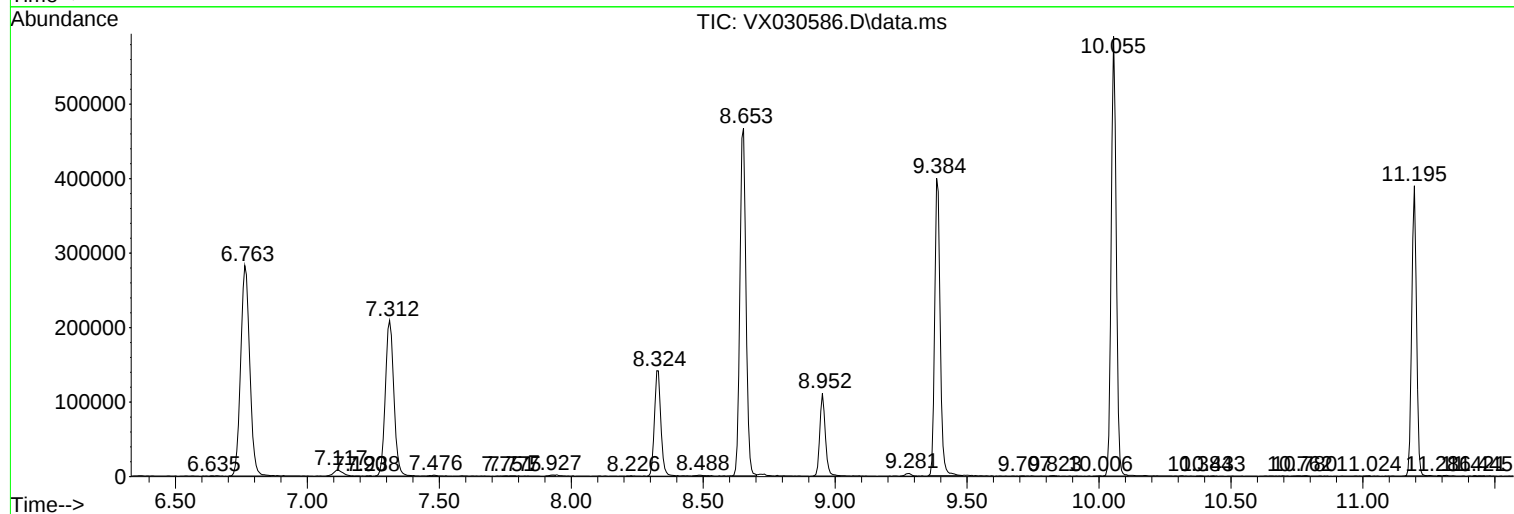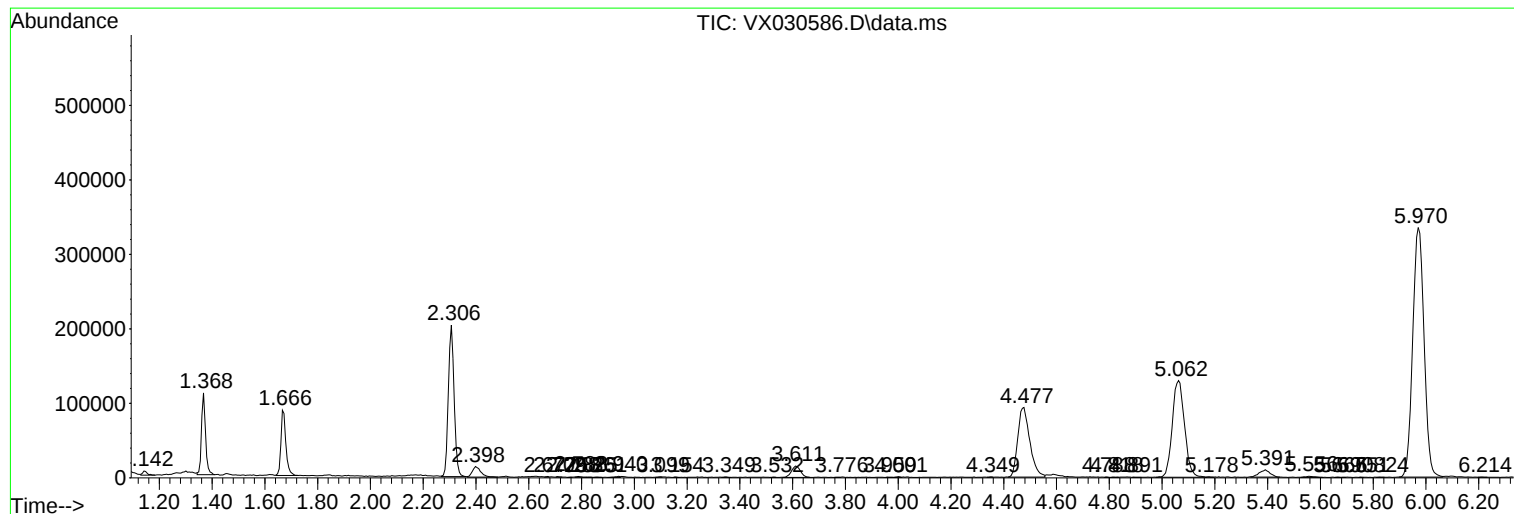

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030586.D
Acq On : 12 Aug 2022 11:58
Operator : JC/MD
Sample : N4144-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EY150

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030586.D
Acq On : 12 Aug 2022 11:58
Operator : JC/MD
Sample : N4144-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EY150

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
