

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030587.D
 Acq On : 12 Aug 2022 12:26
 Operator : JC/MD
 Sample : N4144-06DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EY153DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	120312	123631	10.93%	1.288%
2	1.666	91	95	105	rVB	98171	124202	10.98%	1.294%
3	2.307	194	200	211	rVB	217612	336924	29.79%	3.510%
4	2.502	229	232	233	rBV2	447	413	0.04%	0.004%
5	2.684	258	262	263	rBV2	610	695	0.06%	0.007%
6	2.745	270	272	273	rBV2	445	359	0.03%	0.004%
7	2.764	273	275	276	rVV	435	326	0.03%	0.003%
8	2.788	276	279	285	rVV3	1930	2746	0.24%	0.029%
9	2.947	298	305	311	rBV2	4622	9613	0.85%	0.100%
10	3.093	322	329	340	rBV	71116	129508	11.45%	1.349%
11	3.379	375	376	381	rVB2	515	449	0.04%	0.005%
12	3.434	383	385	387	rVB2	498	438	0.04%	0.005%
13	3.520	398	399	403	rBV2	387	301	0.03%	0.003%
14	3.709	428	430	433	rVB2	396	425	0.04%	0.004%
15	3.825	446	449	452	rVB2	306	385	0.03%	0.004%
16	3.959	468	471	473	rVB2	427	425	0.04%	0.004%
17	3.983	473	475	476	rBV2	412	415	0.04%	0.004%
18	4.239	515	517	518	rVV	407	296	0.03%	0.003%
19	4.257	518	520	522	rBV2	636	534	0.05%	0.006%
20	4.312	528	529	533	rBV2	249	309	0.03%	0.003%
21	4.410	542	545	546	rBV2	354	318	0.03%	0.003%
22	4.477	546	556	573	rBV2	155322	517179	45.72%	5.388%
23	4.769	603	604	608	rBV3	632	687	0.06%	0.007%
24	4.867	619	620	622	rBV	719	562	0.05%	0.006%
25	4.916	626	628	633	rVV2	332	560	0.05%	0.006%
26	5.062	640	652	670	rVB	157185	476512	42.13%	4.964%
27	5.263	683	685	690	rBV3	434	596	0.05%	0.006%
28	5.355	697	700	701	rBV2	369	310	0.03%	0.003%
29	5.391	701	706	708	rBV3	917	1566	0.14%	0.016%
30	5.477	717	720	722	rBV2	567	705	0.06%	0.007%
31	5.550	728	732	733	rBV3	1579	2284	0.20%	0.024%
32	5.812	772	775	777	rVV	445	425	0.04%	0.004%
33	5.970	788	801	816	rBV2	381816	1131094	100.00%	11.783%
34	6.153	829	831	832	rBV2	379	364	0.03%	0.004%
35	6.220	839	842	843	rBV2	372	357	0.03%	0.004%
36	6.440	876	878	880	rVB	636	509	0.05%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030587.D
 Acq On : 12 Aug 2022 12:26
 Operator : JC/MD
 Sample : N4144-06DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EY153DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.470	880	883	885	rBV2	687	749	0.07%	0.008%
38	6.489	885	886	890	rBV2	557	639	0.06%	0.007%
39	6.617	906	907	910	rVB2	374	295	0.03%	0.003%
40	6.763	922	931	949	rBV	287811	676712	59.83%	7.050%
41	7.123	981	990	1001	rBV	289167	645753	57.09%	6.727%
42	7.312	1011	1021	1036	rBV2	245005	531048	46.95%	5.532%
43	7.482	1046	1049	1053	rVB4	920	1027	0.09%	0.011%
44	7.635	1072	1074	1079	rVB3	626	641	0.06%	0.007%
45	7.677	1079	1081	1084	rVB	694	617	0.05%	0.006%
46	7.702	1084	1085	1087	rBV2	517	463	0.04%	0.005%
47	7.775	1095	1097	1099	rVB2	661	524	0.05%	0.005%
48	7.806	1099	1102	1104	rBV	519	478	0.04%	0.005%
49	7.927	1119	1122	1125	rBV2	984	1505	0.13%	0.016%
50	8.104	1150	1151	1155	rBV2	414	586	0.05%	0.006%
51	8.141	1155	1157	1159	rBV	559	313	0.03%	0.003%
52	8.330	1181	1188	1196	rBV	158169	271804	24.03%	2.832%
53	8.653	1234	1241	1255	rVV	529444	851720	75.30%	8.873%
54	8.787	1262	1263	1265	rBV	488	333	0.03%	0.003%
55	8.824	1267	1269	1272	rVB2	589	469	0.04%	0.005%
56	8.952	1282	1290	1303	rBV	123616	186121	16.45%	1.939%
57	9.385	1356	1361	1375	rBV	472737	672756	59.48%	7.008%
58	9.586	1392	1394	1395	rVB	740	380	0.03%	0.004%
59	9.799	1427	1429	1431	rBV	446	326	0.03%	0.003%
60	9.909	1445	1447	1450	rVB2	367	360	0.03%	0.004%
61	10.055	1465	1471	1483	rVV	595547	791645	69.99%	8.247%
62	10.287	1506	1509	1510	rBV	335	351	0.03%	0.004%
63	10.329	1514	1516	1519	rVB	588	571	0.05%	0.006%
64	10.360	1519	1521	1524	rBV	589	745	0.07%	0.008%
65	10.390	1524	1526	1527	rVV	497	322	0.03%	0.003%
66	10.421	1530	1531	1534	rVV2	450	389	0.03%	0.004%
67	10.470	1537	1539	1541	rBV2	529	391	0.03%	0.004%
68	10.494	1541	1543	1546	rVB	495	557	0.05%	0.006%
69	10.525	1546	1548	1551	rBV2	423	645	0.06%	0.007%
70	11.146	1648	1650	1652	rBV	427	297	0.03%	0.003%
71	11.195	1652	1658	1666	rVV	439496	555623	49.12%	5.788%
72	11.396	1688	1691	1693	rBV2	389	457	0.04%	0.005%
73	11.439	1696	1698	1700	rVB	548	355	0.03%	0.004%
74	11.469	1700	1703	1704	rBV	585	659	0.06%	0.007%
75	11.530	1712	1713	1716	rVB	489	331	0.03%	0.003%
76	11.561	1716	1718	1721	rBV2	521	721	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030587.D
 Acq On : 12 Aug 2022 12:26
 Operator : JC/MD
 Sample : N4144-06DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EY153DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.750	1746	1749	1756	rBV4	498	1073	0.09%	0.011%
78	11.896	1772	1773	1775	rVB	706	298	0.03%	0.003%
79	11.915	1775	1776	1779	rBV	389	366	0.03%	0.004%
80	11.957	1782	1783	1788	rVB2	452	402	0.04%	0.004%
81	12.024	1789	1794	1806	rVB	618814	738625	65.30%	7.695%
82	12.110	1806	1808	1809	rBV2	488	305	0.03%	0.003%
83	12.232	1826	1828	1829	rBV	547	385	0.03%	0.004%
84	12.323	1837	1843	1851	rBV	621031	783589	69.28%	8.163%
85	12.463	1864	1866	1869	rBV	478	527	0.05%	0.005%
86	12.555	1880	1881	1884	rVV	624	598	0.05%	0.006%
87	12.719	1906	1908	1909	rBV	686	529	0.05%	0.006%
88	12.756	1912	1914	1918	rVB3	557	532	0.05%	0.006%
89	12.975	1949	1950	1952	rBV	529	311	0.03%	0.003%
90	13.280	1998	2000	2002	rBV2	429	335	0.03%	0.003%
91	13.329	2007	2008	2012	rBV2	360	326	0.03%	0.003%
92	13.426	2023	2024	2026	rBV	443	380	0.03%	0.004%
93	13.683	2065	2066	2068	rBV2	471	374	0.03%	0.004%
94	13.865	2093	2096	2097	rBV	556	625	0.06%	0.007%
95	14.042	2124	2125	2129	rBV3	609	636	0.06%	0.007%
96	15.499	2362	2364	2367	rVB	855	658	0.06%	0.007%
97	15.530	2367	2369	2371	rBV	811	776	0.07%	0.008%
98	16.572	2538	2540	2543	rBV2	754	807	0.07%	0.008%
99	16.615	2546	2547	2549	rVV	674	334	0.03%	0.003%
100	16.700	2559	2561	2562	rBV2	675	323	0.03%	0.003%

Sum of corrected areas: 9599214




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030587.D
Acq On : 12 Aug 2022 12:26
Operator : JC/MD
Sample : N4144-06DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EY153DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

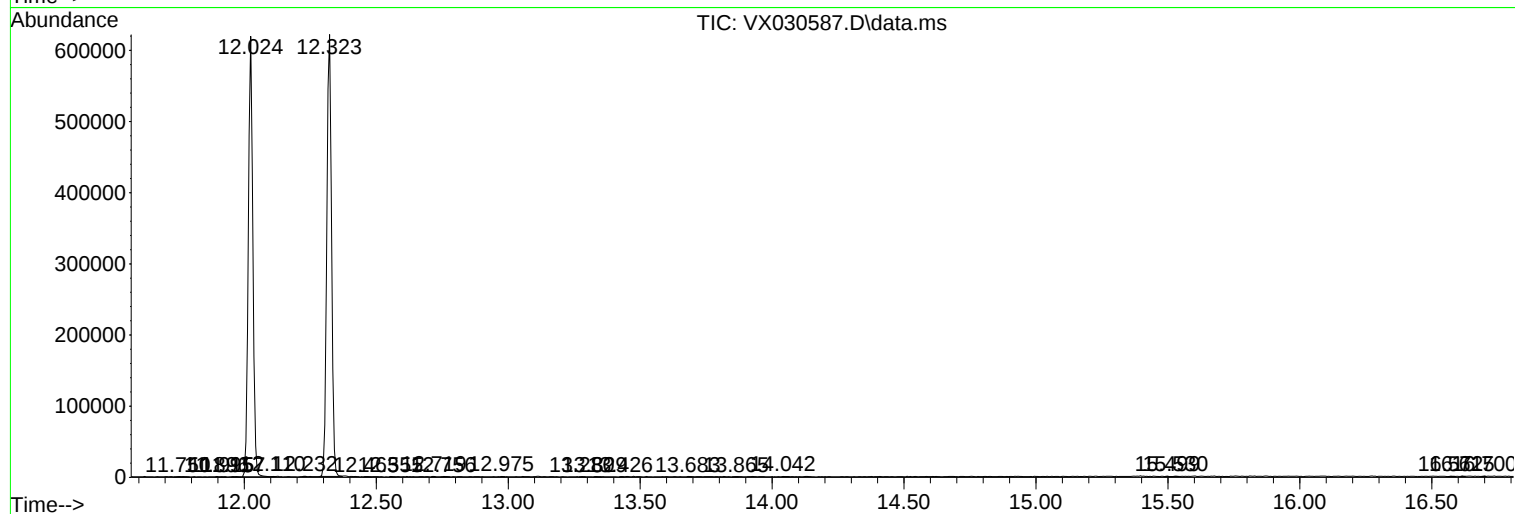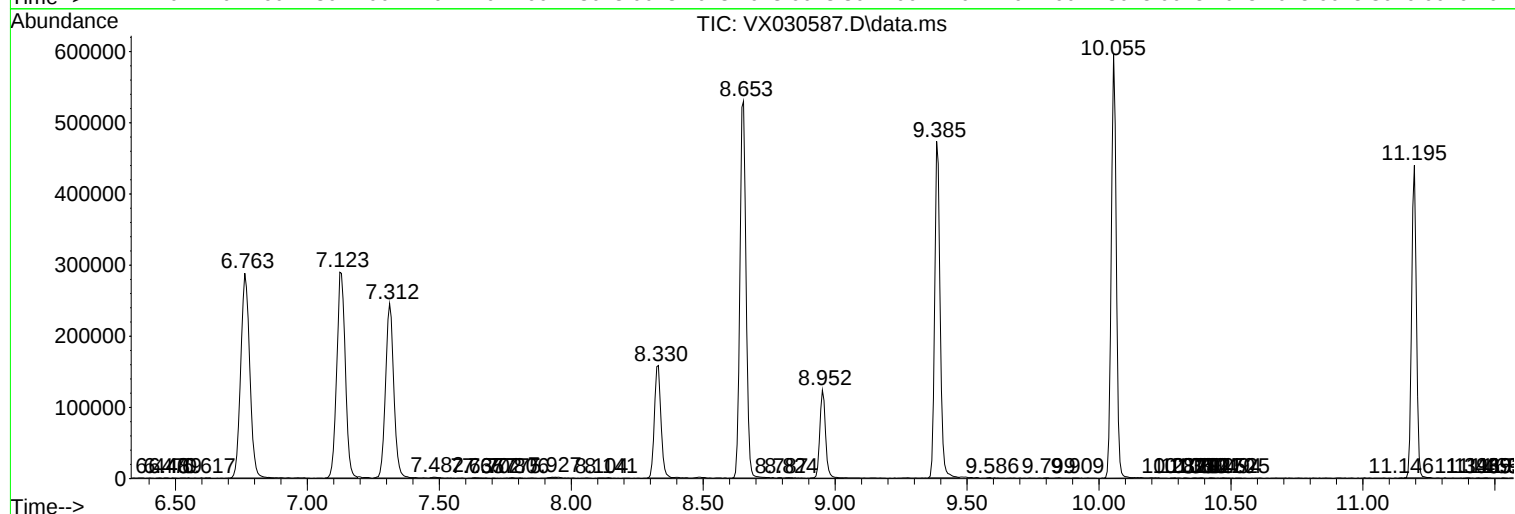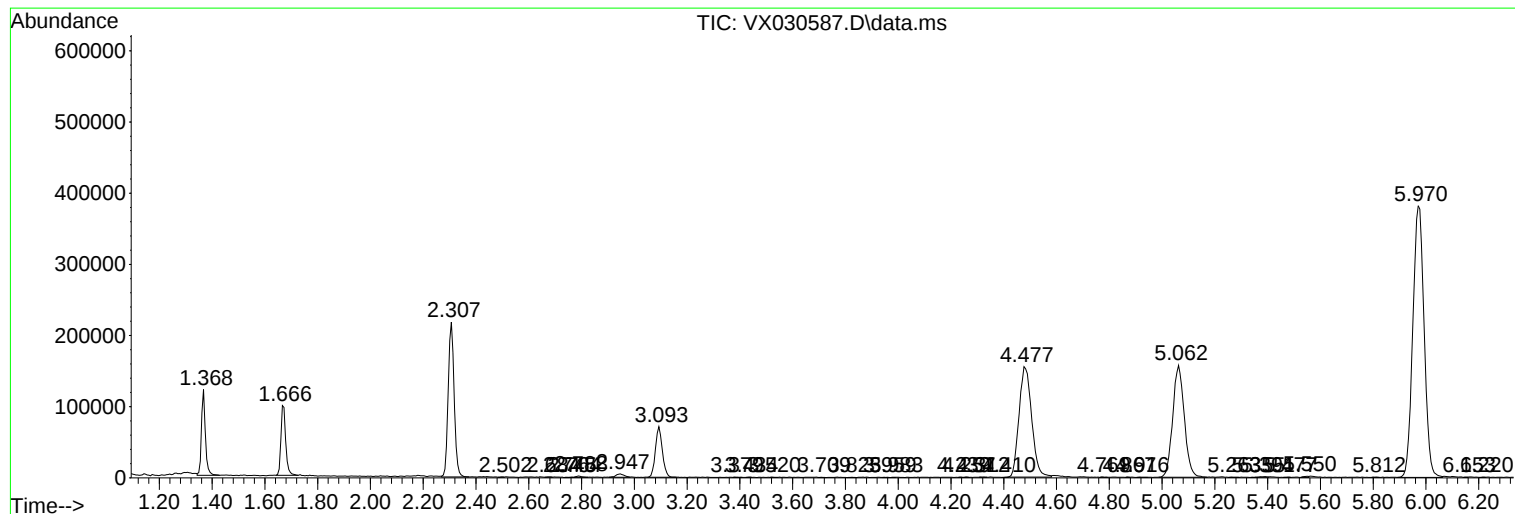

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030587.D
Acq On : 12 Aug 2022 12:26
Operator : JC/MD
Sample : N4144-06DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EY153DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030587.D
Acq On : 12 Aug 2022 12:26
Operator : JC/MD
Sample : N4144-06DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EY153DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc