

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030588.D
 Acq On : 12 Aug 2022 12:50
 Operator : JC/MD
 Sample : N4144-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EY161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030588.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	54	rVB	129519	134206	1.51%	0.577%
2	1.672	91	96	106	rVB	100607	130290	1.46%	0.560%
3	2.306	194	200	209	rVB	209059	327775	3.68%	1.409%
4	2.392	212	214	224	rVB3	2154	4628	0.05%	0.020%
5	2.501	231	232	235	rBV2	634	741	0.01%	0.003%
6	2.575	241	244	245	rBV2	1737	1677	0.02%	0.007%
7	2.794	278	280	284	rVB3	813	673	0.01%	0.003%
8	2.861	289	291	292	rBV	598	457	0.01%	0.002%
9	2.946	299	305	310	rBV4	2210	4929	0.06%	0.021%
10	3.093	320	329	350	rBV	4710846	8908755	100.00%	38.297%
11	3.501	394	396	400	rVB3	567	484	0.01%	0.002%
12	3.562	403	406	408	rBV2	539	536	0.01%	0.002%
13	3.593	408	411	415	rBV3	434	562	0.01%	0.002%
14	3.660	420	422	424	rBV	379	398	0.00%	0.002%
15	3.763	438	439	442	rBV2	331	441	0.00%	0.002%
16	4.093	490	493	496	rVB3	446	619	0.01%	0.003%
17	4.123	496	498	501	rBV2	508	764	0.01%	0.003%
18	4.336	531	533	537	rVB2	331	375	0.00%	0.002%
19	4.495	546	559	582	rBV2	1780022	4856766	54.52%	20.878%
20	4.897	623	625	626	rBV	463	380	0.00%	0.002%
21	5.068	641	653	667	rVB	162431	481558	5.41%	2.070%
22	5.385	702	705	706	rBV3	897	981	0.01%	0.004%
23	5.476	718	720	722	rBV2	533	559	0.01%	0.002%
24	5.562	729	734	742	rVB7	2364	5819	0.07%	0.025%
25	5.653	747	749	752	rBV2	622	711	0.01%	0.003%
26	5.800	772	773	776	rBV2	393	428	0.00%	0.002%
27	5.891	786	788	790	rBV2	500	495	0.01%	0.002%
28	5.976	790	802	818	rBV2	397726	1169211	13.12%	5.026%
29	6.299	852	855	858	rBV2	469	690	0.01%	0.003%
30	6.360	862	865	868	rBV2	510	756	0.01%	0.003%
31	6.537	891	894	895	rBV	444	425	0.00%	0.002%
32	6.616	904	907	908	rBV	433	447	0.01%	0.002%
33	6.769	922	932	948	rBV	273665	664627	7.46%	2.857%
34	7.013	971	972	975	rBV2	633	638	0.01%	0.003%
35	7.129	980	991	1004	rBV	492604	1056847	11.86%	4.543%
36	7.311	1013	1021	1034	rVB	243039	545091	6.12%	2.343%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030588.D
 Acq On : 12 Aug 2022 12:50
 Operator : JC/MD
 Sample : N4144-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EY161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.482	1046	1049	1053	rVB4	985	1382	0.02%	0.006%
38	7.732	1088	1090	1091	rBV	443	425	0.00%	0.002%
39	7.781	1096	1098	1100	rBV2	519	512	0.01%	0.002%
40	7.824	1100	1105	1106	rBV	505	644	0.01%	0.003%
41	7.872	1111	1113	1116	rVV3	326	485	0.01%	0.002%
42	7.939	1119	1124	1129	rVV6	2141	3788	0.04%	0.016%
43	8.019	1133	1137	1140	rBV2	426	700	0.01%	0.003%
44	8.110	1149	1152	1157	rBV2	458	752	0.01%	0.003%
45	8.330	1181	1188	1200	rBV	167890	279780	3.14%	1.203%
46	8.482	1210	1213	1217	rBV5	1652	3205	0.04%	0.014%
47	8.653	1233	1241	1251	rBV	556917	869330	9.76%	3.737%
48	8.951	1284	1290	1304	rBV	121597	189511	2.13%	0.815%
49	9.226	1332	1335	1337	rVB2	509	503	0.01%	0.002%
50	9.281	1340	1344	1347	rVB3	1435	2052	0.02%	0.009%
51	9.311	1347	1349	1353	rBV2	440	461	0.01%	0.002%
52	9.390	1356	1362	1373	rBV	480962	710063	7.97%	3.052%
53	9.567	1390	1391	1396	rBV3	583	741	0.01%	0.003%
54	9.622	1396	1400	1402	rVV3	469	620	0.01%	0.003%
55	9.829	1430	1434	1435	rBV2	510	769	0.01%	0.003%
56	9.945	1449	1453	1454	rBV2	456	442	0.00%	0.002%
57	10.012	1462	1464	1465	rBV2	624	370	0.00%	0.002%
58	10.055	1465	1471	1482	rBV	573589	771506	8.66%	3.317%
59	10.189	1491	1493	1497	rVB3	657	688	0.01%	0.003%
60	10.280	1504	1508	1511	rBV	639	851	0.01%	0.004%
61	10.372	1521	1523	1524	rBV	513	552	0.01%	0.002%
62	10.463	1537	1538	1543	rVV2	494	592	0.01%	0.003%
63	10.506	1543	1545	1547	rVB2	454	367	0.00%	0.002%
64	10.524	1547	1548	1550	rVB	668	475	0.01%	0.002%
65	10.963	1618	1620	1622	rVB2	488	499	0.01%	0.002%
66	11.195	1652	1658	1667	rBV	471827	580953	6.52%	2.497%
67	11.262	1667	1669	1672	rVB3	765	610	0.01%	0.003%
68	11.366	1684	1686	1688	rVB2	450	368	0.00%	0.002%
69	11.402	1688	1692	1693	rBV2	434	494	0.01%	0.002%
70	11.463	1700	1702	1705	rVB2	471	488	0.01%	0.002%
71	11.628	1725	1729	1731	rBV2	472	738	0.01%	0.003%
72	11.768	1748	1752	1754	rBV2	573	751	0.01%	0.003%
73	11.817	1758	1760	1763	rVB2	562	568	0.01%	0.002%
74	11.878	1763	1770	1771	rBV3	432	811	0.01%	0.003%
75	11.933	1776	1779	1780	rBV	405	367	0.00%	0.002%
76	12.024	1788	1794	1805	rBV	580095	703672	7.90%	3.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030588.D
 Acq On : 12 Aug 2022 12:50
 Operator : JC/MD
 Sample : N4144-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EY161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.183	1818	1820	1823	rVB2	423	386	0.00%	0.002%
78	12.219	1823	1826	1836	rBV5	5090	9588	0.11%	0.041%
79	12.323	1836	1843	1850	rBV	656251	803530	9.02%	3.454%
80	12.597	1884	1888	1889	rBV2	431	471	0.01%	0.002%
81	13.048	1960	1962	1965	rVV2	458	419	0.00%	0.002%
82	13.146	1976	1978	1981	rVB2	564	413	0.00%	0.002%
83	13.280	1998	2000	2004	rBV3	568	639	0.01%	0.003%
84	13.603	2052	2053	2058	rBV3	547	703	0.01%	0.003%
85	13.688	2064	2067	2070	rBV2	799	636	0.01%	0.003%
86	13.743	2074	2076	2079	rBV	376	461	0.01%	0.002%
87	14.060	2125	2128	2130	rVB2	764	913	0.01%	0.004%
88	14.085	2130	2132	2134	rBV2	399	501	0.01%	0.002%
89	14.109	2134	2136	2138	rBV	429	461	0.01%	0.002%
90	14.133	2138	2140	2144	rVB2	713	805	0.01%	0.003%
91	14.316	2168	2170	2173	rBV	453	406	0.00%	0.002%
92	14.530	2204	2205	2208	rBV2	522	634	0.01%	0.003%
93	14.627	2219	2221	2224	rBV2	524	690	0.01%	0.003%
94	14.658	2224	2226	2228	rVB	745	390	0.00%	0.002%
95	14.743	2238	2240	2246	rVB3	847	889	0.01%	0.004%
96	15.017	2284	2285	2289	rVB2	929	653	0.01%	0.003%
97	15.578	2375	2377	2380	rBV3	554	623	0.01%	0.003%
98	15.968	2439	2441	2442	rBV	490	372	0.00%	0.002%
99	16.054	2454	2455	2457	rBV	737	642	0.01%	0.003%
100	16.340	2500	2502	2505	rBV4	496	654	0.01%	0.003%




Sum of corrected areas: 23262503

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030588.D
Acq On : 12 Aug 2022 12:50
Operator : JC/MD
Sample : N4144-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EY161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

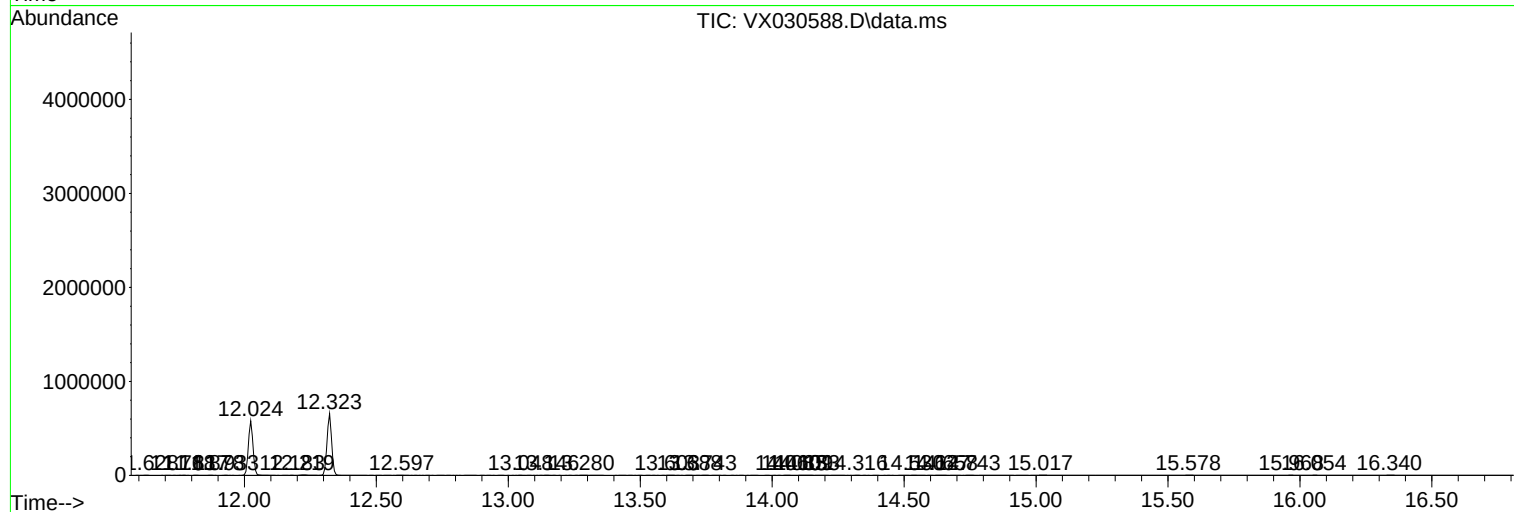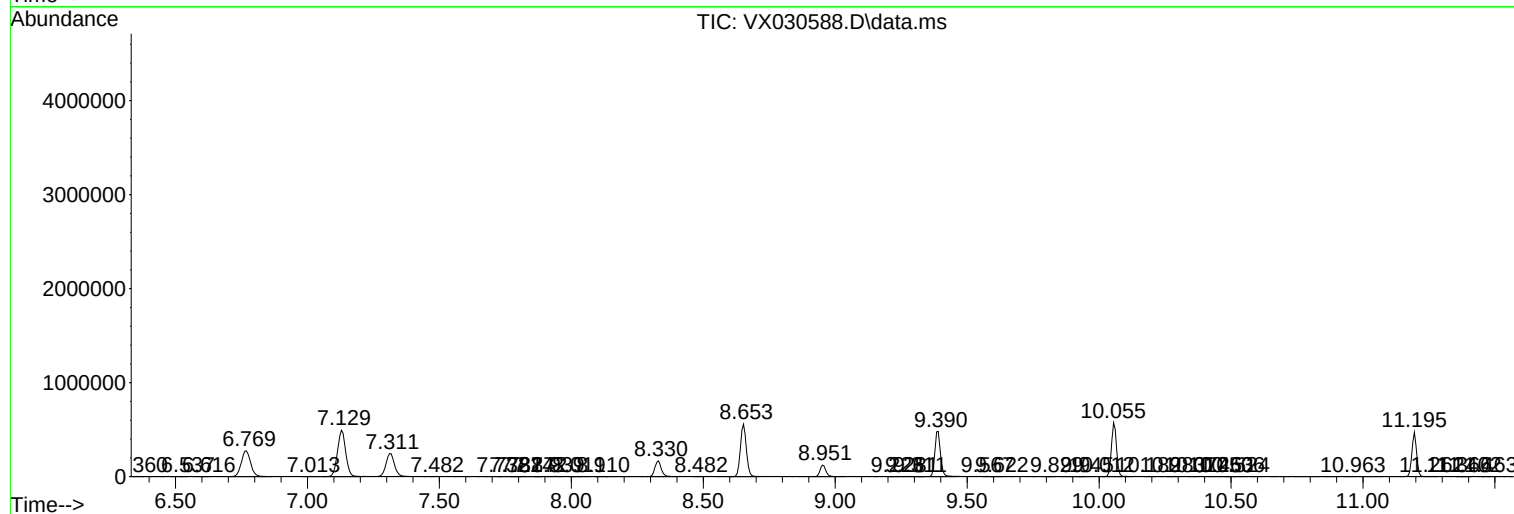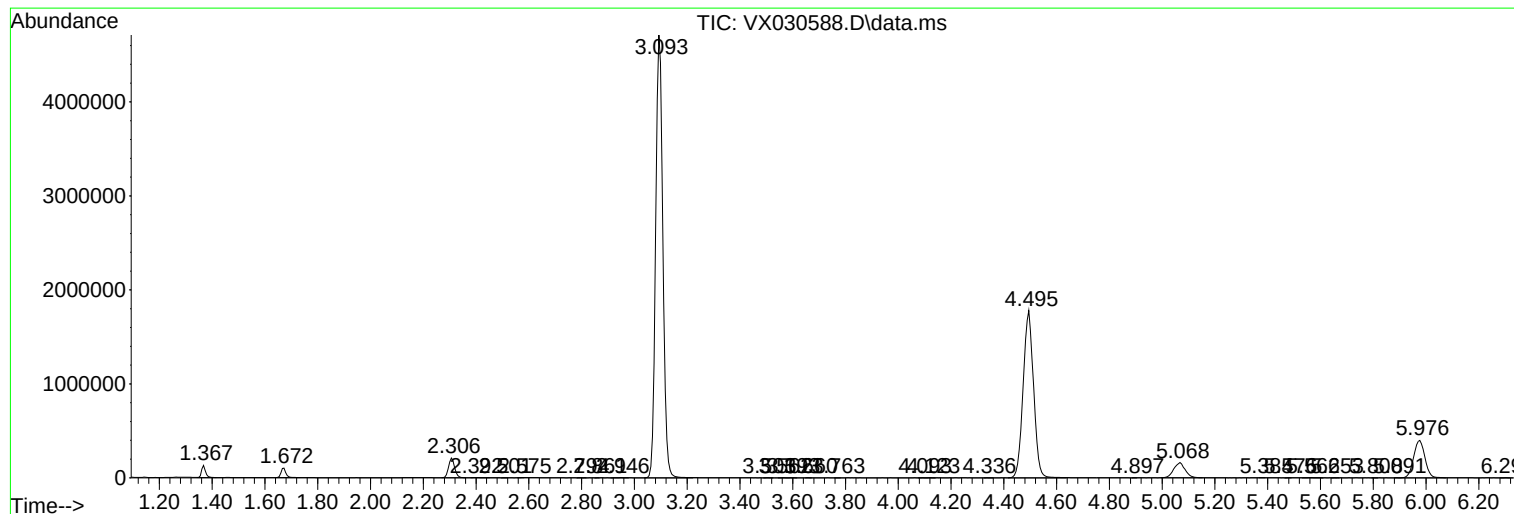

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030588.D
Acq On : 12 Aug 2022 12:50
Operator : JC/MD
Sample : N4144-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EY161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030588.D
Acq On : 12 Aug 2022 12:50
Operator : JC/MD
Sample : N4144-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EY161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc