

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030589.D
 Acq On : 12 Aug 2022 13:13
 Operator : JC/MD
 Sample : VIBLK672
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK672

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	118856	124911	10.60%	1.402%
2	1.666	91	95	103	rVB	99513	128840	10.93%	1.446%
3	2.307	194	200	211	rVB	214235	331304	28.11%	3.719%
4	2.636	253	254	256	rVB	751	473	0.04%	0.005%
5	2.794	275	280	286	rVB6	3923	7656	0.65%	0.086%
6	2.849	286	289	291	rBV2	627	814	0.07%	0.009%
7	2.947	298	305	315	rVB	16554	39359	3.34%	0.442%
8	3.014	315	316	319	rVB2	421	372	0.03%	0.004%
9	3.038	319	320	322	rBV2	396	370	0.03%	0.004%
10	3.093	323	329	337	rVB2	18812	37339	3.17%	0.419%
11	3.361	369	373	377	rBV2	407	543	0.05%	0.006%
12	3.532	400	401	403	rBV2	448	424	0.04%	0.005%
13	3.617	413	415	416	rBV	382	299	0.03%	0.003%
14	3.733	433	434	438	rVB2	423	392	0.03%	0.004%
15	3.855	452	454	456	rVB	517	417	0.04%	0.005%
16	4.111	494	496	500	rVB2	575	424	0.04%	0.005%
17	4.172	504	506	507	rBV2	370	271	0.02%	0.003%
18	4.239	516	517	522	rBV2	428	636	0.05%	0.007%
19	4.355	533	536	537	rBV2	558	617	0.05%	0.007%
20	4.477	545	556	569	rBV	108840	337592	28.64%	3.789%
21	4.861	617	619	621	rBV2	395	395	0.03%	0.004%
22	5.062	639	652	673	rVB	153998	491640	41.71%	5.518%
23	5.202	673	675	676	rBV	620	401	0.03%	0.005%
24	5.556	720	733	735	rBV3	2200	5234	0.44%	0.059%
25	5.885	784	787	788	rBV2	340	310	0.03%	0.003%
26	5.903	788	790	791	rBV2	389	397	0.03%	0.004%
27	5.971	791	801	820	rVV2	395987	1178694	100.00%	13.230%
28	6.227	841	843	849	rVB3	484	875	0.07%	0.010%
29	6.288	849	853	855	rBV2	662	983	0.08%	0.011%
30	6.349	859	863	864	rBV2	369	393	0.03%	0.004%
31	6.428	873	876	878	rBV2	744	832	0.07%	0.009%
32	6.769	922	932	948	rBV	270052	652093	55.32%	7.319%
33	6.970	964	965	966	rBV	465	276	0.02%	0.003%
34	7.111	982	988	999	rVB5	10836	28071	2.38%	0.315%
35	7.184	999	1000	1003	rBV2	564	396	0.03%	0.004%
36	7.214	1003	1005	1006	rBV	508	328	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030589.D
 Acq On : 12 Aug 2022 13:13
 Operator : JC/MD
 Sample : VIBLK672
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK672

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.232	1006	1008	1009	rVB	513	272	0.02%	0.003%
38	7.312	1012	1021	1036	rBV	255956	558036	47.34%	6.263%
39	7.452	1042	1044	1046	rVB	558	490	0.04%	0.005%
40	7.635	1072	1074	1075	rBV2	369	334	0.03%	0.004%
41	7.751	1090	1093	1094	rBV2	289	331	0.03%	0.004%
42	7.818	1103	1104	1106	rBV	676	429	0.04%	0.005%
43	7.934	1120	1123	1131	rVB4	1786	3595	0.30%	0.040%
44	8.086	1146	1148	1150	rBV2	397	419	0.04%	0.005%
45	8.159	1159	1160	1162	rBV	485	393	0.03%	0.004%
46	8.177	1162	1163	1166	rVV2	550	377	0.03%	0.004%
47	8.220	1168	1170	1172	rVB2	644	442	0.04%	0.005%
48	8.330	1181	1188	1201	rBV	171187	284011	24.10%	3.188%
49	8.464	1209	1210	1211	rBV	494	346	0.03%	0.004%
50	8.653	1234	1241	1253	rBV	582096	886523	75.21%	9.950%
51	8.811	1265	1267	1269	rVB	658	425	0.04%	0.005%
52	8.952	1285	1290	1300	rBV	124294	189642	16.09%	2.129%
53	9.147	1320	1322	1323	rBV2	479	474	0.04%	0.005%
54	9.391	1356	1362	1380	rBV	500175	724750	61.49%	8.135%
55	9.708	1410	1414	1419	rVB2	2762	4892	0.42%	0.055%
56	9.750	1419	1421	1424	rBV2	548	714	0.06%	0.008%
57	9.799	1428	1429	1435	rVB2	757	844	0.07%	0.009%
58	10.055	1466	1471	1488	rVB	561636	760420	64.51%	8.535%
59	10.195	1490	1494	1495	rBV2	463	405	0.03%	0.005%
60	10.378	1522	1524	1526	rBV2	464	454	0.04%	0.005%
61	10.817	1594	1596	1599	rBV	562	731	0.06%	0.008%
62	10.939	1614	1616	1618	rVB	582	412	0.03%	0.005%
63	11.085	1639	1640	1642	rBV2	463	425	0.04%	0.005%
64	11.195	1652	1658	1671	rVB	453692	586538	49.76%	6.583%
65	11.342	1679	1682	1685	rBV2	494	675	0.06%	0.008%
66	11.384	1685	1689	1691	rVB2	580	736	0.06%	0.008%
67	11.415	1691	1694	1695	rBV2	446	501	0.04%	0.006%
68	11.488	1704	1706	1707	rBV	429	298	0.03%	0.003%
69	11.543	1713	1715	1717	rBV2	328	307	0.03%	0.003%
70	11.573	1718	1720	1722	rVV2	444	331	0.03%	0.004%
71	11.659	1731	1734	1736	rBV2	659	712	0.06%	0.008%
72	11.793	1754	1756	1760	rVB2	628	758	0.06%	0.009%
73	11.921	1776	1777	1780	rBV2	594	565	0.05%	0.006%
74	11.951	1780	1782	1783	rBV	370	359	0.03%	0.004%
75	12.024	1788	1794	1803	rBV	570353	701485	59.51%	7.874%
76	12.207	1822	1824	1826	rBV2	526	350	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030589.D
 Acq On : 12 Aug 2022 13:13
 Operator : JC/MD
 Sample : VIBLK672
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK672

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.226	1826	1827	1830	rBV	703	534	0.05%	0.006%
78	12.323	1837	1843	1852	rBV	650890	809023	68.64%	9.081%
79	12.677	1899	1901	1903	rBV2	491	579	0.05%	0.006%
80	12.927	1941	1942	1945	rVB	430	269	0.02%	0.003%
81	13.177	1981	1983	1985	rVB	675	467	0.04%	0.005%
82	13.280	1998	2000	2003	rVB2	689	594	0.05%	0.007%
83	13.329	2006	2008	2012	rBV2	530	713	0.06%	0.008%
84	13.366	2012	2014	2015	rBV	576	384	0.03%	0.004%
85	13.451	2026	2028	2032	rVB2	482	483	0.04%	0.005%
86	13.609	2052	2054	2057	rBV2	413	491	0.04%	0.006%
87	13.750	2075	2077	2079	rVB2	517	448	0.04%	0.005%
88	13.774	2079	2081	2084	rBV	473	318	0.03%	0.004%
89	13.841	2090	2092	2095	rVB	541	444	0.04%	0.005%
90	13.890	2098	2100	2102	rBV	431	390	0.03%	0.004%
91	13.951	2108	2110	2111	rBV	537	371	0.03%	0.004%
92	14.109	2134	2136	2137	rBV	432	416	0.04%	0.005%
93	14.499	2196	2200	2201	rBV2	532	604	0.05%	0.007%
94	14.542	2205	2207	2208	rBV	483	346	0.03%	0.004%
95	14.749	2238	2241	2244	rBV2	739	904	0.08%	0.010%
96	14.999	2278	2282	2286	rBV2	656	891	0.08%	0.010%
97	15.347	2337	2339	2340	rBV2	744	443	0.04%	0.005%
98	15.731	2400	2402	2403	rBV2	657	299	0.03%	0.003%
99	15.822	2415	2417	2420	rBV4	748	722	0.06%	0.008%
100	16.719	2562	2564	2566	rVB	931	729	0.06%	0.008%




Sum of corrected areas: 8909434

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030589.D
Acq On : 12 Aug 2022 13:13
Operator : JC/MD
Sample : VIBLK672
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK672

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

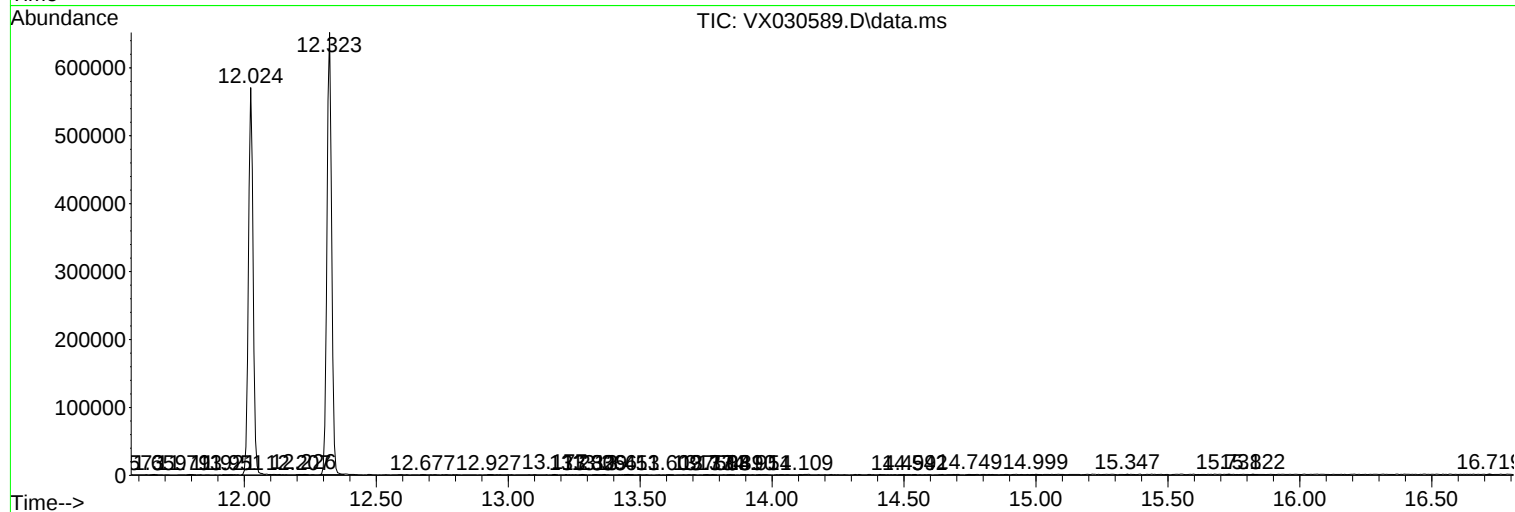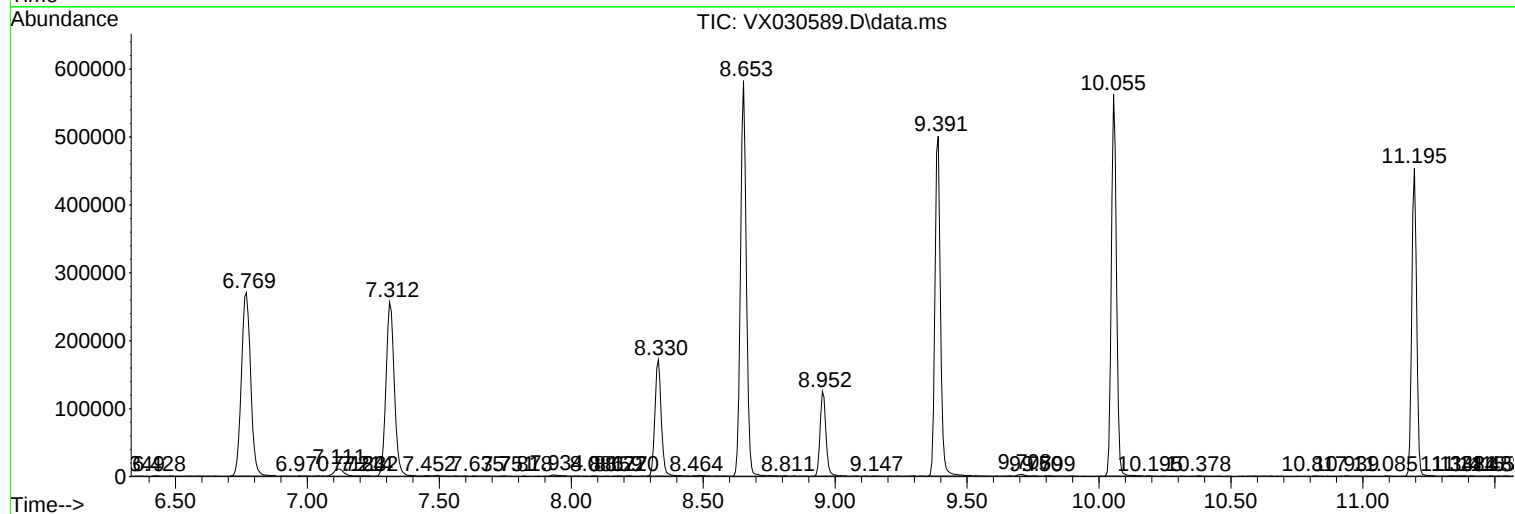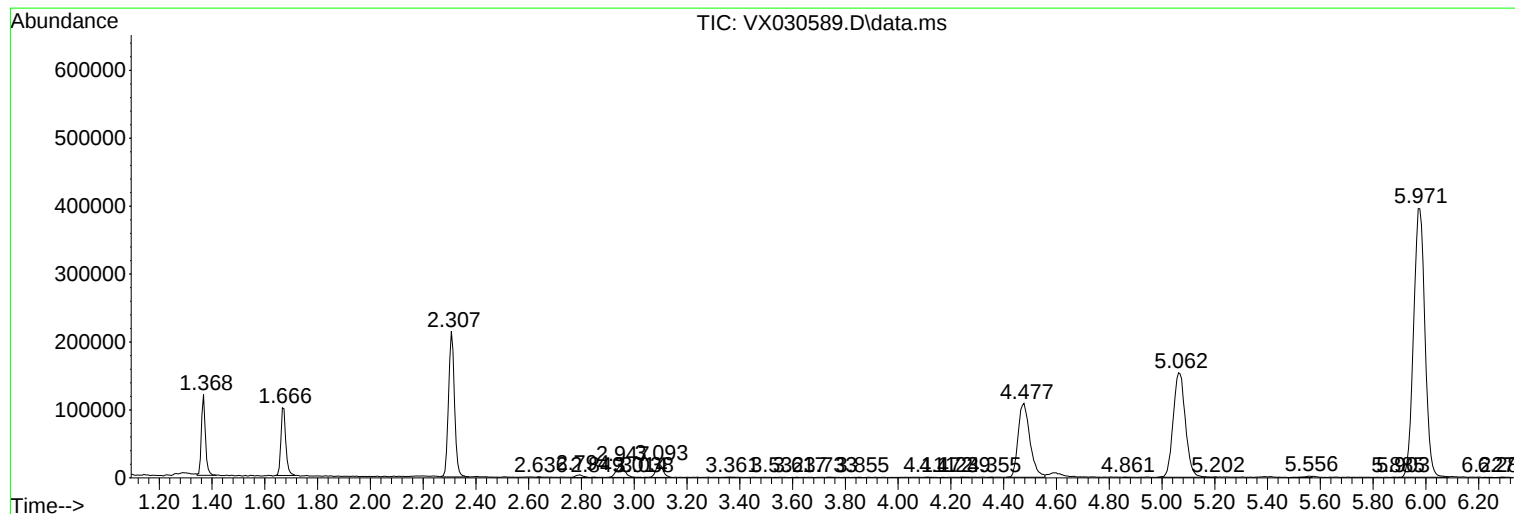

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030589.D
Acq On : 12 Aug 2022 13:13
Operator : JC/MD
Sample : VIBLK672
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK672

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030589.D
Acq On : 12 Aug 2022 13:13
Operator : JC/MD
Sample : VIBLK672
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK672

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc