

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030590.D
 Acq On : 12 Aug 2022 13:37
 Operator : JC/MD
 Sample : N4144-11DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EY161DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030590.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	118261	121543	10.76%	1.302%
2	1.666	91	95	104	rBV	92972	121654	10.77%	1.303%
3	2.014	150	152	154	rBV3	1038	1023	0.09%	0.011%
4	2.307	194	200	210	rVB	206787	314548	27.85%	3.369%
5	2.508	231	233	236	rVB3	999	804	0.07%	0.009%
6	2.587	244	246	248	rBV3	524	606	0.05%	0.006%
7	2.788	275	279	280	rBV2	1978	2256	0.20%	0.024%
8	2.947	297	305	314	rVV	23733	54351	4.81%	0.582%
9	3.093	322	329	340	rBV	215635	406871	36.02%	4.358%
10	3.282	358	360	362	rBV2	546	375	0.03%	0.004%
11	3.489	391	394	398	rBV	447	773	0.07%	0.008%
12	3.758	437	438	440	rBV2	492	381	0.03%	0.004%
13	3.812	445	447	450	rVV3	495	585	0.05%	0.006%
14	4.105	493	495	499	rVB2	584	596	0.05%	0.006%
15	4.385	539	541	544	rBV	715	810	0.07%	0.009%
16	4.483	546	557	571	rBV2	159405	532002	47.10%	5.698%
17	4.757	601	602	604	rBV2	568	379	0.03%	0.004%
18	4.794	606	608	609	rBV2	590	478	0.04%	0.005%
19	4.959	632	635	638	rBV4	393	498	0.04%	0.005%
20	5.062	639	652	672	rVV	157109	474822	42.04%	5.086%
21	5.318	690	694	696	rBV	681	695	0.06%	0.007%
22	5.385	702	705	714	rVB4	1765	4435	0.39%	0.048%
23	5.465	714	718	721	rVB3	663	941	0.08%	0.010%
24	5.501	723	724	728	rVB	690	531	0.05%	0.006%
25	5.556	728	733	739	rBV4	2076	4938	0.44%	0.053%
26	5.769	764	768	769	rBV	579	508	0.04%	0.005%
27	5.867	782	784	785	rBV	481	429	0.04%	0.005%
28	5.977	789	802	820	rBV2	389876	1129443	100.00%	12.097%
29	6.263	847	849	852	rVB2	728	491	0.04%	0.005%
30	6.294	852	854	856	rBV	451	438	0.04%	0.005%
31	6.355	861	864	866	rBV2	592	871	0.08%	0.009%
32	6.611	904	906	908	rBV	415	408	0.04%	0.004%
33	6.653	911	913	917	rVB	584	527	0.05%	0.006%
34	6.769	922	932	944	rBV	287038	684670	60.62%	7.333%
35	7.044	975	977	978	rBV	522	422	0.04%	0.005%
36	7.129	980	991	1001	rBV4	28714	74368	6.58%	0.797%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030590.D
 Acq On : 12 Aug 2022 13:37
 Operator : JC/MD
 Sample : N4144-11DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EY161DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1038	rBV	236961	535199	47.39%	5.732%
38	7.470	1044	1047	1049	rBV2	894	995	0.09%	0.011%
39	7.678	1079	1081	1085	rVB2	608	641	0.06%	0.007%
40	7.714	1085	1087	1090	rBV	449	491	0.04%	0.005%
41	7.812	1100	1103	1106	rBV2	405	565	0.05%	0.006%
42	7.848	1106	1109	1110	rVB2	609	465	0.04%	0.005%
43	7.891	1113	1116	1118	rBV3	707	632	0.06%	0.007%
44	7.940	1120	1124	1125	rBV4	1695	1824	0.16%	0.020%
45	8.080	1144	1147	1150	rBV	249	400	0.04%	0.004%
46	8.330	1181	1188	1200	rVV	159904	265653	23.52%	2.845%
47	8.488	1210	1214	1218	rBV3	956	1525	0.14%	0.016%
48	8.562	1223	1226	1227	rBV2	558	630	0.06%	0.007%
49	8.586	1227	1230	1234	rBV4	1046	1465	0.13%	0.016%
50	8.653	1234	1241	1256	rBV	554811	840095	74.38%	8.998%
51	8.952	1285	1290	1299	rBV	121916	177240	15.69%	1.898%
52	9.055	1305	1307	1309	rBV2	858	517	0.05%	0.006%
53	9.141	1319	1321	1326	rBV4	584	825	0.07%	0.009%
54	9.287	1342	1345	1350	rVB2	597	988	0.09%	0.011%
55	9.391	1356	1362	1375	rBV	480506	696545	61.67%	7.460%
56	9.750	1420	1421	1424	rBV2	589	631	0.06%	0.007%
57	10.000	1458	1462	1463	rBV2	494	605	0.05%	0.006%
58	10.055	1465	1471	1480	rBV	595091	795114	70.40%	8.516%
59	10.336	1516	1517	1519	rBV	551	468	0.04%	0.005%
60	10.390	1524	1526	1528	rVV2	1067	828	0.07%	0.009%
61	10.421	1528	1531	1533	rVV2	513	550	0.05%	0.006%
62	10.458	1533	1537	1538	rVV	521	651	0.06%	0.007%
63	10.506	1544	1545	1549	rVB2	511	487	0.04%	0.005%
64	10.549	1549	1552	1557	rBV2	609	943	0.08%	0.010%
65	10.701	1574	1577	1579	rVB	387	449	0.04%	0.005%
66	10.750	1584	1585	1588	rVB	730	477	0.04%	0.005%
67	10.872	1604	1605	1608	rVV	507	459	0.04%	0.005%
68	10.933	1612	1615	1617	rBV	417	483	0.04%	0.005%
69	10.957	1617	1619	1623	rVB2	420	470	0.04%	0.005%
70	11.079	1637	1639	1641	rVV2	460	370	0.03%	0.004%
71	11.195	1652	1658	1667	rBV	435542	562897	49.84%	6.029%
72	11.360	1683	1685	1688	rVB	681	542	0.05%	0.006%
73	11.402	1691	1692	1696	rVV	509	420	0.04%	0.004%
74	11.476	1702	1704	1707	rVB	863	881	0.08%	0.009%
75	11.506	1707	1709	1711	rBV2	361	426	0.04%	0.005%
76	11.677	1734	1737	1738	rBV	433	380	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030590.D
 Acq On : 12 Aug 2022 13:37
 Operator : JC/MD
 Sample : N4144-11DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EY161DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

77	11.744	1745	1748	1749	rVB2	409	376	0.03%	0.004%
78	11.768	1749	1752	1754	rBV3	461	626	0.06%	0.007%
79	11.854	1764	1766	1769	rBV	498	496	0.04%	0.005%
80	11.902	1772	1774	1777	rVB2	308	374	0.03%	0.004%
81	12.024	1789	1794	1801	rVV	607042	728174	64.47%	7.799%
82	12.226	1825	1827	1829	rVB2	729	619	0.05%	0.007%
83	12.274	1833	1835	1837	rBV2	407	363	0.03%	0.004%
84	12.323	1837	1843	1853	rBV	609120	762436	67.51%	8.166%
85	12.494	1870	1871	1874	rVB2	634	512	0.05%	0.005%
86	12.530	1874	1877	1878	rBV2	325	386	0.03%	0.004%
87	12.573	1880	1884	1885	rBV	803	719	0.06%	0.008%
88	12.652	1893	1897	1898	rBV2	538	687	0.06%	0.007%
89	12.823	1923	1925	1929	rBV	524	747	0.07%	0.008%
90	13.122	1971	1974	1976	rBV	764	783	0.07%	0.008%
91	13.372	2013	2015	2018	rBV2	551	660	0.06%	0.007%
92	13.530	2039	2041	2042	rVB2	576	357	0.03%	0.004%
93	13.884	2095	2099	2100	rBV2	422	427	0.04%	0.005%
94	13.957	2109	2111	2112	rBV	387	372	0.03%	0.004%
95	14.079	2128	2131	2133	rBV	485	367	0.03%	0.004%
96	14.134	2138	2140	2144	rBV3	854	859	0.08%	0.009%
97	14.475	2194	2196	2200	rBV3	445	507	0.04%	0.005%
98	14.871	2259	2261	2262	rBV	477	355	0.03%	0.004%
99	15.627	2383	2385	2386	rVB	774	451	0.04%	0.005%
100	15.993	2443	2445	2446	rBV2	625	367	0.03%	0.004%




Sum of corrected areas: 9336716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030590.D
Acq On : 12 Aug 2022 13:37
Operator : JC/MD
Sample : N4144-11DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EY161DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

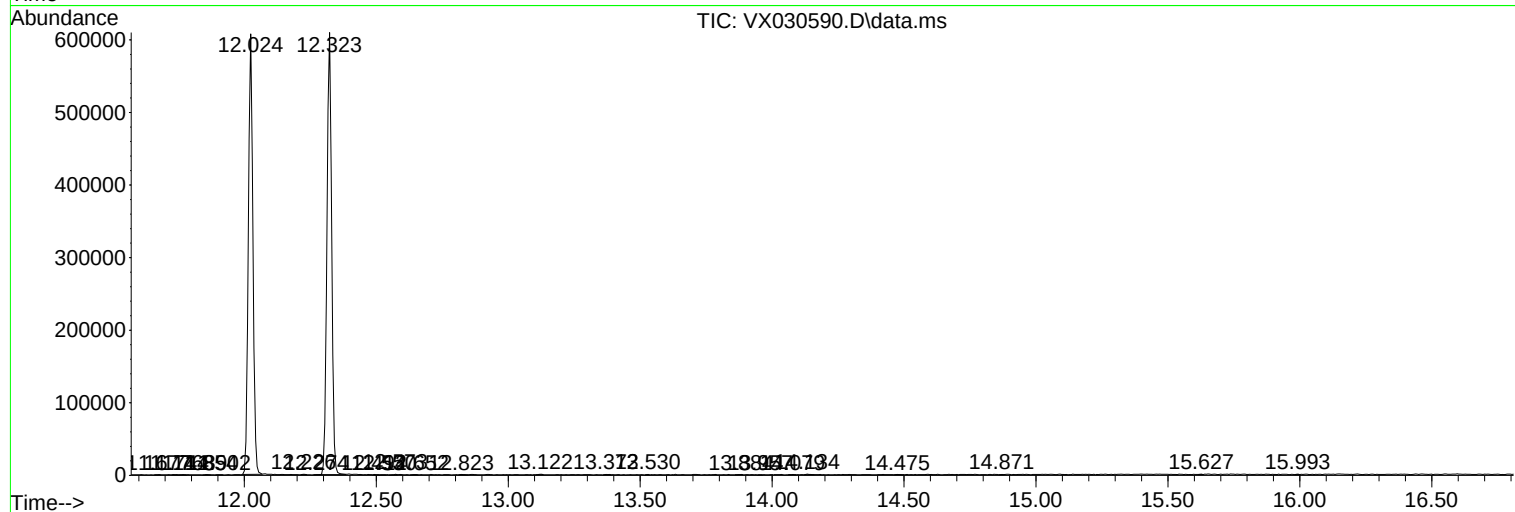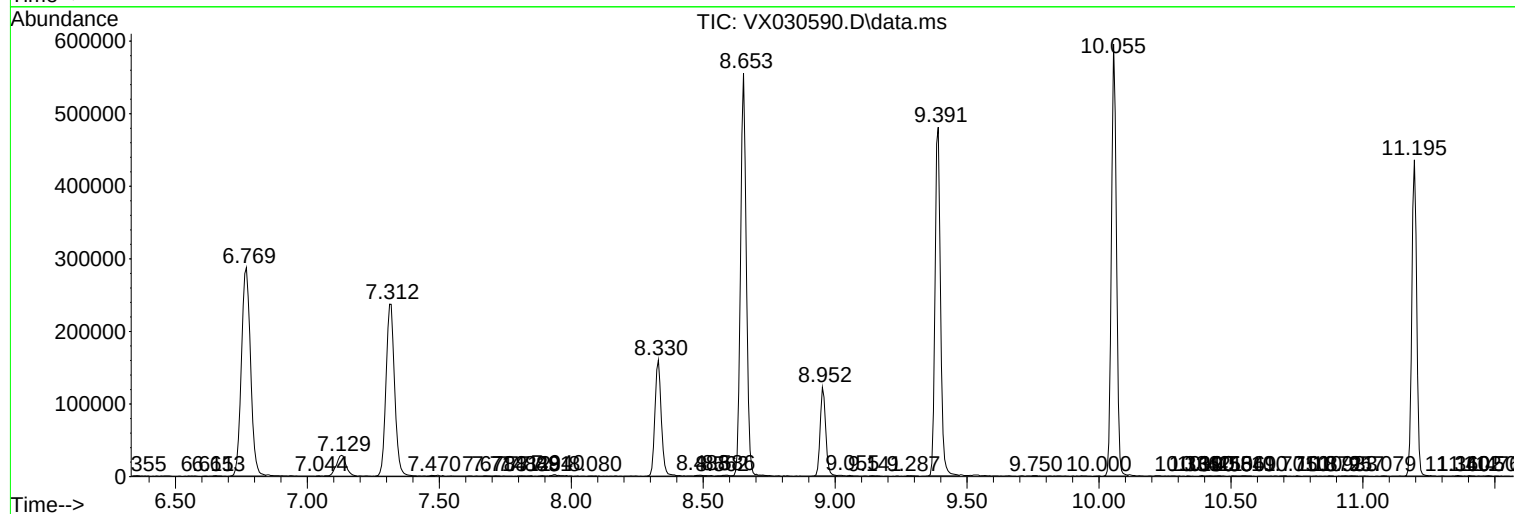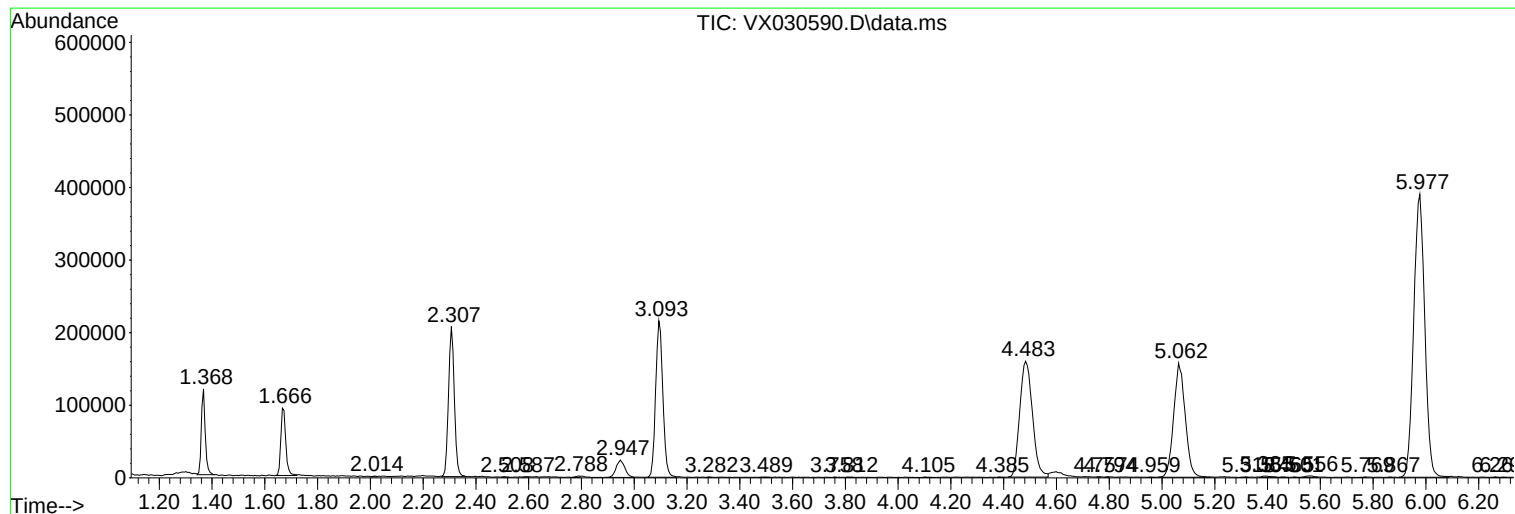

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030590.D
Acq On : 12 Aug 2022 13:37
Operator : JC/MD
Sample : N4144-11DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EY161DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030590.D
Acq On : 12 Aug 2022 13:37
Operator : JC/MD
Sample : N4144-11DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EY161DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc