

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030591.D
 Acq On : 12 Aug 2022 14:00
 Operator : JC/MD
 Sample : N4144-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030591.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	119840	126424	11.07%	1.469%
2	1.672	91	96	103	rVB	97238	121833	10.67%	1.416%
3	2.307	194	200	210	rVB	205515	315383	27.61%	3.665%
4	2.508	231	233	237	rBV3	590	608	0.05%	0.007%
5	2.788	275	279	285	rVB3	4210	7739	0.68%	0.090%
6	2.953	300	306	311	rBV2	969	2156	0.19%	0.025%
7	3.002	311	314	317	rVB2	571	662	0.06%	0.008%
8	3.038	318	320	323	rVB	537	322	0.03%	0.004%
9	3.093	323	329	335	rBV4	4190	7593	0.66%	0.088%
10	3.197	343	346	347	rBV	376	393	0.03%	0.005%
11	3.270	356	358	361	rVB2	677	835	0.07%	0.010%
12	3.300	361	363	365	rBV2	409	377	0.03%	0.004%
13	3.379	373	376	377	rBV3	491	470	0.04%	0.005%
14	3.447	385	387	390	rBV2	264	333	0.03%	0.004%
15	3.544	400	403	404	rBV2	352	319	0.03%	0.004%
16	3.825	447	449	451	rBV	549	483	0.04%	0.006%
17	3.867	455	456	458	rVB2	522	362	0.03%	0.004%
18	3.898	458	461	462	rBV	491	386	0.03%	0.004%
19	3.977	473	474	476	rBV	479	315	0.03%	0.004%
20	4.117	495	497	499	rBV	429	415	0.04%	0.005%
21	4.178	506	507	509	rBV	487	334	0.03%	0.004%
22	4.471	546	555	570	rBV	104128	325656	28.51%	3.785%
23	4.806	609	610	613	rVB2	524	353	0.03%	0.004%
24	5.068	641	653	668	rBV2	146539	476720	41.73%	5.540%
25	5.245	681	682	686	rVB4	695	645	0.06%	0.007%
26	5.367	699	702	703	rBV2	470	500	0.04%	0.006%
27	5.385	703	705	706	rBV2	805	520	0.05%	0.006%
28	5.556	725	733	739	rBV3	2277	5316	0.47%	0.062%
29	5.635	743	746	748	rBV3	441	615	0.05%	0.007%
30	5.977	790	802	818	rBV2	392175	1142350	100.00%	13.276%
31	6.330	859	860	863	rVB2	495	364	0.03%	0.004%
32	6.367	863	866	867	rBV2	460	503	0.04%	0.006%
33	6.525	889	892	894	rBV	598	590	0.05%	0.007%
34	6.550	894	896	898	rVV3	366	304	0.03%	0.004%
35	6.653	911	913	914	rBV	436	313	0.03%	0.004%
36	6.769	922	932	943	rBV	283689	667780	58.46%	7.761%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030591.D
 Acq On : 12 Aug 2022 14:00
 Operator : JC/MD
 Sample : N4144-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.123	983	990	999	rVB5	8425	21135	1.85%	0.246%
38	7.312	1013	1021	1034	rBV	247846	538439	47.13%	6.257%
39	7.464	1044	1046	1047	rBV	991	640	0.06%	0.007%
40	7.495	1049	1051	1053	rVB2	892	748	0.07%	0.009%
41	7.592	1066	1067	1069	rBV	398	412	0.04%	0.005%
42	7.659	1074	1078	1079	rBV	466	439	0.04%	0.005%
43	7.684	1079	1082	1084	rVB2	339	411	0.04%	0.005%
44	7.708	1084	1086	1087	rBV	428	325	0.03%	0.004%
45	7.940	1118	1124	1129	rBV4	1877	3826	0.33%	0.044%
46	8.055	1142	1143	1145	rVB	491	343	0.03%	0.004%
47	8.177	1161	1163	1165	rBV	384	365	0.03%	0.004%
48	8.263	1176	1177	1180	rVB2	367	362	0.03%	0.004%
49	8.330	1180	1188	1198	rBV	165802	272476	23.85%	3.167%
50	8.482	1211	1213	1217	rVB3	993	1051	0.09%	0.012%
51	8.653	1234	1241	1255	rBV	557687	860141	75.30%	9.996%
52	8.952	1284	1290	1303	rBV	118091	182521	15.98%	2.121%
53	9.110	1314	1316	1318	rBV	397	361	0.03%	0.004%
54	9.220	1331	1334	1337	rBV2	702	896	0.08%	0.010%
55	9.391	1356	1362	1378	rBV	480569	706688	61.86%	8.213%
56	9.793	1425	1428	1429	rBV2	593	380	0.03%	0.004%
57	9.848	1435	1437	1440	rVB	439	326	0.03%	0.004%
58	9.958	1453	1455	1458	rBV2	328	323	0.03%	0.004%
59	10.000	1460	1462	1465	rVB3	506	439	0.04%	0.005%
60	10.055	1465	1471	1483	rBV	580316	787848	68.97%	9.156%
61	10.195	1492	1494	1497	rBV	835	704	0.06%	0.008%
62	10.311	1510	1513	1514	rVV2	579	465	0.04%	0.005%
63	10.390	1523	1526	1527	rBV	370	314	0.03%	0.004%
64	10.427	1530	1532	1535	rBV2	515	484	0.04%	0.006%
65	10.573	1554	1556	1560	rBV2	513	943	0.08%	0.011%
66	10.701	1575	1577	1579	rVB2	488	364	0.03%	0.004%
67	10.848	1597	1601	1602	rBV2	615	710	0.06%	0.008%
68	10.933	1610	1615	1617	rBV2	608	771	0.07%	0.009%
69	11.092	1639	1641	1643	rVV2	468	342	0.03%	0.004%
70	11.116	1643	1645	1647	rVB3	492	368	0.03%	0.004%
71	11.195	1652	1658	1671	rVB	461759	570083	49.90%	6.625%
72	11.482	1703	1705	1708	rBV2	423	507	0.04%	0.006%
73	11.701	1739	1741	1744	rVV2	411	377	0.03%	0.004%
74	11.774	1751	1753	1755	rVB	507	339	0.03%	0.004%
75	12.024	1788	1794	1808	rBV	575589	693058	60.67%	8.054%
76	12.232	1823	1828	1832	rVB4	1954	3219	0.28%	0.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030591.D
 Acq On : 12 Aug 2022 14:00
 Operator : JC/MD
 Sample : N4144-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1852	rBV	593865	729777	63.88%	8.481%
78	12.457	1863	1865	1867	rBV	662	433	0.04%	0.005%
79	12.670	1898	1900	1904	rBV3	389	510	0.04%	0.006%
80	12.713	1905	1907	1911	rVB2	728	713	0.06%	0.008%
81	12.768	1914	1916	1918	rVB	543	316	0.03%	0.004%
82	12.847	1927	1929	1933	rVB	609	628	0.05%	0.007%
83	13.091	1966	1969	1970	rBV	414	369	0.03%	0.004%
84	13.317	2004	2006	2009	rBV	426	480	0.04%	0.006%
85	13.487	2032	2034	2036	rVB	484	403	0.04%	0.005%
86	13.597	2049	2052	2053	rBV2	483	384	0.03%	0.004%
87	13.622	2053	2056	2057	rBV2	445	365	0.03%	0.004%
88	13.743	2074	2076	2080	rBV	323	414	0.04%	0.005%
89	13.957	2109	2111	2112	rVB2	491	324	0.03%	0.004%
90	14.042	2124	2125	2127	rBV	500	333	0.03%	0.004%
91	14.524	2201	2204	2205	rBV	442	509	0.04%	0.006%
92	14.640	2221	2223	2224	rBV2	406	366	0.03%	0.004%
93	14.737	2238	2239	2240	rBV	609	314	0.03%	0.004%
94	14.768	2242	2244	2245	rVB2	804	426	0.04%	0.005%
95	15.079	2291	2295	2296	rBV3	781	999	0.09%	0.012%
96	15.322	2333	2335	2338	rBV2	623	491	0.04%	0.006%
97	15.383	2343	2345	2347	rBV2	700	607	0.05%	0.007%
98	15.487	2360	2362	2363	rVB2	738	385	0.03%	0.004%
99	15.908	2430	2431	2434	rBV3	550	534	0.05%	0.006%
100	16.682	2556	2558	2559	rBV	660	557	0.05%	0.006%




Sum of corrected areas: 8604851

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030591.D
Acq On : 12 Aug 2022 14:00
Operator : JC/MD
Sample : N4144-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

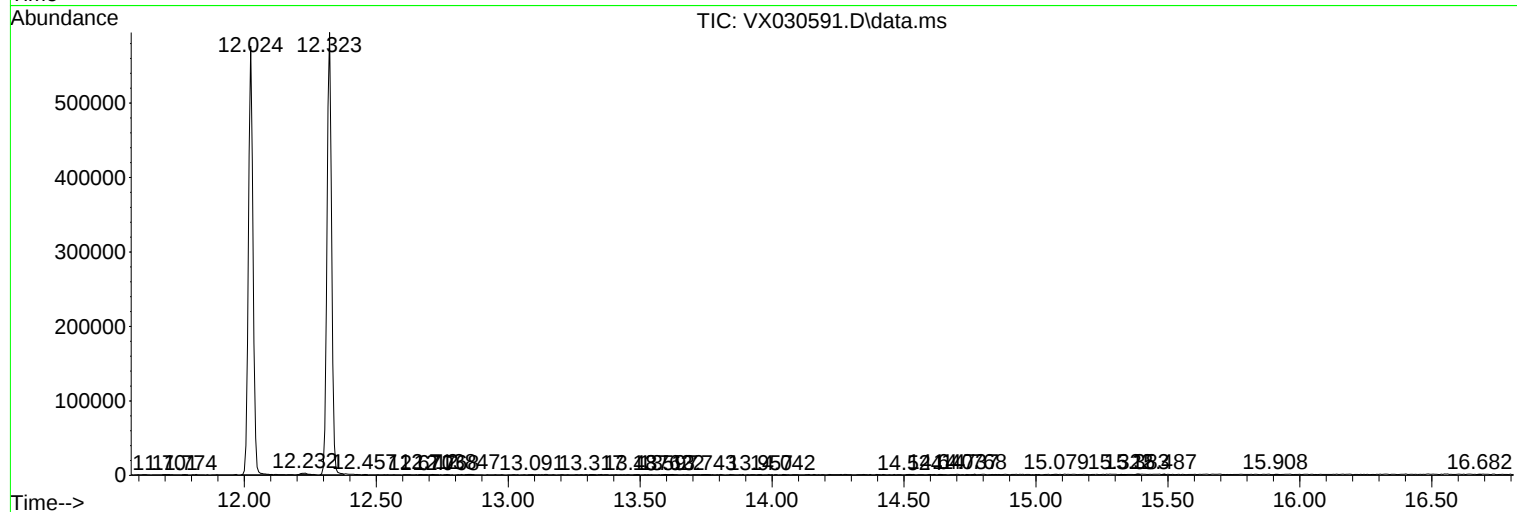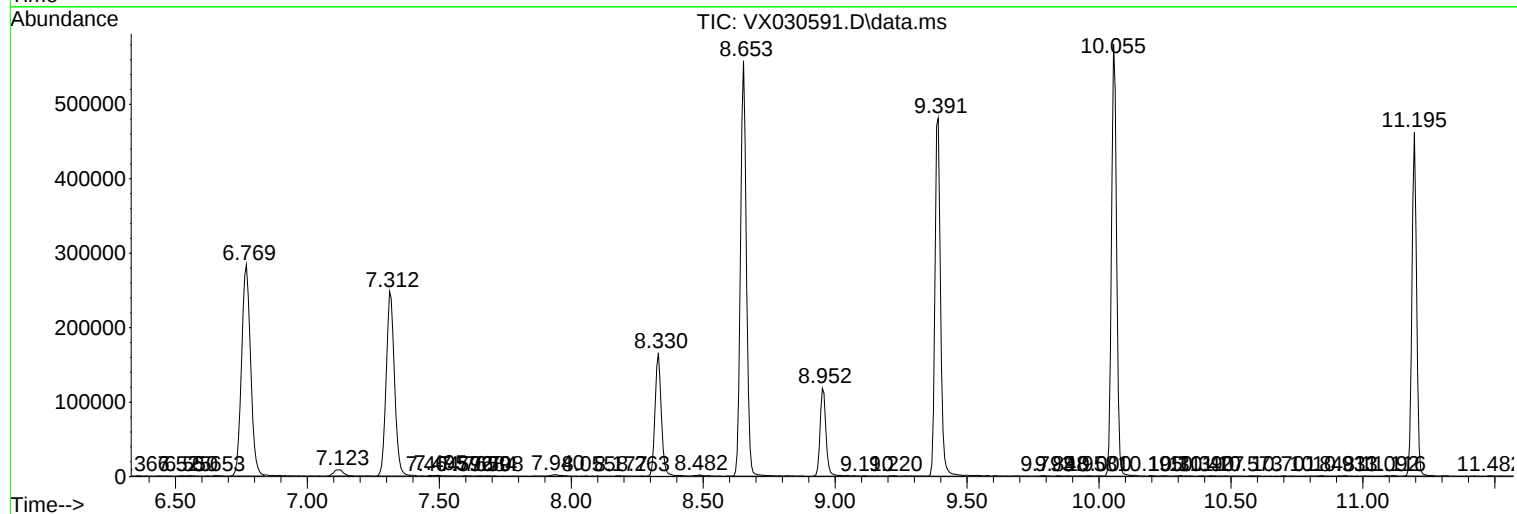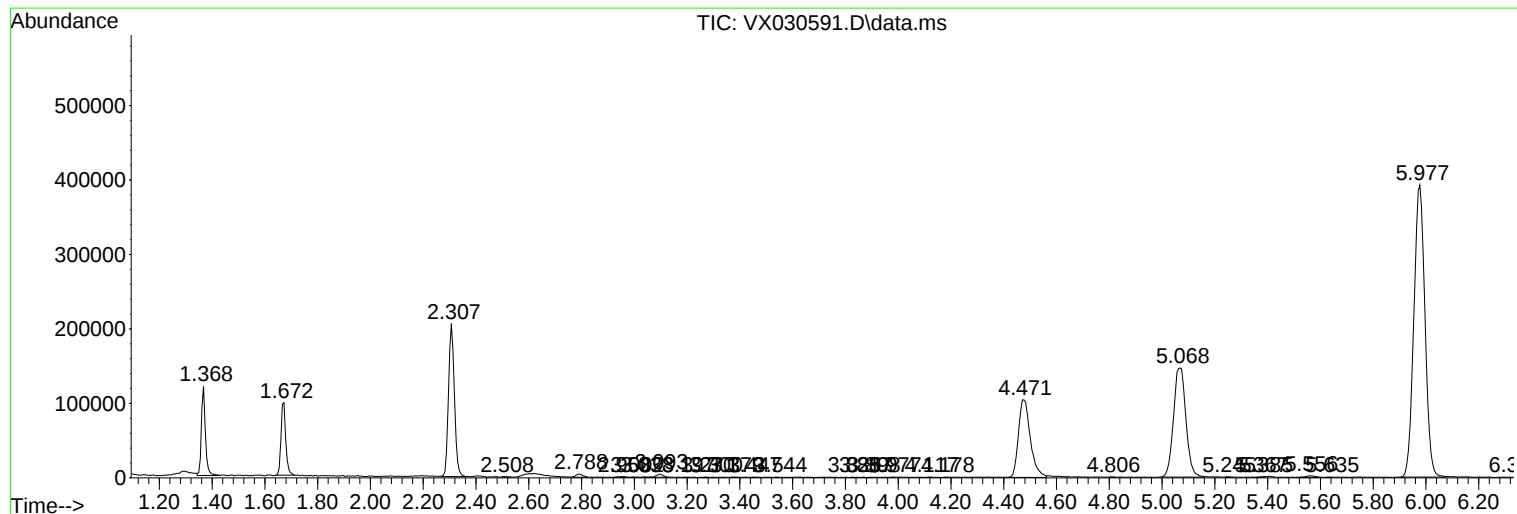

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030591.D
Acq On : 12 Aug 2022 14:00
Operator : JC/MD
Sample : N4144-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030591.D
Acq On : 12 Aug 2022 14:00
Operator : JC/MD
Sample : N4144-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc