

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030592.D
 Acq On : 12 Aug 2022 14:24
 Operator : JC/MD
 Sample : N4110-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	115485	123939	10.91%	1.443%
2	1.672	91	96	106	rVB	94972	125896	11.08%	1.465%
3	2.306	194	200	211	rVB	217031	325227	28.63%	3.785%
4	2.569	240	243	244	rBV3	671	575	0.05%	0.007%
5	2.672	256	260	262	rVB	564	562	0.05%	0.007%
6	2.788	275	279	284	rVB3	1898	2935	0.26%	0.034%
7	2.953	300	306	316	rVB2	7954	18229	1.60%	0.212%
8	3.099	322	330	334	rBV5	2718	5703	0.50%	0.066%
9	3.154	337	339	342	rVV	504	523	0.05%	0.006%
10	3.209	346	348	349	rVB	637	349	0.03%	0.004%
11	3.233	349	352	356	rBV3	428	621	0.05%	0.007%
12	3.318	364	366	368	rBV	516	315	0.03%	0.004%
13	3.361	372	373	377	rBV2	473	475	0.04%	0.006%
14	3.562	404	406	409	rBV2	287	314	0.03%	0.004%
15	3.587	409	410	413	rVB	566	460	0.04%	0.005%
16	3.635	416	418	421	rVB2	598	661	0.06%	0.008%
17	3.666	421	423	425	rBV	589	586	0.05%	0.007%
18	3.739	433	435	437	rVB2	617	452	0.04%	0.005%
19	3.922	463	465	467	rBV	614	454	0.04%	0.005%
20	4.032	479	483	484	rBV	471	646	0.06%	0.008%
21	4.129	496	499	501	rBV	287	369	0.03%	0.004%
22	4.477	547	556	570	rVV	104160	320024	28.18%	3.725%
23	4.788	605	607	609	rBV3	504	375	0.03%	0.004%
24	4.830	612	614	616	rBV2	386	308	0.03%	0.004%
25	5.068	640	653	669	rBV	156837	476033	41.91%	5.541%
26	5.294	689	690	692	rBV2	462	294	0.03%	0.003%
27	5.519	725	727	728	rBV	371	321	0.03%	0.004%
28	5.556	728	733	741	rVV5	2222	5479	0.48%	0.064%
29	5.842	776	780	782	rBV2	354	394	0.03%	0.005%
30	5.976	789	802	818	rBV2	392895	1135786	100.00%	13.220%
31	6.220	841	842	847	rVB2	411	468	0.04%	0.005%
32	6.300	853	855	857	rVB	369	333	0.03%	0.004%
33	6.324	857	859	861	rBV	442	361	0.03%	0.004%
34	6.354	861	864	865	rBV2	385	379	0.03%	0.004%
35	6.452	878	880	882	rVB	590	450	0.04%	0.005%
36	6.556	893	897	899	rBV3	774	843	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030592.D
 Acq On : 12 Aug 2022 14:24
 Operator : JC/MD
 Sample : N4110-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.708	920	922	923	rBV	500	407	0.04%	0.005%
38	6.769	923	932	947	rVV	282653	651258	57.34%	7.580%
39	6.982	966	967	970	rVB2	586	407	0.04%	0.005%
40	7.110	982	988	998	rVB3	10042	23525	2.07%	0.274%
41	7.196	998	1002	1004	rBV2	587	830	0.07%	0.010%
42	7.312	1012	1021	1036	rBV	240959	543415	47.84%	6.325%
43	7.440	1041	1042	1045	rBV	530	454	0.04%	0.005%
44	7.738	1088	1091	1093	rVB2	354	352	0.03%	0.004%
45	7.939	1119	1124	1129	rVB4	2293	3739	0.33%	0.044%
46	7.988	1130	1132	1134	rVB	687	597	0.05%	0.007%
47	8.013	1134	1136	1139	rBV	469	615	0.05%	0.007%
48	8.061	1142	1144	1147	rBV	411	401	0.04%	0.005%
49	8.098	1147	1150	1151	rBV2	344	332	0.03%	0.004%
50	8.202	1163	1167	1169	rVB	285	328	0.03%	0.004%
51	8.330	1182	1188	1200	rVB	162418	266946	23.50%	3.107%
52	8.482	1209	1213	1218	rVB4	1207	2055	0.18%	0.024%
53	8.586	1228	1230	1234	rVB2	687	554	0.05%	0.006%
54	8.653	1234	1241	1252	rBV	559634	853524	75.15%	9.935%
55	8.878	1275	1278	1281	rVB	579	621	0.05%	0.007%
56	8.909	1281	1283	1284	rBV	379	308	0.03%	0.004%
57	8.952	1285	1290	1304	rVV	123183	179837	15.83%	2.093%
58	9.226	1332	1335	1336	rBV	749	521	0.05%	0.006%
59	9.275	1341	1343	1345	rVB	708	466	0.04%	0.005%
60	9.299	1345	1347	1350	rBV	477	372	0.03%	0.004%
61	9.390	1356	1362	1374	rBV	478262	703111	61.91%	8.184%
62	9.701	1409	1413	1421	rVB3	2949	4318	0.38%	0.050%
63	9.835	1431	1435	1438	rVB3	405	632	0.06%	0.007%
64	10.055	1466	1471	1483	rVV	568492	761228	67.02%	8.860%
65	10.171	1489	1490	1493	rVB2	655	388	0.03%	0.005%
66	10.195	1493	1494	1497	rVB2	703	492	0.04%	0.006%
67	10.268	1503	1506	1510	rBV2	348	480	0.04%	0.006%
68	10.378	1522	1524	1526	rBV2	456	306	0.03%	0.004%
69	10.470	1537	1539	1540	rBV2	479	374	0.03%	0.004%
70	10.567	1552	1555	1556	rBV	441	580	0.05%	0.007%
71	10.640	1566	1567	1571	rVB2	535	449	0.04%	0.005%
72	10.841	1598	1600	1602	rBV3	382	297	0.03%	0.003%
73	11.128	1645	1647	1648	rVB2	471	293	0.03%	0.003%
74	11.195	1652	1658	1667	rBV	456781	572037	50.36%	6.658%
75	11.329	1678	1680	1682	rVB3	586	401	0.04%	0.005%
76	11.433	1695	1697	1700	rVB2	464	482	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030592.D
 Acq On : 12 Aug 2022 14:24
 Operator : JC/MD
 Sample : N4110-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.482	1702	1705	1707	rVV2	628	529	0.05%	0.006%
78	11.567	1717	1719	1721	rVB	444	339	0.03%	0.004%
79	11.591	1721	1723	1726	rBV2	333	457	0.04%	0.005%
80	11.664	1732	1735	1739	rBV	449	601	0.05%	0.007%
81	11.756	1748	1750	1752	rVV2	363	345	0.03%	0.004%
82	11.963	1782	1784	1786	rBV2	364	337	0.03%	0.004%
83	12.024	1789	1794	1802	rVV	557697	693630	61.07%	8.074%
84	12.170	1816	1818	1819	rBV	311	297	0.03%	0.003%
85	12.225	1822	1827	1832	rBV7	1697	3402	0.30%	0.040%
86	12.323	1837	1843	1857	rBV	602066	753476	66.34%	8.770%
87	12.494	1869	1871	1873	rBV2	416	422	0.04%	0.005%
88	12.591	1886	1887	1888	rBV	564	330	0.03%	0.004%
89	13.329	2005	2008	2010	rBV2	576	605	0.05%	0.007%
90	13.554	2043	2045	2048	rBV2	406	468	0.04%	0.005%
91	13.981	2114	2115	2120	rVB	522	611	0.05%	0.007%
92	14.127	2134	2139	2142	rBV3	713	1150	0.10%	0.013%
93	14.207	2150	2152	2155	rBV2	469	425	0.04%	0.005%
94	14.542	2206	2207	2210	rBV3	550	447	0.04%	0.005%
95	14.670	2225	2228	2230	rVV2	522	506	0.04%	0.006%
96	14.877	2260	2262	2264	rBV2	447	461	0.04%	0.005%
97	15.591	2377	2379	2382	rBV3	676	776	0.07%	0.009%
98	16.048	2451	2454	2456	rBV	742	826	0.07%	0.010%
99	16.279	2490	2492	2494	rBV2	812	837	0.07%	0.010%
100	16.596	2542	2544	2549	rBV3	751	1243	0.11%	0.014%




Sum of corrected areas: 8591391

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030592.D
Acq On : 12 Aug 2022 14:24
Operator : JC/MD
Sample : N4110-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

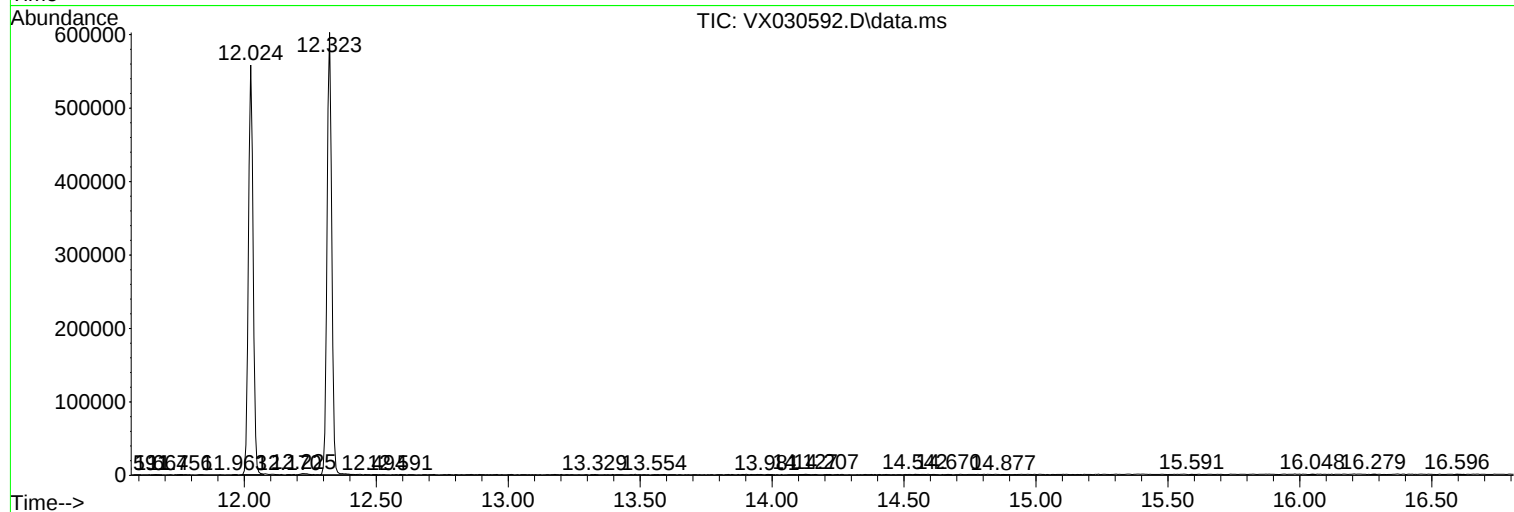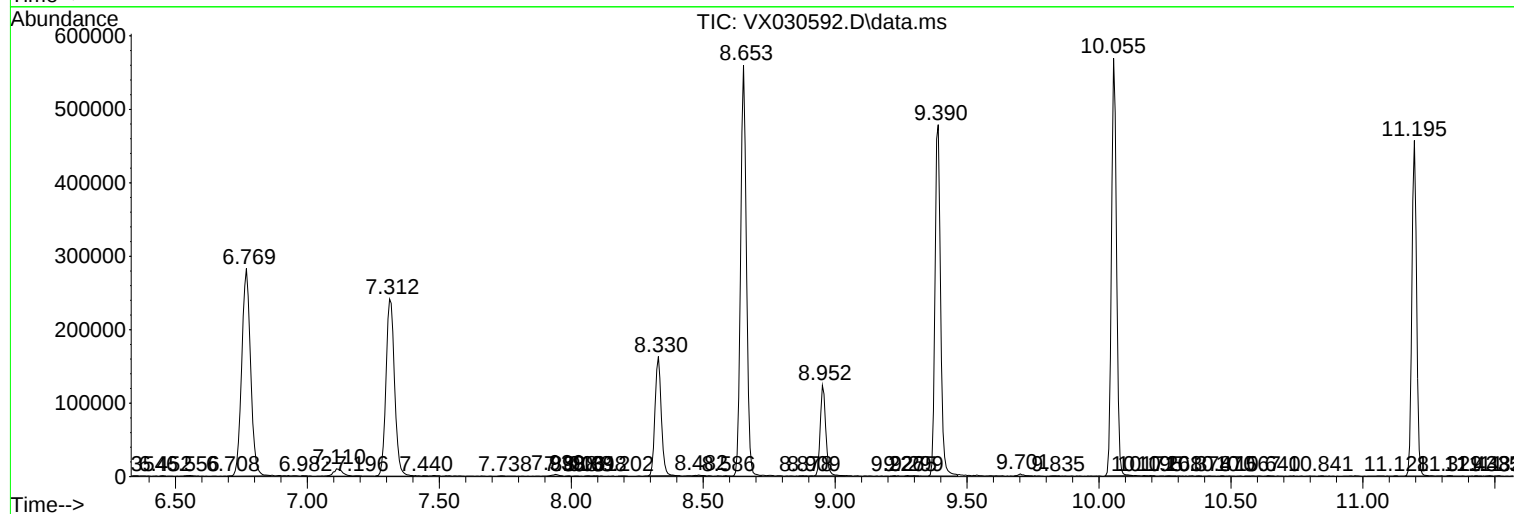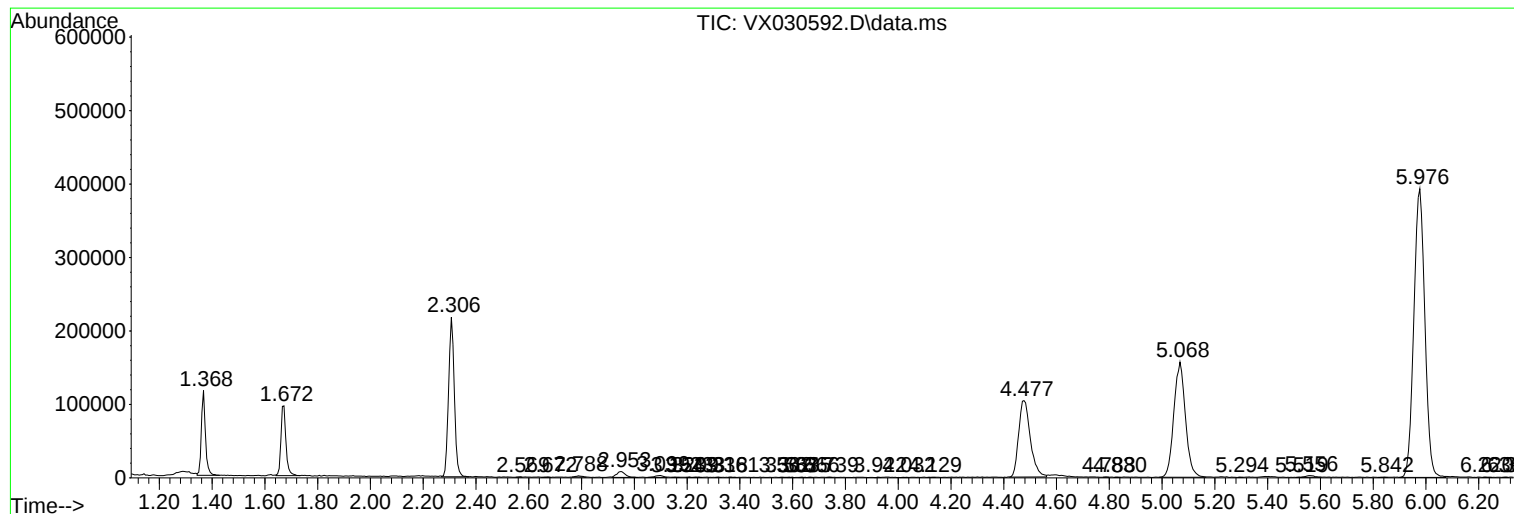

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030592.D
Acq On : 12 Aug 2022 14:24
Operator : JC/MD
Sample : N4110-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030592.D
Acq On : 12 Aug 2022 14:24
Operator : JC/MD
Sample : N4110-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
