

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030593.D
 Acq On : 12 Aug 2022 14:47
 Operator : JC/MD
 Sample : N4131-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB2	267651	311788	5.18%	2.169%
2	1.666	91	95	106	rVB	96783	123391	2.05%	0.858%
3	2.307	194	200	212	rVB	202477	312416	5.19%	2.173%
4	2.489	229	230	231	rBV	608	348	0.01%	0.002%
5	2.617	250	251	254	rBV	555	557	0.01%	0.004%
6	2.727	267	269	270	rVB	617	354	0.01%	0.002%
7	2.831	283	286	287	rBV3	430	462	0.01%	0.003%
8	2.947	303	305	307	rBV2	843	667	0.01%	0.005%
9	3.093	320	329	344	rBV	83715	161044	2.68%	1.120%
10	3.508	394	397	398	rBV2	445	365	0.01%	0.003%
11	3.818	445	448	449	rBV	405	403	0.01%	0.003%
12	3.867	454	456	460	rVB2	642	366	0.01%	0.003%
13	4.032	482	483	487	rBV	302	427	0.01%	0.003%
14	4.074	487	490	493	rVV2	502	607	0.01%	0.004%
15	4.190	506	509	511	rBV2	702	819	0.01%	0.006%
16	4.337	531	533	535	rBV	477	601	0.01%	0.004%
17	4.495	546	559	580	rBV	2202048	6017179	100.00%	41.853%
18	5.068	641	653	669	rBV	147193	463922	7.71%	3.227%
19	5.379	701	704	705	rBV2	1104	1184	0.02%	0.008%
20	5.556	730	733	741	rVB5	2217	4126	0.07%	0.029%
21	5.617	741	743	746	rVB	586	622	0.01%	0.004%
22	5.666	746	751	752	rBV3	654	716	0.01%	0.005%
23	5.727	759	761	764	rBV	497	535	0.01%	0.004%
24	5.891	783	788	790	rBV2	456	728	0.01%	0.005%
25	5.977	790	802	817	rBV2	381861	1098965	18.26%	7.644%
26	6.214	839	841	845	rVB2	552	503	0.01%	0.003%
27	6.251	845	847	849	rVB	621	499	0.01%	0.003%
28	6.367	861	866	869	rVB4	563	1123	0.02%	0.008%
29	6.556	895	897	898	rBV2	472	354	0.01%	0.002%
30	6.684	915	918	921	rVB3	561	509	0.01%	0.004%
31	6.769	921	932	945	rBV	275144	653789	10.87%	4.548%
32	7.123	981	990	997	rBV6	7378	19863	0.33%	0.138%
33	7.312	1013	1021	1034	rBV	230741	515075	8.56%	3.583%
34	7.470	1043	1047	1048	rBV3	613	731	0.01%	0.005%
35	7.848	1108	1109	1115	rVB2	600	623	0.01%	0.004%
36	7.903	1117	1118	1120	rBV2	562	428	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030593.D
 Acq On : 12 Aug 2022 14:47
 Operator : JC/MD
 Sample : N4131-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.934	1120	1123	1130	rVB2	1727	3162	0.05%	0.022%
38	8.043	1138	1141	1144	rVB2	640	721	0.01%	0.005%
39	8.123	1153	1154	1157	rVV2	469	410	0.01%	0.003%
40	8.147	1157	1158	1161	rVB	493	407	0.01%	0.003%
41	8.330	1181	1188	1198	rBV	153307	254513	4.23%	1.770%
42	8.525	1219	1220	1224	rBV3	685	683	0.01%	0.005%
43	8.555	1224	1225	1228	rVB2	617	476	0.01%	0.003%
44	8.653	1234	1241	1249	rBV	539730	818744	13.61%	5.695%
45	8.897	1279	1281	1285	rVB	430	346	0.01%	0.002%
46	8.958	1285	1291	1300	rBV	113128	173904	2.89%	1.210%
47	9.147	1320	1322	1325	rBV2	612	452	0.01%	0.003%
48	9.202	1328	1331	1332	rBV2	397	410	0.01%	0.003%
49	9.275	1339	1343	1349	rBV3	6794	10507	0.17%	0.073%
50	9.391	1356	1362	1374	rBV	461258	660884	10.98%	4.597%
51	9.848	1435	1437	1440	rVB2	529	451	0.01%	0.003%
52	9.884	1440	1443	1447	rBV2	476	665	0.01%	0.005%
53	10.055	1465	1471	1486	rBV	583209	777262	12.92%	5.406%
54	10.384	1523	1525	1528	rVB3	453	378	0.01%	0.003%
55	10.476	1537	1540	1543	rBV3	416	487	0.01%	0.003%
56	10.549	1550	1552	1554	rBV2	429	387	0.01%	0.003%
57	10.610	1557	1562	1564	rBV3	507	844	0.01%	0.006%
58	10.726	1579	1581	1584	rVB2	815	622	0.01%	0.004%
59	10.860	1600	1603	1605	rBV2	363	369	0.01%	0.003%
60	10.994	1623	1625	1628	rVB2	319	382	0.01%	0.003%
61	11.043	1632	1633	1636	rVV2	437	409	0.01%	0.003%
62	11.073	1636	1638	1639	rVV2	486	386	0.01%	0.003%
63	11.104	1642	1643	1647	rVV2	513	729	0.01%	0.005%
64	11.152	1649	1651	1652	rVV	646	532	0.01%	0.004%
65	11.195	1652	1658	1670	rVV	437273	552842	9.19%	3.845%
66	11.281	1670	1672	1675	rVV4	613	740	0.01%	0.005%
67	11.634	1725	1730	1731	rBV	406	399	0.01%	0.003%
68	11.963	1776	1784	1788	rBV2	525	1425	0.02%	0.010%
69	12.024	1788	1794	1802	rBV	563360	688643	11.44%	4.790%
70	12.225	1823	1827	1829	rBV2	1167	1382	0.02%	0.010%
71	12.262	1832	1833	1835	rBV2	478	422	0.01%	0.003%
72	12.323	1837	1843	1850	rBV	569981	706927	11.75%	4.917%
73	12.610	1888	1890	1893	rBV2	406	447	0.01%	0.003%
74	12.817	1922	1924	1927	rVB	536	450	0.01%	0.003%
75	12.933	1941	1943	1945	rBV	686	725	0.01%	0.005%
76	12.981	1949	1951	1954	rVV2	736	736	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030593.D
 Acq On : 12 Aug 2022 14:47
 Operator : JC/MD
 Sample : N4131-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.024	1954	1958	1959	rVV2	528	700	0.01%	0.005%
78	13.067	1963	1965	1968	rBV2	621	606	0.01%	0.004%
79	13.384	2016	2017	2022	rVB2	520	609	0.01%	0.004%
80	13.463	2027	2030	2032	rBV	473	661	0.01%	0.005%
81	13.719	2070	2072	2074	rBV	523	397	0.01%	0.003%
82	13.884	2098	2099	2103	rVV2	529	439	0.01%	0.003%
83	14.024	2121	2122	2125	rBV2	532	546	0.01%	0.004%
84	14.079	2129	2131	2135	rBV2	724	722	0.01%	0.005%
85	14.128	2135	2139	2142	rVV2	449	674	0.01%	0.005%
86	14.189	2147	2149	2150	rBV	578	424	0.01%	0.003%
87	14.329	2170	2172	2175	rVB3	492	602	0.01%	0.004%
88	14.426	2185	2188	2192	rVB2	540	784	0.01%	0.005%
89	14.554	2207	2209	2212	rVB2	535	437	0.01%	0.003%
90	14.737	2238	2239	2243	rBV2	556	607	0.01%	0.004%
91	14.810	2249	2251	2252	rBV2	673	481	0.01%	0.003%
92	14.853	2257	2258	2261	rBV2	532	585	0.01%	0.004%
93	15.261	2323	2325	2330	rBV4	688	1005	0.02%	0.007%
94	15.396	2344	2347	2351	rVB3	1267	1477	0.02%	0.010%
95	15.432	2351	2353	2355	rBV2	641	770	0.01%	0.005%
96	15.780	2408	2410	2414	rVB2	603	683	0.01%	0.005%
97	15.877	2424	2426	2429	rBV3	694	702	0.01%	0.005%
98	16.200	2477	2479	2482	rBV2	550	507	0.01%	0.004%
99	16.328	2498	2500	2501	rBV2	1040	729	0.01%	0.005%
100	16.548	2534	2536	2539	rBV	897	975	0.02%	0.007%




Sum of corrected areas: 14376871

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030593.D
Acq On : 12 Aug 2022 14:47
Operator : JC/MD
Sample : N4131-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

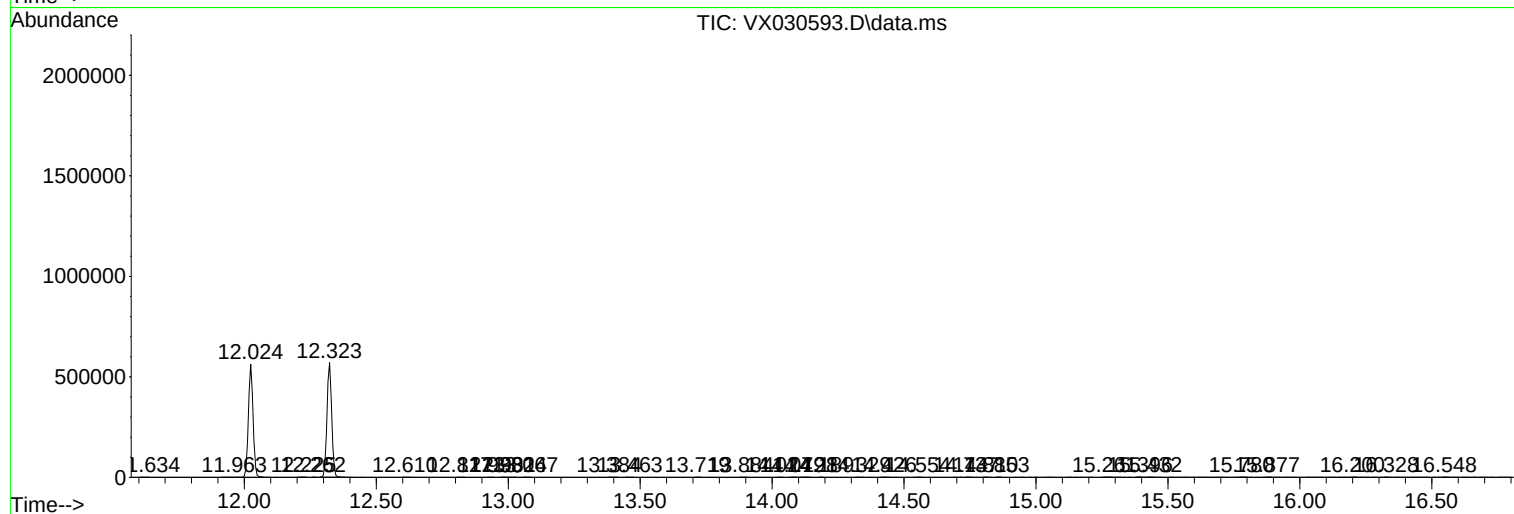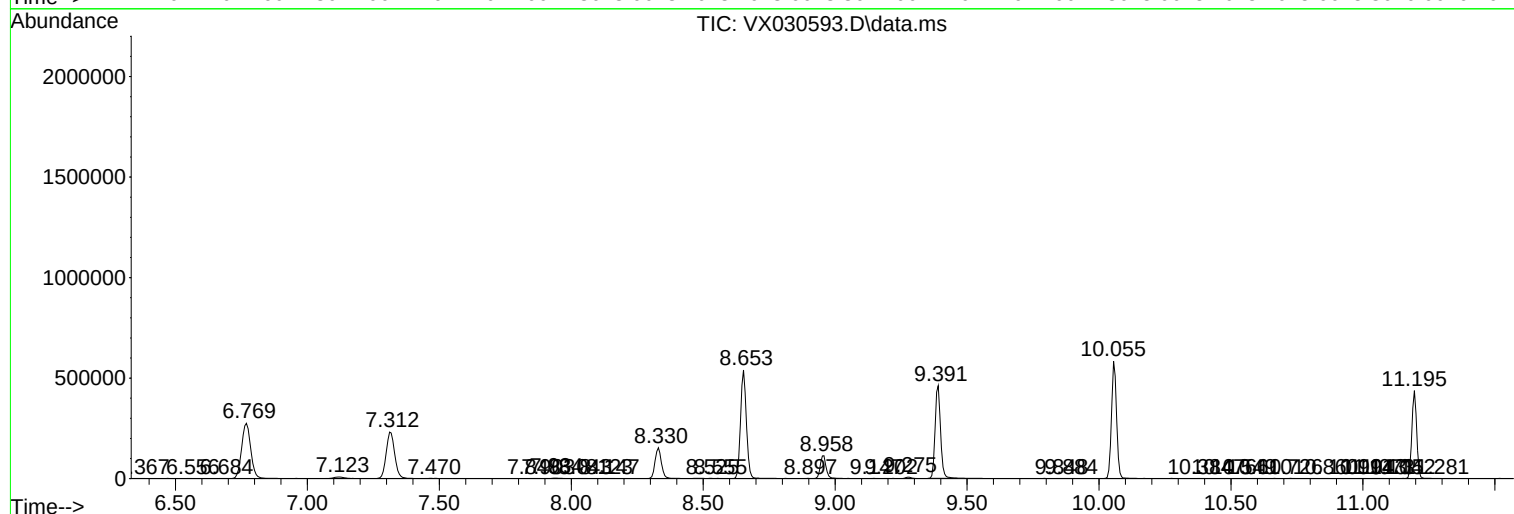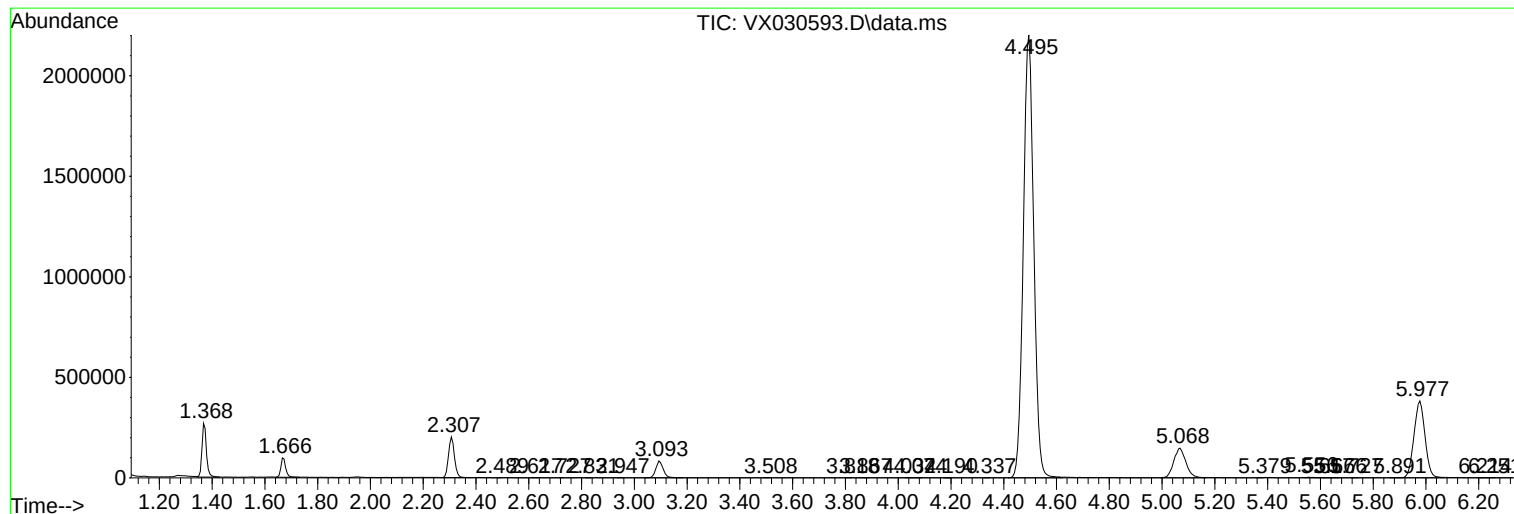

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030593.D
Acq On : 12 Aug 2022 14:47
Operator : JC/MD
Sample : N4131-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030593.D
Acq On : 12 Aug 2022 14:47
Operator : JC/MD
Sample : N4131-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc