

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030594.D
 Acq On : 12 Aug 2022 15:11
 Operator : JC/MD
 Sample : N4131-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	270005	299069	3.03%	1.452%
2	1.666	91	95	103	rVB	96174	121647	1.23%	0.590%
3	2.032	153	155	156	rBV2	1161	806	0.01%	0.004%
4	2.306	194	200	211	rVB	222141	338957	3.43%	1.645%
5	2.569	241	243	245	rBV2	474	549	0.01%	0.003%
6	2.788	277	279	283	rVB2	953	810	0.01%	0.004%
7	2.825	283	285	288	rVB2	597	440	0.00%	0.002%
8	2.855	288	290	293	rBV2	349	521	0.01%	0.003%
9	2.898	295	297	300	rVB2	665	663	0.01%	0.003%
10	3.093	321	329	343	rVB	159042	307364	3.11%	1.492%
11	3.258	354	356	359	rVB2	366	345	0.00%	0.002%
12	3.434	382	385	389	rVB2	315	436	0.00%	0.002%
13	3.678	423	425	427	rVV2	455	394	0.00%	0.002%
14	3.885	456	459	461	rBV2	436	463	0.00%	0.002%
15	3.922	463	465	467	rBV	331	356	0.00%	0.002%
16	4.044	483	485	487	rVV2	513	436	0.00%	0.002%
17	4.111	494	496	498	rBV2	343	427	0.00%	0.002%
18	4.160	501	504	505	rVB	432	350	0.00%	0.002%
19	4.184	505	508	515	rBV2	668	1190	0.01%	0.006%
20	4.245	515	518	519	rBV2	506	474	0.00%	0.002%
21	4.495	546	559	580	rBV	3675483	9885263	100.00%	47.984%
22	4.910	625	627	628	rBV2	547	366	0.00%	0.002%
23	5.068	639	653	671	rVV	144013	461075	4.66%	2.238%
24	5.214	675	677	679	rVB3	978	848	0.01%	0.004%
25	5.385	702	705	707	rBV3	1362	1572	0.02%	0.008%
26	5.495	721	723	725	rBV3	817	613	0.01%	0.003%
27	5.544	728	731	732	rBV2	1123	1279	0.01%	0.006%
28	5.696	754	756	757	rBV	556	420	0.00%	0.002%
29	5.977	789	802	819	rBV2	385713	1111888	11.25%	5.397%
30	6.361	861	865	866	rBV	726	714	0.01%	0.003%
31	6.653	911	913	916	rBV2	419	523	0.01%	0.003%
32	6.769	922	932	947	rBV	275592	645230	6.53%	3.132%
33	6.946	957	961	964	rBV5	390	556	0.01%	0.003%
34	7.025	972	974	977	rBV2	475	456	0.00%	0.002%
35	7.129	980	991	1009	rVV	1001111	2132938	21.58%	10.353%
36	7.312	1013	1021	1037	rVB	241313	525136	5.31%	2.549%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030594.D
 Acq On : 12 Aug 2022 15:11
 Operator : JC/MD
 Sample : N4131-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

37	7.665	1076	1079	1080	rVB2	435	423	0.00%	0.002%
38	7.824	1103	1105	1106	rBV	347	375	0.00%	0.002%
39	7.891	1112	1116	1118	rVB3	532	687	0.01%	0.003%
40	7.940	1118	1124	1130	rBV6	2004	4369	0.04%	0.021%
41	8.068	1143	1145	1148	rBV2	420	550	0.01%	0.003%
42	8.153	1155	1159	1162	rBV3	368	615	0.01%	0.003%
43	8.330	1181	1188	1198	rBV	159305	262911	2.66%	1.276%
44	8.482	1211	1213	1221	rVB5	1976	2584	0.03%	0.013%
45	8.653	1234	1241	1251	rBV	532248	820892	8.30%	3.985%
46	8.872	1276	1277	1280	rBV2	529	529	0.01%	0.003%
47	8.952	1285	1290	1305	rVB	116708	177135	1.79%	0.860%
48	9.055	1305	1307	1308	rBV	768	551	0.01%	0.003%
49	9.232	1334	1336	1338	rVB2	437	347	0.00%	0.002%
50	9.275	1338	1343	1351	rBV2	36007	57230	0.58%	0.278%
51	9.391	1354	1362	1376	rBV	469579	692216	7.00%	3.360%
52	9.598	1395	1396	1401	rVB3	714	758	0.01%	0.004%
53	9.903	1445	1446	1448	rBV	352	361	0.00%	0.002%
54	9.945	1452	1453	1455	rVB2	548	399	0.00%	0.002%
55	9.964	1455	1456	1458	rBV	401	360	0.00%	0.002%
56	10.055	1466	1471	1478	rBV	560089	737013	7.46%	3.578%
57	10.220	1494	1498	1499	rBV	439	414	0.00%	0.002%
58	10.293	1509	1510	1513	rBV2	512	527	0.01%	0.003%
59	10.396	1524	1527	1529	rBV2	677	679	0.01%	0.003%
60	10.421	1529	1531	1536	rVV3	469	447	0.00%	0.002%
61	10.457	1536	1537	1540	rVB2	600	387	0.00%	0.002%
62	10.579	1555	1557	1561	rVB2	557	364	0.00%	0.002%
63	10.756	1583	1586	1589	rBV2	664	1050	0.01%	0.005%
64	11.024	1627	1630	1631	rBV	564	489	0.00%	0.002%
65	11.195	1652	1658	1667	rBV	438676	560143	5.67%	2.719%
66	11.305	1674	1676	1679	rVB4	607	566	0.01%	0.003%
67	11.427	1694	1696	1699	rBV3	572	582	0.01%	0.003%
68	11.476	1703	1704	1707	rVV2	416	416	0.00%	0.002%
69	11.555	1714	1717	1720	rBV2	506	694	0.01%	0.003%
70	11.689	1737	1739	1741	rBV	467	461	0.00%	0.002%
71	11.817	1757	1760	1761	rBV2	483	558	0.01%	0.003%
72	11.933	1778	1779	1781	rBV	559	494	0.00%	0.002%
73	12.024	1788	1794	1802	rBV	540641	661488	6.69%	3.211%
74	12.323	1837	1843	1852	rBV	593714	751009	7.60%	3.645%
75	12.750	1911	1913	1918	rBV3	780	928	0.01%	0.005%
76	12.866	1930	1932	1935	rBV2	474	641	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030594.D
 Acq On : 12 Aug 2022 15:11
 Operator : JC/MD
 Sample : N4131-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

77	12.951	1944	1946	1949	rBV2	609	541	0.01%	0.003%
78	12.994	1951	1953	1955	rBV2	346	417	0.00%	0.002%
79	13.109	1970	1972	1974	rBV3	695	482	0.00%	0.002%
80	13.201	1984	1987	1988	rBV2	522	469	0.00%	0.002%
81	13.262	1995	1997	1999	rBV	630	503	0.01%	0.002%
82	13.384	2015	2017	2021	rVB2	1216	1039	0.01%	0.005%
83	13.420	2021	2023	2025	rVB	564	434	0.00%	0.002%
84	13.439	2025	2026	2030	rBV3	434	484	0.00%	0.002%
85	13.475	2030	2032	2033	rBV	448	419	0.00%	0.002%
86	13.695	2066	2068	2073	rVV2	502	686	0.01%	0.003%
87	13.878	2094	2098	2100	rBV3	588	635	0.01%	0.003%
88	13.908	2100	2103	2107	rVB2	732	956	0.01%	0.005%
89	13.945	2107	2109	2110	rBV2	494	451	0.00%	0.002%
90	14.140	2136	2141	2144	rBV3	625	1112	0.01%	0.005%
91	14.280	2161	2164	2166	rBV2	340	400	0.00%	0.002%
92	14.347	2173	2175	2179	rVB2	673	733	0.01%	0.004%
93	14.536	2204	2206	2208	rBV	647	410	0.00%	0.002%
94	14.621	2218	2220	2221	rBV	682	427	0.00%	0.002%
95	14.762	2241	2243	2245	rBV2	410	409	0.00%	0.002%
96	14.877	2261	2262	2264	rBV2	575	445	0.00%	0.002%
97	14.938	2269	2272	2274	rBV3	599	654	0.01%	0.003%
98	15.060	2290	2292	2296	rBV4	543	708	0.01%	0.003%
99	15.347	2337	2339	2340	rBV2	821	608	0.01%	0.003%
100	16.097	2461	2462	2464	rBV2	650	588	0.01%	0.003%




Sum of corrected areas: 20601226

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030594.D
Acq On : 12 Aug 2022 15:11
Operator : JC/MD
Sample : N4131-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

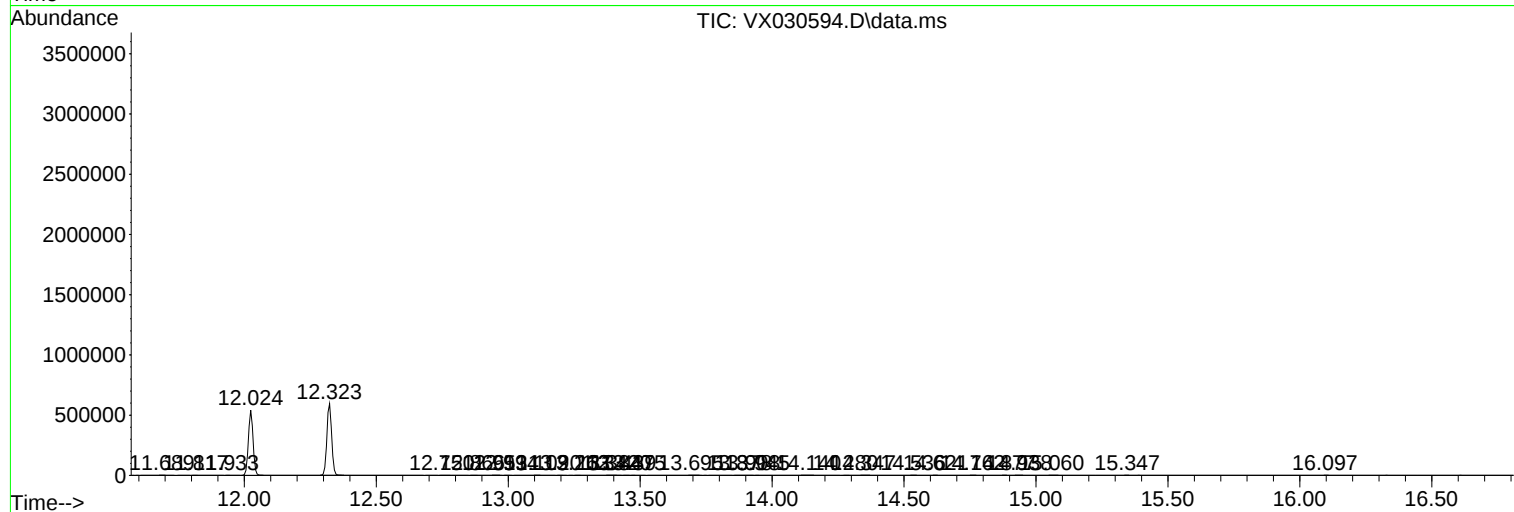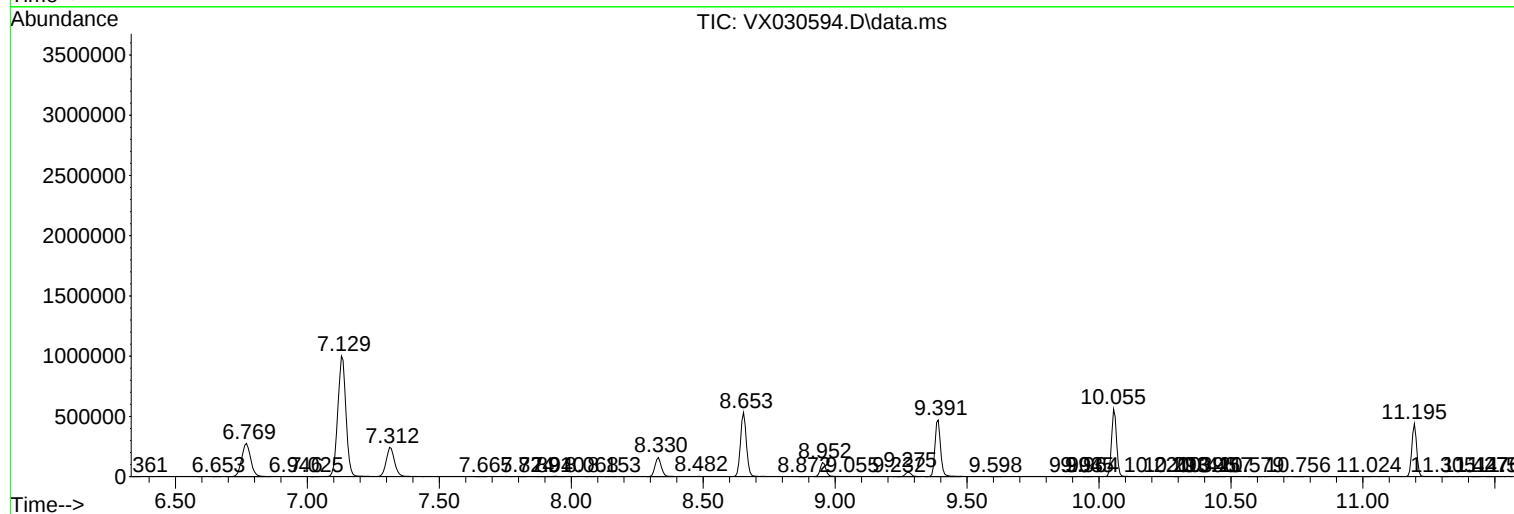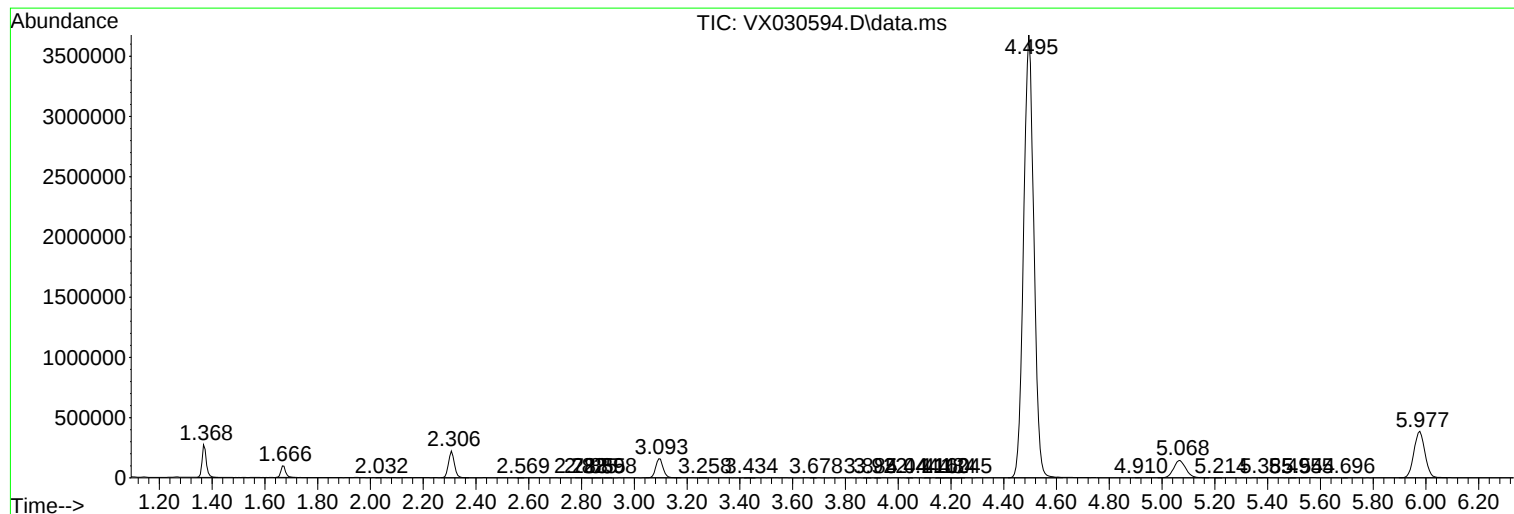

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030594.D
Acq On : 12 Aug 2022 15:11
Operator : JC/MD
Sample : N4131-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030594.D
Acq On : 12 Aug 2022 15:11
Operator : JC/MD
Sample : N4131-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc