

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030597.D
 Acq On : 12 Aug 2022 16:21
 Operator : JC/MD
 Sample : N4131-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030597.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.373	43	47	59	rVB	1369133	1500331	23.42%	9.346%
2	1.666	91	95	104	rVB	96032	122378	1.91%	0.762%
3	2.306	194	200	212	rVB2	234912	383814	5.99%	2.391%
4	2.513	232	234	235	rBV	572	337	0.01%	0.002%
5	2.568	240	243	244	rVB2	478	379	0.01%	0.002%
6	2.587	244	246	247	rBV2	333	335	0.01%	0.002%
7	2.715	266	267	269	rVB	680	376	0.01%	0.002%
8	2.794	277	280	283	rVB3	1020	1087	0.02%	0.007%
9	2.843	286	288	289	rBV	529	359	0.01%	0.002%
10	2.928	300	302	304	rBV2	371	422	0.01%	0.003%
11	3.093	322	329	341	rBV	144604	287182	4.48%	1.789%
12	3.227	350	351	354	rBV	634	446	0.01%	0.003%
13	3.428	383	384	385	rBV	644	351	0.01%	0.002%
14	3.507	394	397	400	rVB2	673	832	0.01%	0.005%
15	3.532	400	401	404	rBV2	475	496	0.01%	0.003%
16	3.763	437	439	443	rVB2	365	527	0.01%	0.003%
17	3.849	449	453	454	rBV2	568	614	0.01%	0.004%
18	3.916	462	464	467	rVB2	427	348	0.01%	0.002%
19	4.013	478	480	481	rBV	393	356	0.01%	0.002%
20	4.135	499	500	503	rVB	548	452	0.01%	0.003%
21	4.166	503	505	509	rBV	413	507	0.01%	0.003%
22	4.245	516	518	521	rBV2	538	556	0.01%	0.003%
23	4.275	521	523	525	rBV	423	374	0.01%	0.002%
24	4.300	525	527	530	rBV2	676	736	0.01%	0.005%
25	4.367	532	538	545	rVB3	1847	4143	0.06%	0.026%
26	4.495	546	559	581	rBV	2348816	6405842	100.00%	39.906%
27	4.928	628	630	631	rVB2	596	348	0.01%	0.002%
28	4.970	634	637	639	rBV2	575	588	0.01%	0.004%
29	5.062	641	652	671	rVV3	140203	453499	7.08%	2.825%
30	5.452	714	716	718	rBV2	590	598	0.01%	0.004%
31	5.476	718	720	721	rVB2	712	363	0.01%	0.002%
32	5.793	769	772	773	rBV2	620	417	0.01%	0.003%
33	5.867	780	784	785	rBV	602	568	0.01%	0.004%
34	5.976	788	802	818	rBV2	372768	1097540	17.13%	6.837%
35	6.202	835	839	840	rBV3	497	542	0.01%	0.003%
36	6.354	861	864	870	rBV5	663	1530	0.02%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030597.D
 Acq On : 12 Aug 2022 16:21
 Operator : JC/MD
 Sample : N4131-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.403	870	872	874	rVB2	593	454	0.01%	0.003%
38	6.433	874	877	878	rBV	463	499	0.01%	0.003%
39	6.519	887	891	892	rBV2	487	574	0.01%	0.004%
40	6.769	923	932	945	rBV	265249	627812	9.80%	3.911%
41	6.982	965	967	969	rBV2	356	347	0.01%	0.002%
42	7.055	975	979	981	rBV3	436	658	0.01%	0.004%
43	7.122	981	990	999	rVV7	8929	23536	0.37%	0.147%
44	7.317	1012	1022	1035	rBV	229786	516322	8.06%	3.216%
45	7.598	1066	1068	1071	rVV	390	375	0.01%	0.002%
46	7.939	1120	1124	1131	rVV4	1418	2957	0.05%	0.018%
47	7.994	1131	1133	1136	rVB2	548	477	0.01%	0.003%
48	8.098	1148	1150	1152	rVV2	419	391	0.01%	0.002%
49	8.165	1158	1161	1163	rBV2	476	712	0.01%	0.004%
50	8.329	1180	1188	1197	rBV	156680	255353	3.99%	1.591%
51	8.482	1211	1213	1217	rVB3	1331	1573	0.02%	0.010%
52	8.518	1217	1219	1222	rBV2	487	454	0.01%	0.003%
53	8.653	1234	1241	1250	rBV	531820	816734	12.75%	5.088%
54	8.884	1278	1279	1282	rVB3	577	463	0.01%	0.003%
55	8.951	1285	1290	1297	rBV	110201	167968	2.62%	1.046%
56	9.134	1319	1320	1322	rBV	489	411	0.01%	0.003%
57	9.250	1336	1339	1341	rBV	595	682	0.01%	0.004%
58	9.281	1341	1344	1347	rVB3	927	1203	0.02%	0.007%
59	9.341	1352	1354	1356	rBV	350	365	0.01%	0.002%
60	9.390	1356	1362	1376	rBV	474972	669034	10.44%	4.168%
61	9.579	1391	1393	1398	rVV4	551	623	0.01%	0.004%
62	9.616	1398	1399	1404	rVB2	1004	1175	0.02%	0.007%
63	9.659	1404	1406	1408	rBV2	793	746	0.01%	0.005%
64	9.701	1411	1413	1416	rBV	367	343	0.01%	0.002%
65	9.805	1429	1430	1433	rVB2	511	329	0.01%	0.002%
66	9.988	1458	1460	1463	rBV2	412	592	0.01%	0.004%
67	10.055	1465	1471	1489	rVV	525968	739280	11.54%	4.605%
68	10.201	1494	1495	1499	rVB2	524	579	0.01%	0.004%
69	10.238	1499	1501	1507	rBV2	546	718	0.01%	0.004%
70	10.323	1512	1515	1517	rVB3	734	773	0.01%	0.005%
71	10.354	1517	1520	1523	rBV2	597	720	0.01%	0.004%
72	10.652	1567	1569	1571	rVB	516	335	0.01%	0.002%
73	10.756	1584	1586	1590	rBV3	413	460	0.01%	0.003%
74	11.018	1628	1629	1631	rBV	528	415	0.01%	0.003%
75	11.195	1652	1658	1672	rBV	446598	560464	8.75%	3.491%
76	11.335	1680	1681	1683	rVB	532	324	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030597.D
 Acq On : 12 Aug 2022 16:21
 Operator : JC/MD
 Sample : N4131-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

77	11.414	1691	1694	1695	rBV2	327	394	0.01%	0.002%
78	11.573	1718	1720	1721	rBV	429	317	0.00%	0.002%
79	11.628	1728	1729	1733	rBV2	606	422	0.01%	0.003%
80	11.707	1740	1742	1743	rBV	743	464	0.01%	0.003%
81	11.780	1753	1754	1757	rVB	461	319	0.00%	0.002%
82	11.817	1757	1760	1762	rBV2	413	573	0.01%	0.004%
83	11.963	1781	1784	1786	rBV2	448	428	0.01%	0.003%
84	12.024	1789	1794	1803	rVV	532817	660019	10.30%	4.112%
85	12.323	1837	1843	1854	rBV	585241	714108	11.15%	4.449%
86	12.506	1871	1873	1876	rVB	699	684	0.01%	0.004%
87	13.079	1964	1967	1968	rBV	320	359	0.01%	0.002%
88	13.402	2018	2020	2023	rBV	445	369	0.01%	0.002%
89	13.493	2033	2035	2037	rBV	520	387	0.01%	0.002%
90	13.755	2075	2078	2079	rBV	451	465	0.01%	0.003%
91	13.841	2086	2092	2097	rBV2	881	1544	0.02%	0.010%
92	14.042	2124	2125	2128	rBV	507	518	0.01%	0.003%
93	14.389	2180	2182	2183	rBV	371	343	0.01%	0.002%
94	14.463	2191	2194	2197	rBV2	676	1056	0.02%	0.007%
95	14.804	2248	2250	2252	rBV3	522	318	0.00%	0.002%
96	14.956	2273	2275	2277	rVB2	617	314	0.00%	0.002%
97	14.975	2277	2278	2282	rVB2	439	352	0.01%	0.002%
98	15.054	2287	2291	2293	rBV3	640	1092	0.02%	0.007%
99	15.450	2355	2356	2358	rBV2	514	410	0.01%	0.003%
100	16.255	2486	2488	2489	rBV2	607	426	0.01%	0.003%


Sum of corrected areas: 16052484

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030597.D
Acq On : 12 Aug 2022 16:21
Operator : JC/MD
Sample : N4131-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

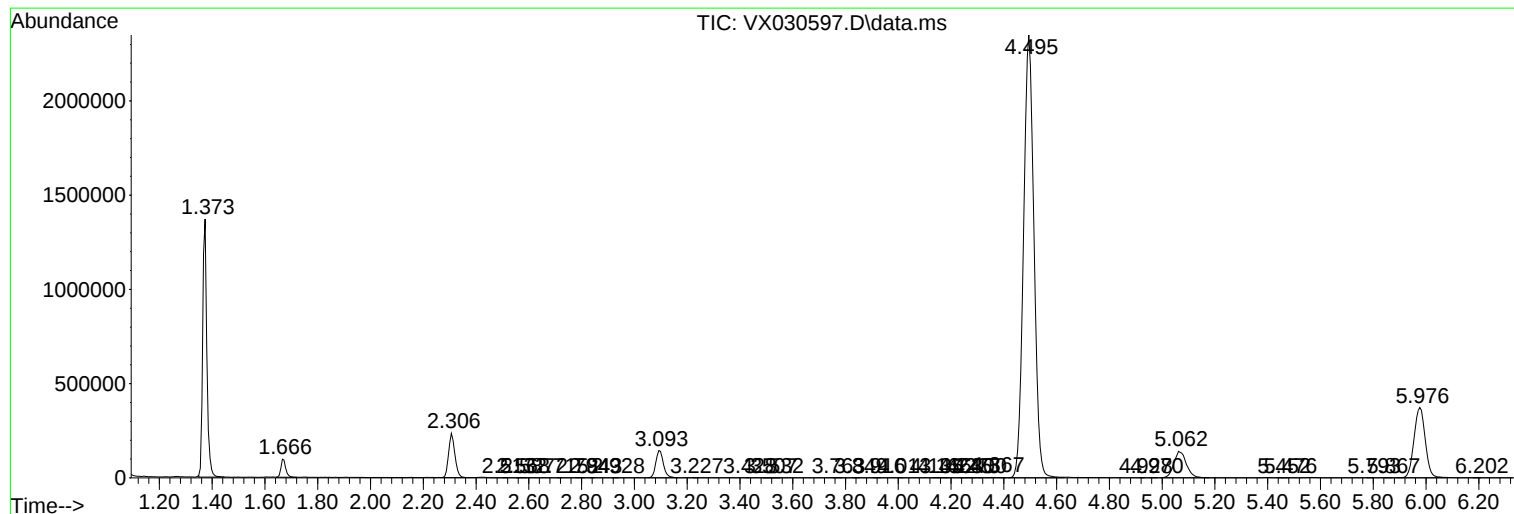

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030597.D
Acq On : 12 Aug 2022 16:21
Operator : JC/MD
Sample : N4131-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030597.D
Acq On : 12 Aug 2022 16:21
Operator : JC/MD
Sample : N4131-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc