

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030601.D
 Acq On : 12 Aug 2022 17:55
 Operator : JC/MD
 Sample : N4131-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	13	rVB	7684	6782	0.63%	0.074%
2	1.368	42	46	58	rVB2	710681	796044	73.60%	8.737%
3	1.666	91	95	102	rBV	87830	113623	10.50%	1.247%
4	2.306	194	200	208	rVB	206453	317907	29.39%	3.489%
5	2.404	212	216	221	rVB3	2212	3590	0.33%	0.039%
6	2.508	231	233	235	rBV	721	477	0.04%	0.005%
7	2.575	242	244	246	rBV3	586	730	0.07%	0.008%
8	2.788	277	279	281	rVV3	572	361	0.03%	0.004%
9	2.898	292	297	299	rBV	597	592	0.05%	0.006%
10	2.995	311	313	315	rVV3	447	478	0.04%	0.005%
11	3.093	323	329	335	rBV4	5315	10254	0.95%	0.113%
12	3.282	356	360	363	rBV2	489	669	0.06%	0.007%
13	3.373	372	375	376	rBV	452	443	0.04%	0.005%
14	3.440	383	386	389	rBV3	401	650	0.06%	0.007%
15	3.568	405	407	409	rBV	632	607	0.06%	0.007%
16	3.733	431	434	437	rBV2	466	665	0.06%	0.007%
17	4.129	496	499	500	rVB2	367	345	0.03%	0.004%
18	4.148	500	502	504	rBV	421	387	0.04%	0.004%
19	4.227	513	515	518	rVB2	459	461	0.04%	0.005%
20	4.300	524	527	530	rBV	293	368	0.03%	0.004%
21	4.355	535	536	540	rBV2	239	349	0.03%	0.004%
22	4.489	545	558	575	rBV2	207267	661841	61.19%	7.264%
23	4.897	622	625	626	rBV	387	349	0.03%	0.004%
24	4.971	634	637	638	rBV2	444	477	0.04%	0.005%
25	5.068	640	653	671	rVV	145724	452102	41.80%	4.962%
26	5.391	703	706	708	rVV3	646	806	0.07%	0.009%
27	5.410	708	709	713	rVV2	677	558	0.05%	0.006%
28	5.708	756	758	761	rVB	343	406	0.04%	0.004%
29	5.977	790	802	818	rBV2	368837	1081639	100.00%	11.871%
30	6.184	833	836	837	rBV2	507	423	0.04%	0.005%
31	6.220	840	842	845	rBV3	436	430	0.04%	0.005%
32	6.379	865	868	870	rBV2	595	759	0.07%	0.008%
33	6.440	876	878	879	rVB	600	332	0.03%	0.004%
34	6.501	886	888	889	rBV	501	362	0.03%	0.004%
35	6.556	895	897	900	rVB2	407	345	0.03%	0.004%
36	6.665	913	915	919	rVB	446	515	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030601.D
 Acq On : 12 Aug 2022 17:55
 Operator : JC/MD
 Sample : N4131-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.769	922	932	946	rBV	247630	593955	54.91%	6.519%
38	6.940	958	960	964	rBV3	583	582	0.05%	0.006%
39	7.117	979	989	999	rBV5	10136	24154	2.23%	0.265%
40	7.318	1013	1022	1034	rBV	232484	510803	47.22%	5.606%
41	7.476	1045	1048	1050	rBV2	798	1177	0.11%	0.013%
42	7.598	1067	1068	1069	rBV	728	332	0.03%	0.004%
43	7.714	1084	1087	1090	rVB2	558	637	0.06%	0.007%
44	7.763	1093	1095	1097	rBV2	355	356	0.03%	0.004%
45	7.854	1106	1110	1112	rBV2	427	781	0.07%	0.009%
46	7.934	1119	1123	1124	rBV3	1945	1852	0.17%	0.020%
47	8.141	1153	1157	1160	rBV2	636	822	0.08%	0.009%
48	8.190	1162	1165	1169	rBV2	548	991	0.09%	0.011%
49	8.330	1181	1188	1198	rBV	153119	247321	22.87%	2.714%
50	8.433	1203	1205	1207	rBV	570	372	0.03%	0.004%
51	8.586	1228	1230	1234	rBV4	1554	1790	0.17%	0.020%
52	8.653	1234	1241	1250	rBV	514175	794015	73.41%	8.715%
53	8.952	1285	1290	1299	rBV	107028	164277	15.19%	1.803%
54	9.275	1340	1343	1346	rBV2	1107	1296	0.12%	0.014%
55	9.299	1346	1347	1351	rVB3	765	807	0.07%	0.009%
56	9.348	1351	1355	1356	rBV2	439	711	0.07%	0.008%
57	9.391	1356	1362	1376	rBV	485099	688864	63.69%	7.561%
58	9.525	1383	1384	1385	rBV	804	457	0.04%	0.005%
59	9.641	1401	1403	1405	rVB	743	395	0.04%	0.004%
60	9.695	1410	1412	1415	rBV	361	380	0.04%	0.004%
61	9.793	1427	1428	1433	rVB	563	747	0.07%	0.008%
62	9.836	1433	1435	1439	rBV	562	600	0.06%	0.007%
63	9.872	1439	1441	1443	rVB	482	360	0.03%	0.004%
64	10.055	1465	1471	1486	rBV	530651	701504	64.86%	7.699%
65	10.476	1538	1540	1543	rBV2	448	492	0.05%	0.005%
66	10.628	1563	1565	1567	rBV	544	531	0.05%	0.006%
67	10.646	1567	1568	1571	rVB2	552	406	0.04%	0.004%
68	10.677	1571	1573	1577	rBV2	340	428	0.04%	0.005%
69	10.756	1585	1586	1588	rVB	595	335	0.03%	0.004%
70	10.793	1589	1592	1596	rVV2	320	402	0.04%	0.004%
71	11.085	1638	1640	1645	rVB2	605	696	0.06%	0.008%
72	11.195	1652	1658	1665	rBV	432316	541088	50.02%	5.939%
73	11.421	1692	1695	1699	rBV2	342	575	0.05%	0.006%
74	11.494	1705	1707	1710	rBV	562	568	0.05%	0.006%
75	11.597	1720	1724	1727	rVV2	473	768	0.07%	0.008%
76	11.707	1740	1742	1745	rBV2	589	616	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030601.D
 Acq On : 12 Aug 2022 17:55
 Operator : JC/MD
 Sample : N4131-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.811	1755	1759	1761	rVB2	500	531	0.05%	0.006%
78	12.024	1789	1794	1803	rVV	528395	634752	58.68%	6.967%
79	12.128	1810	1811	1814	rVB	845	550	0.05%	0.006%
80	12.164	1814	1817	1818	rBV	643	623	0.06%	0.007%
81	12.323	1837	1843	1852	rBV	574827	718474	66.42%	7.886%
82	12.823	1923	1925	1928	rBV2	444	542	0.05%	0.006%
83	13.183	1982	1984	1985	rVB2	592	404	0.04%	0.004%
84	13.615	2053	2055	2056	rBV	368	378	0.03%	0.004%
85	13.658	2060	2062	2065	rBV2	457	604	0.06%	0.007%
86	13.731	2070	2074	2076	rBV	520	547	0.05%	0.006%
87	13.914	2102	2104	2106	rBV	441	436	0.04%	0.005%
88	13.951	2108	2110	2113	rVB	505	417	0.04%	0.005%
89	14.036	2123	2124	2126	rBV	504	476	0.04%	0.005%
90	14.128	2138	2139	2144	rBV2	744	956	0.09%	0.010%
91	14.274	2160	2163	2165	rBV2	556	569	0.05%	0.006%
92	14.487	2197	2198	2201	rBV3	461	560	0.05%	0.006%
93	14.768	2241	2244	2247	rBV3	1114	1531	0.14%	0.017%
94	14.896	2263	2265	2268	rBV	575	602	0.06%	0.007%
95	15.103	2296	2299	2300	rBV3	556	569	0.05%	0.006%
96	15.121	2300	2302	2307	rVV3	731	1220	0.11%	0.013%
97	15.261	2323	2325	2327	rBV3	618	610	0.06%	0.007%
98	15.329	2334	2336	2337	rVB	748	346	0.03%	0.004%
99	15.688	2393	2395	2396	rBV2	739	657	0.06%	0.007%
100	16.773	2572	2573	2575	rBV	722	520	0.05%	0.006%

Sum of corrected areas: 9111243




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030601.D
Acq On : 12 Aug 2022 17:55
Operator : JC/MD
Sample : N4131-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

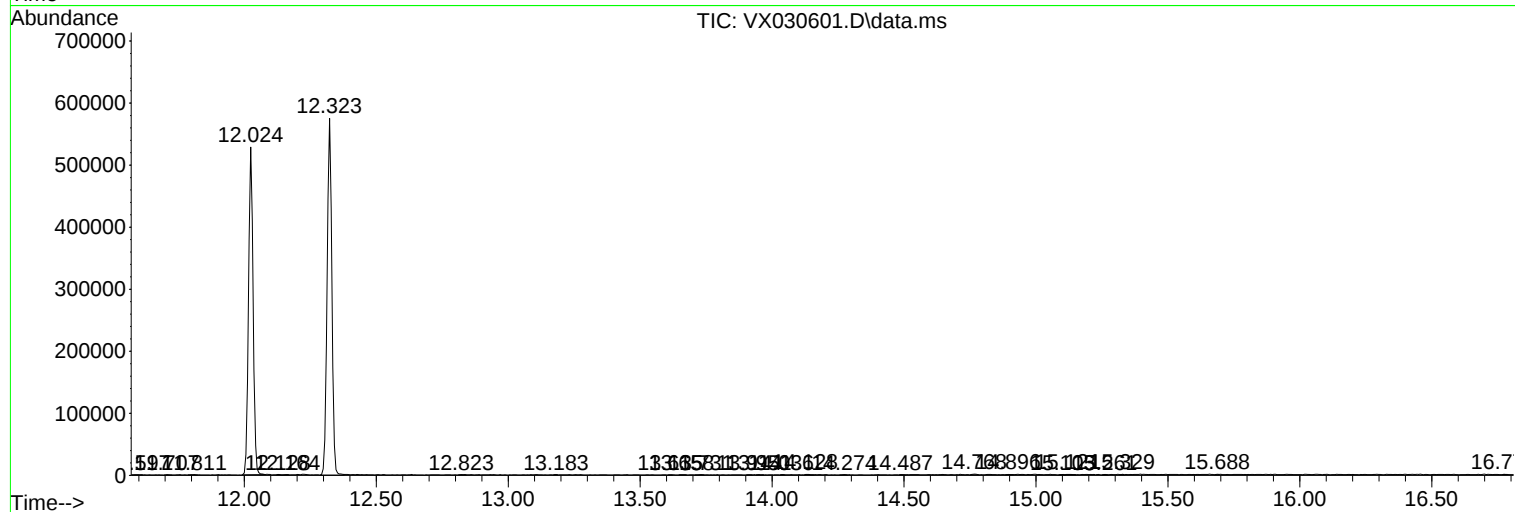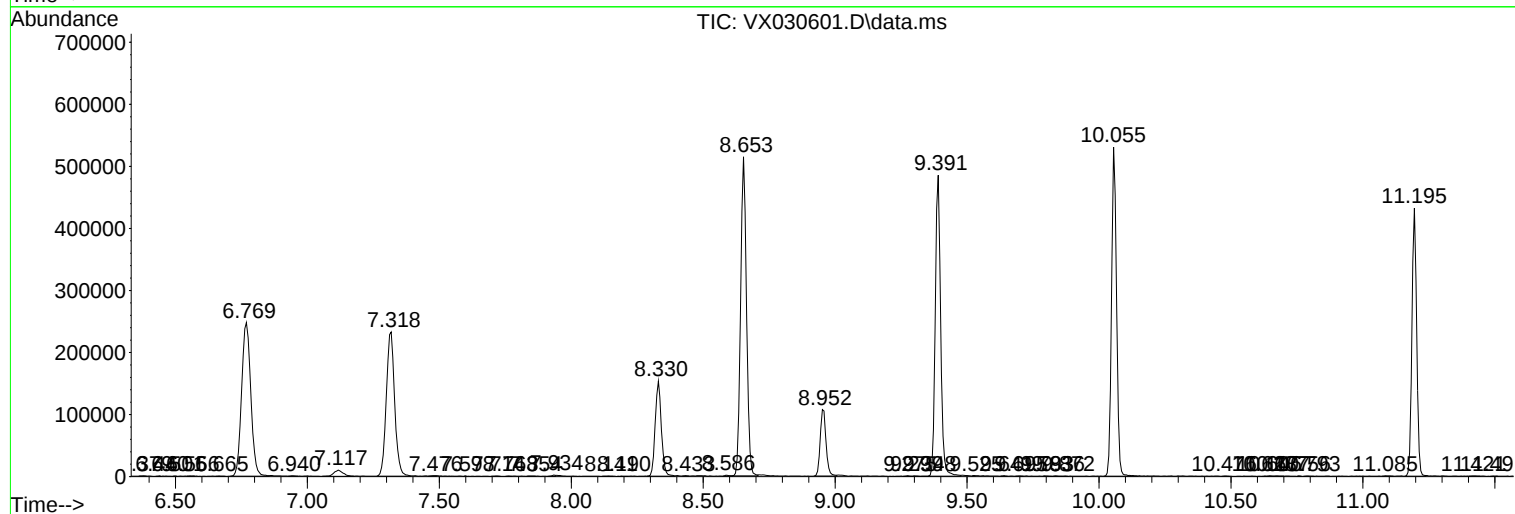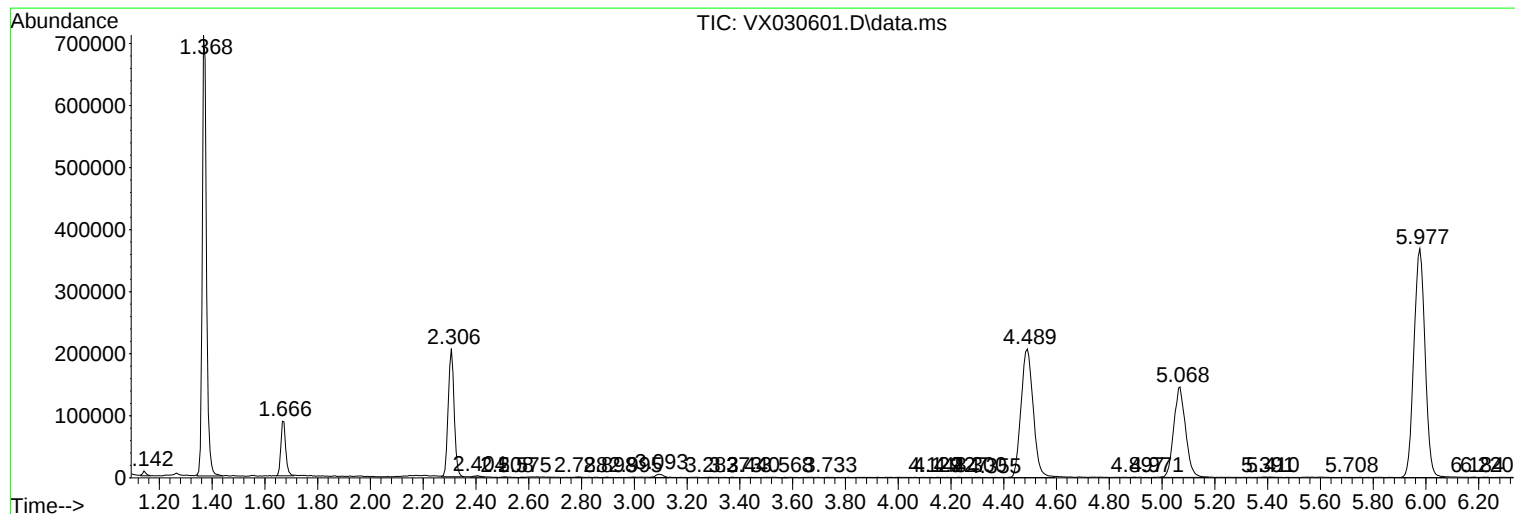

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030601.D
Acq On : 12 Aug 2022 17:55
Operator : JC/MD
Sample : N4131-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030601.D
Acq On : 12 Aug 2022 17:55
Operator : JC/MD
Sample : N4131-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc