

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030602.D
 Acq On : 12 Aug 2022 18:18
 Operator : JC/MD
 Sample : N4131-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D35DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030602.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	53	rVB2	120557	128661	12.17%	1.479%
2	1.666	91	95	103	rBV	86311	113244	10.71%	1.302%
3	2.306	194	200	211	rVB	196771	302683	28.63%	3.480%
4	2.404	211	216	217	rBV3	1068	1549	0.15%	0.018%
5	2.459	223	225	227	rBV	426	410	0.04%	0.005%
6	2.568	240	243	244	rBV2	448	497	0.05%	0.006%
7	2.623	251	252	255	rBV2	611	546	0.05%	0.006%
8	2.648	255	256	258	rVB	636	362	0.03%	0.004%
9	2.678	258	261	263	rBV2	508	665	0.06%	0.008%
10	2.794	274	280	284	rBV4	2662	4686	0.44%	0.054%
11	2.946	299	305	312	rVV4	2611	5873	0.56%	0.068%
12	3.099	323	330	338	rVB	9421	18894	1.79%	0.217%
13	3.392	375	378	380	rBV2	348	449	0.04%	0.005%
14	3.635	417	418	421	rBV2	524	455	0.04%	0.005%
15	3.672	421	424	426	rBV2	354	366	0.03%	0.004%
16	3.971	471	473	476	rVB2	349	372	0.04%	0.004%
17	4.007	476	479	481	rBV2	393	430	0.04%	0.005%
18	4.026	481	482	486	rVV2	621	562	0.05%	0.006%
19	4.190	505	509	510	rBV	362	497	0.05%	0.006%
20	4.300	525	527	530	rBV2	441	384	0.04%	0.004%
21	4.367	537	538	544	rVB	513	767	0.07%	0.009%
22	4.489	544	558	571	rBV2	288115	880798	83.31%	10.126%
23	4.775	603	605	608	rVB2	473	414	0.04%	0.005%
24	4.818	610	612	615	rVB2	656	507	0.05%	0.006%
25	4.891	621	624	626	rVB3	652	739	0.07%	0.008%
26	4.934	629	631	634	rVB	619	431	0.04%	0.005%
27	5.068	639	653	669	rVV	146081	450311	42.59%	5.177%
28	5.190	672	673	677	rBV3	746	821	0.08%	0.009%
29	5.324	693	695	697	rVB2	488	420	0.04%	0.005%
30	5.373	701	703	705	rVV2	652	669	0.06%	0.008%
31	5.416	708	710	712	rVV	675	684	0.06%	0.008%
32	5.452	714	716	718	rVV	367	366	0.03%	0.004%
33	5.550	727	732	733	rBV2	912	1009	0.10%	0.012%
34	5.617	741	743	745	rVB	538	386	0.04%	0.004%
35	5.690	752	755	756	rBV2	491	385	0.04%	0.004%
36	5.976	790	802	817	rBV2	363884	1057223	100.00%	12.154%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030602.D
 Acq On : 12 Aug 2022 18:18
 Operator : JC/MD
 Sample : N4131-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D35DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.360	861	865	868	rBV2	553	906	0.09%	0.010%
38	6.464	878	882	883	rBV2	614	679	0.06%	0.008%
39	6.519	889	891	893	rVB2	397	379	0.04%	0.004%
40	6.549	893	896	899	rBV3	535	693	0.07%	0.008%
41	6.604	902	905	907	rVB2	496	597	0.06%	0.007%
42	6.647	910	912	914	rVB2	426	387	0.04%	0.004%
43	6.671	914	916	920	rBV2	350	524	0.05%	0.006%
44	6.769	920	932	948	rBV	264575	628249	59.42%	7.222%
45	7.123	982	990	999	rBV5	10252	25922	2.45%	0.298%
46	7.220	1004	1006	1010	rVB	561	624	0.06%	0.007%
47	7.318	1012	1022	1038	rBV	232759	510235	48.26%	5.866%
48	7.610	1068	1070	1074	rVV3	385	455	0.04%	0.005%
49	7.683	1079	1082	1084	rBV3	514	392	0.04%	0.005%
50	7.714	1084	1087	1090	rBV2	390	414	0.04%	0.005%
51	7.933	1118	1123	1128	rBV4	2151	4600	0.44%	0.053%
52	8.202	1164	1167	1169	rBV2	417	389	0.04%	0.004%
53	8.330	1180	1188	1199	rBV	144917	247551	23.42%	2.846%
54	8.482	1210	1213	1216	rBV3	1464	2508	0.24%	0.029%
55	8.586	1223	1230	1235	rBV4	2843	4790	0.45%	0.055%
56	8.653	1235	1241	1252	rBV	500040	763153	72.18%	8.773%
57	8.951	1285	1290	1299	rBV	106803	163460	15.46%	1.879%
58	9.281	1339	1344	1349	rVB6	2025	3342	0.32%	0.038%
59	9.329	1349	1352	1354	rBV	469	756	0.07%	0.009%
60	9.390	1356	1362	1374	rBV	488914	694343	65.68%	7.982%
61	9.701	1409	1413	1420	rBV5	3738	6390	0.60%	0.073%
62	9.817	1430	1432	1436	rVB2	386	392	0.04%	0.005%
63	9.915	1444	1448	1449	rBV2	593	640	0.06%	0.007%
64	10.055	1466	1471	1480	rVV	541008	732478	69.28%	8.421%
65	10.201	1492	1495	1500	rBV3	977	1705	0.16%	0.020%
66	10.287	1505	1509	1510	rBV	679	662	0.06%	0.008%
67	10.311	1510	1513	1518	rVB3	1028	1354	0.13%	0.016%
68	10.439	1528	1534	1535	rVB2	372	580	0.05%	0.007%
69	10.494	1540	1543	1544	rBV2	502	424	0.04%	0.005%
70	10.634	1562	1566	1568	rBV	631	874	0.08%	0.010%
71	10.927	1610	1614	1616	rBV2	674	791	0.07%	0.009%
72	10.969	1618	1621	1623	rVV3	814	958	0.09%	0.011%
73	11.000	1624	1626	1629	rVB2	513	408	0.04%	0.005%
74	11.195	1652	1658	1665	rBV	433112	543047	51.37%	6.243%
75	11.414	1690	1694	1695	rBV	673	368	0.03%	0.004%
76	11.640	1728	1731	1733	rBV	423	452	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030602.D
 Acq On : 12 Aug 2022 18:18
 Operator : JC/MD
 Sample : N4131-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D35DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.756	1748	1750	1753	rVB2	647	660	0.06%	0.008%
78	11.933	1776	1779	1781	rVB2	376	361	0.03%	0.004%
79	11.975	1781	1786	1788	rBV4	957	1376	0.13%	0.016%
80	12.024	1789	1794	1803	rVB	530094	655502	62.00%	7.536%
81	12.134	1810	1812	1816	rBV4	628	459	0.04%	0.005%
82	12.256	1829	1832	1833	rBV	370	356	0.03%	0.004%
83	12.323	1837	1843	1851	rBV	567746	704443	66.63%	8.098%
84	12.433	1860	1861	1864	rVB	643	417	0.04%	0.005%
85	12.475	1866	1868	1872	rVB2	788	611	0.06%	0.007%
86	13.103	1967	1971	1972	rBV	446	493	0.05%	0.006%
87	13.115	1972	1973	1976	rVB2	824	581	0.05%	0.007%
88	13.219	1988	1990	1992	rVV	558	398	0.04%	0.005%
89	13.591	2049	2051	2052	rBV	771	401	0.04%	0.005%
90	13.786	2080	2083	2086	rVB3	649	764	0.07%	0.009%
91	14.097	2130	2134	2136	rBV2	403	382	0.04%	0.004%
92	14.121	2136	2138	2140	rVV2	460	539	0.05%	0.006%
93	14.182	2143	2148	2150	rBV2	466	741	0.07%	0.009%
94	14.499	2194	2200	2202	rBV2	564	905	0.09%	0.010%
95	15.109	2297	2300	2303	rBV2	477	646	0.06%	0.007%
96	15.584	2374	2378	2379	rBV2	955	1152	0.11%	0.013%
97	15.658	2388	2390	2393	rBV2	800	815	0.08%	0.009%
98	15.987	2442	2444	2448	rBV3	496	453	0.04%	0.005%
99	16.194	2476	2478	2483	rBV2	751	1150	0.11%	0.013%
100	16.316	2496	2498	2499	rBV	818	507	0.05%	0.006%


Sum of corrected areas: 8698498

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030602.D
Acq On : 12 Aug 2022 18:18
Operator : JC/MD
Sample : N4131-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D35DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

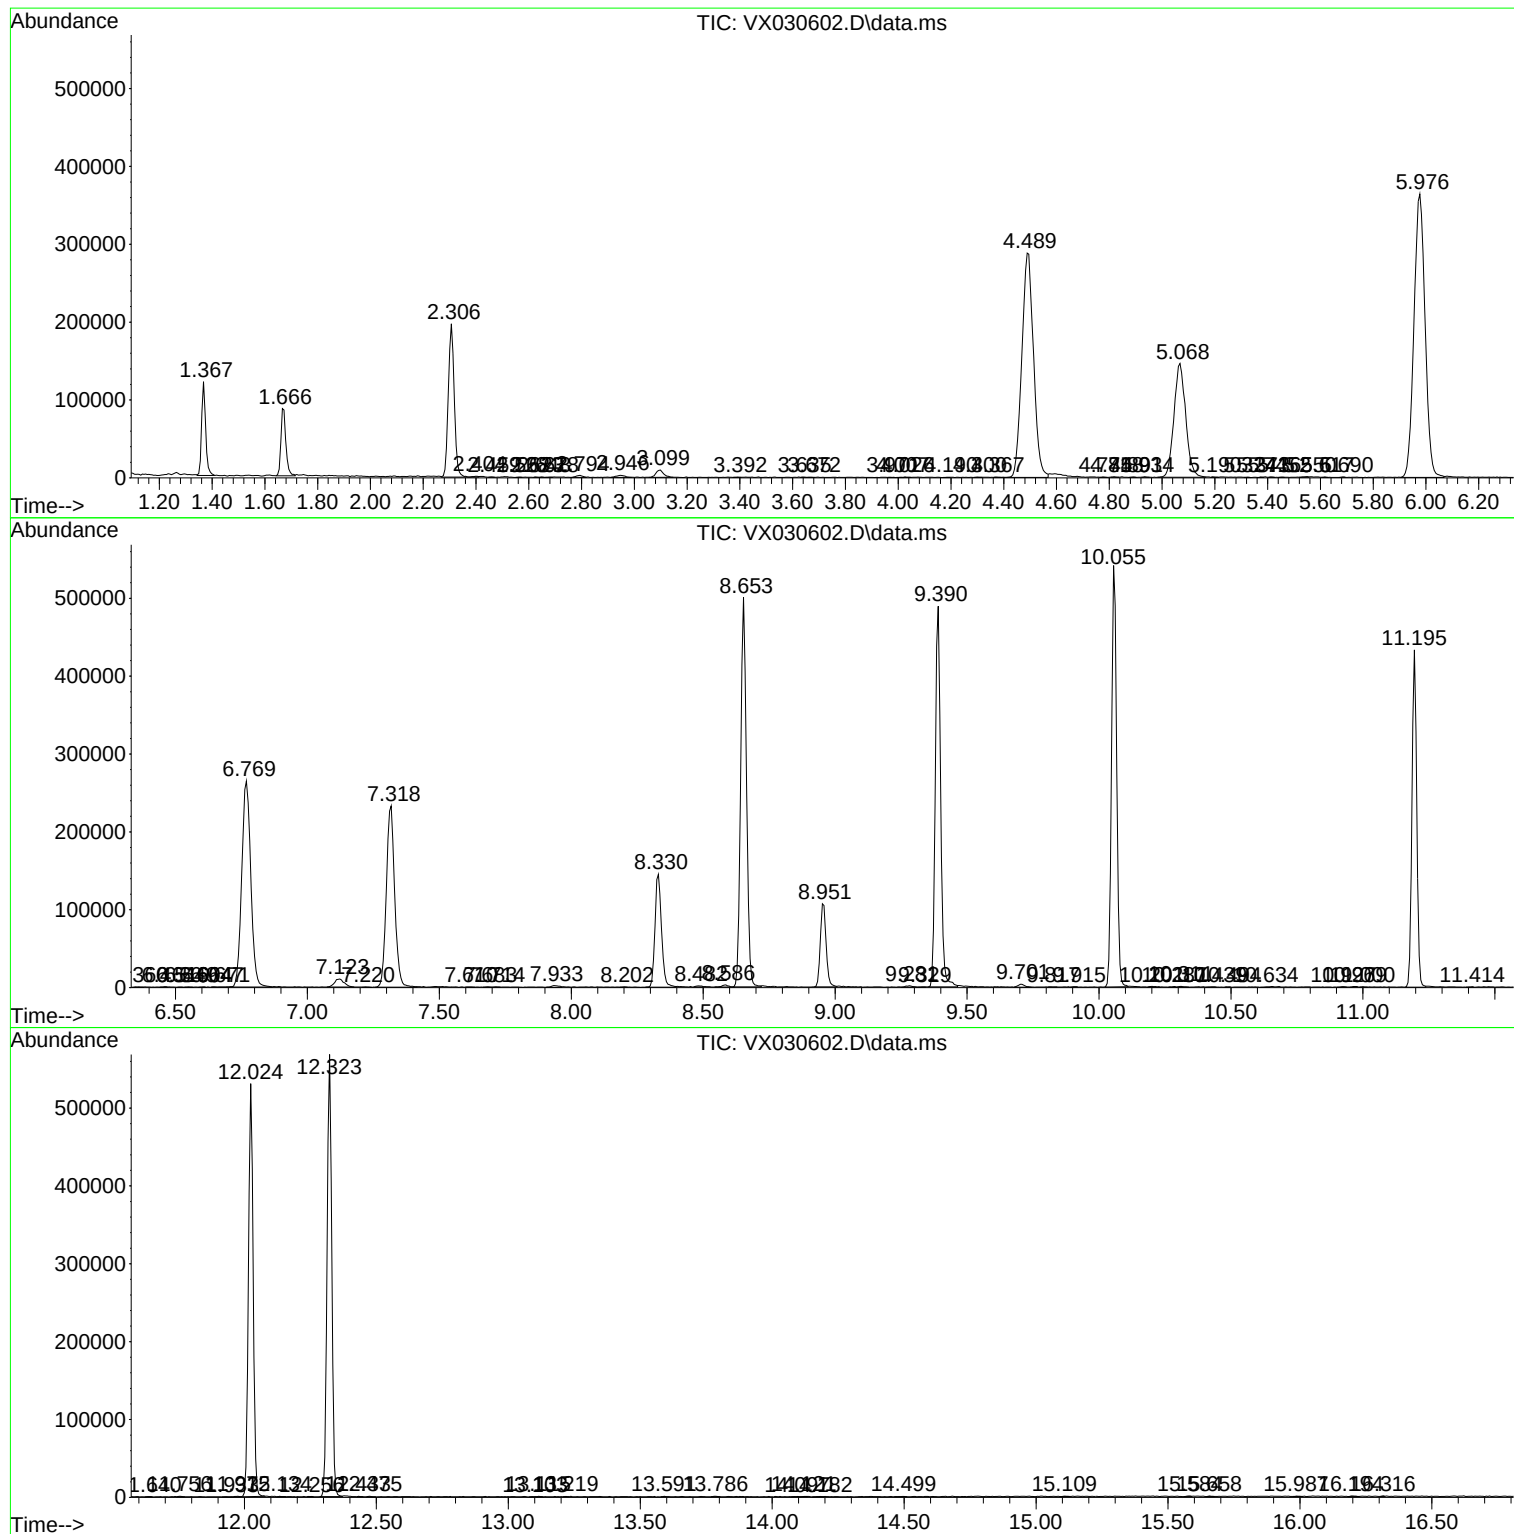

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030602.D
Acq On : 12 Aug 2022 18:18
Operator : JC/MD
Sample : N4131-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D35DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030602.D
Acq On : 12 Aug 2022 18:18
Operator : JC/MD
Sample : N4131-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D35DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc