

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030603.D
 Acq On : 12 Aug 2022 18:42
 Operator : JC/MD
 Sample : N4131-08DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D60DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030603.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	53	rVB	114423	116324	11.04%	1.348%
2	1.666	91	95	106	rVB	88793	111932	10.63%	1.297%
3	2.306	194	200	210	rVB	196913	297835	28.28%	3.452%
4	2.416	216	218	219	rBV2	789	676	0.06%	0.008%
5	2.495	229	231	233	rBV2	549	559	0.05%	0.006%
6	2.708	264	266	269	rBV2	501	646	0.06%	0.007%
7	2.794	275	280	285	rVB3	1827	3485	0.33%	0.040%
8	2.940	300	304	313	rVB5	2036	5421	0.51%	0.063%
9	3.007	313	315	317	rBV	529	503	0.05%	0.006%
10	3.050	320	322	324	rVV2	418	447	0.04%	0.005%
11	3.086	324	328	337	rVV4	8015	16618	1.58%	0.193%
12	3.221	348	350	353	rBV2	556	556	0.05%	0.006%
13	3.324	365	367	370	rVB	390	400	0.04%	0.005%
14	3.538	399	402	405	rVB2	546	714	0.07%	0.008%
15	3.574	405	408	410	rBV	461	503	0.05%	0.006%
16	3.952	467	470	472	rBV2	355	304	0.03%	0.004%
17	3.970	472	473	477	rVB2	490	519	0.05%	0.006%
18	4.013	477	480	481	rBV	529	541	0.05%	0.006%
19	4.489	546	558	572	rBV2	244397	777653	73.83%	9.014%
20	4.745	599	600	603	rBV2	578	312	0.03%	0.004%
21	4.891	623	624	628	rVB	360	364	0.03%	0.004%
22	5.062	640	652	668	rBV	142949	442530	42.02%	5.129%
23	5.568	729	735	737	rBV4	977	1548	0.15%	0.018%
24	5.623	742	744	748	rVB3	465	572	0.05%	0.007%
25	5.732	759	762	765	rBV	403	358	0.03%	0.004%
26	5.824	774	777	779	rBV2	391	418	0.04%	0.005%
27	5.866	782	784	788	rVB	331	477	0.05%	0.006%
28	5.976	788	802	819	rBV2	365731	1053260	100.00%	12.209%
29	6.147	829	830	833	rBV	507	432	0.04%	0.005%
30	6.177	833	835	838	rVB2	324	335	0.03%	0.004%
31	6.208	838	840	843	rVB	370	344	0.03%	0.004%
32	6.238	843	845	847	rBV	626	484	0.05%	0.006%
33	6.379	864	868	874	rVB3	484	839	0.08%	0.010%
34	6.427	874	876	879	rVB	654	537	0.05%	0.006%
35	6.458	879	881	882	rBV2	411	343	0.03%	0.004%
36	6.513	888	890	893	rBV	444	351	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030603.D
 Acq On : 12 Aug 2022 18:42
 Operator : JC/MD
 Sample : N4131-08DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D60DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.769	917	932	947	rBV	266547	638388	60.61%	7.400%
38	7.061	977	980	981	rBV2	365	415	0.04%	0.005%
39	7.134	982	992	1004	rVB4	48735	122008	11.58%	1.414%
40	7.311	1013	1021	1033	rBV	229037	499031	47.38%	5.784%
41	7.604	1066	1069	1070	rBV2	395	321	0.03%	0.004%
42	7.939	1118	1124	1131	rBV5	1851	4315	0.41%	0.050%
43	8.031	1135	1139	1142	rBV2	453	773	0.07%	0.009%
44	8.171	1161	1162	1164	rBV	618	382	0.04%	0.004%
45	8.244	1172	1174	1175	rBV	520	340	0.03%	0.004%
46	8.329	1181	1188	1197	rBV	152728	244238	23.19%	2.831%
47	8.652	1235	1241	1250	rVV	479100	744039	70.64%	8.624%
48	8.835	1269	1271	1273	rBV2	461	373	0.04%	0.004%
49	8.957	1282	1291	1301	rBV	105364	162413	15.42%	1.883%
50	9.079	1309	1311	1314	rVB3	550	388	0.04%	0.004%
51	9.280	1340	1344	1351	rVB3	2447	3700	0.35%	0.043%
52	9.390	1356	1362	1377	rBV	487807	698244	66.29%	8.094%
53	9.646	1402	1404	1405	rBV	409	313	0.03%	0.004%
54	9.707	1411	1414	1420	rVB3	2609	3722	0.35%	0.043%
55	9.756	1420	1422	1423	rBV2	577	322	0.03%	0.004%
56	9.768	1423	1424	1428	rVV	609	682	0.06%	0.008%
57	9.817	1430	1432	1433	rBV2	571	299	0.03%	0.003%
58	9.841	1433	1436	1440	rVB3	475	858	0.08%	0.010%
59	9.890	1440	1444	1447	rBV2	288	328	0.03%	0.004%
60	10.055	1466	1471	1484	rVV	555098	743439	70.58%	8.617%
61	10.146	1484	1486	1489	rVB3	829	678	0.06%	0.008%
62	10.292	1507	1510	1512	rBV2	489	653	0.06%	0.008%
63	10.725	1580	1581	1585	rVB2	434	303	0.03%	0.004%
64	10.914	1608	1612	1616	rBV2	297	607	0.06%	0.007%
65	11.006	1626	1627	1631	rBV2	401	390	0.04%	0.005%
66	11.042	1631	1633	1634	rVV2	426	327	0.03%	0.004%
67	11.097	1641	1642	1644	rVB2	576	308	0.03%	0.004%
68	11.195	1652	1658	1671	rBV	432602	545982	51.84%	6.329%
69	11.439	1697	1698	1701	rBV	491	367	0.03%	0.004%
70	11.536	1713	1714	1717	rBV2	322	312	0.03%	0.004%
71	11.628	1727	1729	1733	rBV2	709	887	0.08%	0.010%
72	11.804	1756	1758	1762	rVB2	468	437	0.04%	0.005%
73	11.951	1781	1782	1784	rBV	468	421	0.04%	0.005%
74	12.024	1789	1794	1804	rVV	549460	660979	62.76%	7.662%
75	12.323	1837	1843	1850	rBV	563270	693738	65.87%	8.041%
76	12.548	1877	1880	1881	rBV2	326	344	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030603.D
 Acq On : 12 Aug 2022 18:42
 Operator : JC/MD
 Sample : N4131-08DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D60DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.841	1924	1928	1930	rBV	722	761	0.07%	0.009%
78	12.883	1932	1935	1936	rBV2	538	359	0.03%	0.004%
79	13.030	1953	1959	1960	rBV2	362	605	0.06%	0.007%
80	13.121	1972	1974	1976	rBV2	578	677	0.06%	0.008%
81	13.146	1976	1978	1981	rVV	590	581	0.06%	0.007%
82	13.188	1984	1985	1988	rBV2	340	377	0.04%	0.004%
83	13.225	1989	1991	1994	rVB2	496	453	0.04%	0.005%
84	13.261	1994	1997	1998	rBV2	461	443	0.04%	0.005%
85	13.280	1998	2000	2001	rBV	444	301	0.03%	0.003%
86	13.572	2046	2048	2050	rBV	369	305	0.03%	0.004%
87	13.676	2064	2065	2067	rBV	468	351	0.03%	0.004%
88	13.883	2097	2099	2101	rBV2	315	385	0.04%	0.004%
89	14.261	2158	2161	2162	rBV	409	386	0.04%	0.004%
90	14.347	2173	2175	2177	rBV2	445	459	0.04%	0.005%
91	14.444	2189	2191	2193	rVB	743	341	0.03%	0.004%
92	14.767	2242	2244	2245	rBV2	518	457	0.04%	0.005%
93	14.798	2247	2249	2251	rBV	611	467	0.04%	0.005%
94	15.328	2334	2336	2338	rBV2	723	520	0.05%	0.006%
95	15.353	2338	2340	2343	rBV2	479	650	0.06%	0.008%
96	15.481	2359	2361	2362	rBV	586	416	0.04%	0.005%
97	15.767	2405	2408	2410	rBV4	916	1255	0.12%	0.015%
98	15.877	2424	2426	2428	rVB2	674	421	0.04%	0.005%
99	16.401	2511	2512	2514	rVB	776	458	0.04%	0.005%
100	16.432	2514	2517	2518	rBV	579	577	0.05%	0.007%




Sum of corrected areas: 8627209

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030603.D
Acq On : 12 Aug 2022 18:42
Operator : JC/MD
Sample : N4131-08DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D60DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

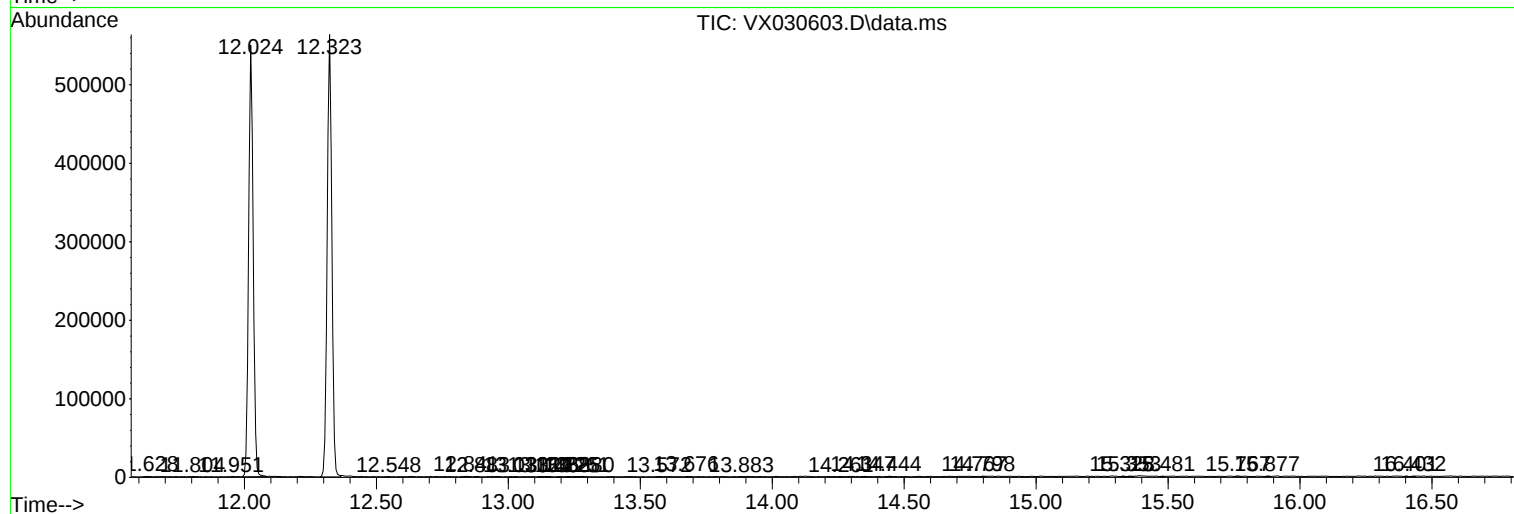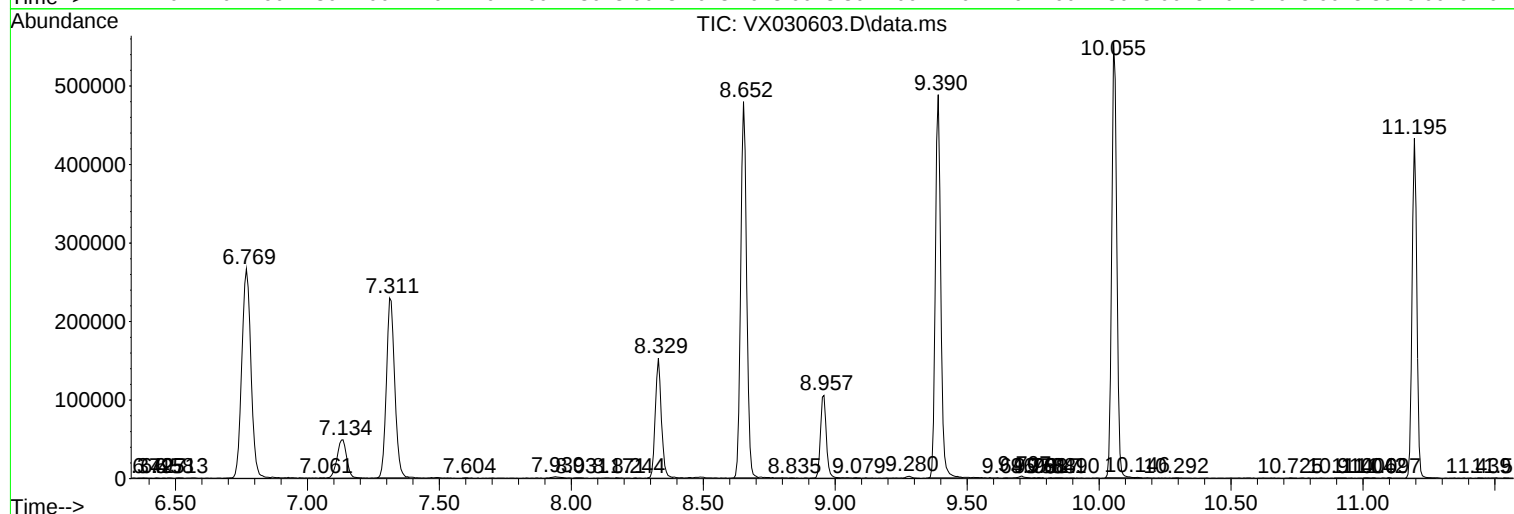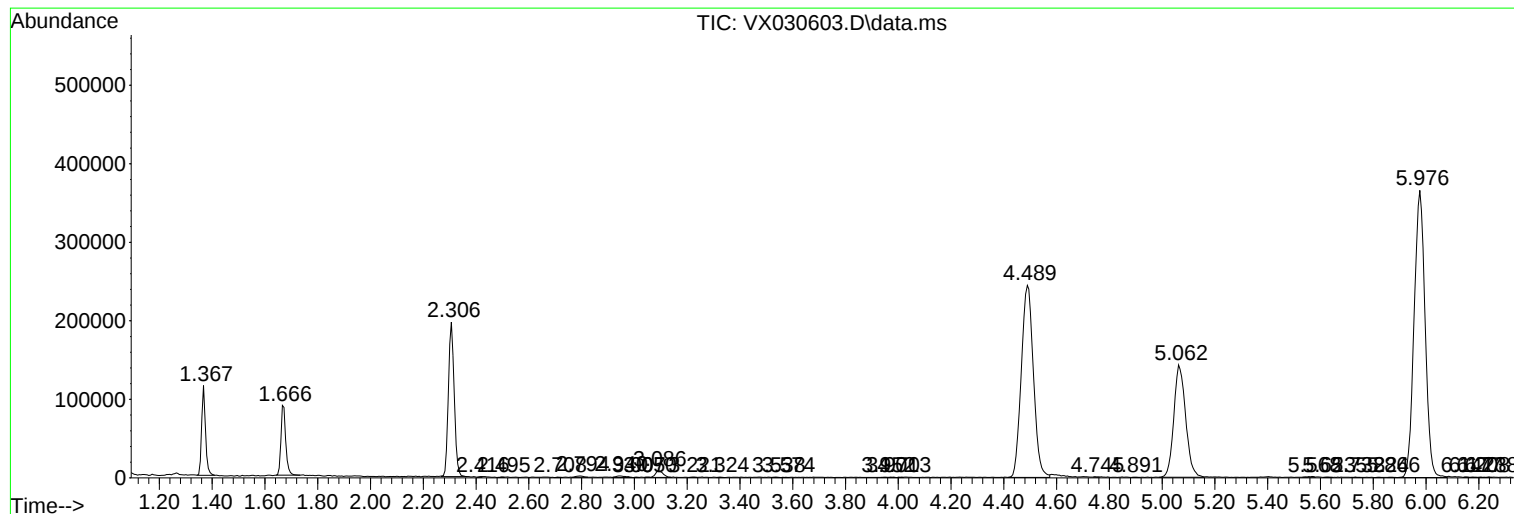

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030603.D
Acq On : 12 Aug 2022 18:42
Operator : JC/MD
Sample : N4131-08DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D60DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030603.D
Acq On : 12 Aug 2022 18:42
Operator : JC/MD
Sample : N4131-08DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D60DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc