

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030604.D
 Acq On : 12 Aug 2022 19:05
 Operator : JC/MD
 Sample : N4131-11DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D90DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	57	rVB2	214231	235613	23.14%	2.750%
2	1.666	91	95	104	rVB	89519	111032	10.90%	1.296%
3	2.306	194	200	210	rVB	190296	296646	29.13%	3.462%
4	2.507	229	233	234	rBV2	477	706	0.07%	0.008%
5	2.642	254	255	258	rBV2	456	423	0.04%	0.005%
6	2.684	258	262	263	rBV3	583	615	0.06%	0.007%
7	2.739	268	271	274	rBV3	633	918	0.09%	0.011%
8	2.788	274	279	288	rVB6	1484	3277	0.32%	0.038%
9	2.946	298	305	315	rVB2	5296	12640	1.24%	0.148%
10	3.020	315	317	319	rVB	566	356	0.03%	0.004%
11	3.093	323	329	337	rVB	13583	26415	2.59%	0.308%
12	3.294	359	362	364	rBV2	358	348	0.03%	0.004%
13	3.483	391	393	395	rVB2	497	391	0.04%	0.005%
14	3.812	444	447	449	rBV	443	570	0.06%	0.007%
15	3.879	456	458	461	rBV	414	522	0.05%	0.006%
16	4.007	476	479	480	rBV2	480	483	0.05%	0.006%
17	4.086	490	492	494	rBV2	491	452	0.04%	0.005%
18	4.123	496	498	501	rBV2	347	383	0.04%	0.004%
19	4.160	501	504	506	rVB2	442	515	0.05%	0.006%
20	4.269	519	522	523	rVB	525	463	0.05%	0.005%
21	4.343	532	534	536	rBV2	373	339	0.03%	0.004%
22	4.489	546	558	572	rBV3	284350	884587	86.86%	10.324%
23	4.745	597	600	602	rBV	726	674	0.07%	0.008%
24	4.824	611	613	617	rVB2	554	649	0.06%	0.008%
25	4.867	617	620	621	rBV3	586	526	0.05%	0.006%
26	4.885	621	623	627	rBV2	503	560	0.05%	0.007%
27	4.928	627	630	631	rBV	543	531	0.05%	0.006%
28	5.068	640	653	667	rBV	132771	427394	41.97%	4.988%
29	5.208	674	676	680	rVB2	631	601	0.06%	0.007%
30	5.251	680	683	686	rBV3	488	632	0.06%	0.007%
31	5.373	698	703	704	rBV2	709	937	0.09%	0.011%
32	5.513	725	726	728	rBV	353	375	0.04%	0.004%
33	5.812	774	775	777	rBV	550	336	0.03%	0.004%
34	5.842	777	780	783	rVB2	396	434	0.04%	0.005%
35	5.873	783	785	788	rBV	385	422	0.04%	0.005%
36	5.976	790	802	819	rVV2	353453	1018399	100.00%	11.886%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030604.D
 Acq On : 12 Aug 2022 19:05
 Operator : JC/MD
 Sample : N4131-11DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D90DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

37	6.287	852	853	855	rBV	386	343	0.03%	0.004%
38	6.324	857	859	862	rBV2	666	536	0.05%	0.006%
39	6.373	865	867	869	rBV2	554	563	0.06%	0.007%
40	6.440	876	878	879	rBV2	441	361	0.04%	0.004%
41	6.769	922	932	947	rBV	263554	612569	60.15%	7.149%
42	6.982	965	967	971	rBV3	491	589	0.06%	0.007%
43	7.123	982	990	999	rBV5	9898	23462	2.30%	0.274%
44	7.190	999	1001	1003	rBV2	407	478	0.05%	0.006%
45	7.312	1013	1021	1034	rBV	228000	499475	49.05%	5.829%
46	7.470	1044	1047	1048	rBV2	708	626	0.06%	0.007%
47	7.586	1063	1066	1068	rVB2	437	417	0.04%	0.005%
48	7.622	1071	1072	1075	rBV	418	473	0.05%	0.006%
49	7.848	1107	1109	1112	rVB2	516	490	0.05%	0.006%
50	7.878	1112	1114	1116	rBV	427	488	0.05%	0.006%
51	7.933	1119	1123	1125	rBV4	1669	2580	0.25%	0.030%
52	8.116	1152	1153	1158	rVB	540	436	0.04%	0.005%
53	8.189	1163	1165	1168	rBV	413	415	0.04%	0.005%
54	8.330	1181	1188	1200	rBV	141942	237848	23.36%	2.776%
55	8.482	1210	1213	1220	rVB6	1314	2624	0.26%	0.031%
56	8.653	1234	1241	1254	rBV	475980	727792	71.46%	8.494%
57	8.738	1254	1255	1258	rBV3	599	544	0.05%	0.006%
58	8.860	1273	1275	1277	rBV	496	493	0.05%	0.006%
59	8.958	1285	1291	1298	rBV	104882	157062	15.42%	1.833%
60	9.232	1334	1336	1338	rVB2	450	393	0.04%	0.005%
61	9.275	1341	1343	1346	rBV3	419	487	0.05%	0.006%
62	9.390	1356	1362	1375	rBV	471498	682739	67.04%	7.968%
63	9.707	1411	1414	1420	rVB2	2687	3661	0.36%	0.043%
64	9.963	1454	1456	1459	rBV	402	347	0.03%	0.004%
65	10.055	1465	1471	1482	rBV	515306	702830	69.01%	8.203%
66	10.201	1493	1495	1496	rVB2	712	403	0.04%	0.005%
67	10.250	1502	1503	1505	rBV	575	412	0.04%	0.005%
68	10.384	1522	1525	1526	rBV2	384	385	0.04%	0.004%
69	10.500	1543	1544	1546	rBV	792	535	0.05%	0.006%
70	10.927	1611	1614	1615	rVB2	400	347	0.03%	0.004%
71	10.951	1616	1618	1622	rBV3	394	512	0.05%	0.006%
72	11.006	1624	1627	1628	rBV2	572	553	0.05%	0.006%
73	11.024	1629	1630	1633	rVB2	438	349	0.03%	0.004%
74	11.067	1636	1637	1641	rBV	495	447	0.04%	0.005%
75	11.134	1646	1648	1652	rBV3	291	479	0.05%	0.006%
76	11.195	1652	1658	1668	rBV	439133	535066	52.54%	6.245%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030604.D
 Acq On : 12 Aug 2022 19:05
 Operator : JC/MD
 Sample : N4131-11DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D90DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.408	1691	1693	1697	rBV2	448	547	0.05%	0.006%
78	11.481	1703	1705	1706	rBV	626	441	0.04%	0.005%
79	11.622	1724	1728	1731	rBV	588	621	0.06%	0.007%
80	11.762	1748	1751	1755	rBV2	469	584	0.06%	0.007%
81	11.902	1773	1774	1777	rVB2	729	563	0.06%	0.007%
82	12.024	1789	1794	1807	rVB	511915	642111	63.05%	7.494%
83	12.323	1837	1843	1851	rBV	541210	684181	67.18%	7.985%
84	12.554	1878	1881	1882	rBV	512	482	0.05%	0.006%
85	12.762	1913	1915	1918	rVB2	644	648	0.06%	0.008%
86	12.786	1918	1919	1922	rBV	399	423	0.04%	0.005%
87	13.566	2045	2047	2050	rVB2	515	454	0.04%	0.005%
88	13.591	2050	2051	2054	rVB	534	521	0.05%	0.006%
89	13.883	2095	2099	2101	rBV2	595	625	0.06%	0.007%
90	13.987	2115	2116	2118	rBV	433	335	0.03%	0.004%
91	14.103	2132	2135	2137	rBV2	489	611	0.06%	0.007%
92	14.121	2137	2138	2140	rBV	446	340	0.03%	0.004%
93	14.213	2151	2153	2155	rBV2	356	342	0.03%	0.004%
94	14.231	2155	2156	2158	rVB	724	501	0.05%	0.006%
95	14.828	2252	2254	2258	rVV3	492	700	0.07%	0.008%
96	15.024	2284	2286	2287	rBV	885	523	0.05%	0.006%
97	15.353	2338	2340	2343	rBV2	670	548	0.05%	0.006%
98	16.657	2552	2554	2556	rVB2	700	441	0.04%	0.005%
99	16.682	2556	2558	2559	rBV	797	391	0.04%	0.005%
100	16.743	2566	2568	2569	rBV2	434	369	0.04%	0.004%




Sum of corrected areas: 8568075

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030604.D
Acq On : 12 Aug 2022 19:05
Operator : JC/MD
Sample : N4131-11DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

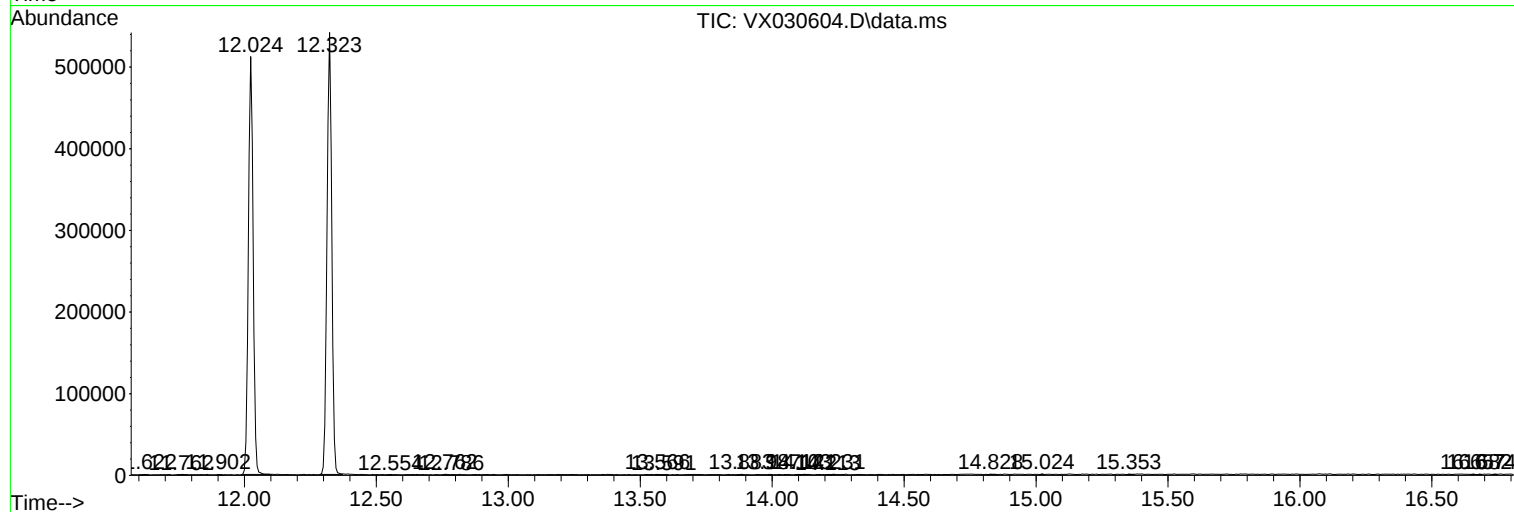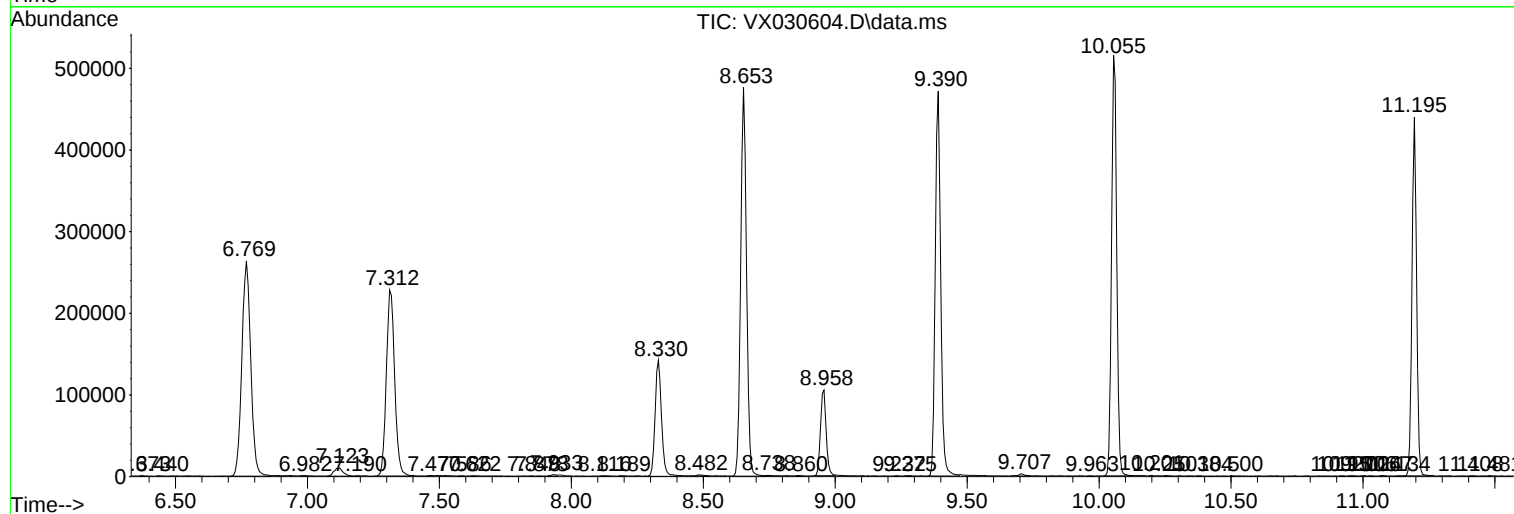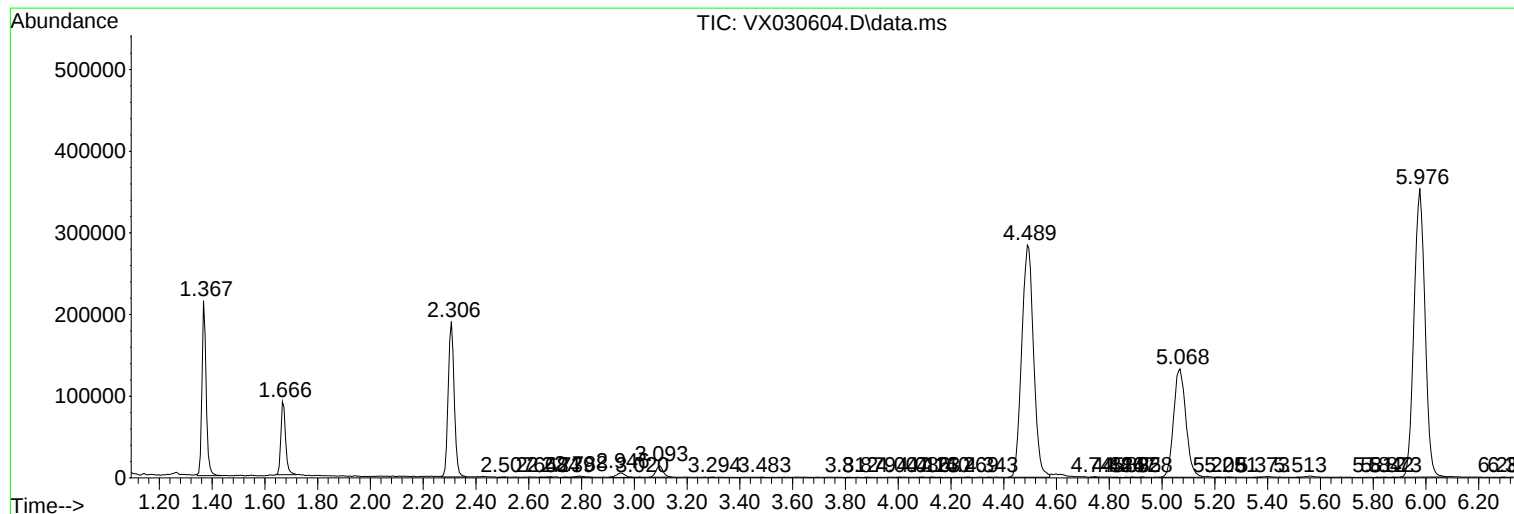

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030604.D
Acq On : 12 Aug 2022 19:05
Operator : JC/MD
Sample : N4131-11DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030604.D
Acq On : 12 Aug 2022 19:05
Operator : JC/MD
Sample : N4131-11DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc