
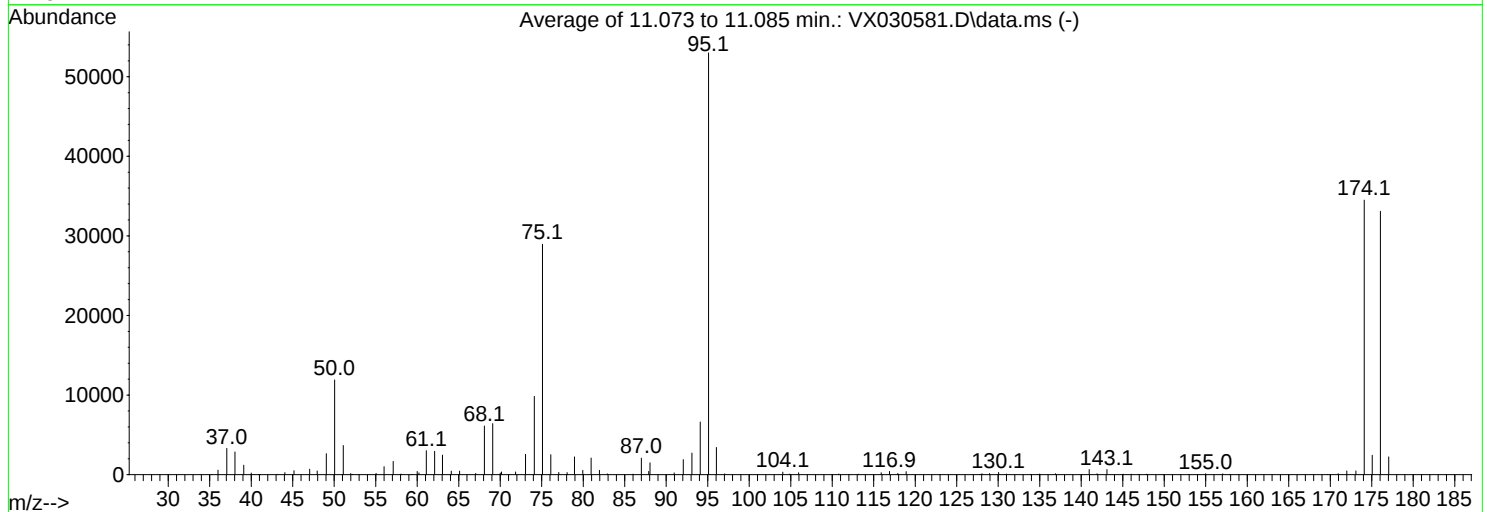


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030581.D
 Acq On : 12 Aug 2022 08:39
 Operator : JC/MD
 Sample : BFB677
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB677

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Fri Aug 12 23:28:07 2022

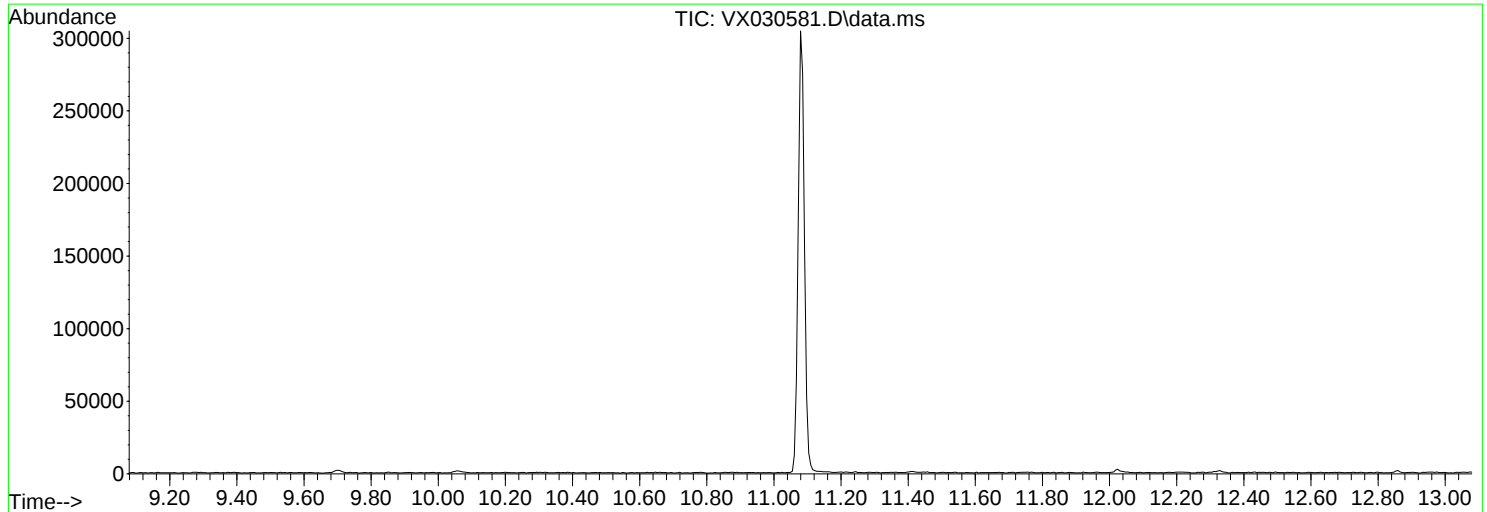

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	11909	PASS
75	95	30	80	54.6	28952	PASS
95	95	100	100	100.0	53000	PASS
96	95	5	9	6.4	3416	PASS
173	174	0.00	2	1.3	455	PASS
174	95	50	120	65.1	34509	PASS
175	174	5	9	7.0	2424	PASS
176	174	95	101	95.9	33096	PASS
177	176	5	9	6.8	2236	PASS

m/z	Abundance
36.00	92.0
40.00	413.0
44.10	409.0

Instrument :
MSVOA_X
ClientSampleId :
BFB677

m/z	Abundance
36.00	469.0
37.00	2798.0
38.10	2500.0
39.10	906.0
40.00	710.0
40.90	72.0
44.00	436.0
45.20	380.0
47.10	516.0
48.00	436.0
49.00	2161.0
50.00	9768.0
51.10	3148.0
52.10	81.0
52.90	72.0
55.00	228.0
56.00	781.0
57.10	1288.0
58.00	71.0
60.00	670.0
61.10	2471.0
62.10	2771.0
63.00	2181.0
64.10	383.0
65.10	220.0
67.10	68.0
68.10	4817.0
69.10	4776.0
70.00	577.0
71.10	51.0
71.80	249.0
73.00	1907.0
74.10	7079.0
75.10	21960.0
76.10	1870.0
77.10	136.0
78.00	141.0
78.90	1662.0
79.90	432.0
80.90	1784.0
81.90	468.0
82.90	77.0
87.00	1942.0
87.90	1238.0
90.90	183.0
92.00	1455.0
93.10	2016.0
94.10	5377.0
95.10	40744.0
96.10	2809.0
97.20	71.0
104.00	300.0
104.90	132.0
105.90	251.0
111.00	72.0
112.00	69.0
115.90	194.0
116.90	198.0
117.90	85.0
118.90	219.0
127.80	98.0
129.00	147.0
130.20	123.0
131.00	58.0
134.80	80.0
136.80	56.0
141.00	449.0
141.80	126.0
143.10	500.0
148.00	74.0
149.90	78.0
155.10	74.0
157.10	77.0
171.90	278.0
173.10	221.0
174.10	20360.0
175.10	1619.0
176.10	20560.0
177.00	1292.0

Instrument :
MSVOA_X
ClientSampleId :
BFB677

m/z	Abundance
36.10	917.0
37.10	3549.0
38.00	3259.0
39.10	1334.0
40.00	444.0
41.10	54.0
44.10	959.0
45.10	720.0
46.90	574.0
47.90	505.0
49.10	3219.0
50.10	14201.0
51.10	3943.0
52.00	366.0
55.10	243.0
56.00	1198.0
57.10	2004.0
58.10	106.0
59.30	55.0
60.20	661.0
61.10	3734.0
62.10	3513.0
63.00	2751.0
64.20	529.0
65.00	555.0
67.10	212.0
68.10	7213.0
69.10	7863.0
70.20	590.0
71.90	549.0
73.10	3216.0
74.10	11914.0
75.10	34408.0
76.10	3178.0
77.10	299.0
78.10	325.0
78.90	2567.0
80.00	608.0
81.00	2508.0
81.90	597.0
82.90	155.0
86.00	68.0
87.00	2187.0
88.10	2455.0
91.00	216.0
92.10	2142.0
93.10	3207.0
94.10	7756.0
95.10	62456.0
96.10	4280.0
97.00	167.0
104.00	354.0
104.90	142.0
105.90	199.0
110.80	62.0
112.00	70.0
113.10	95.0
115.90	292.0
116.90	597.0
117.90	141.0
118.90	432.0
128.00	221.0
128.90	111.0
130.00	363.0
131.00	124.0
133.90	60.0
135.00	176.0
136.90	221.0
140.10	89.0
141.00	845.0
141.90	68.0
143.10	711.0
145.00	133.0
146.00	110.0
146.90	58.0
147.80	68.0
155.00	229.0
157.10	90.0
159.00	61.0
171.10	92.0
172.00	485.0
173.20	585.0
174.10	42504.0
175.10	2932.0
176.10	39088.0
177.10	2699.0

Instrument :
MSVOA_X
ClientSampleId :
BFB677

m/z	Abundance
35.30	79.0
36.10	593.0
37.10	3522.0
38.10	2789.0
39.10	1333.0
40.00	676.0
43.20	110.0
44.10	622.0
45.20	415.0
47.10	970.0
48.00	440.0
49.00	2546.0
50.10	11758.0
51.10	3910.0
52.20	151.0
56.00	1009.0
57.10	1697.0
58.10	88.0
60.00	524.0
61.10	2865.0
62.10	2514.0
63.10	2438.0
64.00	428.0
65.20	542.0
67.00	189.0
68.10	6317.0
69.10	6634.0
70.10	469.0
71.80	234.0
73.10	2509.0
74.10	10475.0
75.10	30488.0
76.10	2467.0
77.00	445.0
78.10	313.0
79.00	2501.0
80.00	611.0
80.90	2001.0
82.00	541.0
83.00	62.0
86.00	98.0
87.00	2107.0
88.00	2035.0
90.90	236.0
92.00	2101.0
93.10	2946.0
94.10	6701.0
95.10	55800.0
96.00	3158.0
97.00	59.0
104.10	296.0
106.00	267.0
110.70	100.0
113.20	62.0
115.90	263.0
116.90	411.0
117.90	252.0
118.90	473.0
122.90	59.0
128.10	170.0
128.90	151.0
130.10	348.0
131.00	77.0
135.00	96.0
137.00	91.0
140.90	660.0
142.00	149.0
143.10	749.0
145.10	74.0
146.10	62.0
147.80	69.0
152.90	61.0
155.10	82.0
157.00	144.0
157.90	52.0
169.70	84.0
170.90	245.0
172.10	600.0
173.00	560.0
174.10	40664.0
175.00	2720.0
176.00	39640.0
177.00	2716.0

Instrument :
MSVOA_X
ClientSampleId :
BFB677