

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081318\
 Data File : VX004002.D
 Acq On : 13 Aug 2018 16:08
 Operator : JC/MD
 Sample : J4447-15
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SP-1-7


Quant Time: Aug 14 03:08:51 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 13 01:34:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	308377	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	514170	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	478042	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	257878	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	225710	55.22	ug/l	0.00
Spiked Amount			Recovery	=	110.44%	
35) Dibromofluoromethane	5.51	113	183126	47.01	ug/l	0.00
Spiked Amount			Recovery	=	94.02%	
50) Toluene-d8	8.72	98	731476	48.29	ug/l	0.00
Spiked Amount			Recovery	=	96.58%	
62) 4-Bromofluorobenzene	11.14	95	251057	51.22	ug/l	0.00
Spiked Amount			Recovery	=	102.44%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.65	94	869	0.32	ug/l	98
6) Chloroethane	1.59	64	14162	5.22	ug/l #	55
11) Tert butyl alcohol	3.04	59	2074	2.11	ug/l #	73
13) Acrolein	2.28	56	164	0.30	ug/l	87
16) Acetone	2.43	43	13897	5.71	ug/l	100
18) Methyl Acetate	2.77	43	5561	1.05	ug/l	91
20) Methylene Chloride	2.86	84	7407	1.26	ug/l	93
25) 2-Butanone	4.70	43	3348	0.92	ug/l	93
29) Tetrahydrofuran	5.16	42	1439	0.77	ug/l	98
30) Chloroform	5.21	83	5170	0.79	ug/l	94
31) Cyclohexane	5.59	56	5305	0.90	ug/l	95
36) 1,1-Dichloropropene	5.67	75	21241	3.69	ug/l #	50
38) Carbon Tetrachloride	5.67	117	27308	4.98	ug/l #	15
39) Methylcyclohexane	7.47	83	5271	0.78	ug/l	92
43) Isopropyl Acetate	6.46	43	151206	15.86	ug/l	99
47) Bromodichloromethane	7.90	83	1338	0.24	ug/l #	95
48) Methyl methacrylate	7.88	41	17434	3.60	ug/l #	42
51) 4-Methyl-2-Pentanone	8.62	43	2541	0.32	ug/l #	34
59) 2-Hexanone	9.55	43	10336	1.75	ug/l #	55
67) Ethyl Benzene	10.26	91	12079	0.59	ug/l	99
68) m/p-Xylenes	10.36	106	16100	2.02	ug/l	97
69) o-Xylene	10.70	106	2105	0.28	ug/l	99
74) N-ethyl acetate	6.46	43	151206	15.24	ug/l #	99
76) 1,2,3-Trichloropropane	11.14	75	121793	21.38	ug/l #	36
80) 1,3,5-Trimethylbenzene	11.51	105	3524	0.23	ug/l	91
81) trans-1,4-Dichloro-2-buten	11.14	75	121793	65.17	ug/l #	9
84) 1,2,4-Trimethylbenzene	11.81	105	9822	0.63	ug/l	92
95) Naphthalene	13.83	128	17075	0.89	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

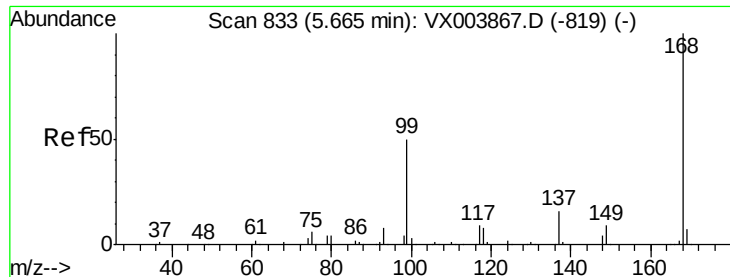

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 833

Delta R.T. 0.00 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08

Instrument :

MSVOA_X

ClientSampled :


SP-1-7

Tot Ion:168 Resp: 308377

Ion Ratio Lower Upper

168 100

99 51.5 40.1 60.1

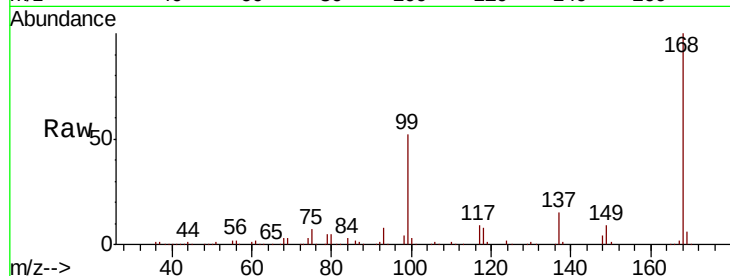

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

120000

100000

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

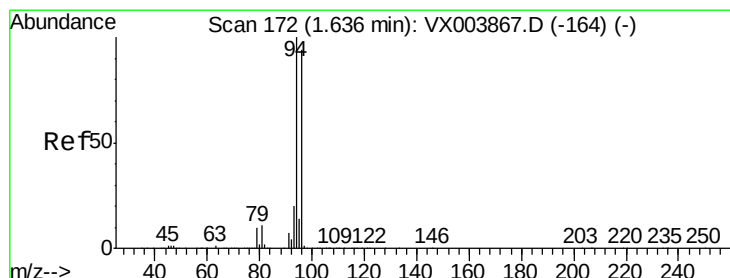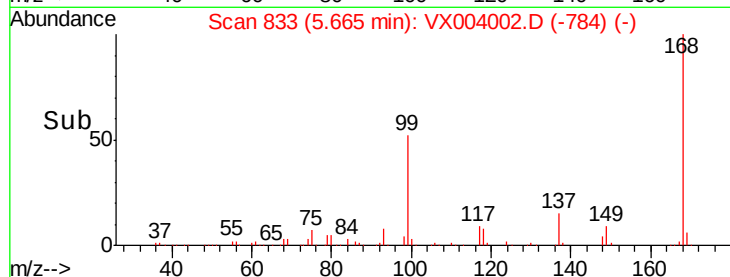

#5

Bromomethane

Concen: 0.32 ug/l

RT: 1.65 min Scan# 174

Delta R.T. 0.01 min

Lab File: VX004002.D


Acq: 13 Aug 2018 16:08

Tgt Ion: 94 Resp: 869

Ion Ratio Lower Upper

94 100

96 95.5 75.2 112.8

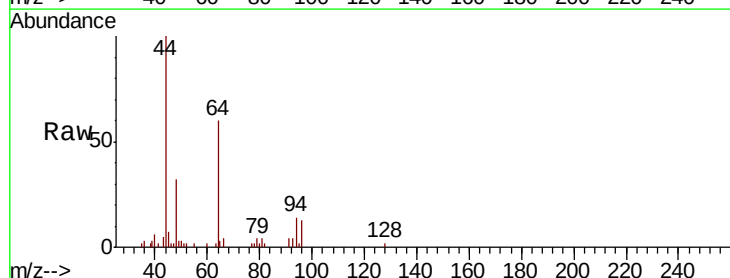

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.65

600

500

400


300


200

100

0

Time--> 1.60 1.65 1.70

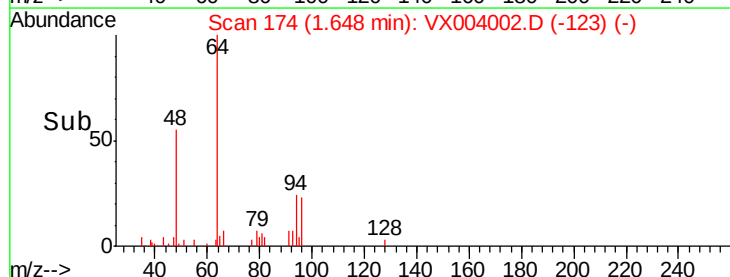

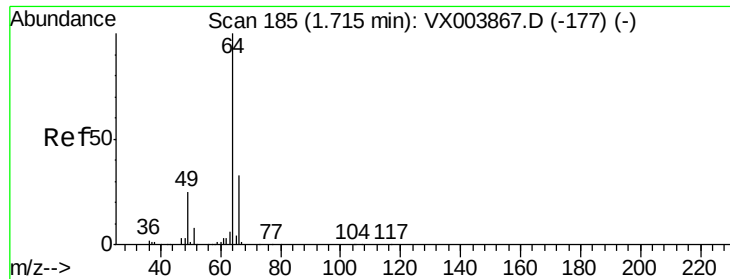

#6

Chloroethane

Concen: 5.22 ug/l

RT: 1.59 min Scan# 165

Delta R.T. -0.12 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08

Instrument :

MSVOA_X

ClientSampled :





SP-1-7

Tot Ion: 64 Resp: 14162

Ion Ratio Lower Upper

64 100

66 7.4 26.5 39.7#

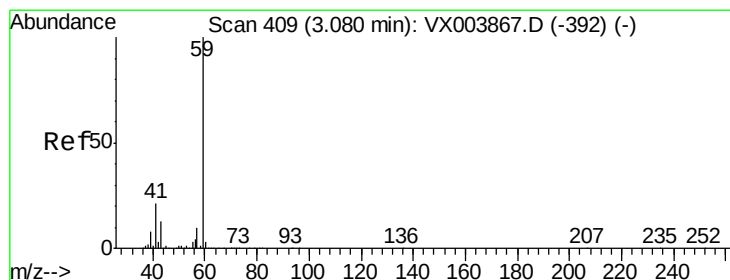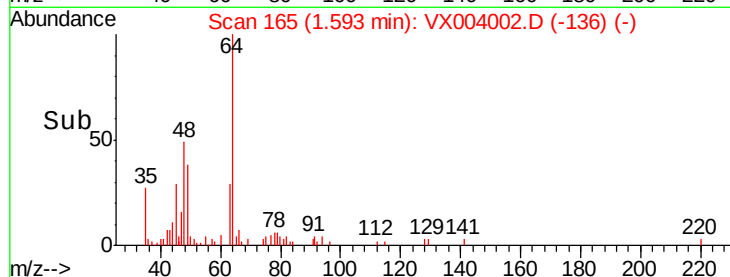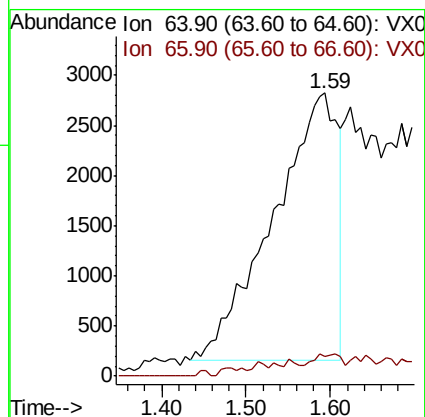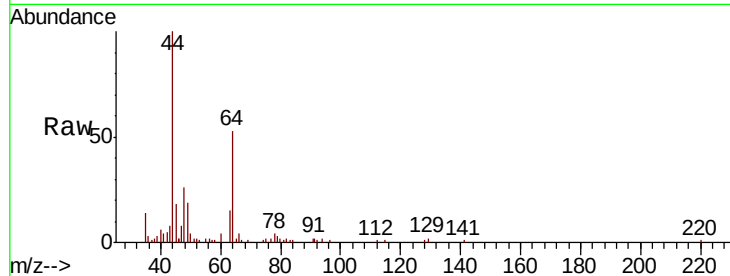

#11

Tert butyl alcohol

Concen: 2.11 ug/l

RT: 3.04 min Scan# 402

Delta R.T. -0.04 min

Lab File: VX004002.D




Acq: 13 Aug 2018 16:08


Tgt Ion: 59 Resp: 2074

Ion Ratio Lower Upper

59 100

57 0.0 8.1 12.1#

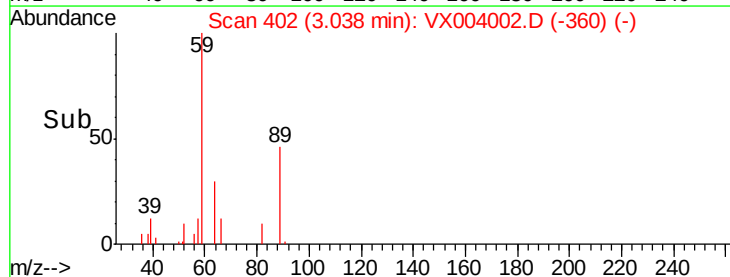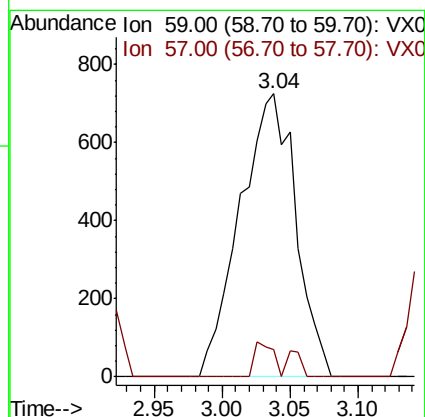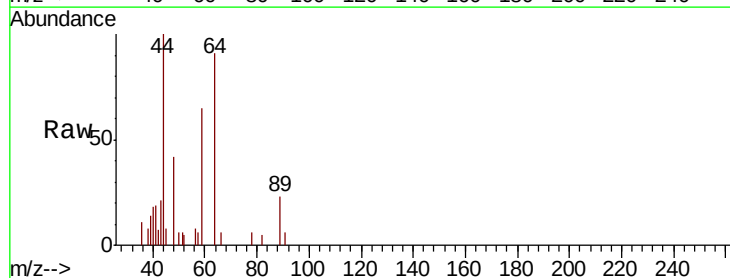

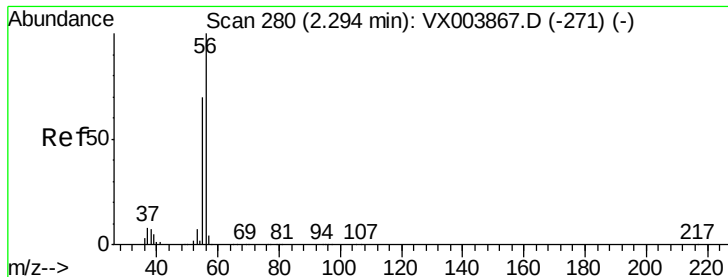

#13

Acrolein

Concen: 0.30 ug/l

RT: 2.28 min Scan# 278

Delta R.T. -0.01 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08

Instrument :

MSVOA_X

ClientSampled :





SP-1-7

Tot Ion: 56 Resp: 164

Ion Ratio Lower Upper

56 100

55 59.8 56.1 84.1

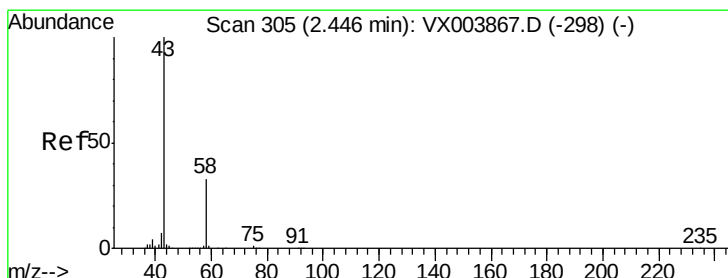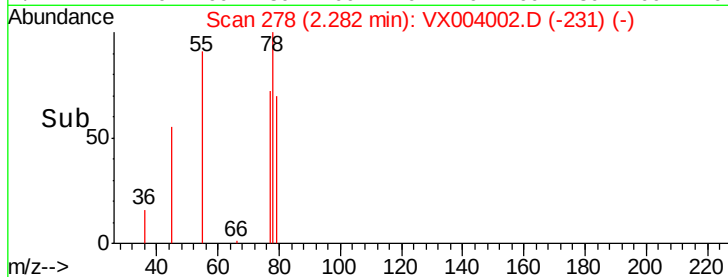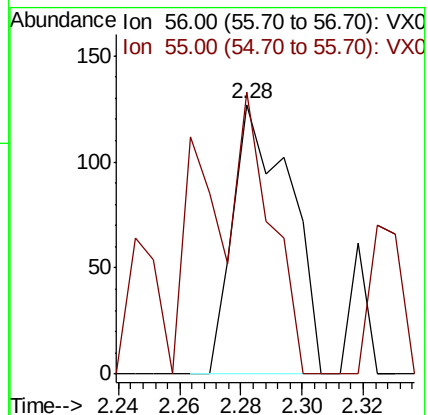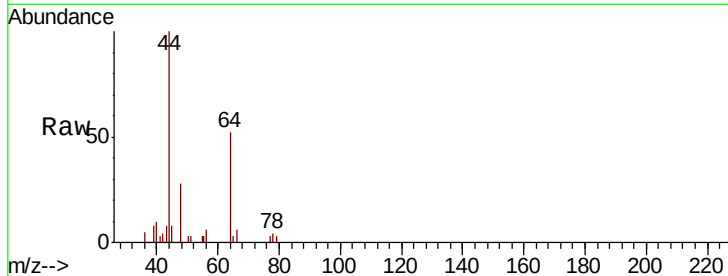

#16

Acetone

Concen: 5.71 ug/l

RT: 2.43 min Scan# 303

Delta R.T. -0.01 min

Lab File: VX004002.D




Acq: 13 Aug 2018 16:08


Tgt Ion: 43 Resp: 13897

Ion Ratio Lower Upper

43 100

58 33.0 26.4 39.6


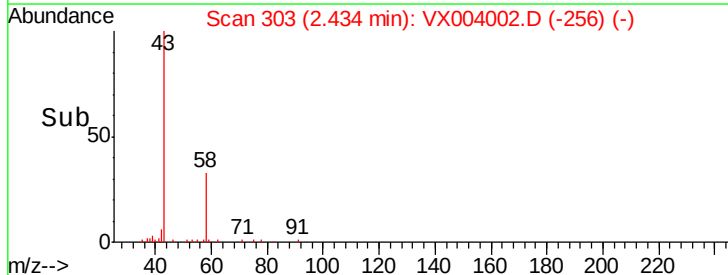
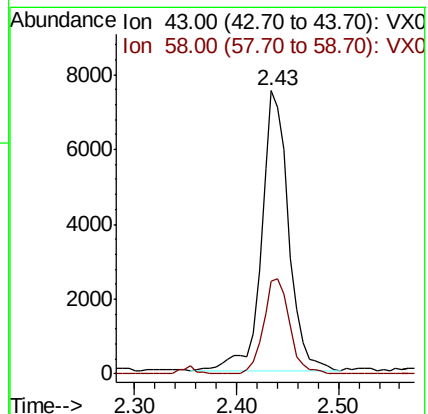
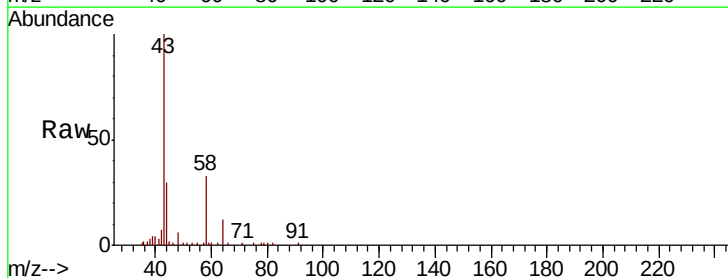




#18
Methvl Acetate
Concen: 1.05 ug/l
RT: 2.77 min Scan# 358
Delta R.T. -0.01 min
Lab File: VX004002.D
Acq: 13 Aug 2018 16:08




Instrument :
MSVOA_X
ClientSampleId :
SP-1-7


Tot Ion: 43 Resp: 5561
Ion Ratio Lower Upper
43 100
74 27.9 18.9 28.3

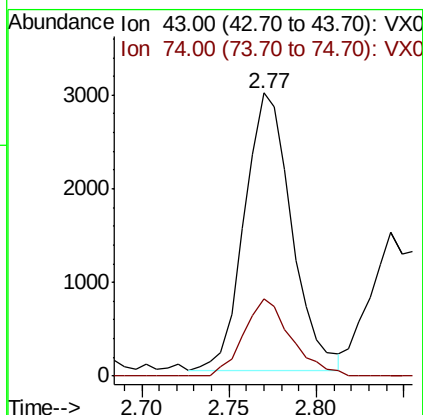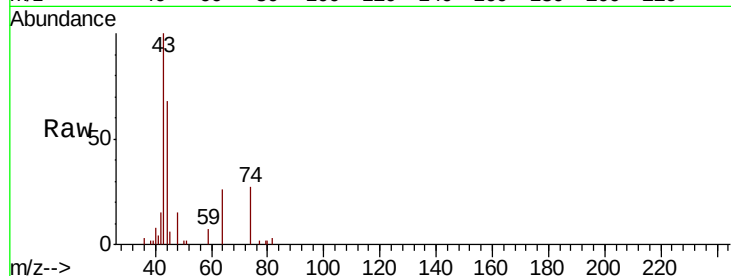

#20
Methylene Chloride
Concen: 1.26 ug/l
RT: 2.86 min Scan# 373
Delta R.T. 0.01 min
Lab File: VX004002.D
Acq: 13 Aug 2018 16:08

Tgt Ion: 84 Resp: 7407
Ion Ratio Lower Upper
84 100
49 110.9 98.9 148.3
51 38.4 29.9 44.9
86 64.9 51.0 76.6

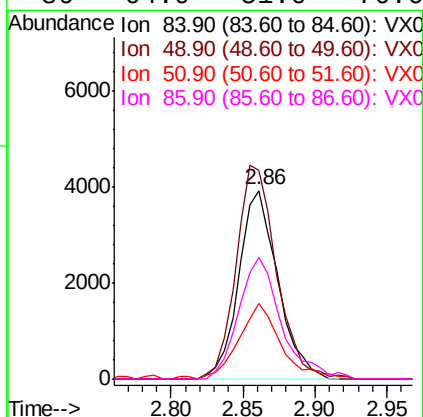



#25

2-Butanone

Concen: 0.92 ug/l

RT: 4.70 min Scan# 674

Delta R.T. -0.01 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08

Instrument :

MSVOA_X

ClientSampled :


SP-1-7

Tot Ion: 43 Resp: 3348

Ion Ratio Lower Upper

43 100

72 23.3 21.4 32.0

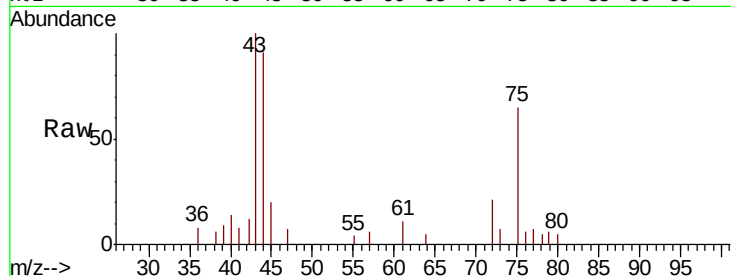

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

1500



1000

500

0

4.60 4.65 4.70 4.75

Time-->



#29

Tetrahydrofuran

Concen: 0.77 ug/l

RT: 5.16 min Scan# 750

Delta R.T. -0.01 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08


Tgt Ion: 42 Resp: 1439

Ion Ratio Lower Upper

42 100

72 47.9 37.7 56.5

71 42.3 35.0 52.6



Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

600


400


200

0

5.05 5.10 5.15 5.20 5.25

Time-->









#30
Chloroform
Concen: 0.79 ug/l
RT: 5.21 min Scan# 759
Delta R.T. 0.00 min
Lab File: VX004002.D
Acq: 13 Aug 2018 16:08




Instrument :
MSVOA_X
ClientSampleId :
SP-1-7


Tot Ion: 83 Resp: 5170
Ion Ratio Lower Upper
83 100
85 68.3 50.7 76.1

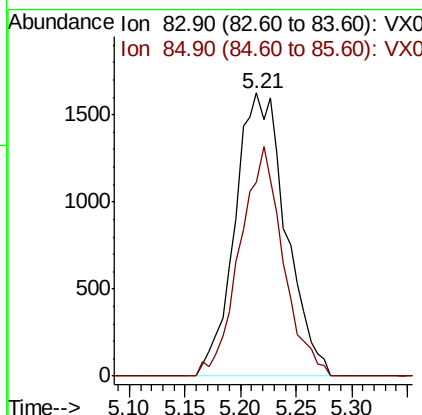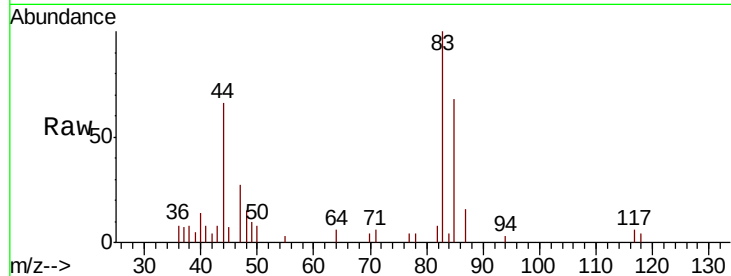

#31
Cyclohexane
Concen: 0.90 ug/l
RT: 5.59 min Scan# 820
Delta R.T. 0.01 min
Lab File: VX004002.D
Acq: 13 Aug 2018 16:08

Tgt Ion: 56 Resp: 5305
Ion Ratio Lower Upper
56 100
69 33.0 24.9 37.3
84 84.1 71.7 107.5



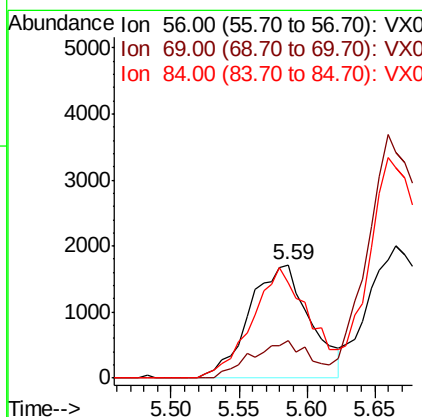
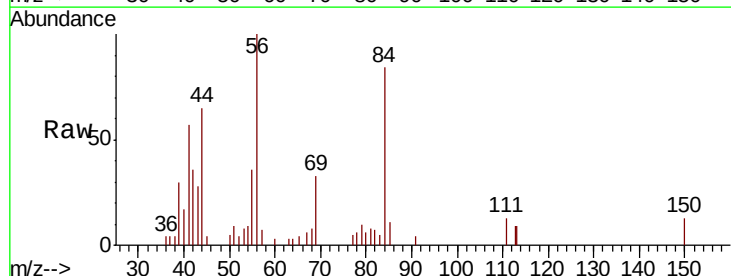


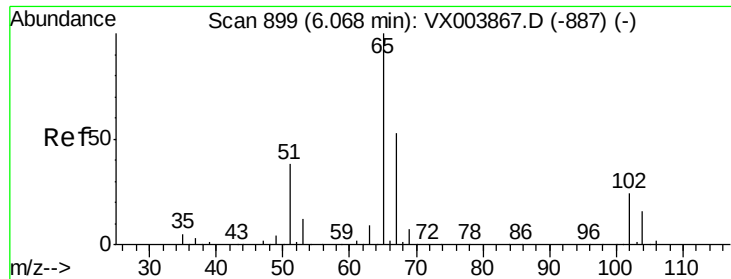

#33
 1,2-Dichloroethane-d4
 Concen: 55.22 ug/l
 RT: 6.07 min Scan# 899
 Delta R.T. 0.00 min
 Lab File: VX004002.D
 Acq: 13 Aug 2018 16:08




Instrument :
 MSVOA_X
 ClientSampleID :
 SP-1-7


Tot Ion: 65 Resp: 225710
 Ion Ratio Lower Upper
 65 100
 67 53.2 0.0 105.8

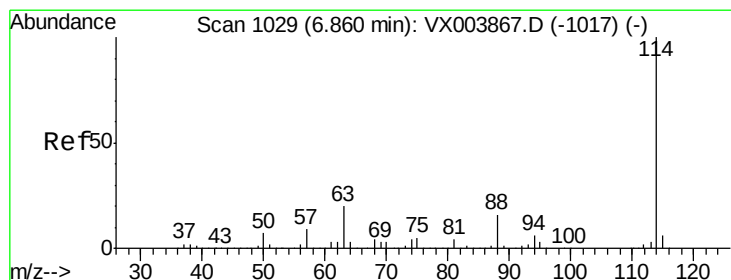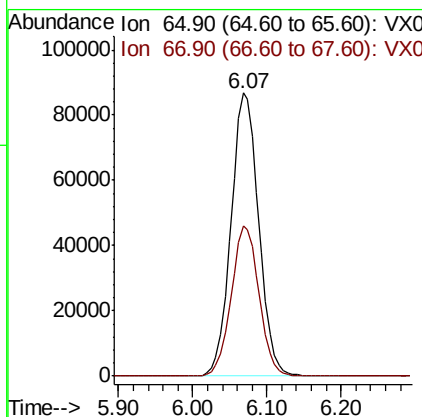

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. 0.01 min
 Lab File: VX004002.D
 Acq: 13 Aug 2018 16:08

Tgt Ion: 114 Resp: 514170
 Ion Ratio Lower Upper
 114 100
 63 20.1 0.0 39.0
 88 15.2 0.0 32.0

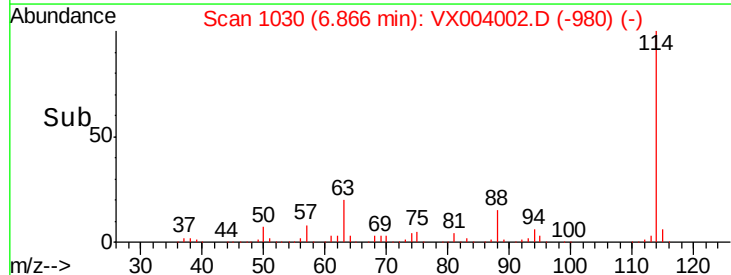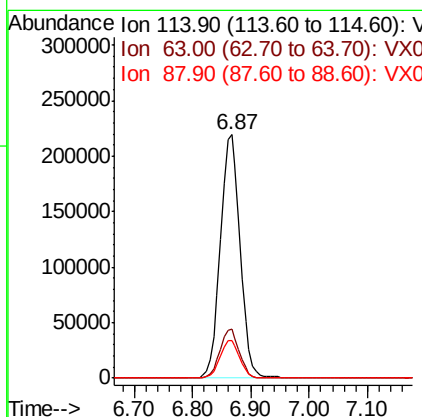

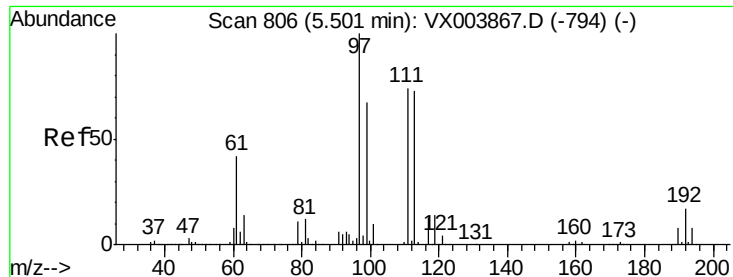

#35

Dibromofluoromethane

Concen: 47.01 ug/l

RT: 5.51 min Scan# 807

Delta R.T. 0.01 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08

Instrument :

MSVOA_X

ClientSampleId :

SP-1-7





Tot Ion:113 Resp: 183126

Ion Ratio Lower Upper

113 100

111 101.6 82.0 123.0

192 22.8 19.0 28.4

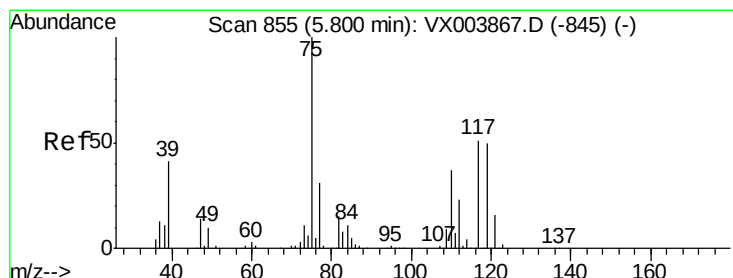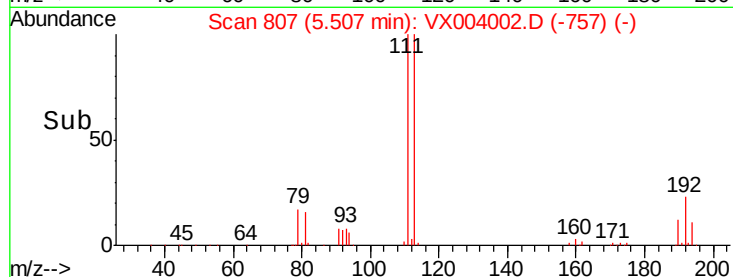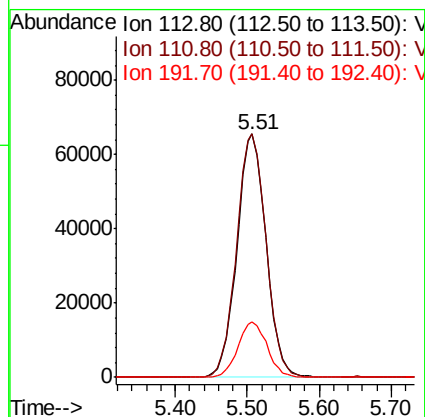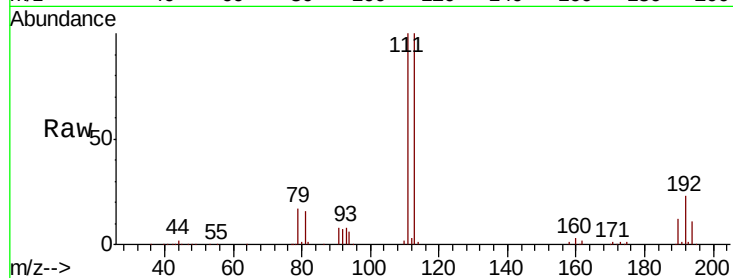

#36

1,1-Dichloropropene

Concen: 3.69 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.13 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08




Tgt Ion: 75 Resp: 21241


Ion Ratio Lower Upper

75 100

110 9.7 18.2 54.6#

77 0.3 25.0 37.4#

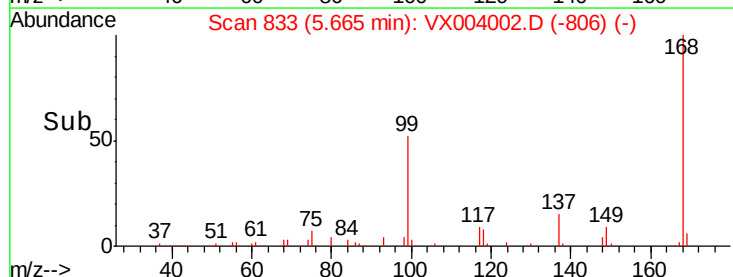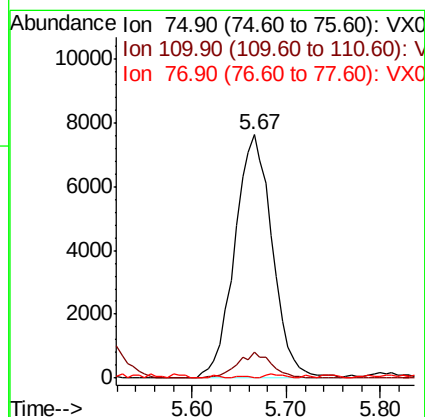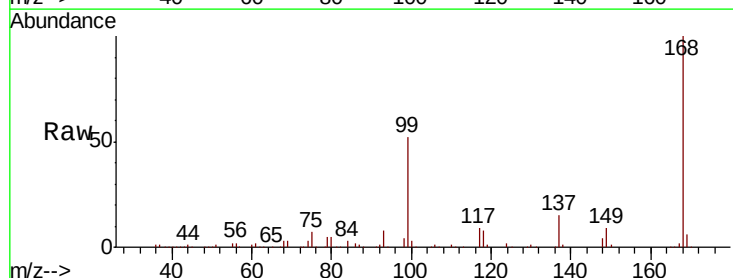

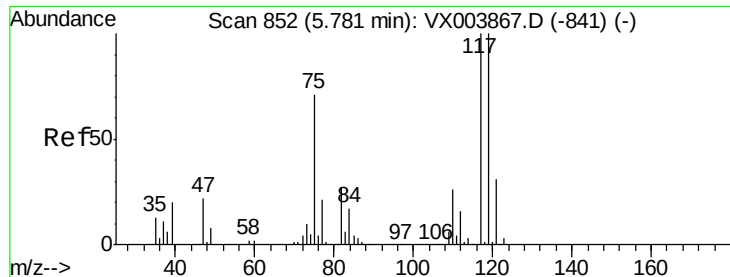

#38

Carbon Tetrachloride

Concen: 4.98 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.12 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08

Instrument :

MSVOA_X

ClientSampled :

SP-1-7


Tot Ion:117 Resp: 27308

Ion Ratio Lower Upper

117 100

119 5.7 79.5 119.3#




121 0.0 25.0 37.4#

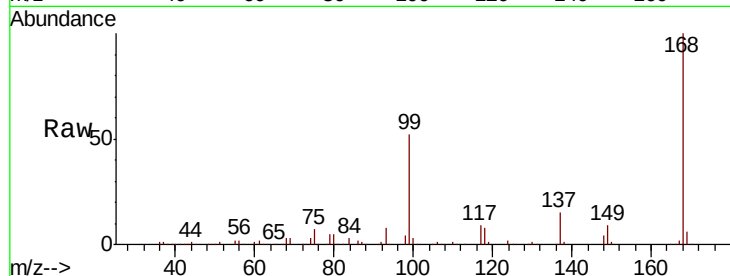

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

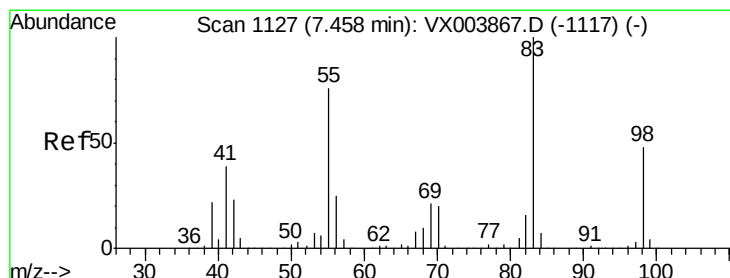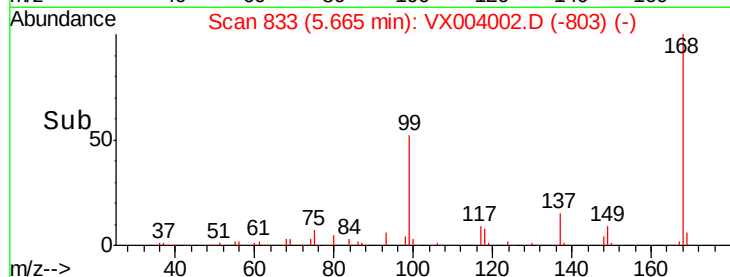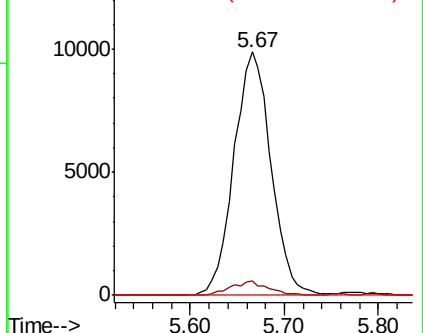

#39

Methylcyclohexane

Concen: 0.78 ug/l

RT: 7.47 min Scan# 1129

Delta R.T. 0.01 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08


Tgt Ion: 83 Resp: 5271

Ion Ratio Lower Upper

83 100

55 70.0 61.0 91.6



98 41.6 38.6 57.8

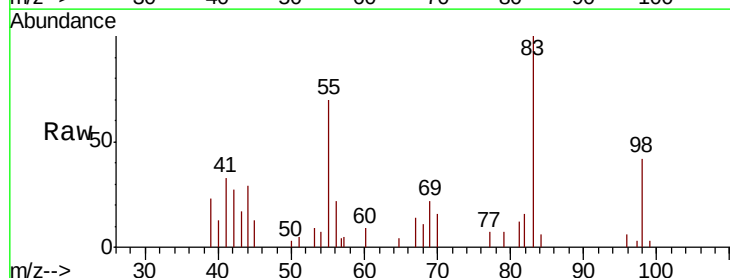


Abundance Ion 83.00 (82.70 to 83.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 98.00 (97.70 to 98.70): VX0

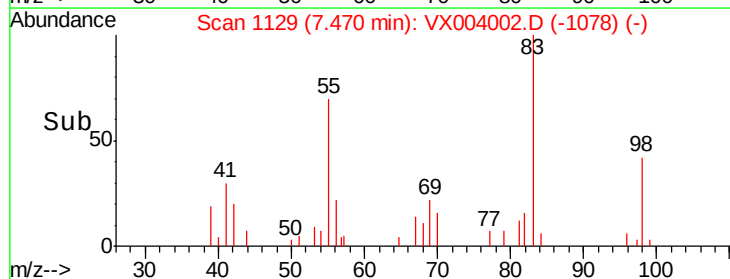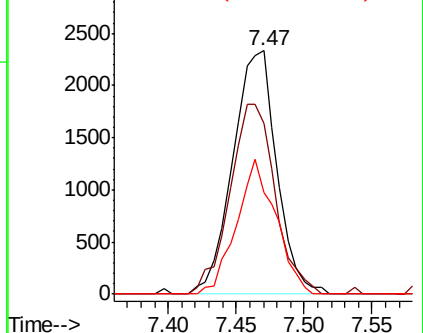

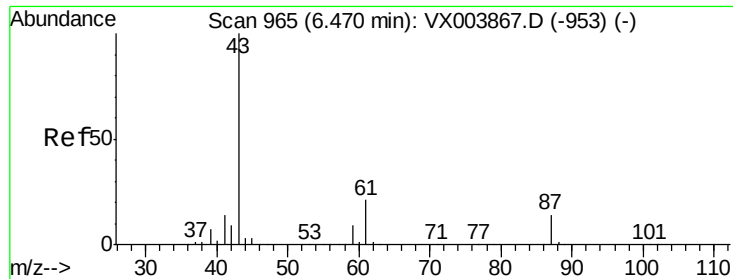

#43

Isopropyl Acetate

Concen: 15.86 ug/l

RT: 6.46 min Scan# 964

Delta R.T. -0.01 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08

Instrument :

MSVOA_X

ClientSampleId :

SP-1-7


Tot Ion: 43 Resp: 151206

Ion Ratio Lower Upper




43 100

61 20.4 16.9 25.3

87 14.2 11.3 16.9

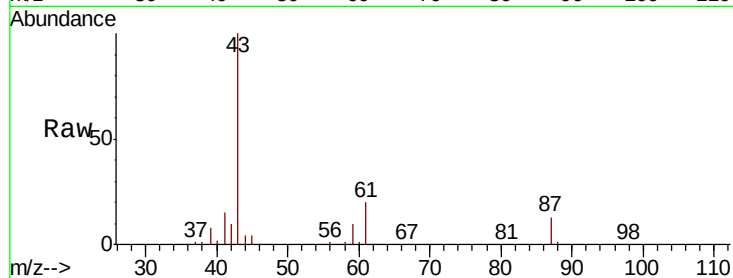

Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 61.00 (60.70 to 61.70): VX0
Ion 87.00 (86.70 to 87.70): VX0

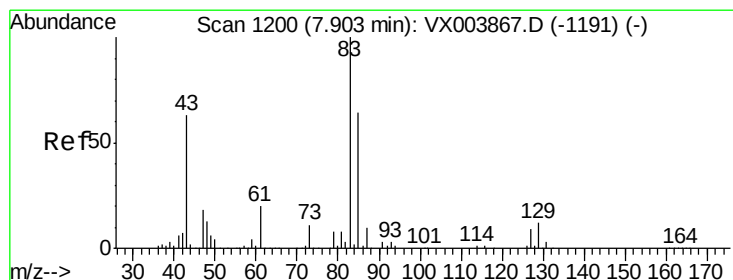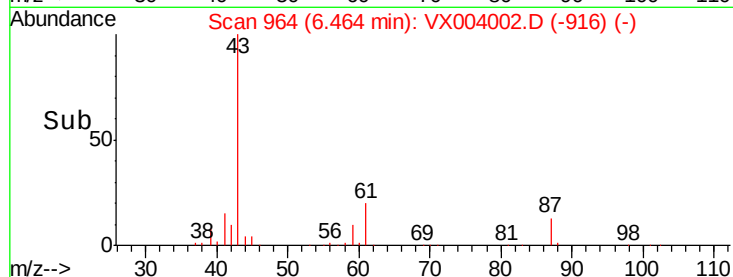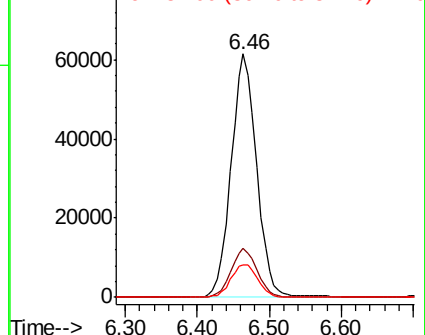

#47

Bromodichloromethane

Concen: 0.24 ug/l

RT: 7.90 min Scan# 1200

Delta R.T. 0.00 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08


Tgt Ion: 83 Resp: 1338

Ion Ratio Lower Upper



83 100


85 60.5 51.2 76.8

127 11.9 7.2 10.8#

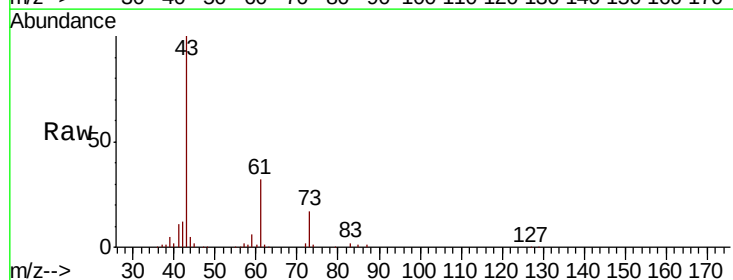

Abundance Ion 82.90 (82.60 to 83.60): VX0
Ion 84.90 (84.60 to 85.60): VX0
Ion 126.80 (126.50 to 127.50): V

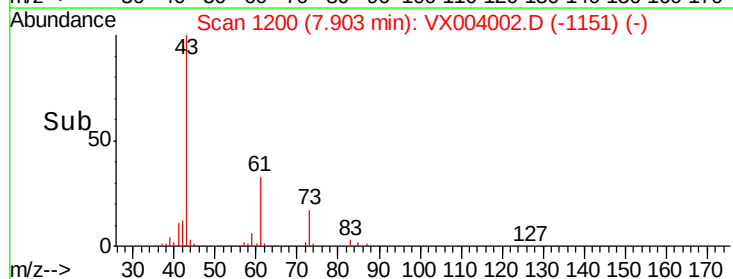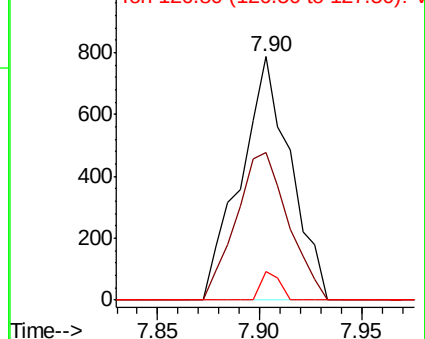

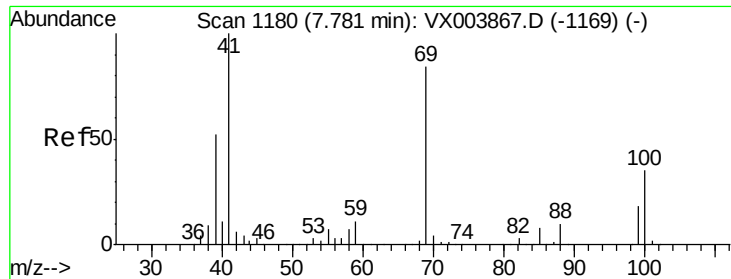

#48

Methvl methacrylate

Concen: 3.60 ug/l

RT: 7.88 min Scan# 1197

Delta R.T. 0.10 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08

Instrument :

MSVOA_X

ClientSampleId :

SP-1-7


Tot Ion: 41 Resp: 17434

Ion Ratio Lower Upper

41 100

69 0.0 68.8 103.2#




39 53.8 42.3 63.5

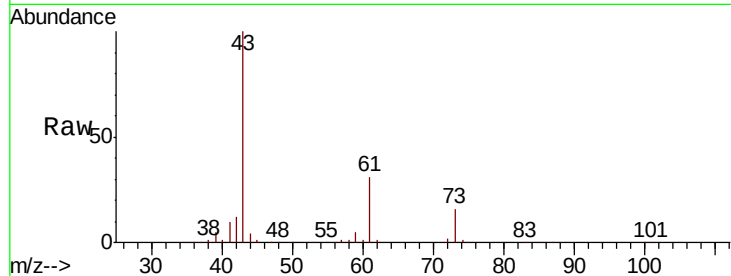

Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

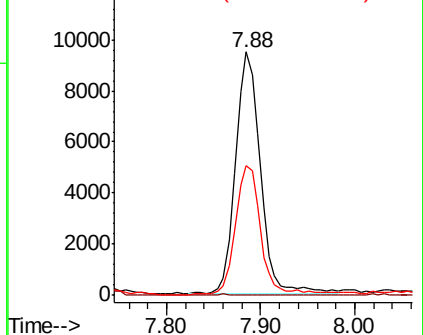

#50

Toluene-d8

Concen: 48.29 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX004002.D


Acq: 13 Aug 2018 16:08

Tgt Ion: 98 Resp: 731476

Ion Ratio Lower Upper



98 100


100 65.7 53.3 79.9



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

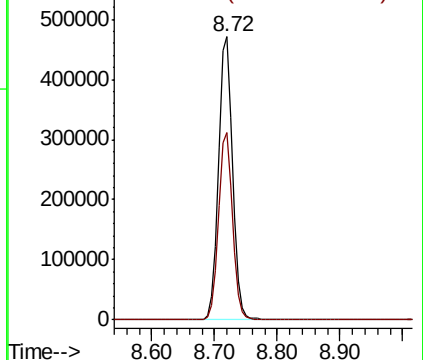



#51

4-Methyl-2-Pentanone

Concen: 0.32 ug/l

RT: 8.62 min Scan# 1318

Delta R.T. -0.03 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08

Instrument :

MSVOA_X

ClientSampleId :





SP-1-7

Tot Ion: 43 Resp: 2541

Ion Ratio Lower Upper

43 100

58 0.0 33.0 49.6#

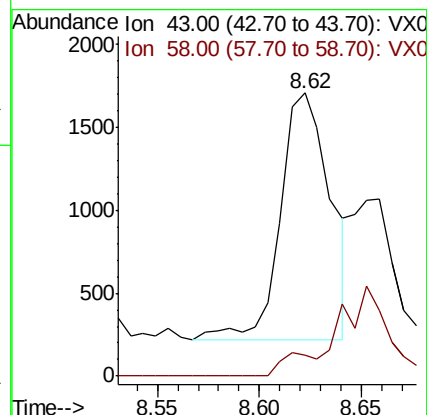

#59

2-Hexanone

Concen: 1.75 ug/l

RT: 9.55 min Scan# 1470

Delta R.T. 0.05 min

Lab File: VX004002.D




Acq: 13 Aug 2018 16:08


Tgt Ion: 43 Resp: 10336

Ion Ratio Lower Upper

43 100

58 24.7 29.0 87.0#



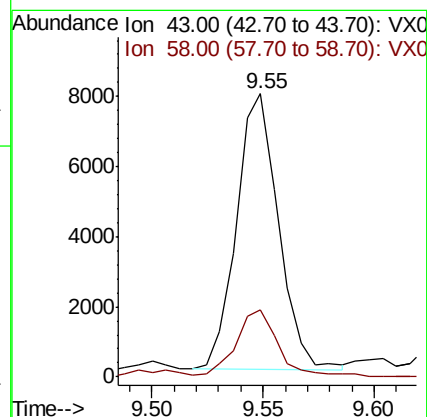



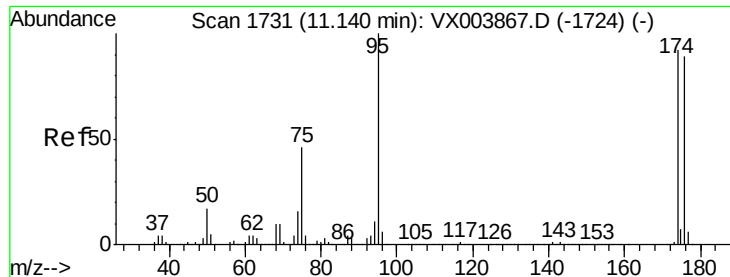

#62
4-Bromofluorobenzene
Concen: 51.22 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. 0.00 min
Lab File: VX004002.D
Acq: 13 Aug 2018 16:08




Instrument :
MSVOA_X
ClientSampled :
SP-1-7


Tot Ion: 95 Resp: 251057
Ion Ratio Lower Upper
95 100
174 90.3 0.0 182.8
176 87.9 0.0 179.0

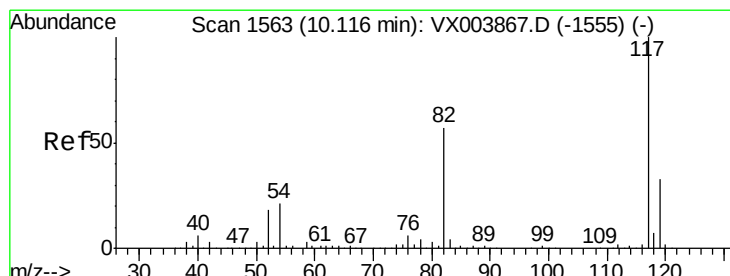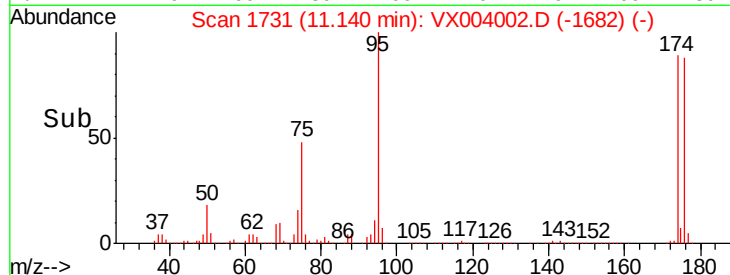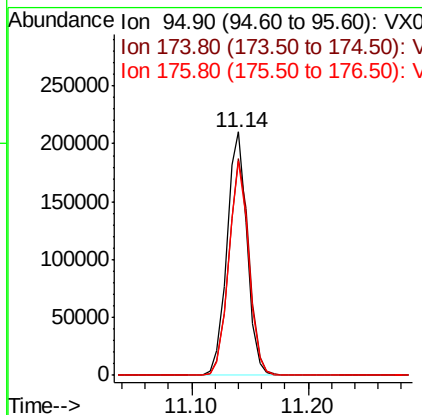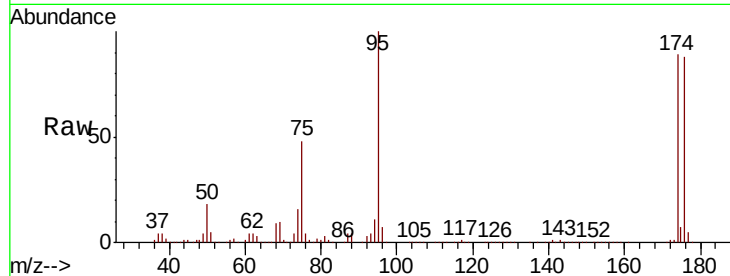

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. 0.00 min
Lab File: VX004002.D
Acq: 13 Aug 2018 16:08

Tgt Ion: 117 Resp: 478042
Ion Ratio Lower Upper
117 100
82 54.4 45.4 68.0
119 33.1 26.6 40.0


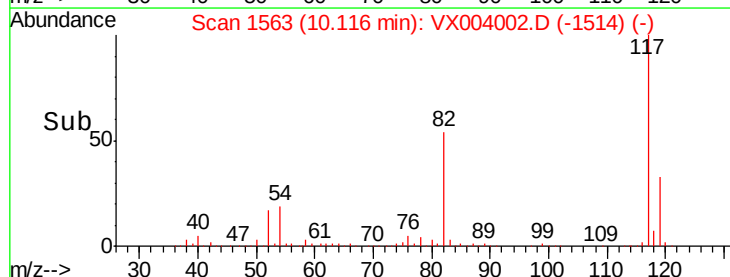
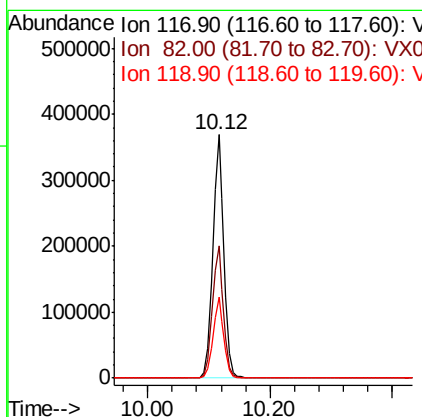
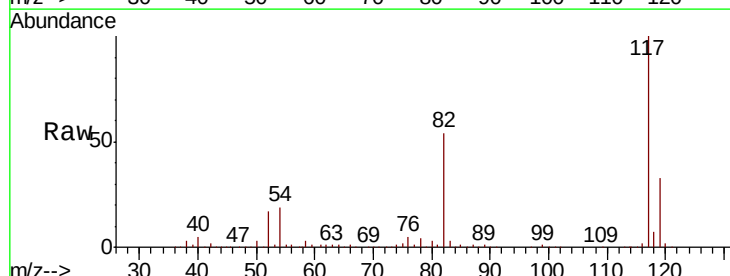


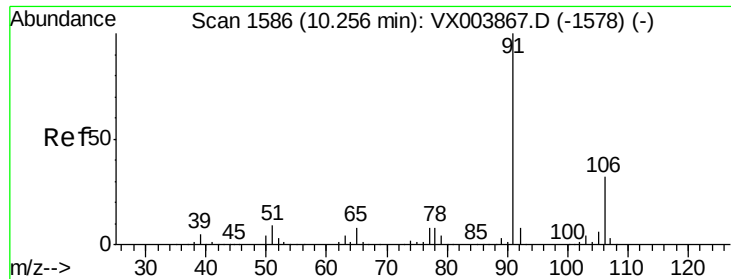

#67
Ethyl Benzene
Concen: 0.59 ug/l
RT: 10.26 min Scan# 1586
Delta R.T. 0.00 min
Lab File: VX004002.D
Acq: 13 Aug 2018 16:08




Instrument :
MSVOA_X
ClientSampled :
SP-1-7


Tot Ion: 91 Resp: 12079
Ion Ratio Lower Upper
91 100
106 31.6 25.9 38.9

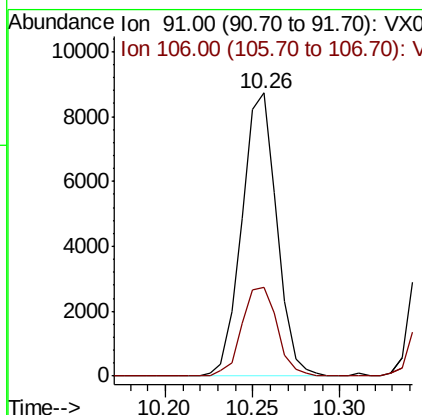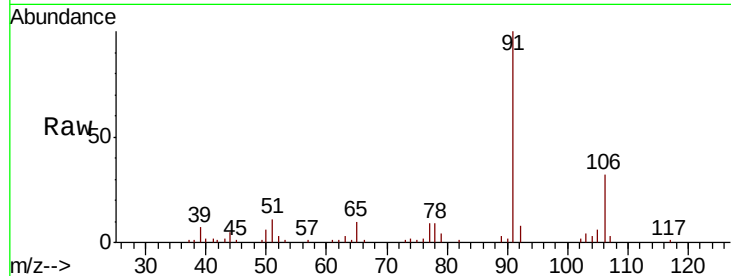

#68
m/p-Xylenes
Concen: 2.02 ug/l
RT: 10.36 min Scan# 1603
Delta R.T. 0.00 min
Lab File: VX004002.D
Acq: 13 Aug 2018 16:08

Tgt Ion: 106 Resp: 16100
Ion Ratio Lower Upper
106 100
91 198.5 162.3 243.5

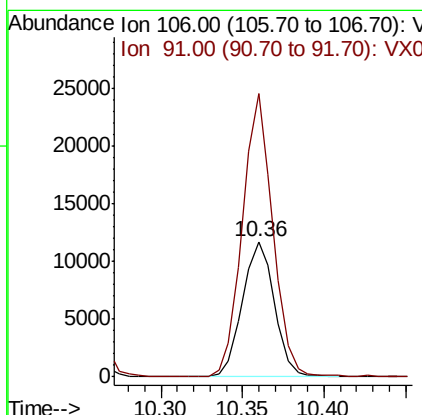


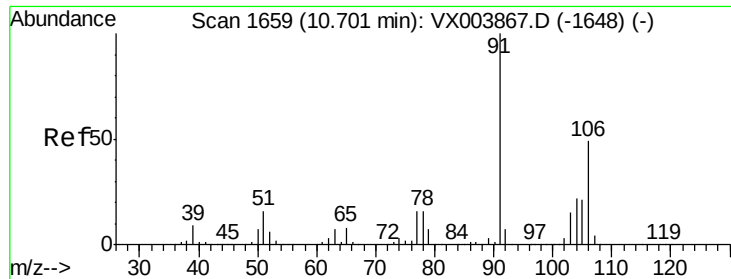




#69
o-Xylene
Concen: 0.28 ug/l
RT: 10.70 min Scan# 1659
Delta R.T. 0.00 min
Lab File: VX004002.D
Acq: 13 Aug 2018 16:08

Instrument :
MSVOA_X
ClientSampleId :
SP-1-7

Tot Ion:106 Resp: 2105
Ion Ratio Lower Upper
106 100
91 205.3 101.9 305.7

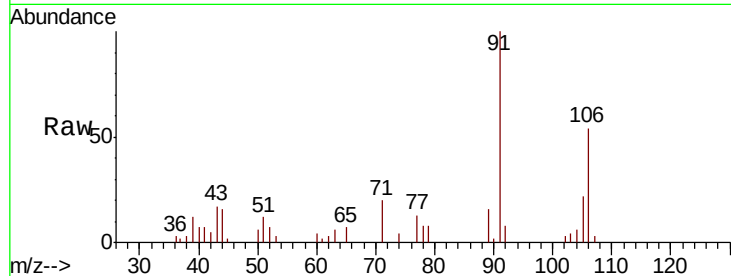


Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VX0


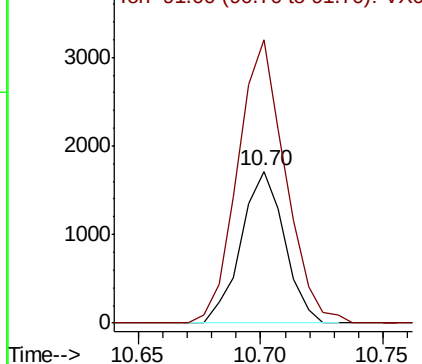



#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.08 min Scan# 1885
Delta R.T. 0.00 min
Lab File: VX004002.D
Acq: 13 Aug 2018 16:08

Tgt Ion:152 Resp: 257878
Ion Ratio Lower Upper
152 100
115 55.1 39.1 117.3
150 156.7 0.0 349.2



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

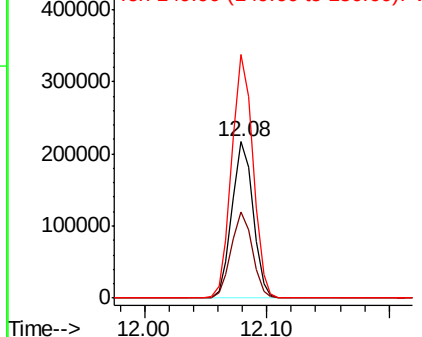

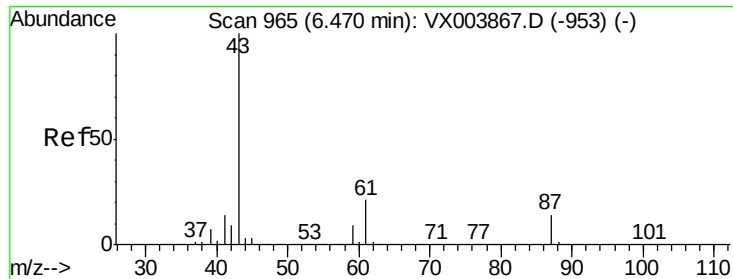

#74

N-amvl acetate

Concen: 15.24 ug/l

RT: 6.46 min Scan# 964

Delta R.T. -0.01 min

Lab File: VX004002.D

Acq: 13 Aug 2018 16:08

Instrument :

MSVOA_X

ClientSampleId :

SP-1-7

Tot Ion: 43 Resp: 151206


Ion Ratio Lower Upper

43 100

70 0.5 0.0 0.0#

55 0.7 0.1 0.1#

61 20.4 16.9 25.3



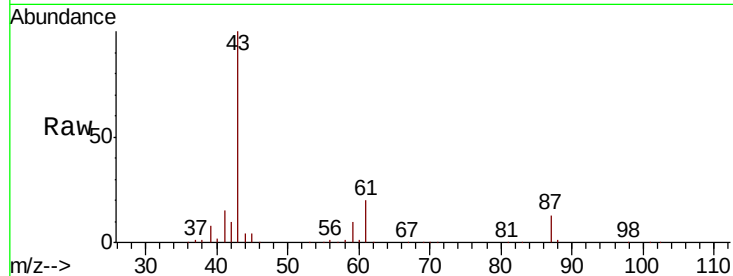


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

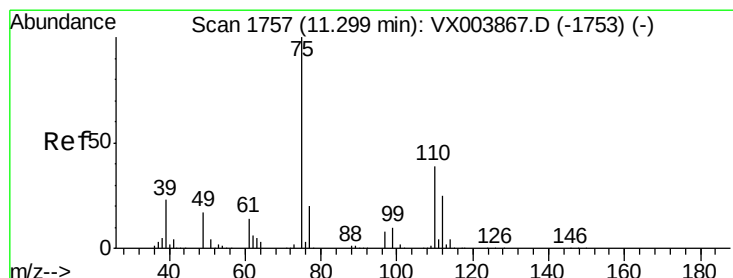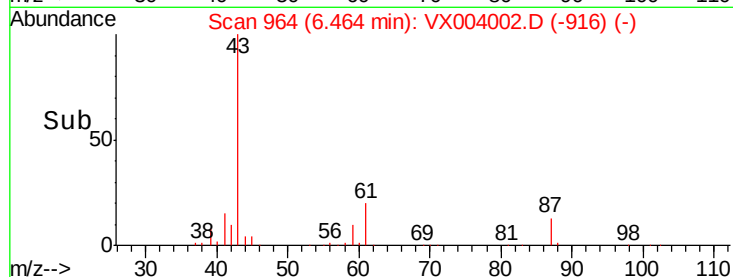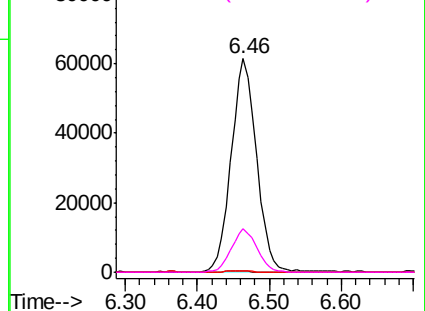

#76

1,2,3-Trichloropropane

Concen: 21.38 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.16 min

Lab File: VX004002.D


Acq: 13 Aug 2018 16:08

Tgt Ion: 75 Resp: 121793

Ion Ratio Lower Upper



75 100


77 1.3 20.8 62.5#

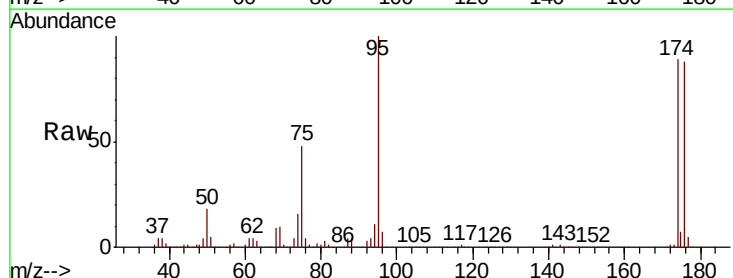

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0



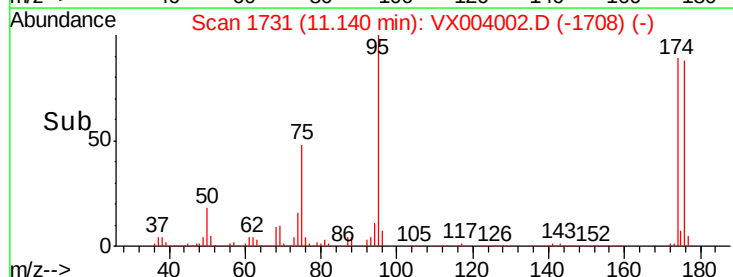
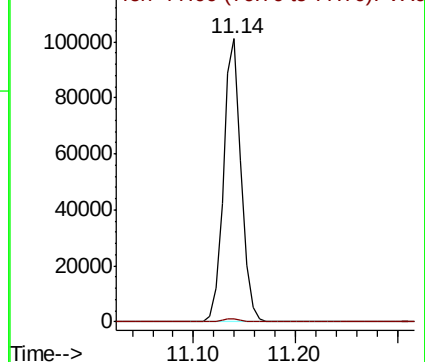


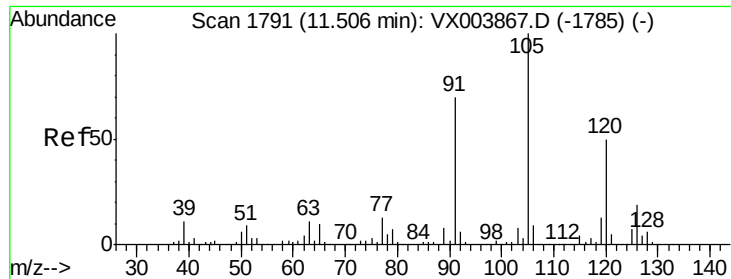

#80
 1,3,5-Trimethylbenzene
 Concen: 0.23 ug/l
 RT: 11.51 min Scan# 1791
 Delta R.T. 0.00 min
 Lab File: VX004002.D
 Acq: 13 Aug 2018 16:08




Instrument :
 MSVOA_X
 ClientSampleId :
 SP-1-7


Tot Ion:105 Resp: 3524
 Ion Ratio Lower Upper
 105 100
 120 57.0 25.4 76.2

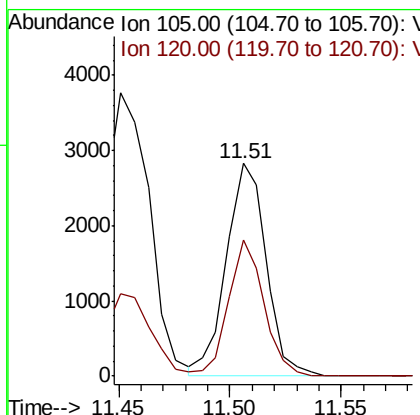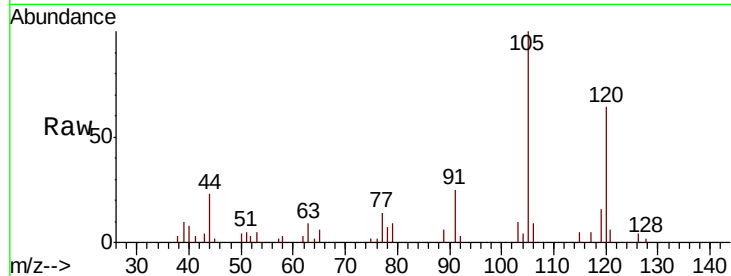

#81
 trans-1,4-Dichloro-2-butene
 Concen: 65.17 ug/l
 RT: 11.14 min Scan# 1731
 Delta R.T. 0.06 min
 Lab File: VX004002.D
 Acq: 13 Aug 2018 16:08

Tgt Ion: 75 Resp: 121793
 Ion Ratio Lower Upper
 75 100
 53 0.2 80.3 120.5#
 89 0.0 37.8 56.8#


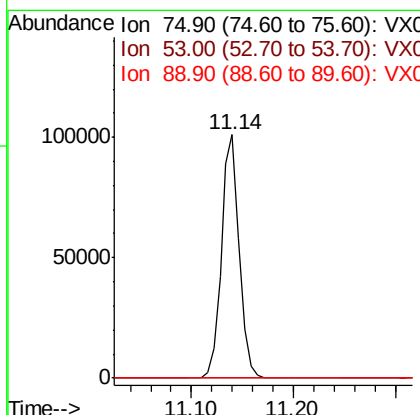




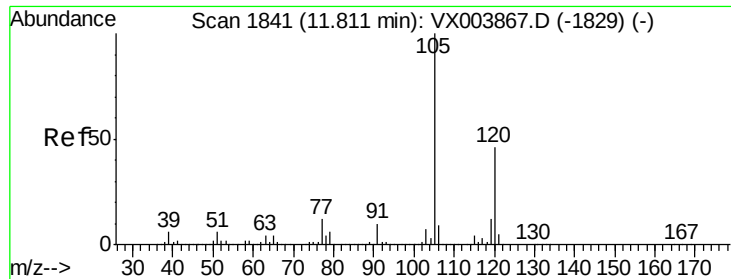

#84
 1,2,4-Trimethylbenzene
 Concen: 0.63 ug/l
 RT: 11.81 min Scan# 1841
 Delta R.T. 0.00 min
 Lab File: VX004002.D
 Acq: 13 Aug 2018 16:08

Instrument :
 MSVOA_X
 ClientSampled :
 SP-1-7

Tot Ion:105 Resp: 9822
 Ion Ratio Lower Upper
 105 100
 120 51.3 23.1 69.2

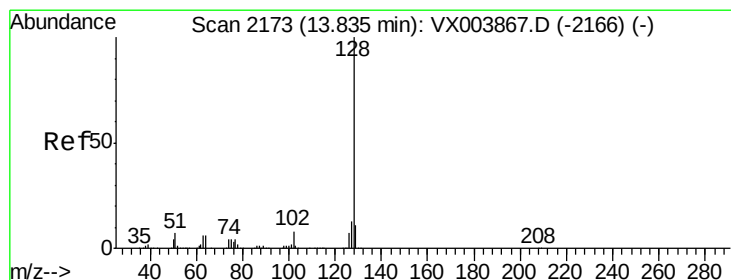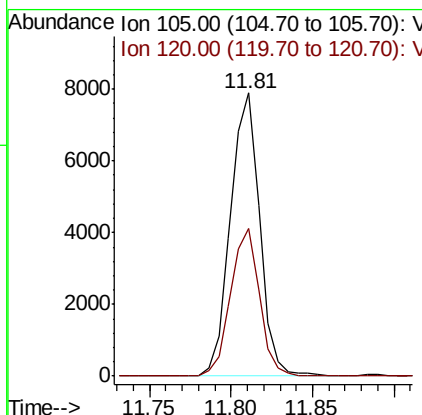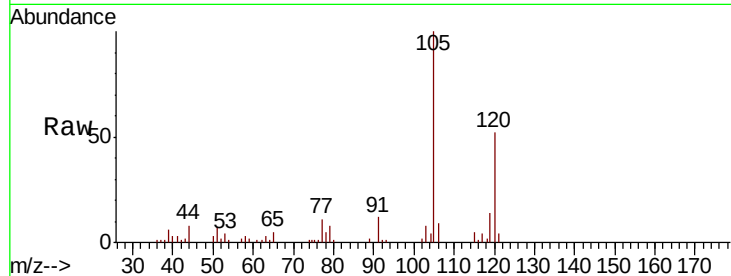

#95
 Naphthalene
 Concen: 0.89 ug/l
 RT: 13.83 min Scan# 2173
 Delta R.T. 0.00 min
 Lab File: VX004002.D
 Acq: 13 Aug 2018 16:08

Tgt Ion:128 Resp: 17075
 Ion Ratio Lower Upper
 128 100
 127 13.4 10.2 15.2
 129 11.7 8.8 13.2

