


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081318\
Data File : VX003990.D
Acq On : 13 Aug 2018 08:54
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Title : SW846 8260
Last Update : Mon Aug 13 01:34:27 2018

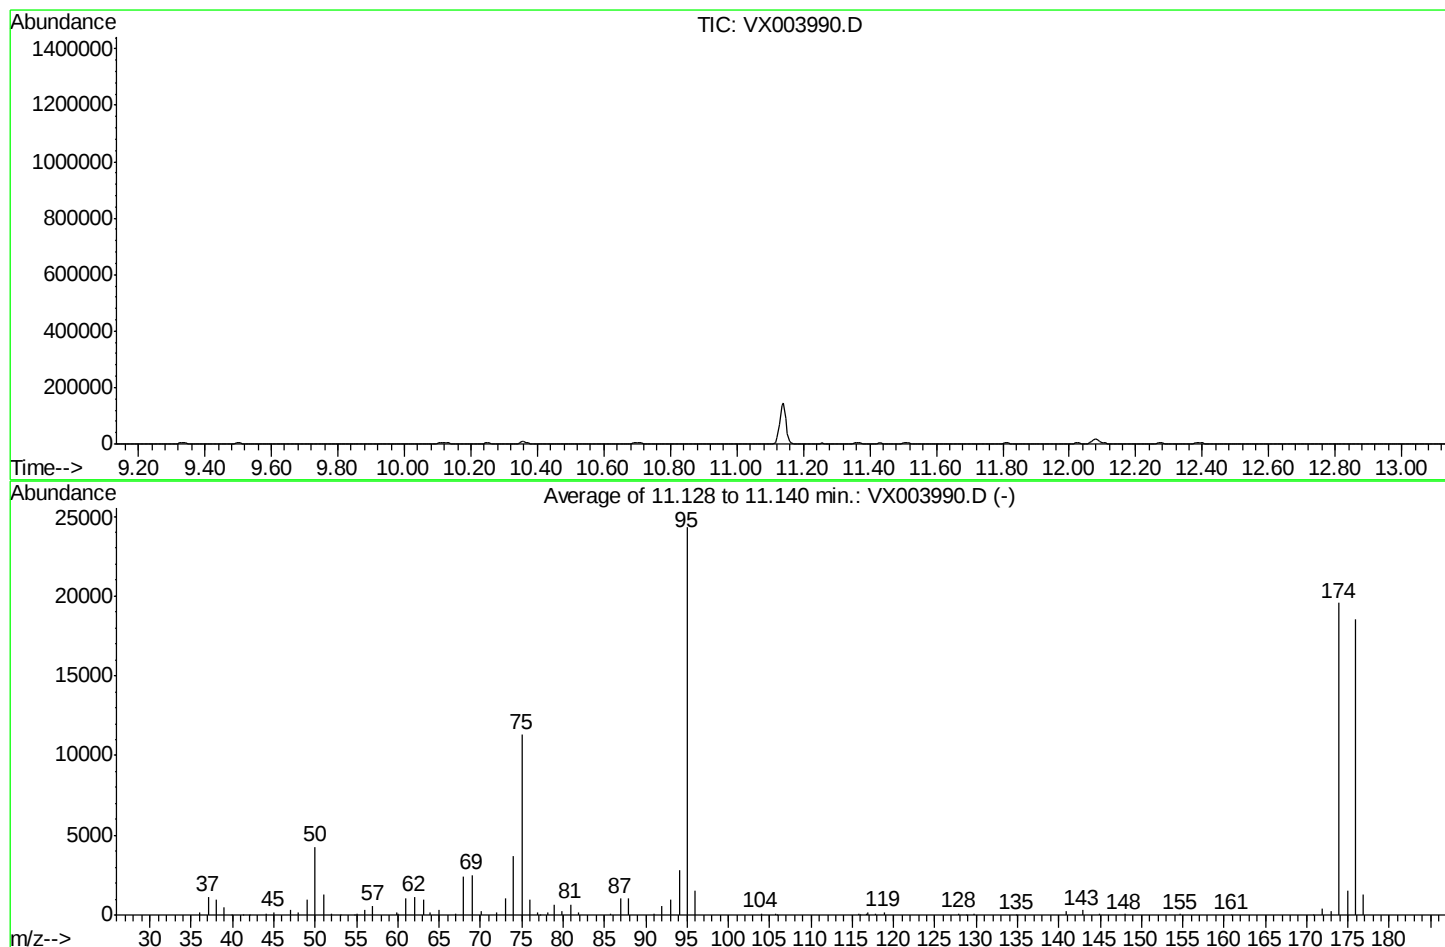

AutoFind: Scans 1729, 1730, 1731; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	4288	PASS
75	95	30	60	46.4	11291	PASS
95	95	100	100	100.0	24308	PASS
96	95	5	9	6.4	1556	PASS
173	174	0.00	2	1.2	231	PASS
174	95	50	100	80.4	19550	PASS
175	174	5	9	7.8	1525	PASS
176	174	95	101	95.0	18574	PASS
177	176	5	9	6.7	1249	PASS