

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081319\
 Data File : VX011525.D
 Acq On : 13 Aug 2019 10:48
 Operator : JC/SP
 Sample : VX0813WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0813WBL01

Quant Time: Aug 14 01:21:30 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 02 01:55:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	192858	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	289662	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	253922	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	112207	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	107083	55.14	ug/l	0.00
Spiked Amount	50.000		Recovery	=	110.28%	
35) Dibromofluoromethane	5.49	113	89761	47.46	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.92%	
50) Toluene-d8	8.71	98	338819	47.46	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.92%	
62) 4-Bromofluorobenzene	11.13	95	109096	42.81	ug/l	0.00
Spiked Amount	50.000		Recovery	=	85.62%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081319\
Data File : VX011525.D
Acq On : 13 Aug 2019 10:48
Operator : JC/SP
Sample : VX0813WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0813WBL01

Quant Time: Aug 14 01:21:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 02 01:55:00 2019
Response via : Initial Calibration

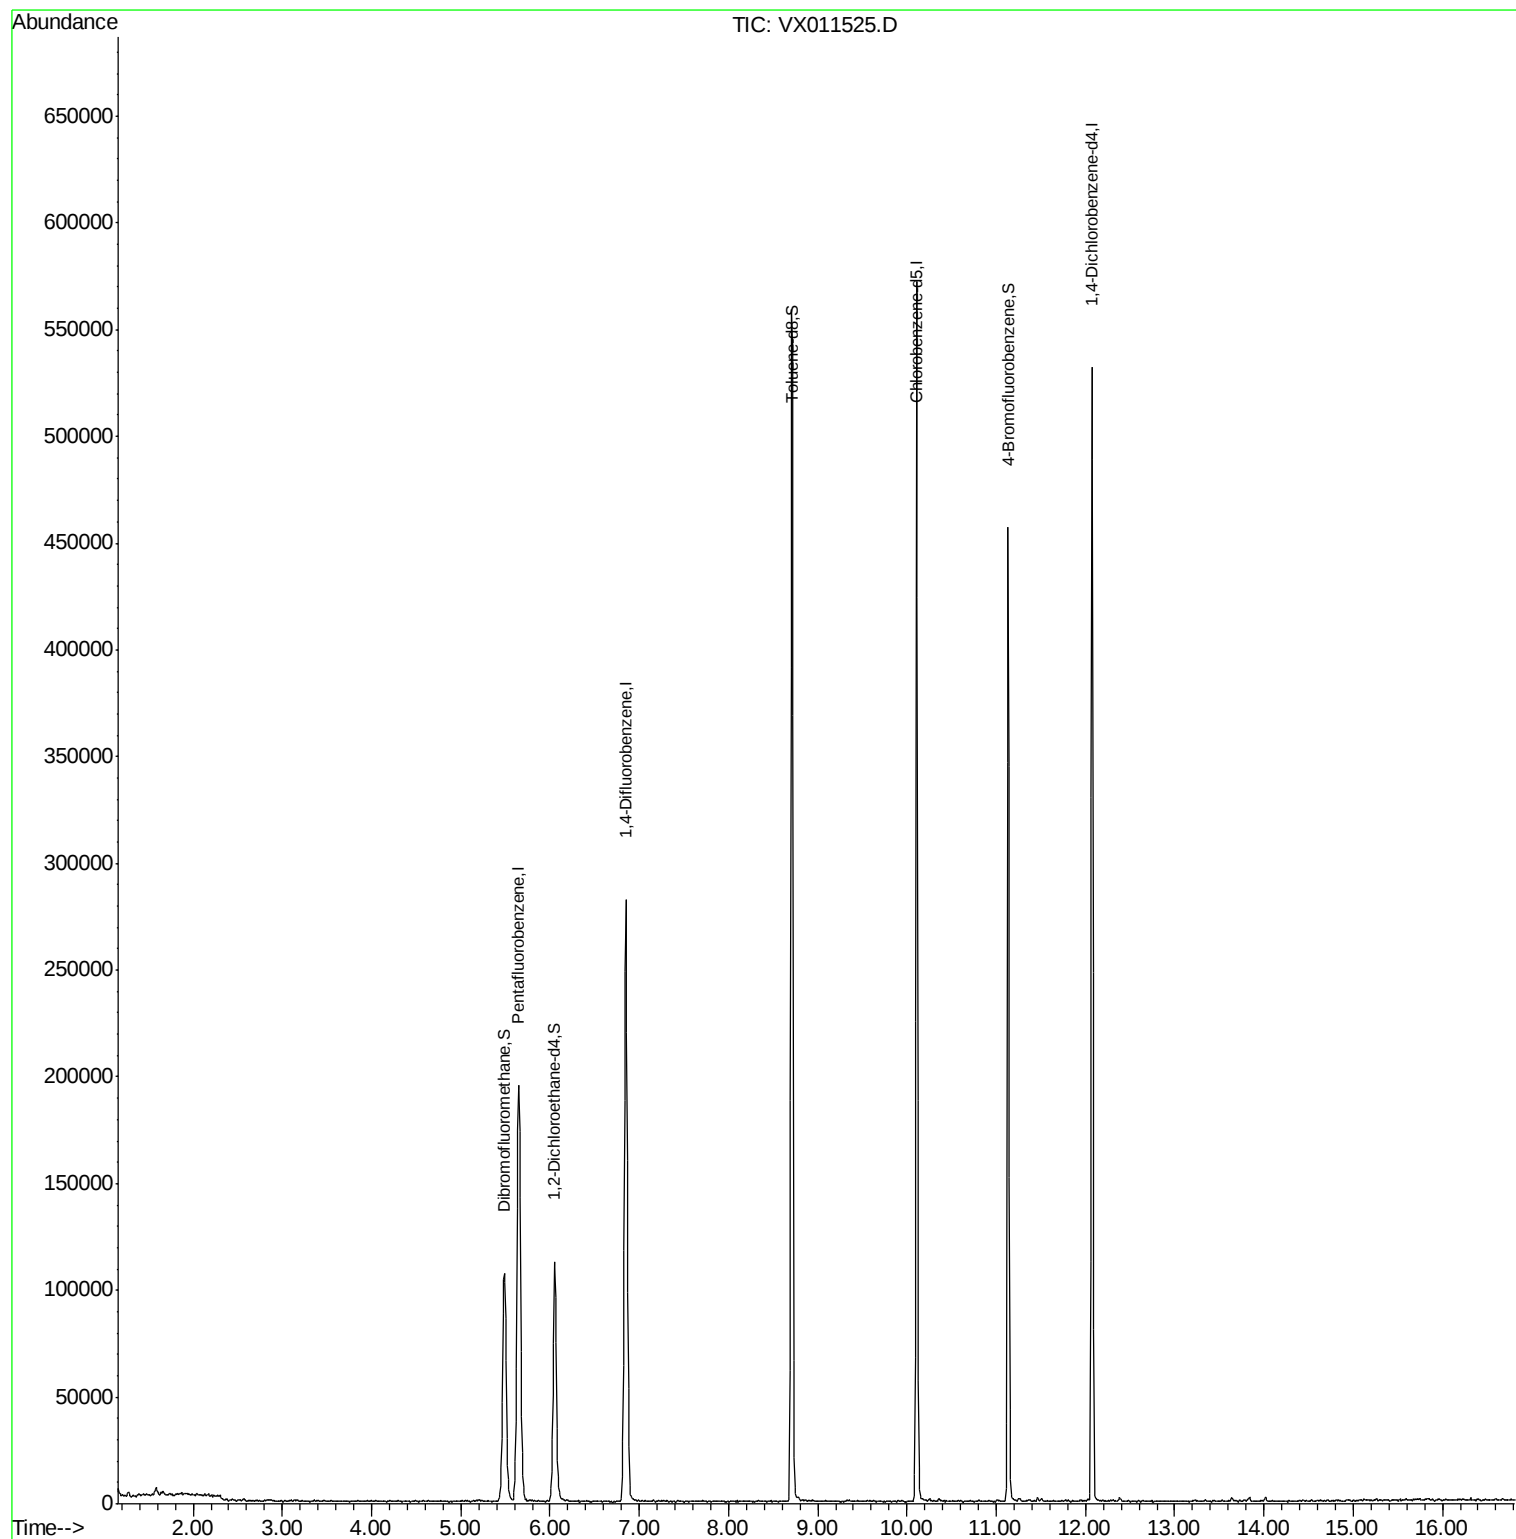

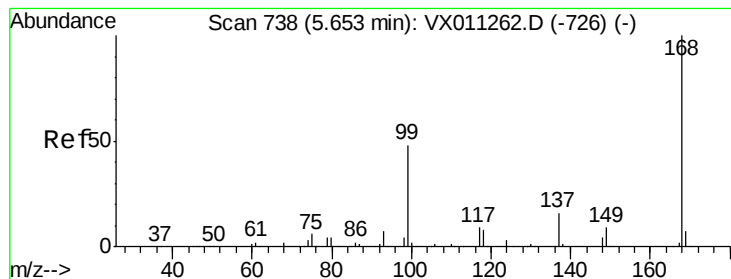

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 738

Delta R.T. 0.00 min

Lab File: VX011525.D

Acq: 13 Aug 2019 10:48

Instrument :

MSVOA_X

ClientSampleId :


VX0813WBL01

Tot Ion:168 Resp: 192858

Ion Ratio Lower Upper

168 100

99 50.3 38.5 57.7

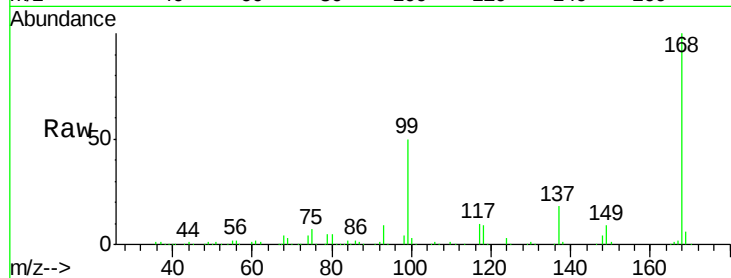

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

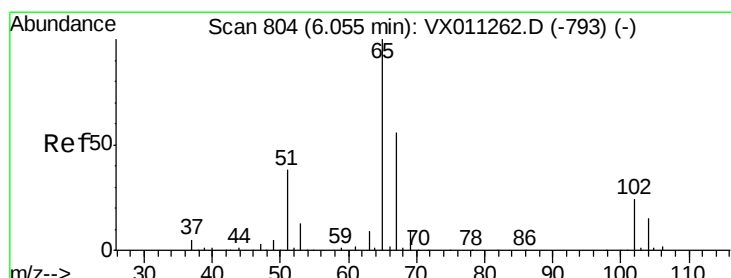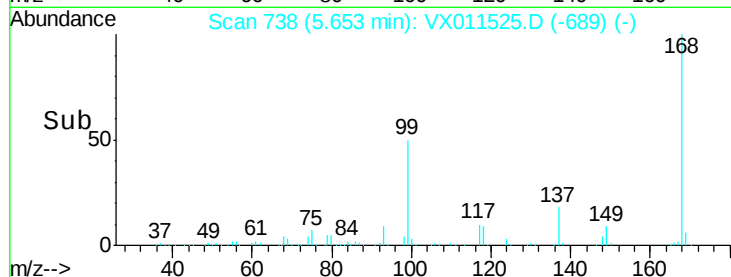

#33

1,2-Dichloroethane-d4

Concen: 55.135 ug/l

RT: 6.06 min Scan# 804

Delta R.T. 0.00 min

Lab File: VX011525.D


Acq: 13 Aug 2019 10:48

Tgt Ion: 65 Resp: 107083

Ion Ratio Lower Upper

65 100

67 51.6 0.0 110.6

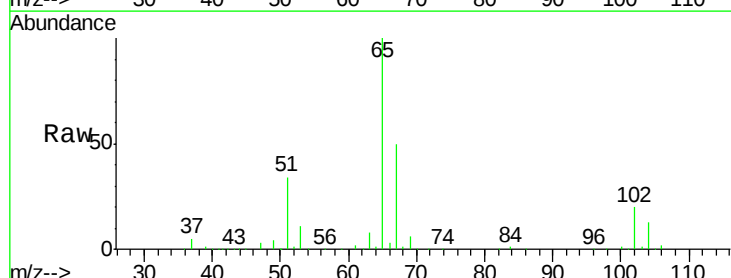

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.06

40000


30000


20000

10000

0

Time--> 5.90 6.00 6.10 6.20




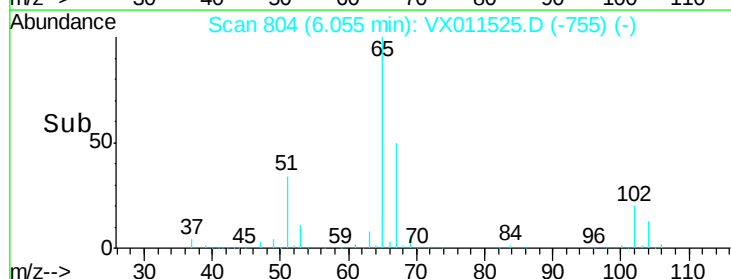


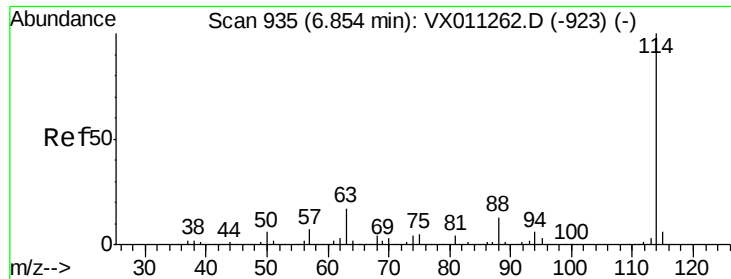

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.85 min Scan# 934
Delta R.T. -0.01 min
Lab File: VX011525.D
Acq: 13 Aug 2019 10:48




Instrument :
MSVOA_X
ClientSampleId :
VX0813WBL01


Tot Ion	Ratio	Lower	Upper
114	100		
63	19.3	0.0	34.0
88	14.7	0.0	26.4

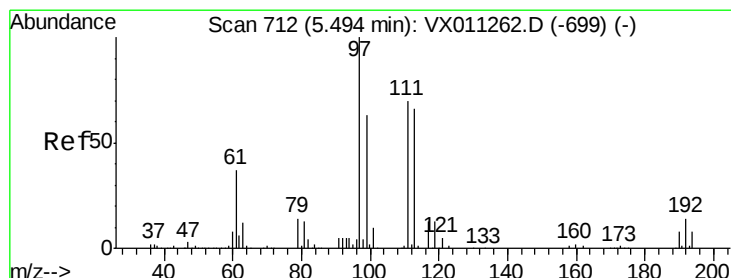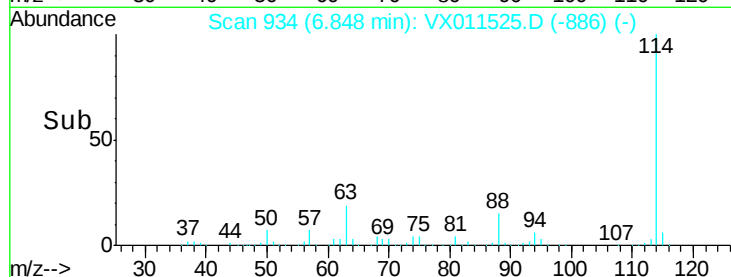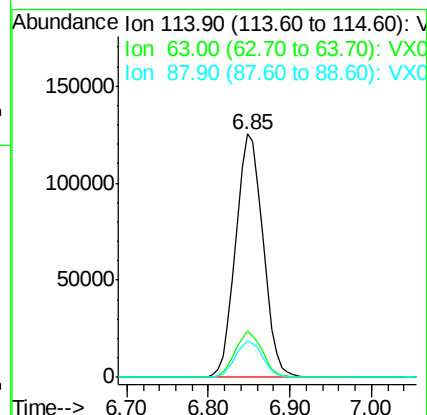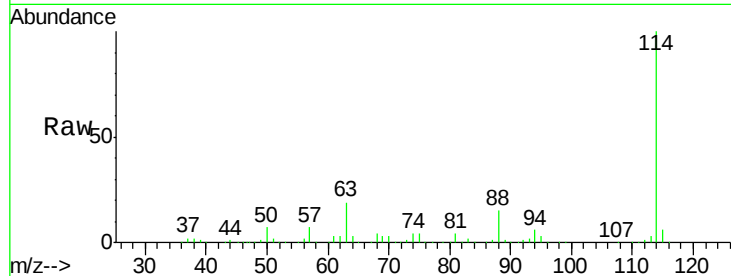

#35
Dibromofluoromethane
Concen: 47.464 ug/l
RT: 5.49 min Scan# 711
Delta R.T. -0.01 min
Lab File: VX011525.D
Acq: 13 Aug 2019 10:48

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.5	81.9	122.9
192	21.8	17.8	26.8

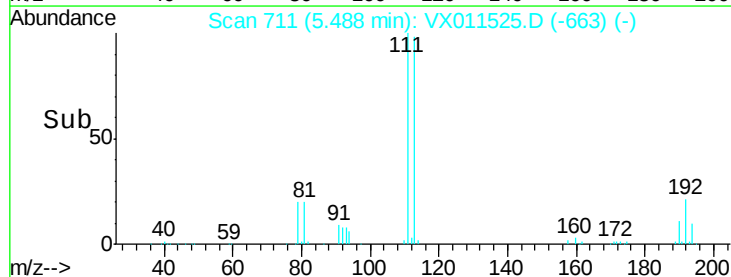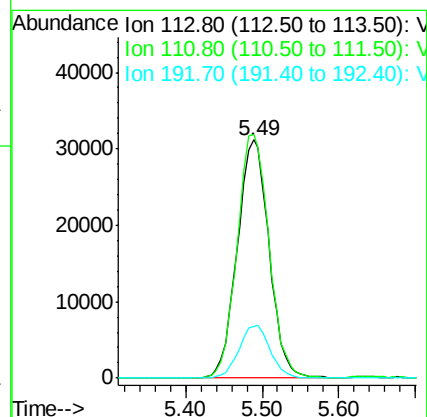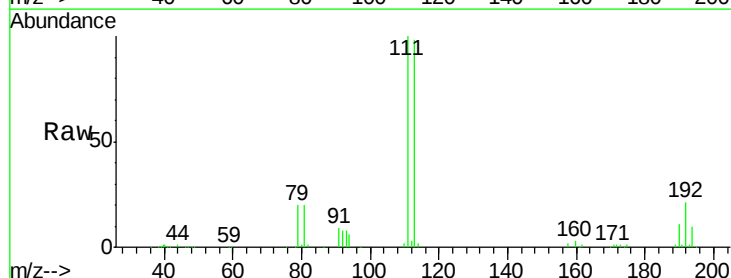

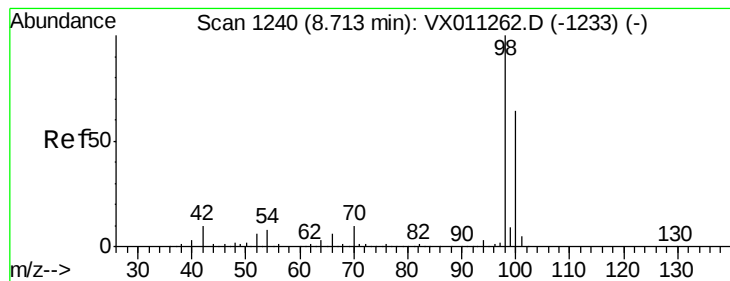

#50

Toluene-d8

Concen: 47.464 ug/l

RT: 8.71 min Scan# 1239

Delta R.T. -0.01 min

Lab File: VX011525.D

Acq: 13 Aug 2019 10:48

Instrument :

MSVOA_X

ClientSampleId :


VX0813WBL01

Tot Ion: 98 Resp: 338819

Ion Ratio Lower Upper

98 100

100 63.9 51.7 77.5

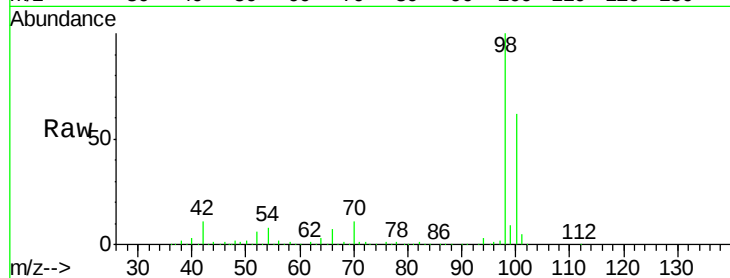

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

8.71

250000

200000



150000

100000

50000

0

Time--> 8.60 8.70 8.80

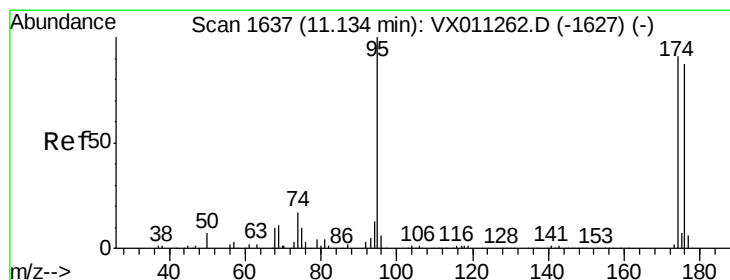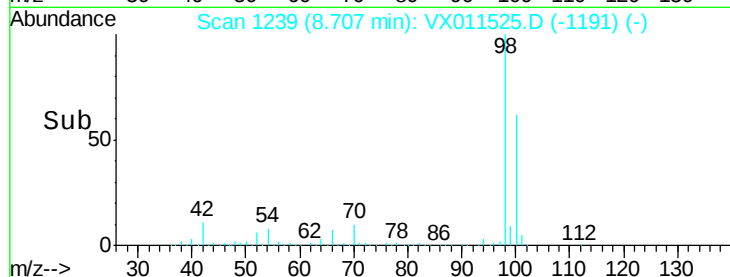

#62

4-Bromofluorobenzene

Concen: 42.806 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX011525.D

Acq: 13 Aug 2019 10:48


Tgt Ion: 95 Resp: 109096

Ion Ratio Lower Upper

95 100

174 90.1 0.0 191.2

176 87.7 0.0 184.8

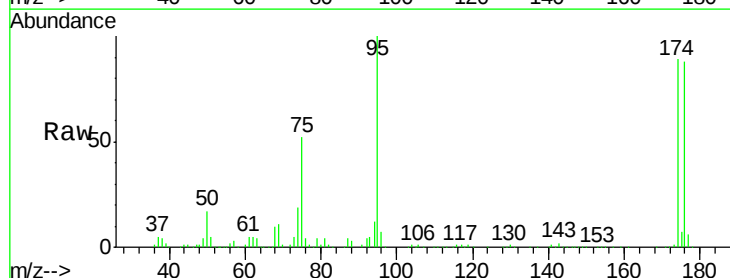

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

120000

100000

80000


60000


40000

20000

0

Time--> 11.05 11.10 11.15 11.20




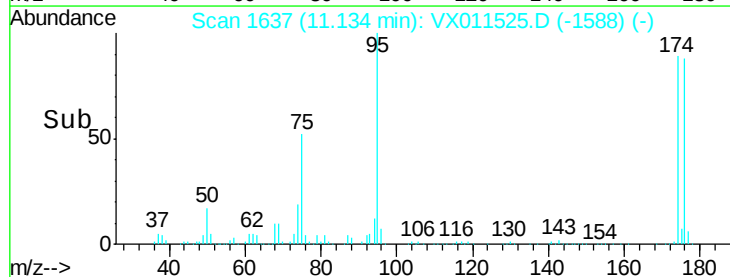


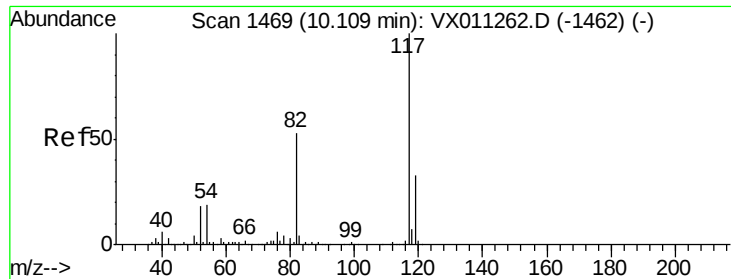

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX011525.D
Acq: 13 Aug 2019 10:48

Instrument :
MSVOA_X
ClientSampled :
VX0813WBL01

Tot Ion:117 Resp: 253922
Ion Ratio Lower Upper
117 100
82 53.6 42.2 63.2
119 31.9 26.6 39.8

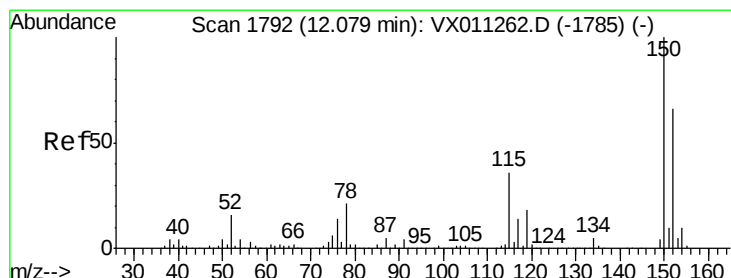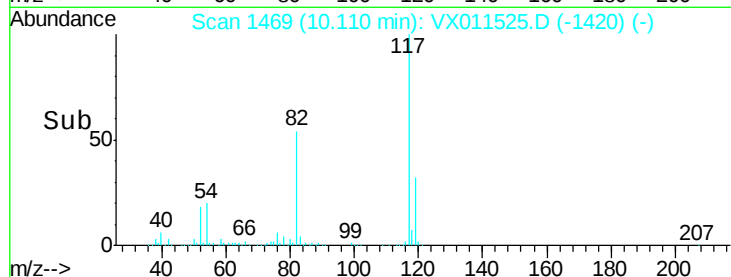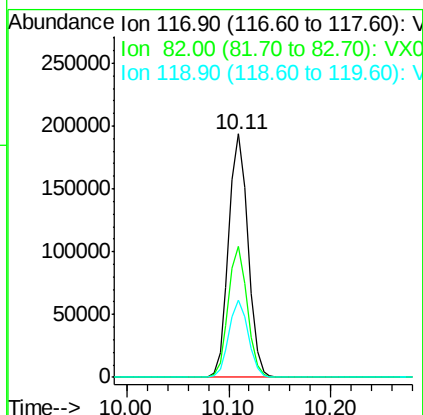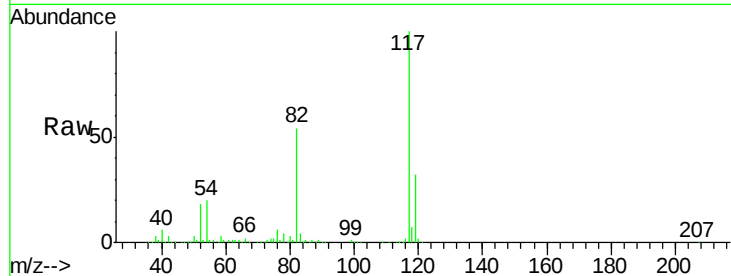

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1791
Delta R.T. -0.01 min
Lab File: VX011525.D
Acq: 13 Aug 2019 10:48

Tgt Ion:152 Resp: 112207
Ion Ratio Lower Upper
152 100
115 56.6 40.0 119.9
150 158.3 0.0 350.4

