

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081319\
 Data File : VX011531.D
 Acq On : 13 Aug 2019 13:20
 Operator : JC/SP
 Sample : K4279-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z3-0671

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.788	98	104	115	rVB	122924	171025	1.69%	0.206%
2	1.995	133	138	147	rVB	159754	221388	2.19%	0.266%
3	2.392	191	203	208	rBV	70256	142624	1.41%	0.172%
4	2.837	258	276	279	rBV2	138499	315232	3.12%	0.379%
5	2.885	279	284	288	rVV	595030	1261997	12.49%	1.518%
6	2.928	288	291	304	rVB	370624	692627	6.85%	0.833%
7	3.166	320	330	344	rBV	570886	1295405	12.82%	1.559%
8	3.519	378	388	403	rBV	388422	883508	8.74%	1.063%
9	4.397	522	532	546	rVB	1082842	3138996	31.06%	3.777%
10	5.232	655	669	690	rVB3	35630	157905	1.56%	0.190%
11	5.495	701	712	716	rBV2	107157	296132	2.93%	0.356%
12	5.580	716	726	735	rBV2	1070920	3399234	33.63%	4.090%
13	5.726	745	750	768	rVB	112199	325704	3.22%	0.392%
14	5.927	770	783	796	rBV4	285204	904562	8.95%	1.088%
15	6.056	796	804	809	rVV	110275	282146	2.79%	0.339%
16	6.141	809	818	829	rVV	1458781	3781672	37.42%	4.550%
17	6.257	829	837	847	rVV4	141449	489868	4.85%	0.589%
18	6.354	847	853	861	rVV2	137110	371358	3.67%	0.447%
19	6.452	861	869	883	rVB	231036	633753	6.27%	0.763%
20	6.854	925	935	943	rBV	286581	670597	6.63%	0.807%
21	7.464	1022	1035	1046	rVB	1521422	3478793	34.42%	4.186%
22	7.732	1072	1079	1089	rVB	147088	283047	2.80%	0.341%
23	7.848	1089	1098	1105	rVB2	49449	102996	1.02%	0.124%
24	8.025	1120	1127	1140	rVB3	50896	115471	1.14%	0.139%
25	8.500	1200	1205	1214	rBV	63198	122633	1.21%	0.148%
26	8.665	1224	1232	1235	rBV2	198989	364671	3.61%	0.439%
27	8.714	1235	1240	1247	rVB	602769	1008508	9.98%	1.213%
28	8.835	1255	1260	1264	rBV	85530	139856	1.38%	0.168%
29	8.909	1268	1272	1279	rVB3	60610	103979	1.03%	0.125%
30	9.037	1288	1293	1300	rVB	175395	278201	2.75%	0.335%
31	9.165	1305	1314	1319	rBV	83207	139845	1.38%	0.168%
32	9.573	1374	1381	1384	rBV3	73849	125463	1.24%	0.151%
33	9.622	1384	1389	1393	rVB	219915	308351	3.05%	0.371%
34	9.677	1393	1398	1402	rBV	101120	146787	1.45%	0.177%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081319\
 Data File : VX011531.D
 Acq On : 13 Aug 2019 13:20
 Operator : JC/SP
 Sample : K4279-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z3-0671

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Title : SW846 8260

35	10.110	1464	1469	1475	rBV	585156	759572	7.52%	0.914%
36	10.183	1475	1481	1486	rVB	84915	128645	1.27%	0.155%
37	10.250	1486	1492	1498	rBV	7793720	10107253	100.00%	12.161%
38	10.360	1501	1510	1516	rVB	2817144	3697615	36.58%	4.449%
39	10.640	1548	1556	1562	rBV4	45957	113151	1.12%	0.136%
40	10.835	1577	1588	1595	rBV2	95365	162329	1.61%	0.195%
41	10.908	1595	1600	1606	rBV3	64803	108695	1.08%	0.131%
42	11.012	1612	1617	1623	rBV	820303	1077223	10.66%	1.296%
43	11.134	1631	1637	1642	rBV	541838	677616	6.70%	0.815%
44	11.359	1668	1674	1680	rBV	948408	1214165	12.01%	1.461%
45	11.451	1681	1689	1693	rVV	1368845	1801407	17.82%	2.167%
46	11.506	1693	1698	1706	rVB	1023541	1288999	12.75%	1.551%
47	11.664	1715	1724	1733	rBV	3715283	4666161	46.17%	5.614%
48	11.804	1742	1747	1752	rVB	7944794	9520522	94.19%	11.455%
49	11.945	1767	1770	1776	rVV	186654	228527	2.26%	0.275%
50	12.024	1776	1783	1786	rVV	144780	178324	1.76%	0.215%
51	12.073	1786	1791	1796	rVB2	754086	1105815	10.94%	1.331%
52	12.140	1797	1802	1807	rBV	3208722	3761395	37.21%	4.526%
53	12.231	1812	1817	1821	rBV	89633	109997	1.09%	0.132%
54	12.298	1822	1828	1835	rBV	1161390	1628263	16.11%	1.959%
55	12.365	1835	1839	1849	rVB3	622413	965902	9.56%	1.162%
56	12.457	1849	1854	1859	rBV2	244108	317068	3.14%	0.382%
57	12.518	1859	1864	1869	rBV	625686	773910	7.66%	0.931%
58	12.585	1869	1875	1877	rBV	602648	824381	8.16%	0.992%
59	12.609	1877	1879	1883	rVB	692207	674024	6.67%	0.811%
60	12.664	1883	1888	1891	rBV	737196	845828	8.37%	1.018%
61	12.701	1891	1894	1898	rVB	155110	185600	1.84%	0.223%
62	12.756	1898	1903	1910	rBV3	470218	851615	8.43%	1.025%
63	12.902	1921	1927	1931	rVB2	471093	605000	5.99%	0.728%
64	12.975	1931	1939	1942	rBV	416163	560251	5.54%	0.674%
65	13.018	1942	1946	1952	rVB	761209	926008	9.16%	1.114%
66	13.079	1952	1956	1961	rBV2	98322	174364	1.73%	0.210%
67	13.194	1971	1975	1977	rBV3	111752	147832	1.46%	0.178%
68	13.219	1977	1979	1983	rVB	138853	156819	1.55%	0.189%
69	13.304	1989	1993	1995	rBV2	120366	153099	1.51%	0.184%
70	13.341	1995	1999	2004	rVB2	1257838	1670470	16.53%	2.010%
71	13.475	2017	2021	2030	rVB	704221	862906	8.54%	1.038%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081319\
Data File : VX011531.D
Acq On : 13 Aug 2019 13:20
Operator : JC/SP
Sample : K4279-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0671

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Title : SW846 8260

72	13.560	2030	2035	2038	rBV3	66486	102955	1.02%	0.124%
73	13.633	2044	2047	2053	rVV3	143251	260295	2.58%	0.313%
74	13.719	2058	2061	2067	rVB2	155493	249537	2.47%	0.300%
75	13.829	2072	2079	2087	rVB	1028940	1434928	14.20%	1.727%
76	13.908	2087	2092	2096	rVB	107825	147629	1.46%	0.178%
77	13.981	2096	2104	2108	rBV2	153515	231206	2.29%	0.278%
78	14.286	2146	2154	2159	rVB2	196236	359712	3.56%	0.433%
79	14.536	2190	2195	2200	rBV2	211962	280896	2.78%	0.338%
80	14.694	2213	2221	2224	rBV	327514	439105	4.34%	0.528%
81	14.834	2239	2244	2249	rBV	322961	419364	4.15%	0.505%


Sum of corrected areas: 83110712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081319\
Data File : VX011531.D
Acq On : 13 Aug 2019 13:20
Operator : JC/SP
Sample : K4279-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0671

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

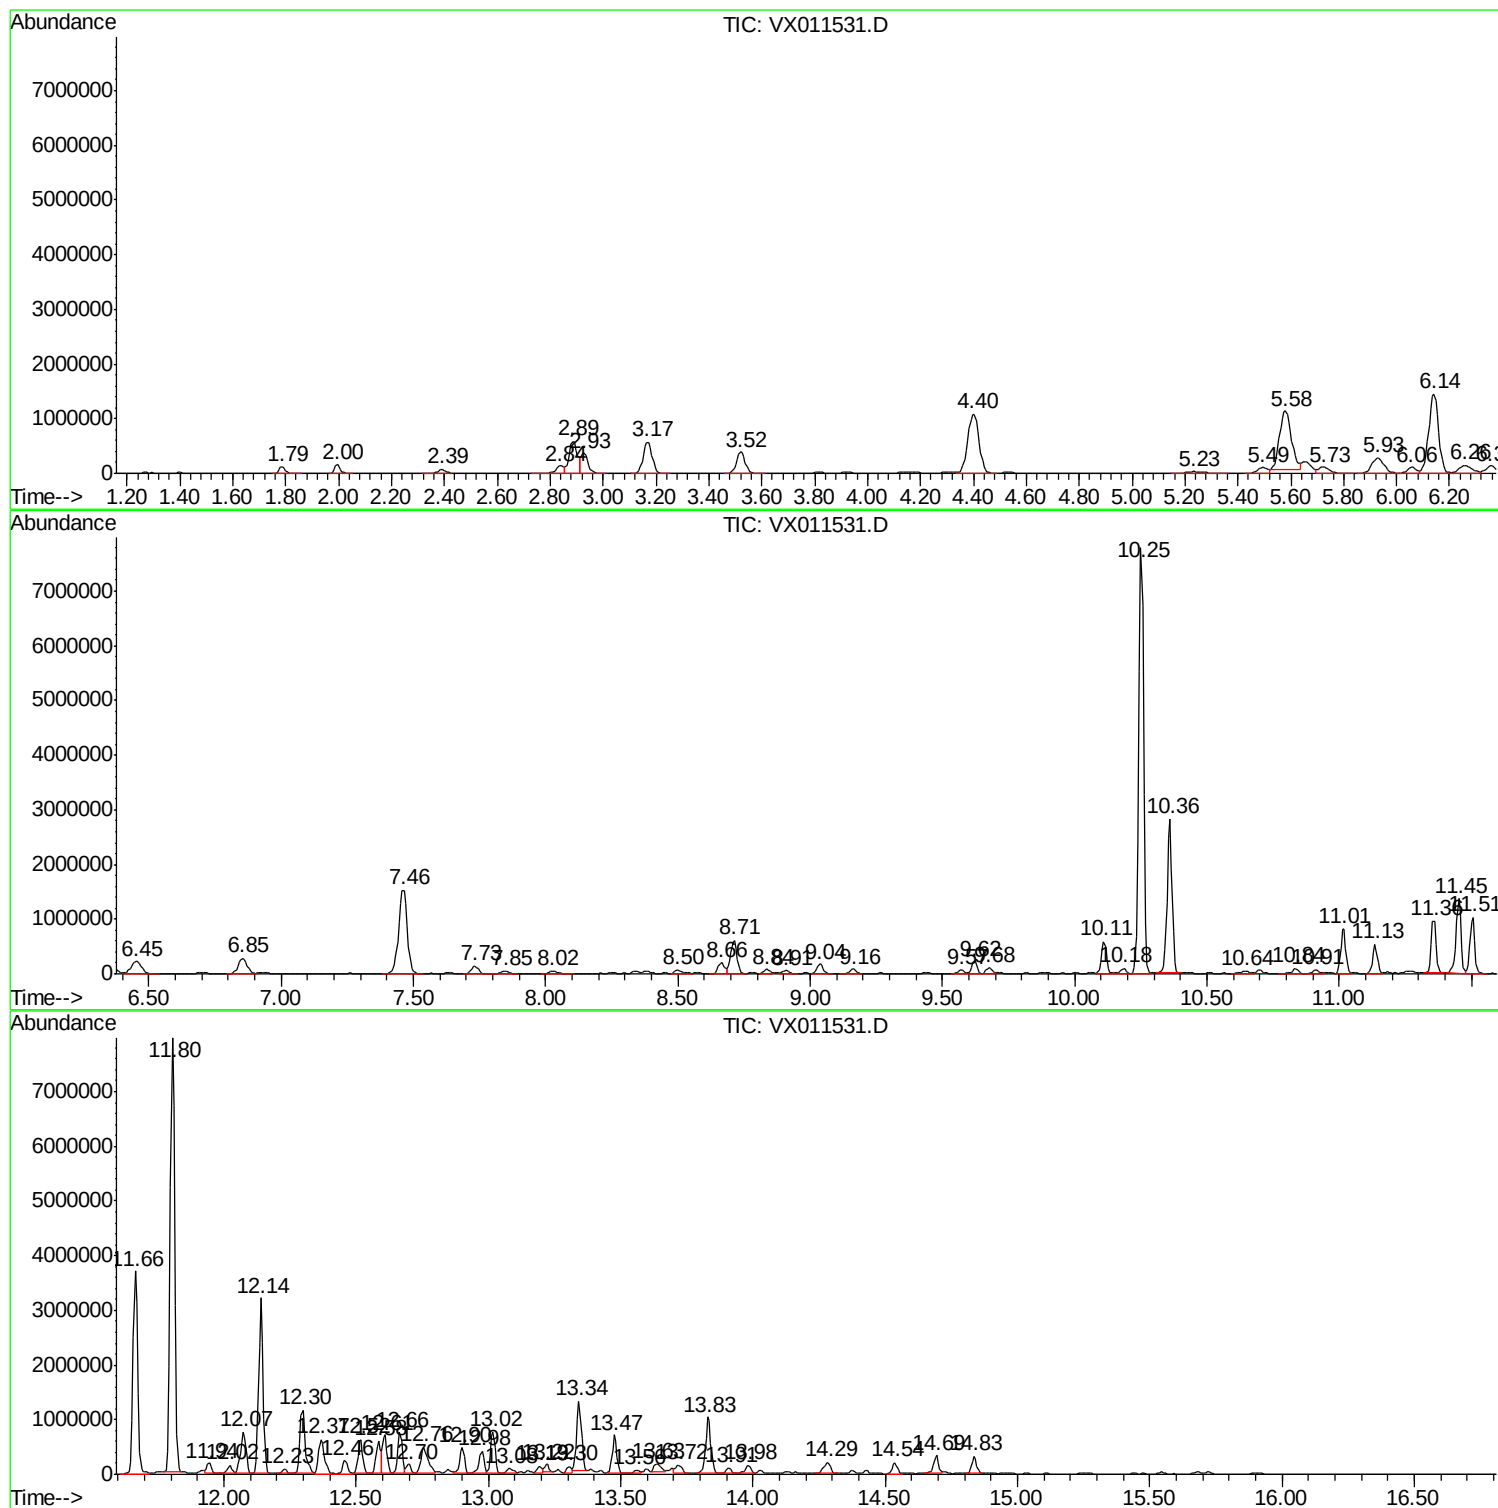

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081319\
Data File : VX011531.D
Acq On : 13 Aug 2019 13:20
Operator : JC/SP
Sample : K4279-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0671

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081319\
Data File : VX011531.D
Acq On : 13 Aug 2019 13:20
Operator : JC/SP
Sample : K4279-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0671

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc