

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081319\
 Data File : VX011533.D
 Acq On : 13 Aug 2019 14:07
 Operator : JC/SP
 Sample : K4279-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z3-0672

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.788	98	104	112	rVB	129967	175927	1.81%	0.212%
2	1.995	133	138	145	rVB	164553	227999	2.34%	0.275%
3	2.391	195	203	208	rBV	72513	147205	1.51%	0.178%
4	2.842	258	277	279	rBV2	147579	330918	3.40%	0.399%
5	2.885	279	284	288	rVV	623644	1328268	13.63%	1.603%
6	2.928	288	291	310	rVB	373646	700138	7.19%	0.845%
7	3.166	321	330	348	rVB	593389	1361340	13.97%	1.643%
8	3.519	377	388	403	rBV	415642	933876	9.59%	1.127%
9	4.397	522	532	547	rVB	1103716	3210806	32.96%	3.874%
10	5.238	655	670	690	rVB3	36645	154292	1.58%	0.186%
11	5.494	698	712	716	rBV3	110946	309815	3.18%	0.374%
12	5.580	716	726	735	rBV2	1077719	3416426	35.07%	4.122%
13	5.726	745	750	766	rVB2	116134	336316	3.45%	0.406%
14	5.927	770	783	796	rBV3	297473	947077	9.72%	1.143%
15	6.055	796	804	809	rVV	113148	287460	2.95%	0.347%
16	6.141	809	818	829	rVV	1380119	3580848	36.75%	4.321%
17	6.256	829	837	847	rVV3	145770	507742	5.21%	0.613%
18	6.354	847	853	861	rVV	141692	387046	3.97%	0.467%
19	6.452	861	869	884	rVB	239788	659525	6.77%	0.796%
20	6.854	924	935	944	rBV	293565	694417	7.13%	0.838%
21	7.464	1022	1035	1046	rBV	1557774	3584822	36.79%	4.326%
22	7.732	1071	1079	1089	rVB	153146	293579	3.01%	0.354%
23	7.848	1089	1098	1105	rVB4	50387	106705	1.10%	0.129%
24	8.024	1121	1127	1141	rVB2	53209	120578	1.24%	0.145%
25	8.500	1200	1205	1209	rBV	68055	109386	1.12%	0.132%
26	8.665	1224	1232	1235	rBV2	212985	378191	3.88%	0.456%
27	8.713	1235	1240	1247	rVB	622054	1046203	10.74%	1.262%
28	8.835	1255	1260	1264	rBV	89022	140593	1.44%	0.170%
29	8.908	1269	1272	1279	rVB2	66544	100016	1.03%	0.121%
30	9.036	1288	1293	1300	rVB	179192	287655	2.95%	0.347%
31	9.164	1305	1314	1319	rBV	87246	143575	1.47%	0.173%
32	9.573	1374	1381	1384	rBV2	76827	127060	1.30%	0.153%
33	9.622	1384	1389	1393	rVV	231789	318643	3.27%	0.384%
34	9.677	1393	1398	1402	rVV	104104	145342	1.49%	0.175%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081319\
 Data File : VX011533.D
 Acq On : 13 Aug 2019 14:07
 Operator : JC/SP
 Sample : K4279-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z3-0672

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Title : SW846 8260

35	10.109	1464	1469	1475	rBV	597068	777416	7.98%	0.938%
36	10.183	1475	1481	1486	rVB	86498	130772	1.34%	0.158%
37	10.250	1486	1492	1498	rBV	7690995	9742974	100.00%	11.756%
38	10.359	1501	1510	1516	rVV	2701054	3533479	36.27%	4.264%
39	10.646	1548	1557	1562	rBV4	43709	114726	1.18%	0.138%
40	10.695	1562	1565	1576	rVB2	60695	101556	1.04%	0.123%
41	10.835	1576	1588	1595	rBV2	95288	164550	1.69%	0.199%
42	10.914	1595	1601	1605	rBV3	62073	105905	1.09%	0.128%
43	11.018	1612	1618	1623	rBV	828875	1072121	11.00%	1.294%
44	11.134	1631	1637	1642	rBV	559472	710023	7.29%	0.857%
45	11.359	1669	1674	1680	rBV	963819	1206585	12.38%	1.456%
46	11.451	1681	1689	1693	rVV	1379189	1838859	18.87%	2.219%
47	11.506	1693	1698	1706	rVB	1079720	1331482	13.67%	1.607%
48	11.664	1719	1724	1734	rBV	3678657	4524255	46.44%	5.459%
49	11.804	1742	1747	1752	rBV	7802415	9339708	95.86%	11.270%
50	11.944	1767	1770	1776	rVV	187505	234404	2.41%	0.283%
51	12.024	1776	1783	1786	rVV	155358	192112	1.97%	0.232%
52	12.073	1786	1791	1797	rVB2	767105	1141460	11.72%	1.377%
53	12.140	1797	1802	1807	rBV	3121557	3644420	37.41%	4.398%
54	12.231	1812	1817	1821	rBV	94588	112875	1.16%	0.136%
55	12.298	1822	1828	1835	rBV2	1148423	1625922	16.69%	1.962%
56	12.365	1835	1839	1848	rVB3	627859	987945	10.14%	1.192%
57	12.457	1849	1854	1859	rBV2	250172	311419	3.20%	0.376%
58	12.518	1859	1864	1869	rVB	638075	781127	8.02%	0.943%
59	12.585	1869	1875	1877	rBV	599659	810551	8.32%	0.978%
60	12.609	1877	1879	1883	rVB	705270	692667	7.11%	0.836%
61	12.664	1883	1888	1892	rBV	745053	871161	8.94%	1.051%
62	12.700	1892	1894	1898	rVB	164725	162396	1.67%	0.196%
63	12.755	1898	1903	1910	rBV3	472096	863611	8.86%	1.042%
64	12.902	1922	1927	1931	rVB2	473000	607548	6.24%	0.733%
65	12.975	1931	1939	1942	rBV	443172	562298	5.77%	0.678%
66	13.017	1942	1946	1952	rVB	759899	923458	9.48%	1.114%
67	13.078	1952	1956	1961	rBV3	101043	179220	1.84%	0.216%
68	13.194	1971	1975	1977	rBV2	112271	149989	1.54%	0.181%
69	13.219	1977	1979	1983	rVB	145921	163311	1.68%	0.197%
70	13.304	1989	1993	1995	rBV2	117600	150442	1.54%	0.182%
71	13.341	1995	1999	2005	rVB2	1244585	1675819	17.20%	2.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081319\
Data File : VX011533.D
Acq On : 13 Aug 2019 14:07
Operator : JC/SP
Sample : K4279-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0672

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Title : SW846 8260

72	13.475	2016	2021	2029	rVB	685851	863842	8.87%	1.042%
73	13.560	2030	2035	2038	rBV4	64107	100111	1.03%	0.121%
74	13.633	2044	2047	2053	rVV4	143332	259678	2.67%	0.313%
75	13.719	2058	2061	2067	rVB2	160944	251044	2.58%	0.303%
76	13.828	2072	2079	2087	rVB	999853	1378526	14.15%	1.663%
77	13.908	2087	2092	2097	rVB2	108214	150871	1.55%	0.182%
78	13.981	2097	2104	2108	rBV2	154574	240037	2.46%	0.290%
79	14.286	2146	2154	2158	rVB2	197642	360536	3.70%	0.435%
80	14.535	2190	2195	2204	rBV2	219751	295088	3.03%	0.356%
81	14.694	2213	2221	2224	rBV	318728	425634	4.37%	0.514%
82	14.834	2239	2244	2249	rBV	305734	410929	4.22%	0.496%


Sum of corrected areas: 82874651

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081319\
Data File : VX011533.D
Acq On : 13 Aug 2019 14:07
Operator : JC/SP
Sample : K4279-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0672

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

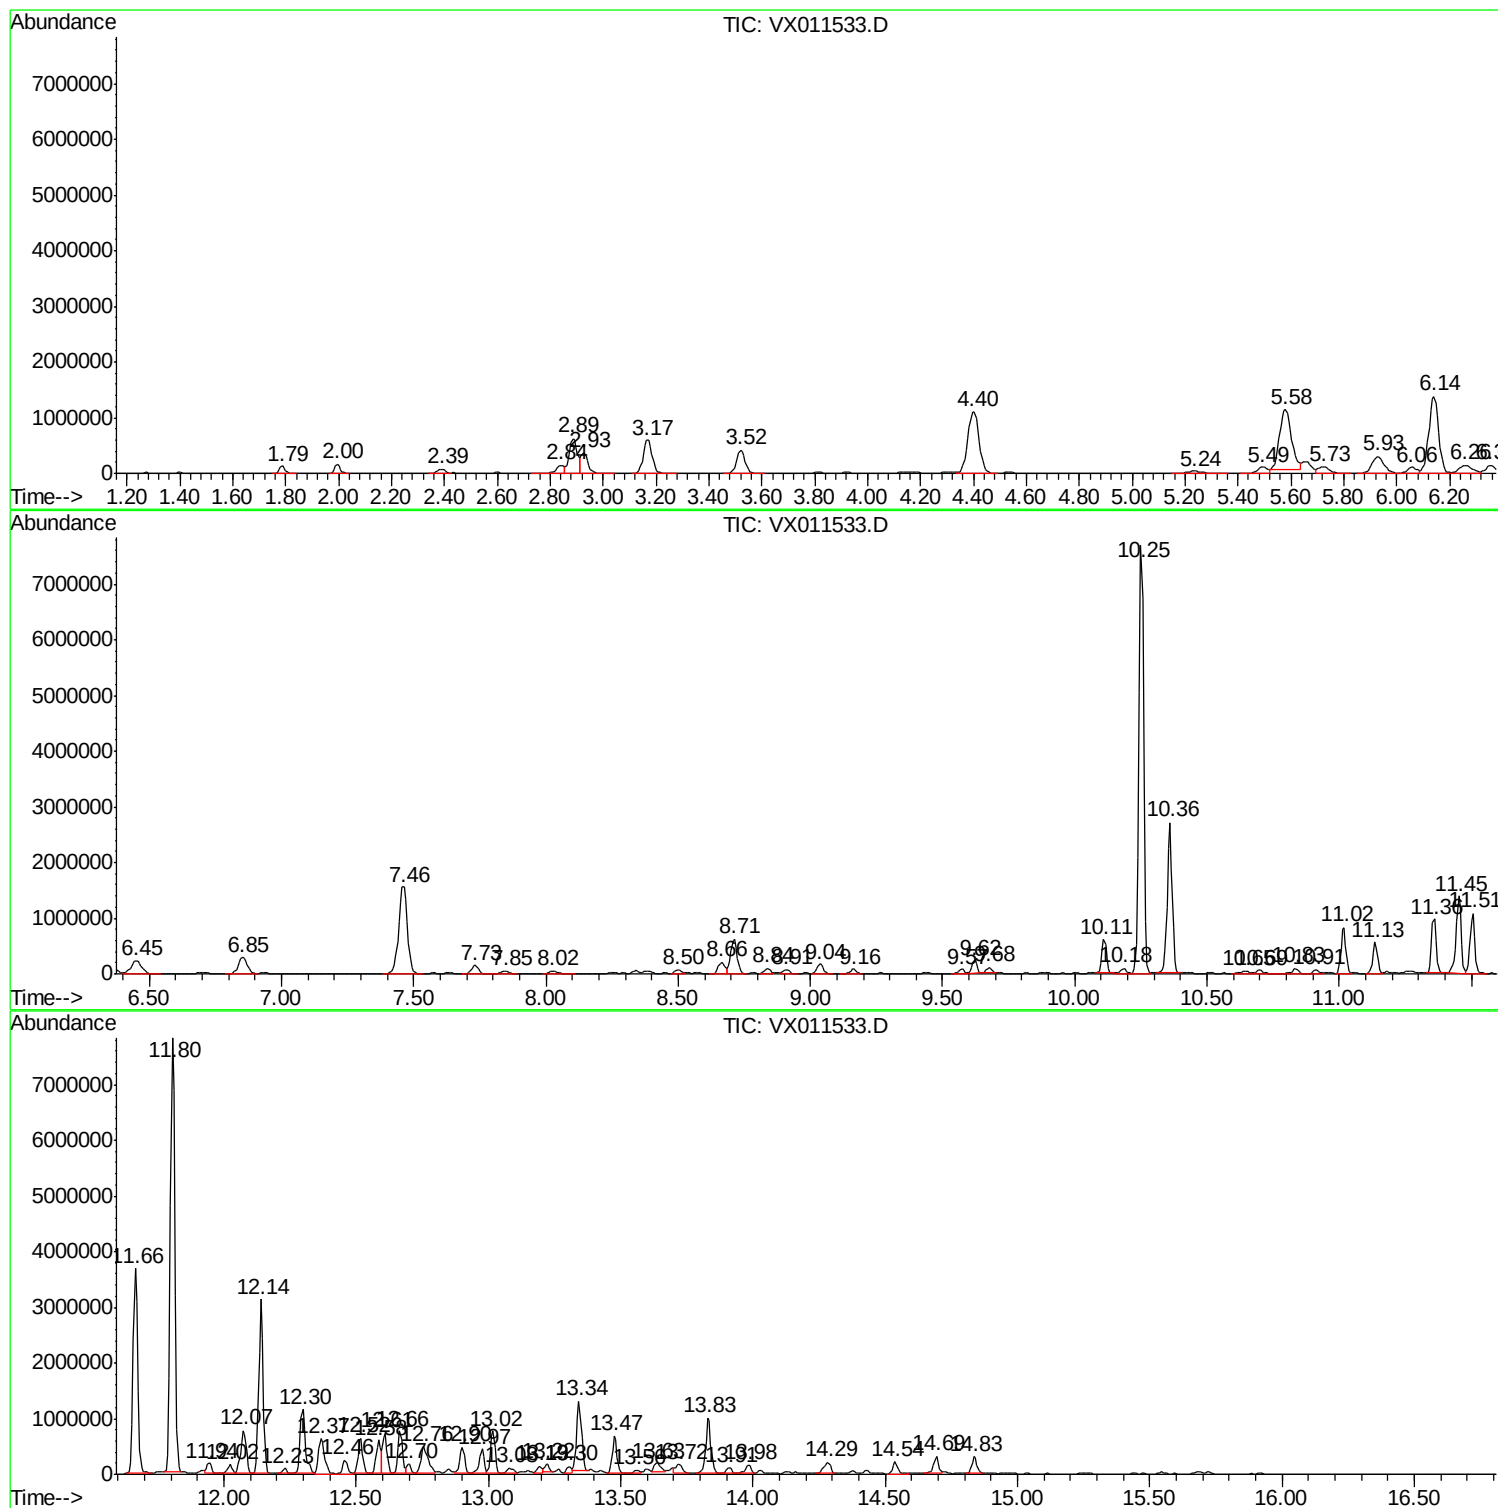

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081319\
Data File : VX011533.D
Acq On : 13 Aug 2019 14:07
Operator : JC/SP
Sample : K4279-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0672

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081319\
Data File : VX011533.D
Acq On : 13 Aug 2019 14:07
Operator : JC/SP
Sample : K4279-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0672

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc