

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081319\  
Data File : VX011545.D  
Acq On : 13 Aug 2019 18:48  
Operator : JC/SP  
Sample : K4336-06  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
KY038PS034-190812

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X080119W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.270       | 15            | 19          | 27           | rBV      | 34458          | 43980         | 4.98%           | 0.890%        |
| 2         | 2.599       | 229           | 237         | 245          | rVB3     | 4600           | 10929         | 1.24%           | 0.221%        |
| 3         | 4.592       | 552           | 564         | 577          | rBV3     | 41925          | 125603        | 14.21%          | 2.541%        |
| 4         | 5.495       | 700           | 712         | 726          | rBV      | 107400         | 308022        | 34.85%          | 6.232%        |
| 5         | 5.659       | 728           | 739         | 753          | rVV      | 197533         | 551658        | 62.41%          | 11.162%       |
| 6         | 6.055       | 793           | 804         | 818          | rBV      | 113336         | 302584        | 34.23%          | 6.122%        |
| 7         | 6.854       | 926           | 935         | 952          | rBV      | 283834         | 666925        | 75.45%          | 13.494%       |
| 8         | 8.713       | 1233          | 1240        | 1253         | rBV      | 583516         | 883886        | 100.00%         | 17.884%       |
| 9         | 10.110      | 1463          | 1469        | 1481         | rBV      | 588844         | 765848        | 86.65%          | 15.495%       |
| 10        | 11.134      | 1632          | 1637        | 1648         | rBV      | 472586         | 586557        | 66.36%          | 11.868%       |
| 11        | 12.073      | 1786          | 1791        | 1800         | rBV      | 538321         | 696452        | 78.79%          | 14.091%       |


Sum of corrected areas: 4942444

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX081319\  
Data File : VX011545.D  
Acq On : 13 Aug 2019 18:48  
Operator : JC/SP  
Sample : K4336-06  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
KY038PS034-190812

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X080119W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

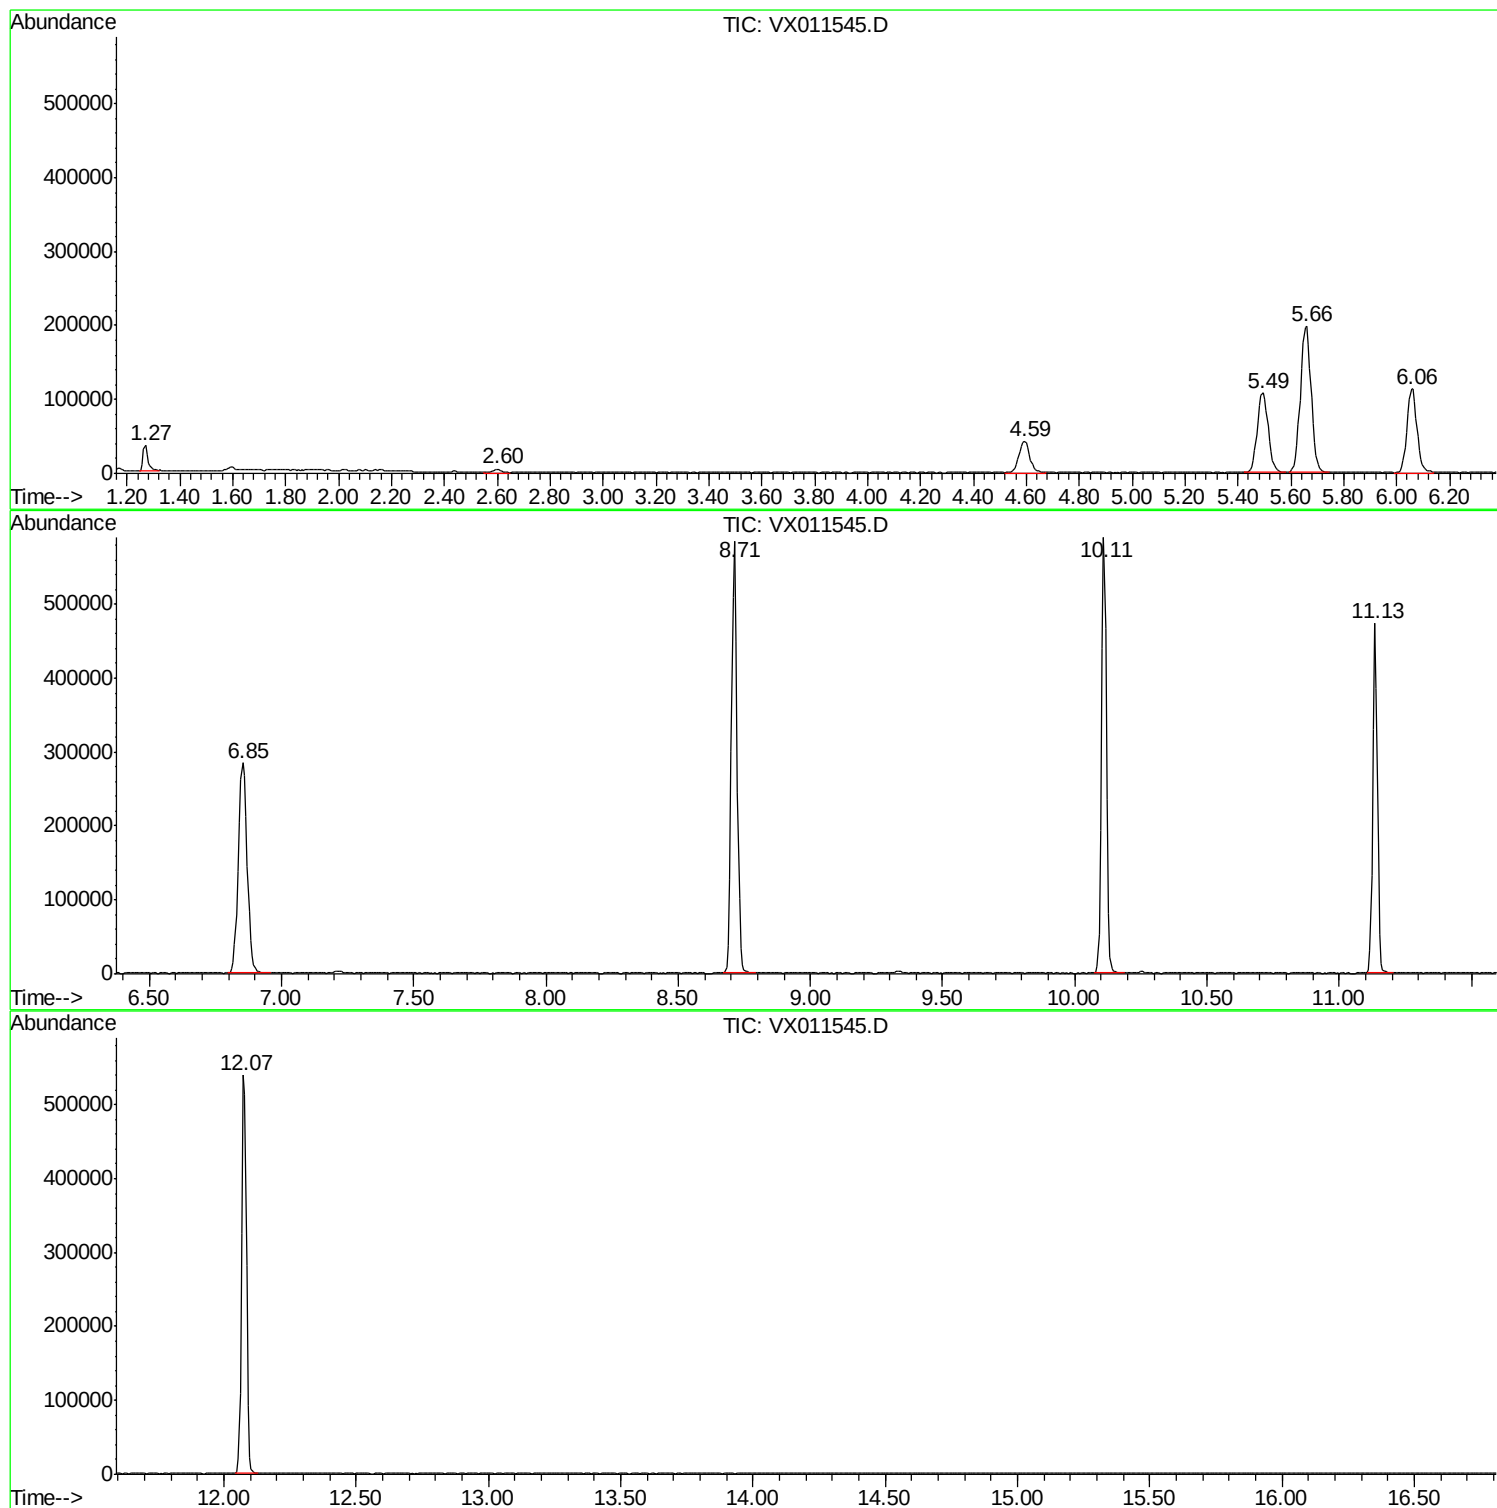

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX081319\  
Data File : VX011545.D  
Acq On : 13 Aug 2019 18:48  
Operator : JC/SP  
Sample : K4336-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
KY038PS034-190812

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X080119W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX081319\  
Data File : VX011545.D  
Acq On : 13 Aug 2019 18:48  
Operator : JC/SP  
Sample : K4336-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
KY038PS034-190812

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X080119W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |