


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081320\
Data File : VX017879.D
Acq On : 13 Aug 2020 16:49
Operator : JC/SP
Sample : L3643-03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Aug 14 08:26:56 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 14 07:35:30 2020
Response via : Initial Calibration

Instrument :
MSVOA_X
Client Sampled :
BG0A4

Manual Integrations
APPROVED

MMDadoda
8/14/2020 10:06:40 AM

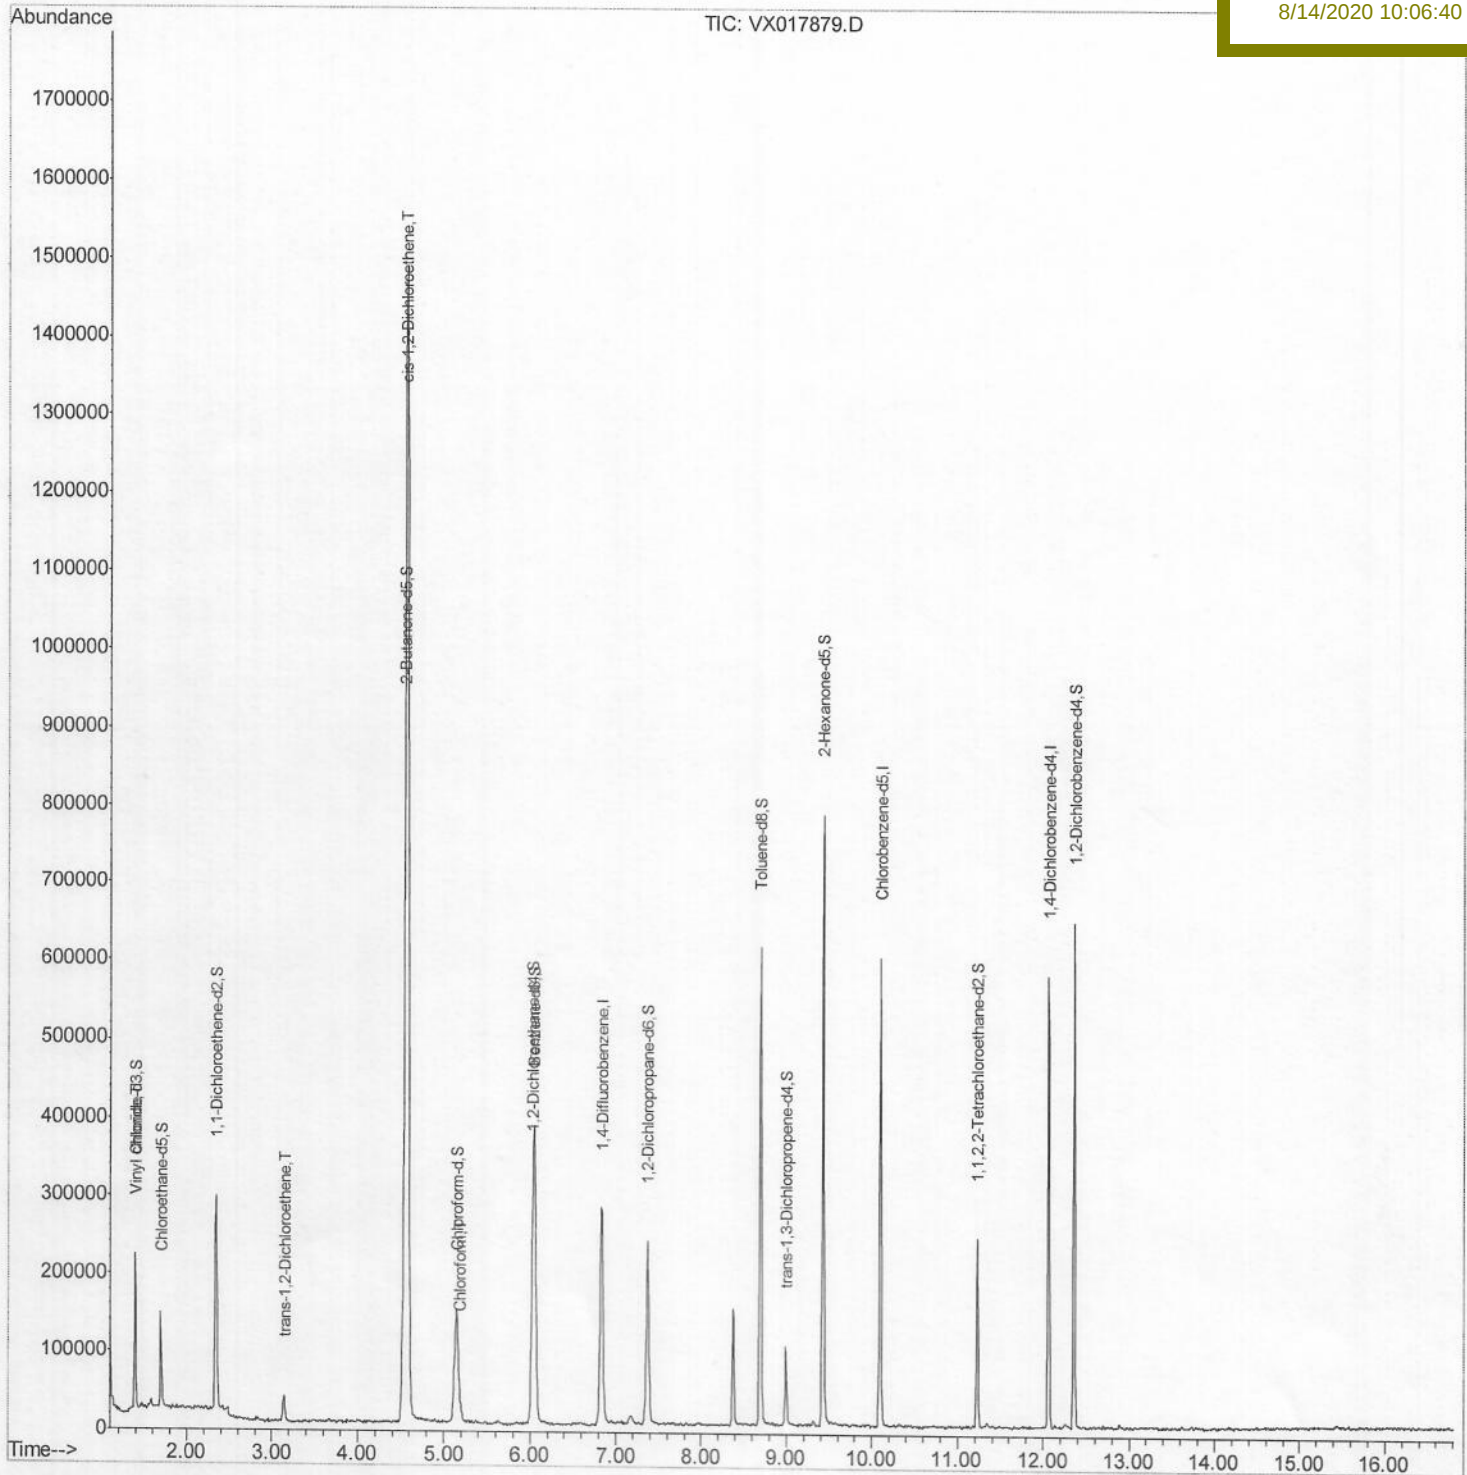

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081320\
 Data File : VX017879.D
 Acq On : 13 Aug 2020 16:49
 Operator : JC/SP
 Sample : L3643-03
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Aug 14 07:38:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 14 07:35:30 2020
 Response via : Initial Calibration

Instrument :
 MSVOA_X
 ClientSampled :
 BG0A4

Manual Integrations
 APPROVED

MMDadoda
 8/14/2020 10:06:40 AM

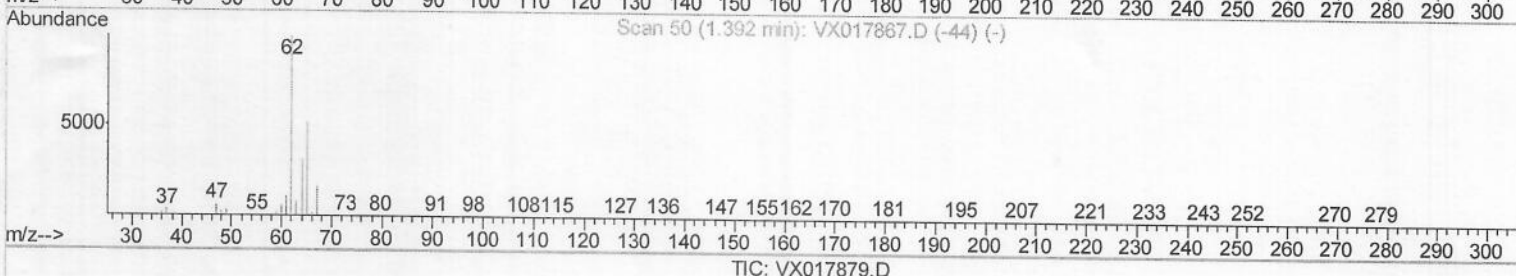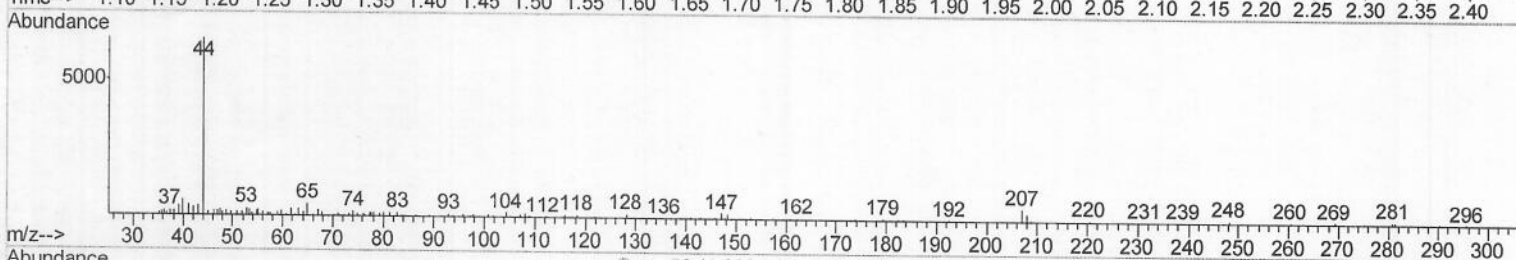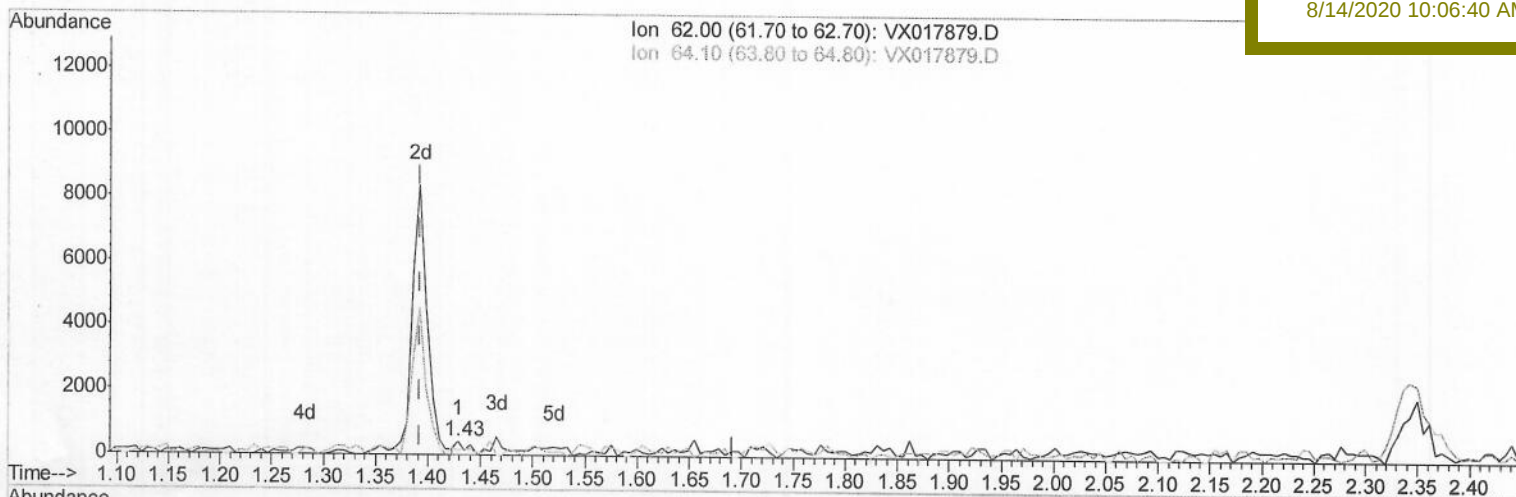

TIC: VX017879.D

(5) Vinyl chloride (T)

1.429min (+0.037) 0.01ug/L

response 335

Ion	Exp%	Act%
62.00	100	100
64.10	30.50	39.21
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081320\

Data File : VX017879.D

Acq On : 13 Aug 2020 16:49

Operator : JC/SP

Sample : L3643-03

Misc : 25.0mL/MSVOA_X/WATER

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Aug 14 07:38:05 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Fri Aug 14 07:35:30 2020




Response via : Initial Calibration

Instrument :

MSVOA_X

ClientSampled :

BG0A4

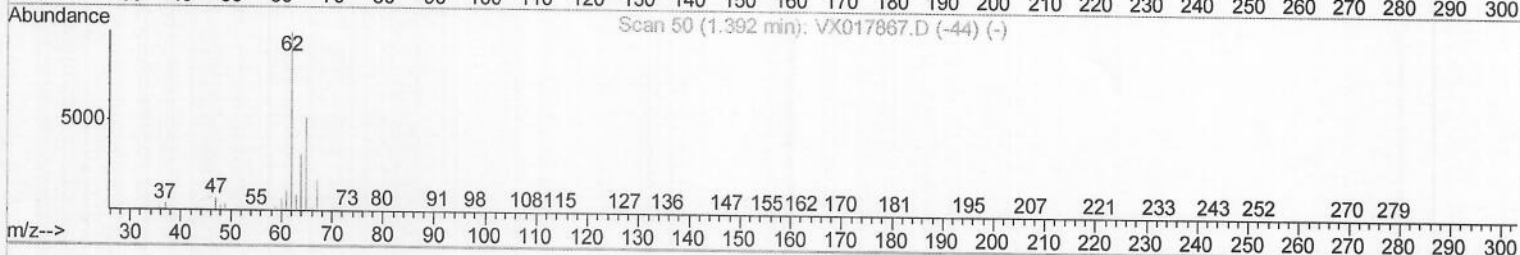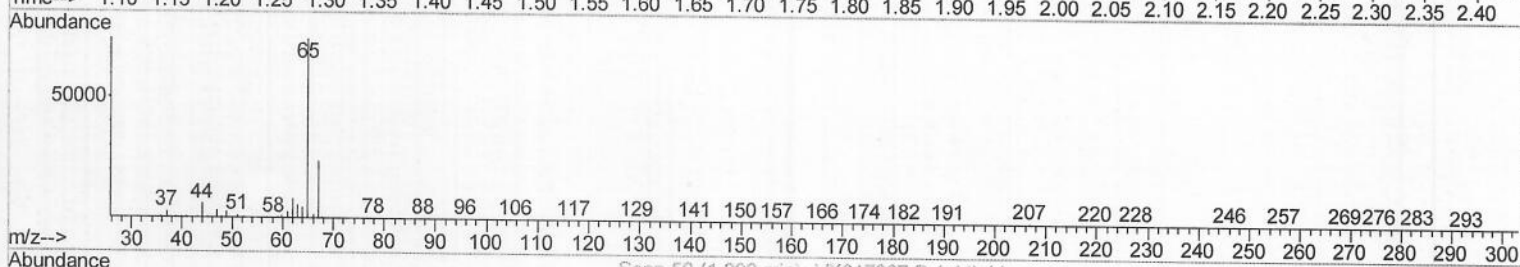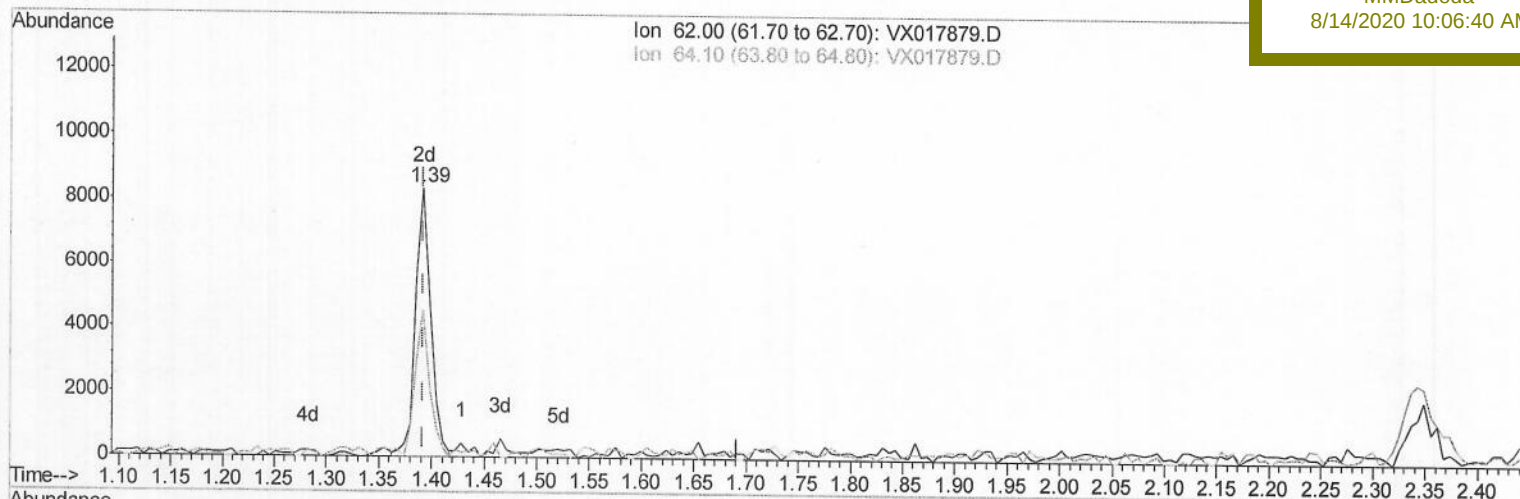Manual Integrations
APPROVEDMMDadoda
8/14/2020 10:06:40 AM

TIC: VX017879.D

(5) Vinyl chloride (T)

1.392min (+0.000) 0.31ug/L m ->

response 8229

Ion Exp% Act%

62.00 100 100

64.10 30.50 54.43#

0.00 0.00 0.00

0.00 0.00 0.00

MD
08/14/20

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081320\
 Data File : VX017879.D
 Acq On : 13 Aug 2020 16:49
 Operator : JC/SP
 Sample : L3643-03
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 Client Sampled :
 BG0A4

Quant Time: Aug 14 08:26:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 14 07:35:30 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 8/14/2020 10:06:40 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	6.83	114	280645	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	265243	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	118221	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	108950	5.62	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	112.40%
7) Chloroethane-d5	1.69	69	83676	5.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.80%
11) 1,1-Dichloroethene-d2	2.34	63	156411	3.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.40%
20) 2-Butanone-d5	4.54	46	264415	51.34	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.68%
24) Chloroform-d	5.14	84	176181	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
26) 1,2-Dichloroethane-d4	6.03	65	111692	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.40%
32) Benzene-d6	6.05	84	389869	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.00%
36) 1,2-Dichloropropane-d6	7.37	67	122170	5.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.60%
41) Toluene-d8	8.70	98	349030	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
45) trans-1,3-Dichloropropene-	8.99	79	48447	4.97	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.40%
48) 2-Hexanone-d5	9.43	63	204132	50.39	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.78%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	89281	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.40%
65) 1,2-Dichlorobenzene-d4	12.36	152	130356	5.73	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.60%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Vinyl chloride	1.39	62	8229m ->	0.311	ug/L	
18) trans-1,2-Dichloroethene	3.14	96	12794	0.524	ug/L	97
22) cis-1,2-Dichloroethene	4.56	96	905310	35.347	ug/L #	99
25) Chloroform	5.18	83	32006	0.683	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed