


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081320\
 Data File : VX017866.D
 Acq On : 13 Aug 2020 08:49
 Operator : JC/SP
 Sample : BFB68
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB68

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Aug 14 13:36:03 2020

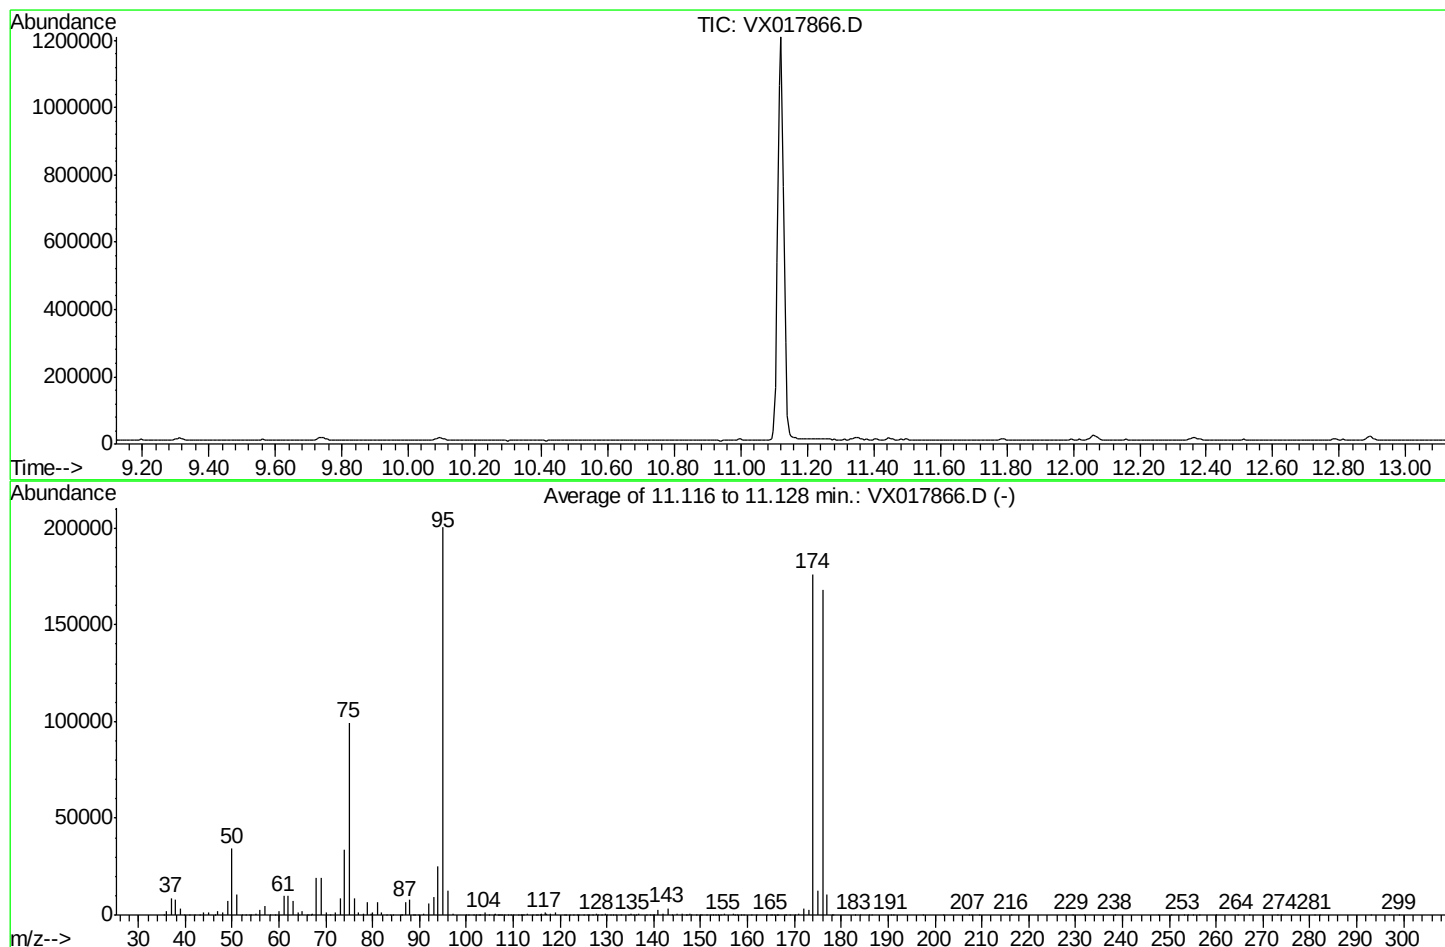

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	34304	PASS
75	95	30	80	49.5	99253	PASS
95	95	100	100	100.0	200341	PASS
96	95	5	9	6.2	12508	PASS
173	174	0.00	2	1.4	2467	PASS
174	95	50	120	88.0	176256	PASS
175	174	5	9	7.3	12814	PASS
176	174	95	101	95.5	168367	PASS
177	176	5	9	6.2	10415	PASS

m/z	Abundance
36.00	2415.0
37.00	11209.0
38.00	9146.0
39.00	4626.0
40.00	615.0
41.20	236.0
42.20	145.0
42.90	208.0
44.00	2158.0
44.90	1968.0
46.90	2804.0
47.90	1586.0
49.00	9168.0
50.00	40336.0
51.00	13696.0
52.20	701.0
52.80	284.0
53.70	208.0
55.10	800.0
56.00	3245.0
57.00	5589.0
58.00	497.0
58.80	118.0
59.20	139.0
60.00	2185.0
61.00	10820.0
62.00	11881.0
63.00	8642.0
64.00	1926.0
64.90	2645.0
65.90	365.0
66.90	751.0
68.00	20872.0
69.00	23152.0
70.10	1831.0
70.80	283.0
72.00	1744.0
73.00	10148.0
74.00	38096.0
75.00	114400.0
76.00	11015.0
77.10	1281.0
77.90	909.0
78.90	7053.0
79.80	2393.0
80.90	7114.0
81.90	1851.0
83.10	139.0
83.70	164.0
84.30	62.0
86.20	659.0
87.00	7570.0
87.90	8431.0
88.80	312.0
90.00	159.0
91.00	1153.0
92.00	5669.0
93.00	10392.0
94.00	27472.0
95.00	215616.0
96.00	14081.0
97.10	319.0
97.90	66.0
99.90	73.0
100.30	52.0
102.10	153.0
102.60	220.0
103.00	214.0
104.00	1208.0
104.80	340.0
105.90	879.0
106.70	194.0
107.20	167.0
108.30	80.0
109.00	72.0
110.00	229.0
110.90	383.0
111.70	192.0
112.20	180.0
113.00	406.0
114.90	397.0
115.80	810.0
116.80	2157.0
117.80	902.0
118.90	1487.0
120.80	61.0
122.10	69.0
123.70	97.0
126.10	153.0
127.80	1155.0
129.00	435.0
129.80	602.0

Instrument :
MSVOA_X
ClientSampleId :
BFB68

130.90	301.0
131.80	63.0
132.90	57.0
134.00	88.0
135.00	588.0
136.10	305.0
136.90	426.0
138.30	159.0
139.70	161.0
141.00	2269.0
142.00	599.0
142.90	3004.0
144.00	351.0
145.00	888.0
145.90	335.0
147.00	306.0
147.80	751.0
149.10	146.0
149.80	380.0
152.10	96.0
152.60	100.0
153.20	103.0
154.20	165.0
155.00	508.0
156.20	55.0
156.90	293.0
157.20	264.0
157.90	61.0
158.70	296.0
159.10	297.0
160.90	360.0
161.80	78.0
164.80	130.0
166.60	157.0
167.90	130.0
168.30	87.0
169.10	191.0
170.00	149.0
171.00	506.0
172.00	3047.0
173.00	2391.0
174.00	165568.0
175.10	12454.0
176.00	154816.0
177.00	10157.0
177.90	521.0
184.10	51.0
185.90	74.0
190.80	118.0
192.80	63.0
201.90	52.0
207.10	388.0
207.70	85.0
216.30	69.0
250.40	56.0
253.10	89.0
255.10	64.0
267.20	54.0
273.00	83.0
273.90	63.0
281.20	308.0
282.20	67.0

Instrument :
MSVOA_X
ClientSampleId :
BFB68

m/z	Abundance
35.30	198.0
36.00	2124.0
37.00	10334.0
38.00	8415.0
39.10	4104.0
39.90	701.0
40.90	130.0
41.90	249.0
43.00	336.0
43.90	2444.0
45.00	1909.0
46.30	474.0
46.90	2778.0
48.00	1548.0
49.00	8470.0
50.00	40768.0
51.00	12358.0
51.90	707.0
53.10	222.0
53.90	133.0
54.90	991.0
56.00	3625.0
56.90	6115.0
57.90	276.0
58.80	68.0
59.90	2172.0
61.00	11284.0
62.00	10847.0
63.00	8729.0
64.00	1440.0
65.00	1917.0
66.00	272.0
66.20	272.0
67.10	772.0
68.00	24248.0
69.00	21744.0
70.10	1700.0
70.90	195.0
72.00	1496.0
73.00	9838.0
74.00	40080.0
75.00	116800.0
76.00	9807.0
76.90	1586.0
77.80	776.0
78.90	8125.0
80.00	2537.0
80.90	8605.0
81.80	1678.0
83.00	224.0
83.60	118.0
85.90	410.0
87.00	8241.0
87.90	9357.0
89.90	295.0
90.90	753.0
92.00	7385.0
93.00	10663.0
94.00	28880.0
95.00	241472.0
96.00	15494.0
97.20	787.0
99.90	60.0
102.10	104.0
102.80	189.0
103.10	177.0
103.90	1389.0
104.80	539.0
106.10	864.0
106.90	166.0
108.80	56.0
110.00	213.0
111.00	310.0
111.90	223.0
112.90	512.0
115.10	466.0
116.00	1182.0
116.80	1775.0
117.90	1360.0
119.00	1405.0
121.30	90.0
122.10	218.0
122.90	321.0
124.00	193.0
125.10	70.0
126.00	197.0
127.10	152.0
128.00	797.0
129.10	500.0
129.80	855.0
130.80	370.0
131.80	89.0

Instrument :
MSVOA_X
ClientSampleId :
BFB68

134.00	122.0
134.70	556.0
135.00	541.0
135.60	283.0
136.10	140.0
136.90	690.0
138.40	169.0
139.10	204.0
140.90	2706.0
141.90	544.0
143.00	4637.0
143.90	214.0
144.80	1098.0
146.00	391.0
146.80	373.0
147.80	752.0
149.00	139.0
149.80	317.0
150.10	318.0
151.10	177.0
152.00	266.0
152.70	263.0
154.20	121.0
154.90	859.0
156.90	443.0
157.90	68.0
159.00	234.0
161.00	436.0
161.80	100.0
164.20	94.0
164.80	57.0
165.10	58.0
165.70	51.0
166.50	78.0
167.90	94.0
169.10	167.0
170.10	187.0
171.00	684.0
172.00	3671.0
173.00	2738.0
174.00	212480.0
175.00	14022.0
176.00	209216.0
177.00	12574.0
178.20	504.0
186.60	69.0
192.80	131.0
207.10	399.0
247.60	108.0
260.00	68.0
264.60	78.0
273.00	59.0
273.90	172.0
281.10	153.0
282.10	83.0
293.00	86.0
299.20	82.0

Instrument :
MSVOA_X
ClientSampleId :
BFB68

m/z	Abundance
36.00	1310.0
36.90	5136.0
38.00	6089.0
39.00	2334.0
39.80	385.0
40.80	230.0
42.00	295.0
43.10	420.0
44.00	1762.0
44.90	1166.0
46.10	394.0
47.00	1386.0
47.90	996.0
49.00	4948.0
50.00	21808.0
51.00	6501.0
52.10	317.0
53.00	244.0
54.00	304.0
55.00	599.0
55.90	2125.0
57.00	3139.0
58.10	203.0
59.00	107.0
60.00	1413.0
61.00	7124.0
62.00	6453.0
63.00	5298.0
63.90	632.0
64.20	693.0
65.00	1177.0
66.20	219.0
67.10	372.0
68.00	12171.0
69.00	13515.0
70.10	875.0
71.30	132.0
71.90	646.0
73.00	6168.0
74.00	23656.0
75.00	66560.0
76.00	6103.0
77.00	844.0
78.00	407.0
78.90	4652.0
79.90	1391.0
80.90	4136.0
82.00	1163.0
83.00	214.0
84.10	59.0
86.00	237.0
87.00	5043.0
88.00	5162.0
89.00	179.0
89.80	128.0
90.80	561.0
91.00	558.0
92.10	5004.0
93.00	7340.0
94.00	18272.0
95.00	143936.0
96.00	8539.0
97.00	422.0
100.00	130.0
101.50	141.0
102.70	124.0
103.80	633.0
105.00	239.0
106.00	684.0
106.90	246.0
107.60	85.0
108.10	97.0
109.50	54.0
110.10	192.0
110.90	169.0
111.90	183.0
113.10	227.0
114.10	103.0
115.20	206.0
116.00	733.0
117.10	1258.0
117.80	792.0
119.00	1014.0
122.10	170.0
122.90	162.0
124.00	167.0
125.80	92.0
126.10	99.0
127.00	90.0
127.80	725.0
128.90	506.0
130.00	912.0

Instrument :
MSVOA_X
ClientSampleId :
BFB68

130.70	233.0
131.30	118.0
131.80	113.0
133.20	66.0
135.00	421.0
136.80	471.0
139.10	272.0
139.90	221.0
140.90	2176.0
141.80	391.0
142.90	3311.0
143.90	204.0
144.90	882.0
145.90	423.0
147.10	149.0
148.00	520.0
149.00	191.0
149.90	312.0
151.10	59.0
152.00	137.0
153.00	74.0
153.70	105.0
154.90	583.0
156.90	531.0
159.10	127.0
160.90	447.0
164.00	99.0
165.10	276.0
166.20	121.0
167.80	113.0
168.30	100.0
170.20	175.0
170.80	298.0
171.90	2436.0
173.10	2272.0
174.00	150720.0
175.00	11967.0
176.00	141312.0
177.00	8515.0
178.20	113.0
182.80	79.0
190.60	82.0
191.10	119.0
192.90	105.0
193.90	86.0
197.50	94.0
206.80	222.0
207.10	248.0
209.30	58.0
229.30	69.0
231.90	56.0
238.50	75.0
253.00	68.0
253.90	87.0
256.50	105.0
264.60	68.0
267.20	67.0
281.00	405.0
299.10	54.0

Instrument :
MSVOA_X
ClientSampleId :
BFB68

m/z	Abundance
35.90	183.0
36.80	171.0
37.50	183.0
37.90	131.0
38.50	127.0
38.90	172.0
39.80	387.0
41.20	152.0
41.80	140.0
42.30	88.0
42.90	233.0
44.10	1055.0
45.10	142.0
47.30	67.0
48.20	77.0
49.00	50.0
50.30	192.0
52.00	240.0
53.00	172.0
54.40	94.0
56.20	190.0
57.10	131.0
58.10	103.0
58.60	156.0
59.60	93.0
60.20	57.0
60.70	97.0
64.10	118.0
64.90	104.0
65.70	111.0
67.90	54.0
68.70	86.0
71.10	107.0
71.90	90.0
72.50	126.0
73.10	229.0
76.10	115.0
78.00	143.0
79.00	142.0
79.70	161.0
80.50	119.0
82.70	68.0
85.30	78.0
86.00	148.0
91.80	119.0
94.60	76.0
95.50	75.0
96.10	196.0
97.80	165.0
100.60	143.0
102.60	59.0
105.00	129.0
107.00	67.0
117.50	173.0
118.00	71.0
119.30	50.0
128.90	129.0
129.70	62.0
133.20	188.0
134.00	100.0
137.30	157.0
145.50	58.0
147.00	125.0
147.90	54.0
155.80	116.0
156.40	110.0
160.80	107.0
162.80	161.0
176.00	81.0
192.00	59.0
192.70	104.0
193.70	83.0
195.70	60.0
206.80	151.0
207.30	184.0
212.80	51.0
221.00	116.0
248.80	77.0
251.30	57.0
266.90	117.0
268.80	148.0
269.70	154.0
277.00	72.0
280.80	224.0
281.20	157.0
286.30	53.0
291.60	54.0

Instrument :
MSVOA_X
ClientSampleId :
BFB68