

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081321\
 Data File : VX023709.D
 Acq On : 13 Aug 2021 23:41
 Operator : JC/MD
 Sample : PB138358ZHE#20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Aug 14 05:32:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 23 06:05:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	148981	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	259408	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	245940	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	95525	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	105867	56.967	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 113.940%			
35) Dibromofluoromethane	5.397	113	82981	51.162	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 102.320%			
50) Toluene-d8	8.653	98	322861	54.180	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 108.360%			
62) 4-Bromofluorobenzene	11.085	95	108145	53.370	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 106.740%			
Target Compounds					Qvalue	
3) Chloromethane	1.301	50	390	0.244	ug/l	99
5) Bromomethane	1.630	94	608	0.634	ug/l	82
6) Chloroethane	1.685	64	285	0.287	ug/l #	86
10) Methyl Iodide	2.471	142	1596	0.864	ug/l #	95
11) Tert butyl alcohol	2.965	59	1160	2.732	ug/l #	78
13) Acrolein	2.240	56	105	1.848	ug/l #	1
15) Acrylonitrile	3.087	53	340	0.355	ug/l #	62
16) Acetone	2.386	43	28580	31.351	ug/l	90
17) Carbon Disulfide	2.514	76	1189	0.329	ug/l #	93
18) Methyl Acetate	2.715	43	1599	0.738	ug/l #	88
20) Methylene Chloride	2.794	84	12587	7.098	ug/l	91
25) 2-Butanone	4.581	43	4424	3.126	ug/l #	85
29) Tetrahydrofuran	5.038	42	1666	1.796	ug/l #	83
36) 1,1-Dichloropropene	5.562	75	12039	5.130	ug/l #	50
38) Carbon Tetrachloride	5.562	117	15113	6.333	ug/l #	15
43) Isopropyl Acetate	6.349	43	23162	5.052	ug/l #	90
48) Methyl methacrylate	7.604	41	6010	2.830	ug/l #	10
49) 1,4-Dioxane	7.806	88	170	3.760	ug/l #	1
51) 4-Methyl-2-Pentanone	8.555	43	81904	29.207	ug/l #	46
53) t-1,3-Dichloropropene	8.982	75	221	1.891	ug/l #	44
54) cis-1,3-Dichloropropene	8.555	75	34093	12.155	ug/l #	72
57) 1,3-Dichloropropane	9.488	76	21903	7.385	ug/l #	43
59) 2-Hexanone	9.488	43	320420	150.470	ug/l #	43
60) Dibromochloromethane	9.275	129	199	2.082	ug/l #	11
74) N-amyl acetate	10.768	43	952	0.289	ug/l #	43
76) 1,2,3-Trichloropropane	11.085	75	58617	27.885	ug/l #	39
80) 1,3,5-Trimethylbenzene	11.457	105	1316	0.224	ug/l	96
81) trans-1,4-Dichloro-2-b...	11.085	75	58617	74.979	ug/l #	12
93) 1,2,4-Trichlorobenzene	13.591	180	528	0.270	ug/l #	85
94) Hexachlorobutadiene	13.725	225	192	0.219	ug/l	85
96) 1,2,3-Trichlorobenzene	13.963	180	499	0.253	ug/l	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081321\
Data File : VX023709.D
Acq On : 13 Aug 2021 23:41
Operator : JC/MD
Sample : PB138358ZHE#20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Aug 14 05:32:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 23 06:05:38 2021
Response via : Initial Calibration




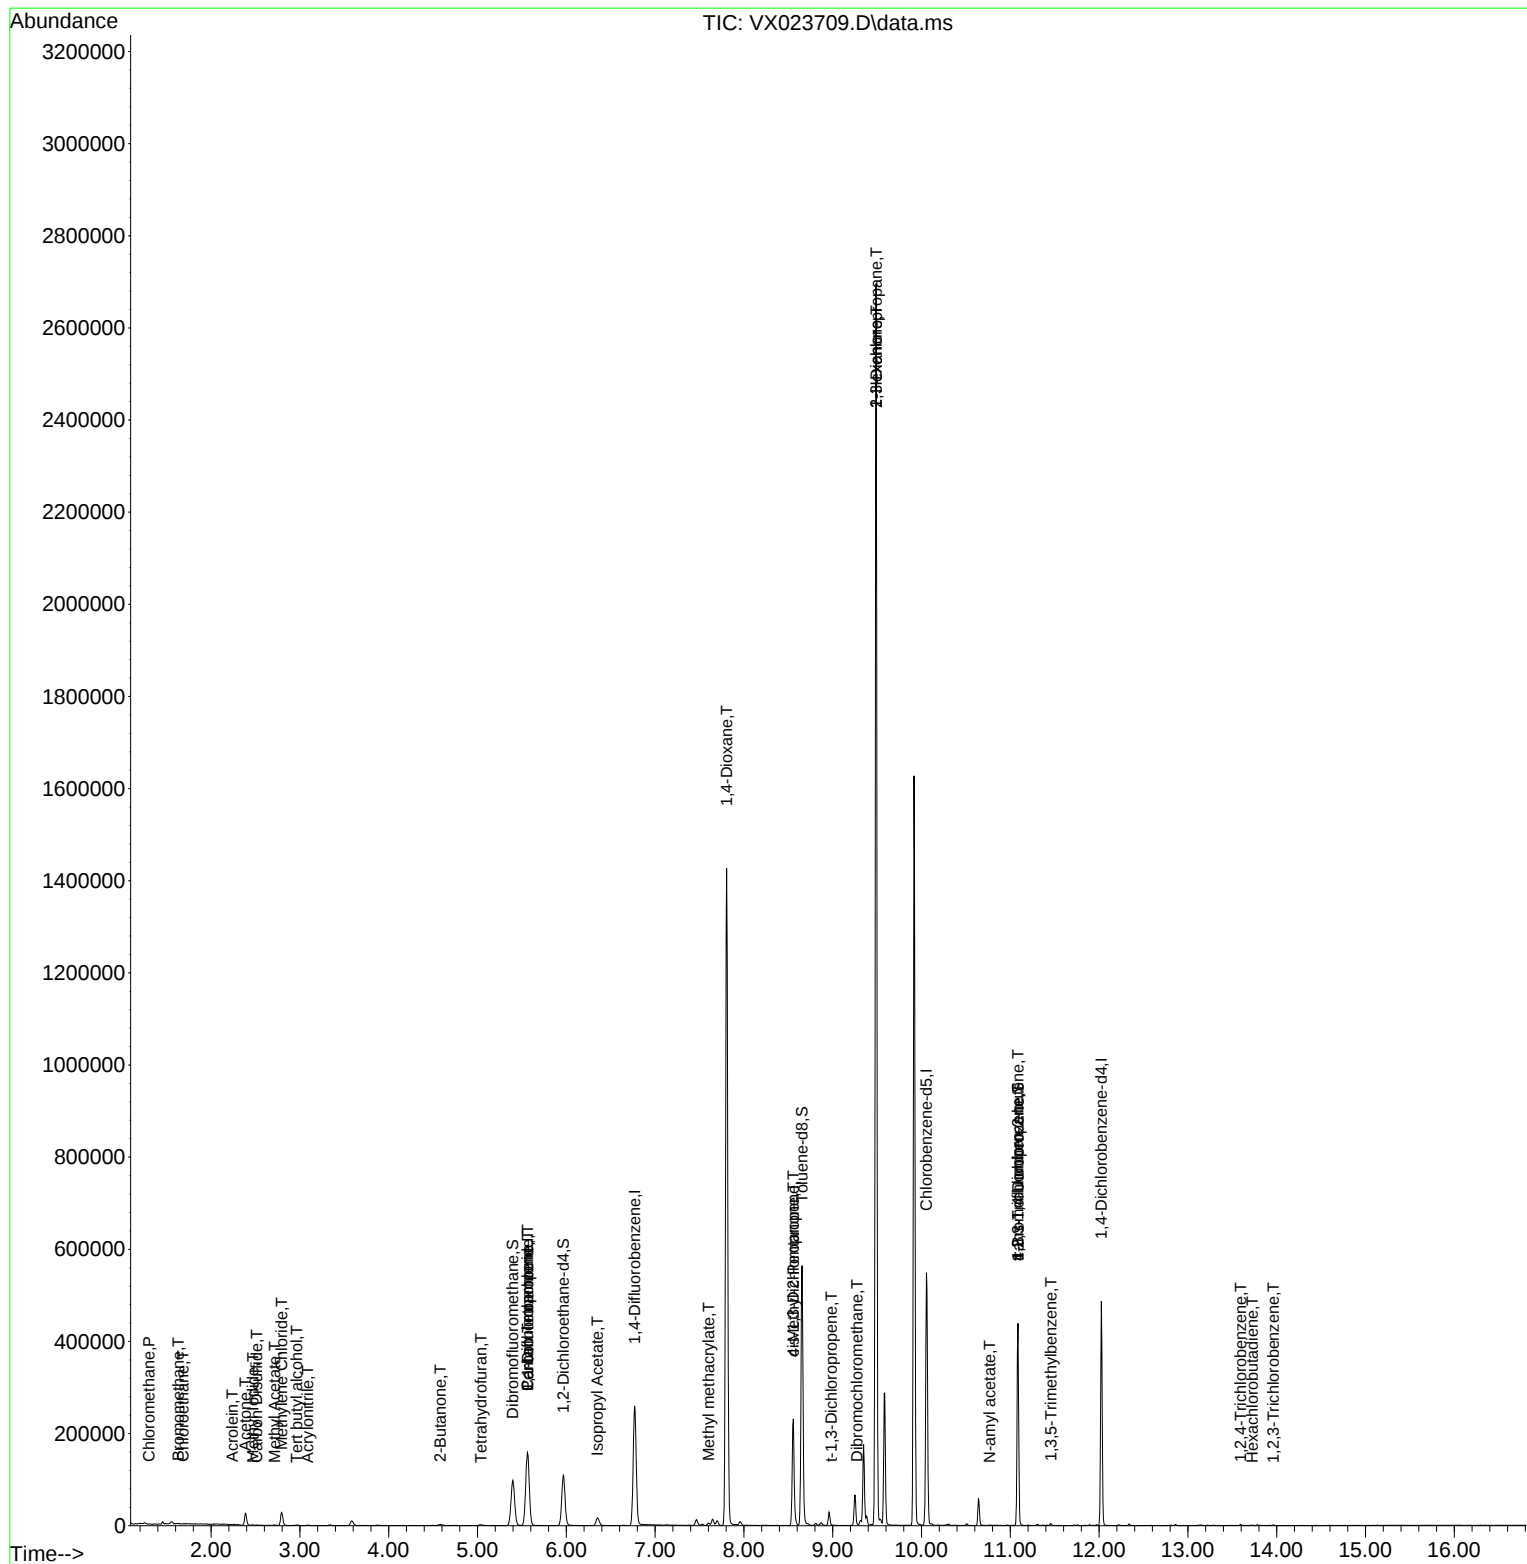




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:168 Resp: 148981
Ion Ratio Lower Upper
168 100
99 62.1 45.8 68.6

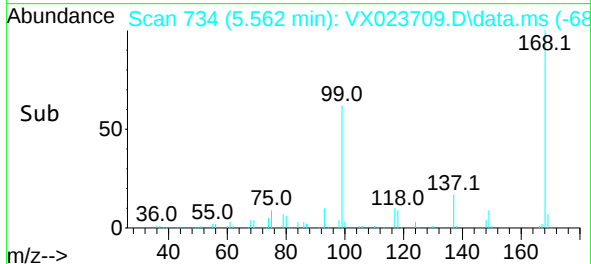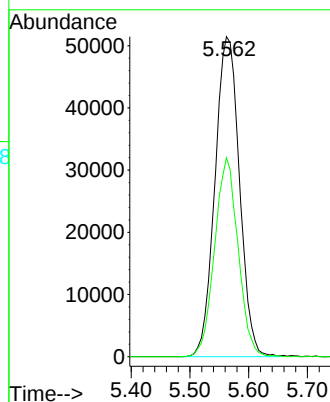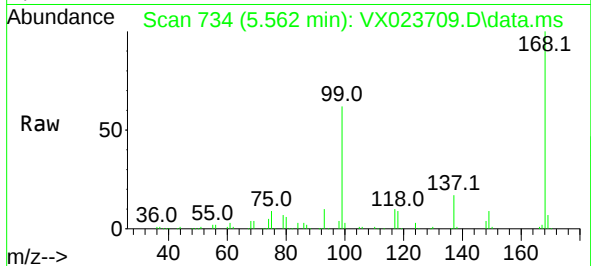

#3
Chloromethane
Concen: 0.244 ug/l
RT: 1.301 min Scan# 35
Delta R.T. 0.007 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Tgt Ion: 50 Resp: 390
Ion Ratio Lower Upper
50 100
52 33.7 26.4 39.6


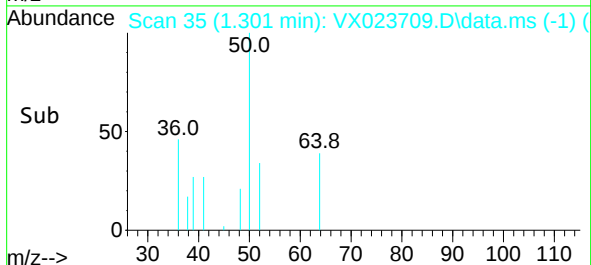
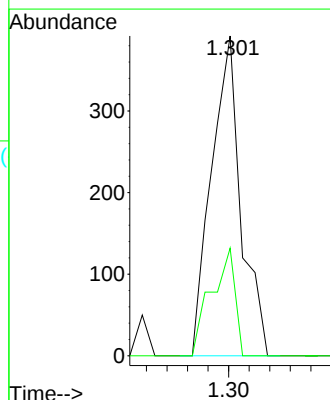
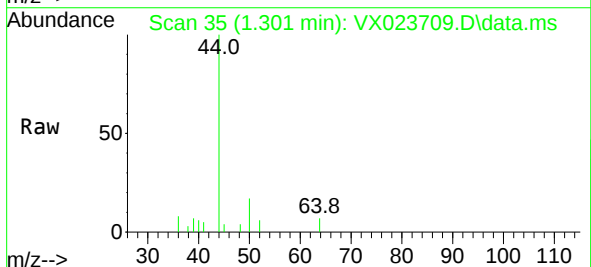


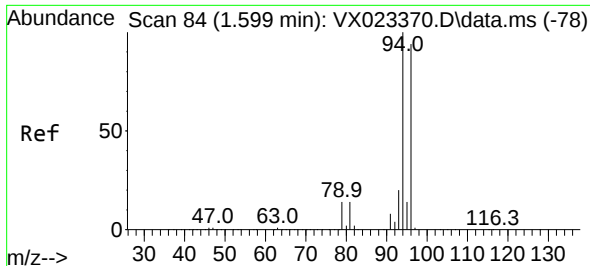

#5
Bromomethane
Concen: 0.634 ug/l
RT: 1.630 min Scan# 89
Delta R.T. 0.031 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 94 Resp: 608
Ion Ratio Lower Upper
94 100
96 77.8 76.4 114.6

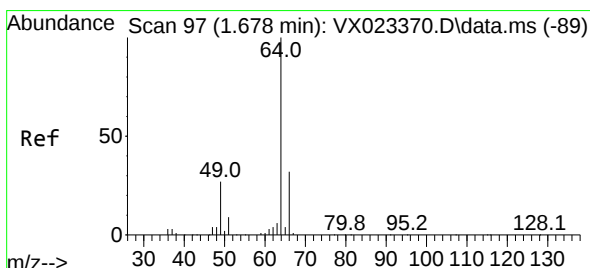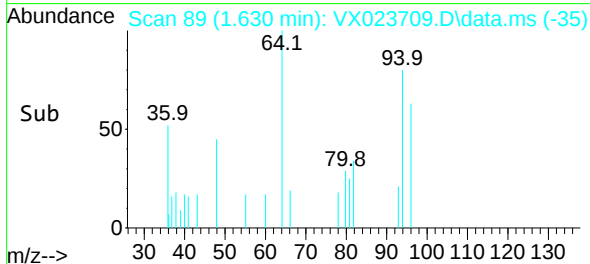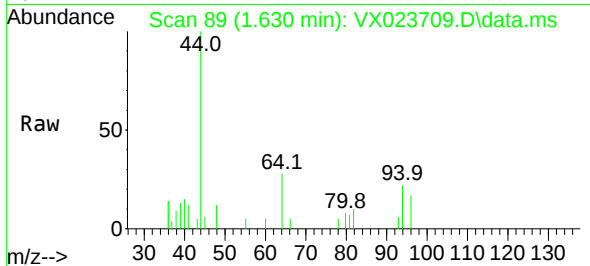

#6
Chloroethane
Concen: 0.287 ug/l
RT: 1.685 min Scan# 98
Delta R.T. 0.007 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41


Tgt Ion: 64 Resp: 285
Ion Ratio Lower Upper
64 100
66 39.3 25.4 38.0#

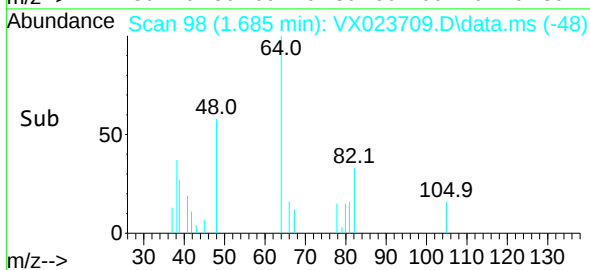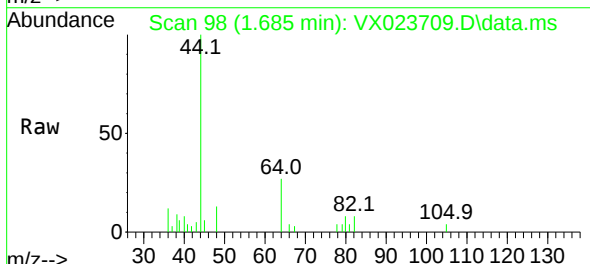



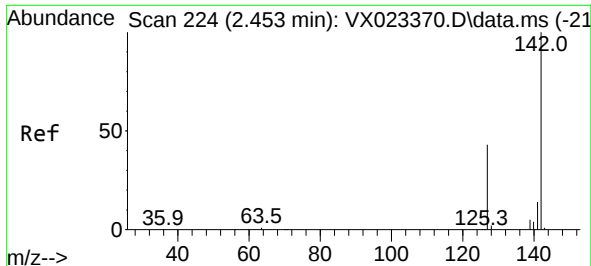


#10
Methyl Iodide
Concen: 0.864 ug/l
RT: 2.471 min Scan# 227
Delta R.T. 0.018 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Instrument :
MSVOA_X
ClientSampled :







Tgt Ion:142 Resp: 1596
Ion Ratio Lower Upper
142 100
127 39.8 33.3 49.9
141 8.9 11.4 17.0#

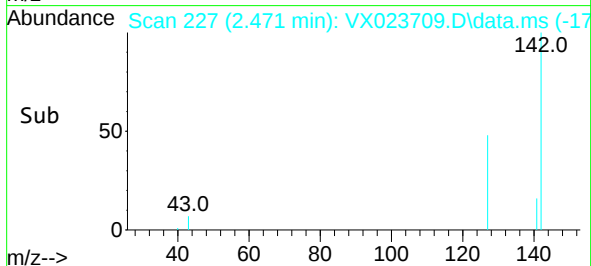

#11
Tert butyl alcohol
Concen: 2.732 ug/l
RT: 2.965 min Scan# 308
Delta R.T. -0.018 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41


Tgt Ion: 59 Resp: 1160
Ion Ratio Lower Upper
59 100
57 1.8 7.8 11.8#

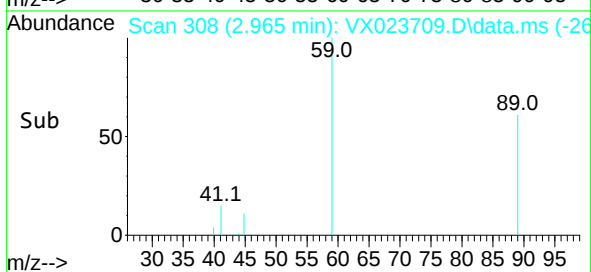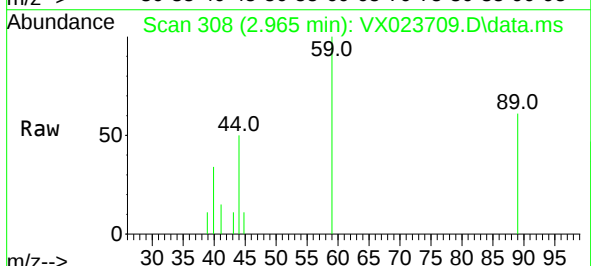






#13
Acrolein
Concen: 1.848 ug/l
RT: 2.240 min Scan# 189
Delta R.T. 0.001 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41


Instrument :
MSVOA_X
ClientSampled :

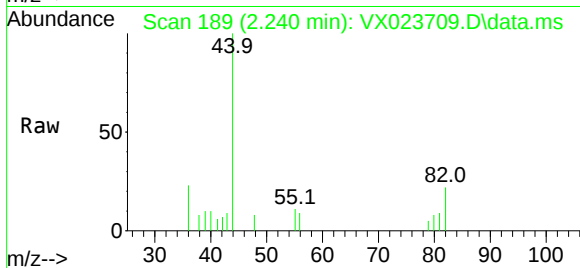



Tgt Ion: 56 Resp: 105
Ion Ratio Lower Upper
56 100
55 304.8 56.4 84.6#




#15
Acrylonitrile
Concen: 0.355 ug/l
RT: 3.087 min Scan# 328
Delta R.T. 0.012 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

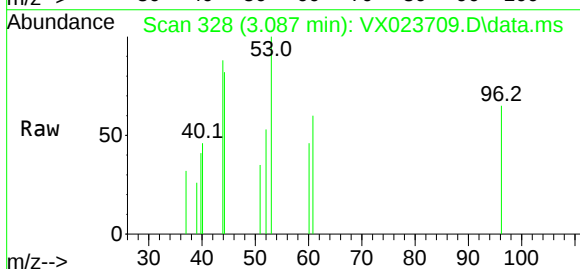

Tgt Ion: 53 Resp: 340
Ion Ratio Lower Upper
53 100
52 56.5 65.3 97.9#
51 0.0 28.2 42.2#



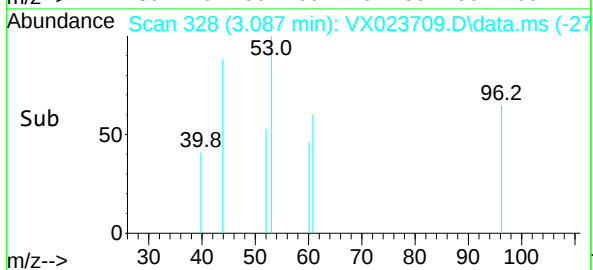





#16
Acetone
Concen: 31.351 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 28580
Ion Ratio Lower Upper
43 100
58 29.1 27.8 41.8

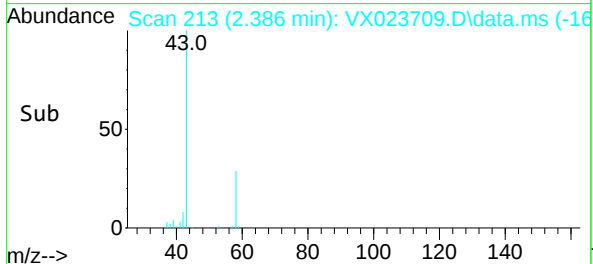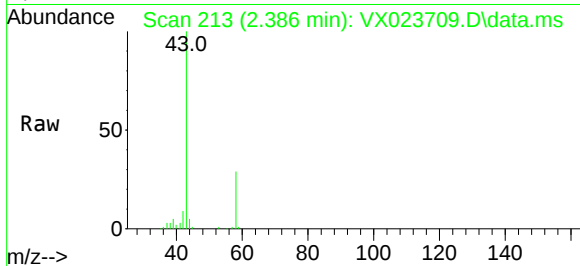

#17
Carbon Disulfide
Concen: 0.329 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Tgt Ion: 76 Resp: 1189
Ion Ratio Lower Upper
76 100
78 11.7 7.2 10.8#


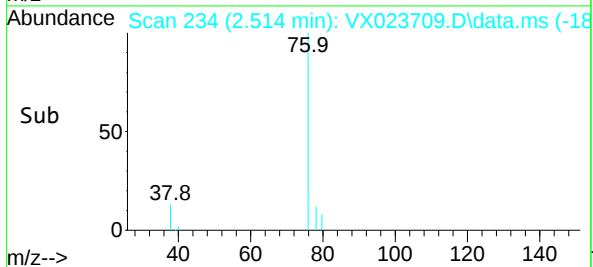

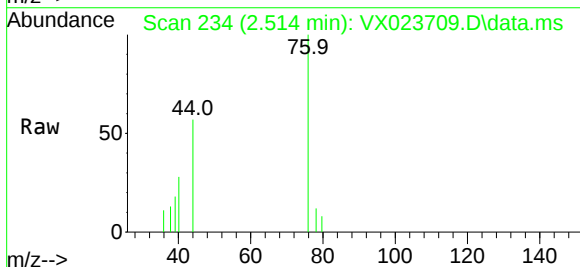


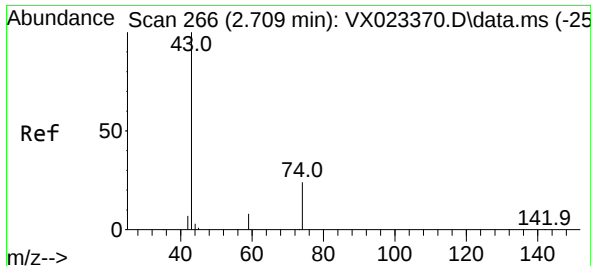

#18
Methyl Acetate
Concen: 0.738 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 1599
Ion Ratio Lower Upper
43 100
74 21.1 21.9 32.9#

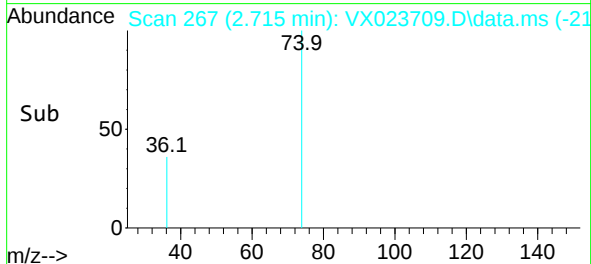

#20
Methylene Chloride
Concen: 7.098 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Tgt Ion: 84 Resp: 12587
Ion Ratio Lower Upper
84 100
49 124.7 88.6 132.8
51 37.9 27.0 40.6
86 64.6 50.3 75.5


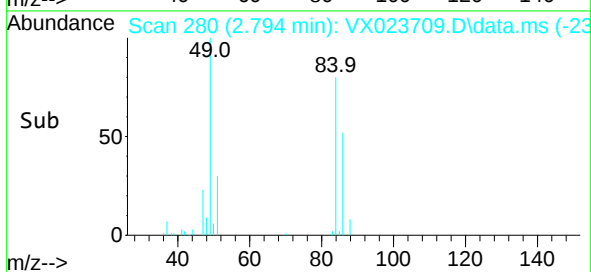

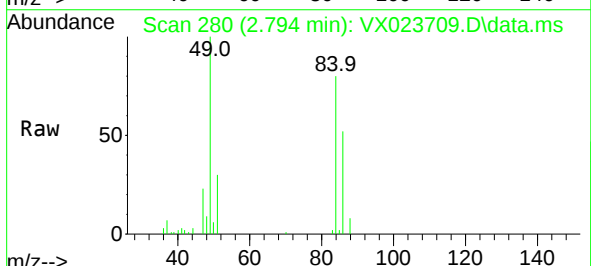




#25
2-Butanone
Concen: 3.126 ug/l
RT: 4.581 min Scan# 573
Delta R.T. 0.013 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 4424
Ion Ratio Lower Upper
43 100
72 21.4 23.7 35.5#

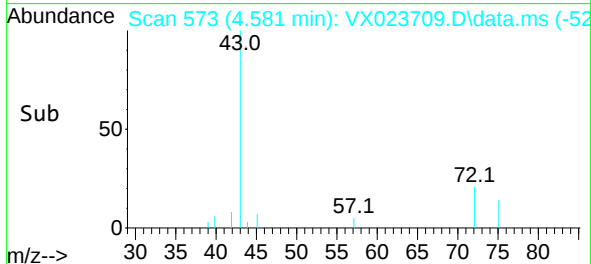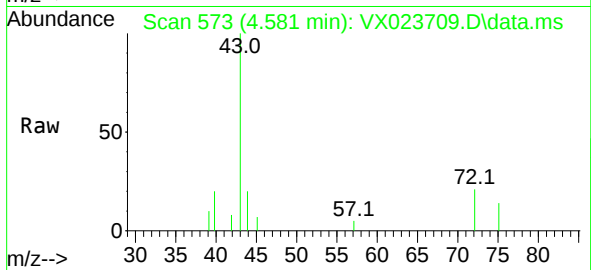

#29
Tetrahydrofuran
Concen: 1.796 ug/l
RT: 5.038 min Scan# 648
Delta R.T. 0.025 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Tgt Ion: 42 Resp: 1666
Ion Ratio Lower Upper
42 100
72 42.1 41.7 62.5
71 34.1 38.4 57.6#

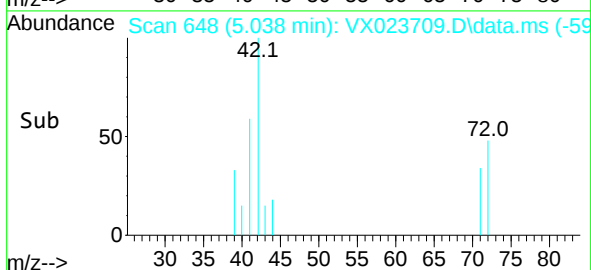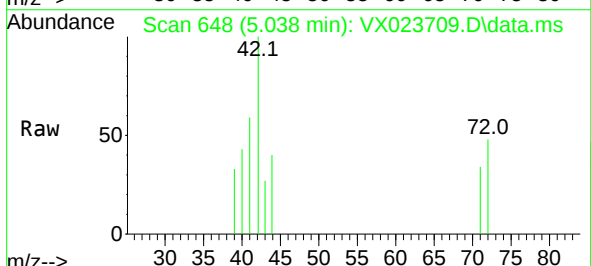







#33

1,2-Dichloroethane-d4
Concen: 56.967 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Instrument :
MSVOA_X
ClientSampled :




Tgt Ion: 65 Resp: 105867
Ion Ratio Lower Upper
65 100
67 51.5 0.0 105.4

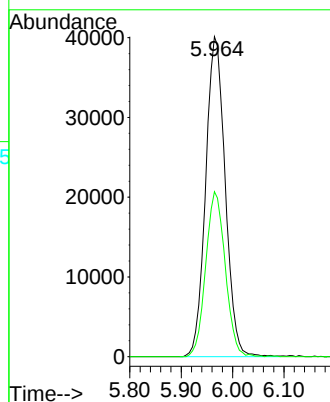


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Tgt Ion: 114 Resp: 259408
Ion Ratio Lower Upper
114 100
63 21.1 0.0 40.8
88 15.7 0.0 32.8


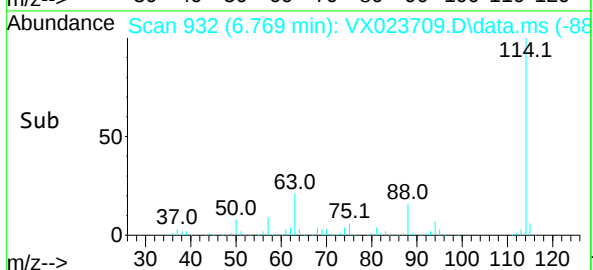
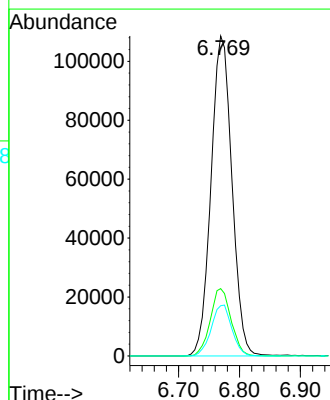





#35
Dibromofluoromethane
Concen: 51.162 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:113 Resp: 82981
Ion Ratio Lower Upper
113 100
111 102.5 81.9 122.9
192 19.7 16.7 25.1

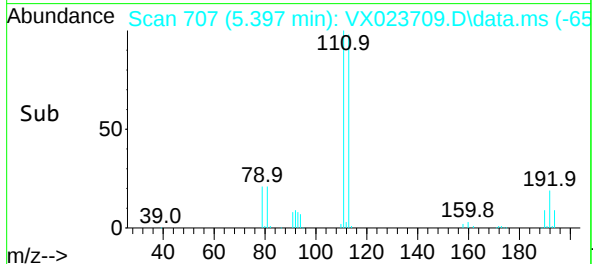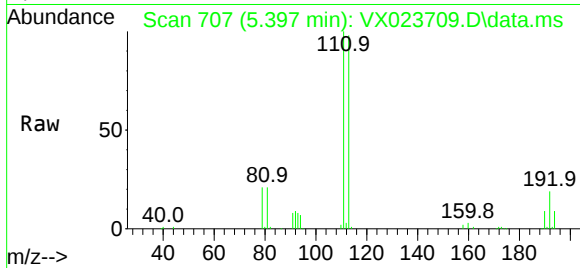

#36
1,1-Dichloropropene
Concen: 5.130 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.134 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41


Tgt Ion: 75 Resp: 12039
Ion Ratio Lower Upper
75 100
110 10.3 18.1 54.4#
77 0.0 25.3 37.9#

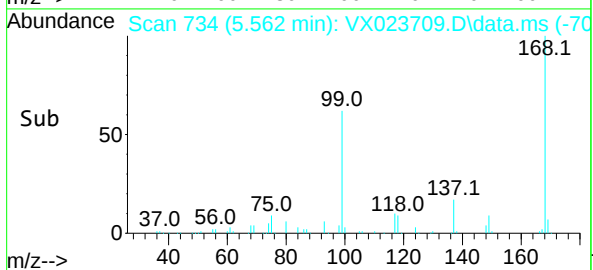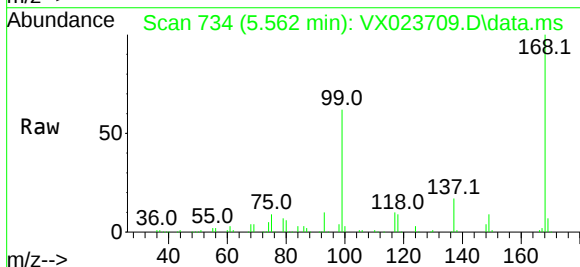






#38
Carbon Tetrachloride
Concen: 6.333 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.122 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41


Instrument :
MSVOA_X
ClientSampled :





Tgt Ion:117 Resp: 15113
Ion Ratio Lower Upper
117 100
119 3.3 76.2 114.2#
121 0.0 24.8 37.2#




#43
Isopropyl Acetate
Concen: 5.052 ug/l
RT: 6.349 min Scan# 863
Delta R.T. 0.001 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

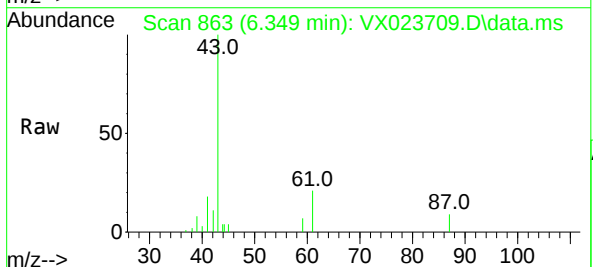


Tgt Ion: 43 Resp: 23162
Ion Ratio Lower Upper
43 100
61 17.7 18.2 27.4#
87 12.1 12.5 18.7#








#48
Methyl methacrylate
Concen: 2.830 ug/l
RT: 7.604 min Scan# 1069
Delta R.T. -0.098 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Instrument :
MSVOA_X
ClientSampled :



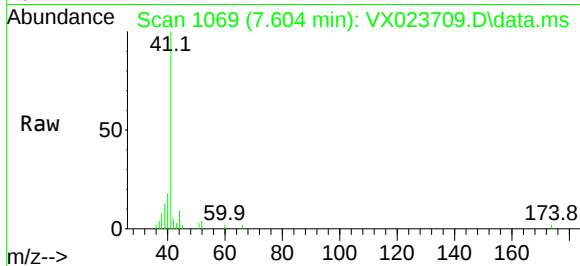



Tgt Ion: 41 Resp: 6010
Ion Ratio Lower Upper
41 100
69 0.0 76.0 114.0#
39 0.0 44.6 67.0#

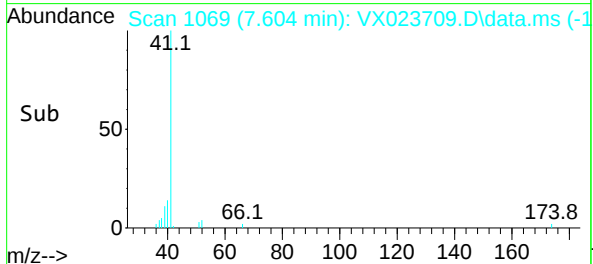

#49
1,4-Dioxane
Concen: 3.760 ug/l
RT: 7.806 min Scan# 1102
Delta R.T. 0.141 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Tgt Ion: 88 Resp: 170
Ion Ratio Lower Upper
88 100
43 765932.4 23.2 34.8#
58 3401.8 55.0 82.4#

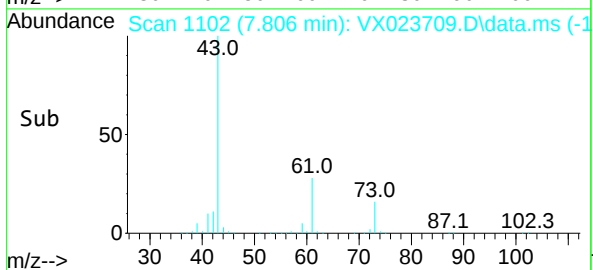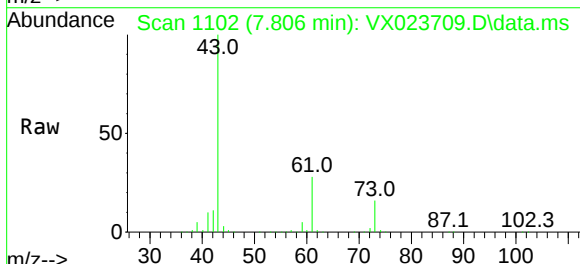



#50

Toluene-d8

Concen: 54.180 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.000 min

Lab File: VX023709.D





Acq: 13 Aug 2021 23:41

Tgt Ion: 98 Resp: 322861

Ion Ratio Lower Upper

98 100

100 64.2 51.9 77.9

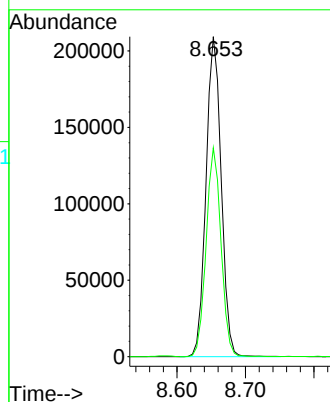

#51

4-Methyl-2-Pentanone

Concen: 29.207 ug/l

RT: 8.555 min Scan# 1225

Delta R.T. -0.025 min

Lab File: VX023709.D




Acq: 13 Aug 2021 23:41


Tgt Ion: 43 Resp: 81904

Ion Ratio Lower Upper

43 100

58 8.9 35.4 53.0#


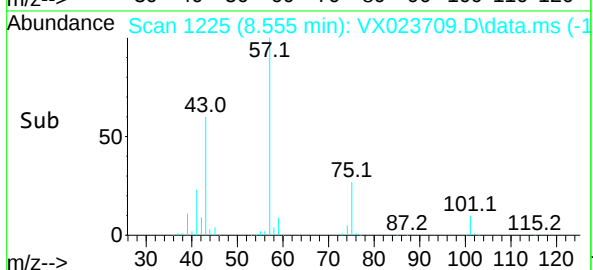
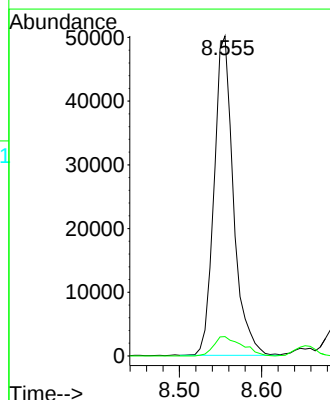





#53
t-1,3-Dichloropropene
Concen: 1.891 ug/l
RT: 8.982 min Scan# 1295
Delta R.T. 0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 75 Resp: 221
Ion Ratio Lower Upper
75 100
77 0.0 24.9 37.3#

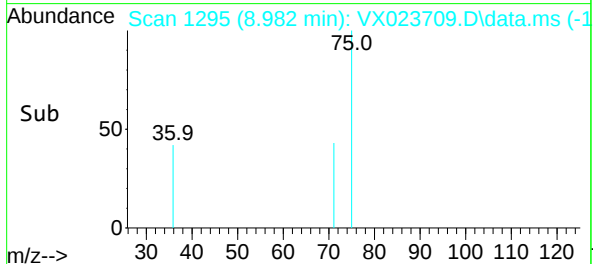

#54
cis-1,3-Dichloropropene
Concen: 12.155 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. 0.183 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Tgt Ion: 75 Resp: 34093
Ion Ratio Lower Upper
75 100
77 0.8 25.7 38.5#
39 38.5 35.1 52.7


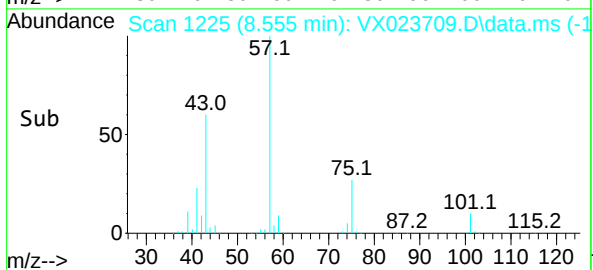

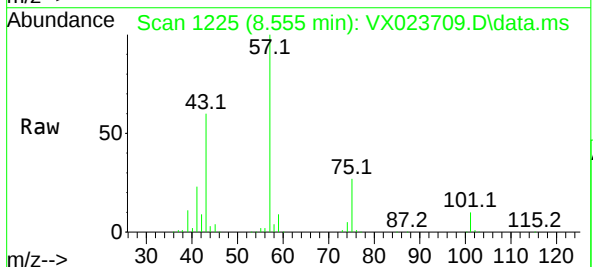




#57
1,3-Dichloropropane
Concen: 7.385 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.177 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 76 Resp: 21903
Ion Ratio Lower Upper
76 100
78 0.5 26.2 39.2#

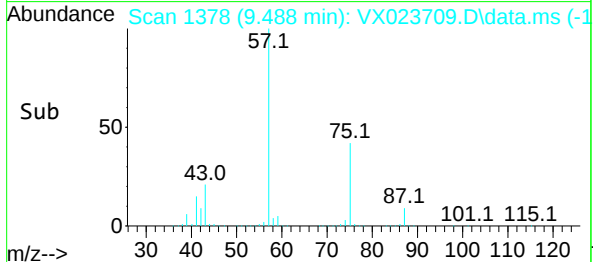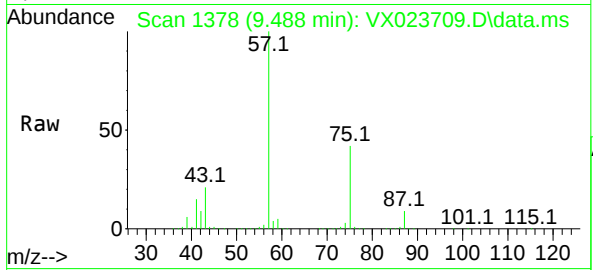

#59
2-Hexanone
Concen: 150.470 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.055 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Tgt Ion: 43 Resp: 320420
Ion Ratio Lower Upper
43 100
58 18.0 30.9 92.8#


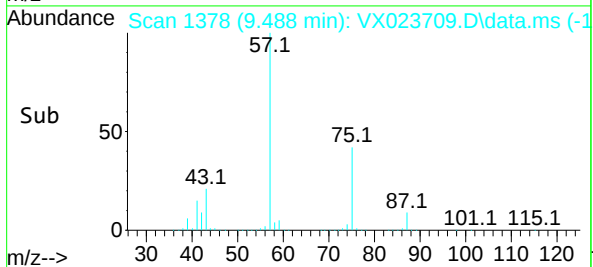

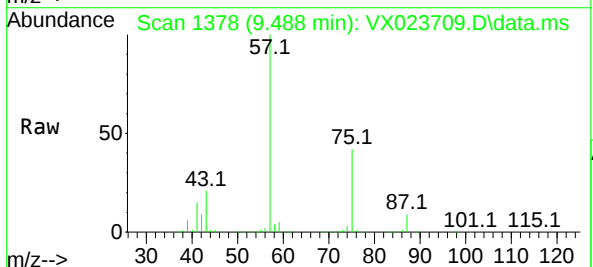




#60
Dibromochloromethane
Concen: 2.082 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.250 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:129 Resp: 199
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#

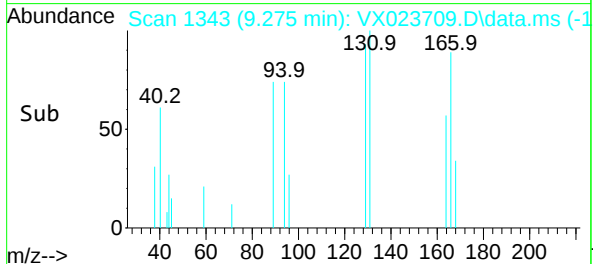

#62
4-Bromofluorobenzene
Concen: 53.370 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Tgt Ion: 95 Resp: 108145
Ion Ratio Lower Upper
95 100
174 80.6 0.0 154.6
176 78.5 0.0 155.8


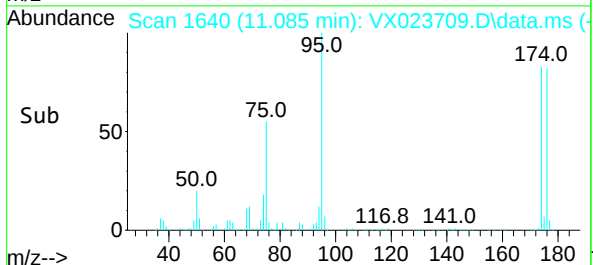

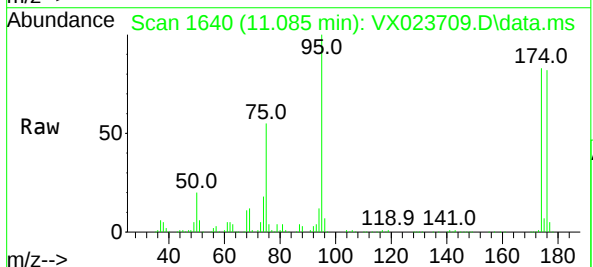


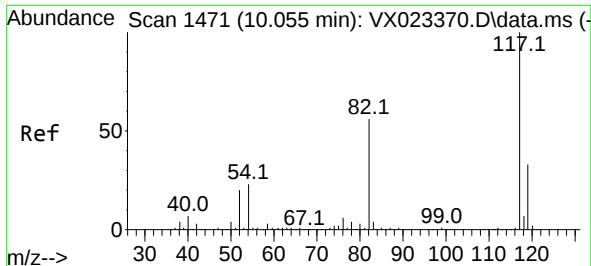

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:117 Resp: 245940
Ion Ratio Lower Upper
117 100
82 58.2 47.4 71.2
119 31.6 26.6 39.8

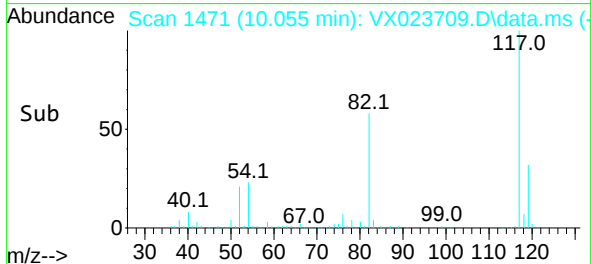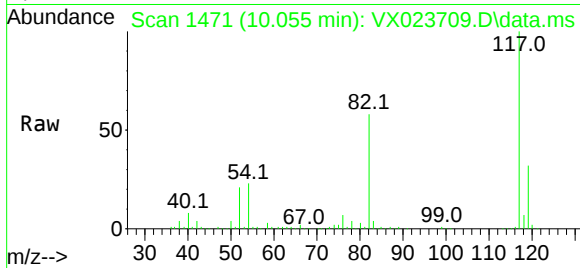

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Tgt Ion:152 Resp: 95525
Ion Ratio Lower Upper
152 100
115 59.0 41.1 123.3
150 156.9 0.0 349.0


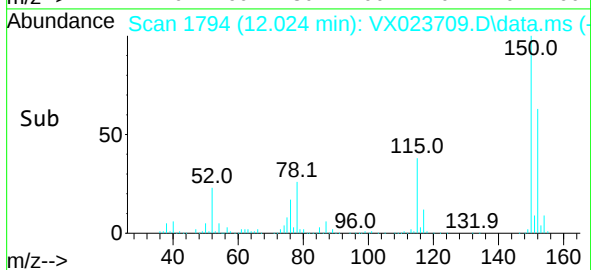

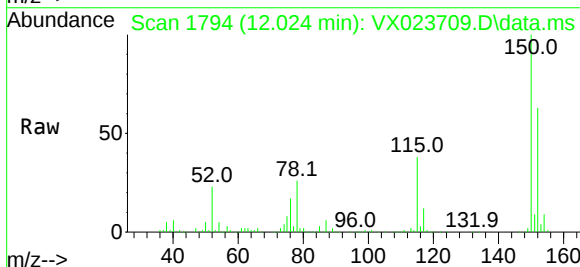




#74
N-amy1 acetate
Concen: 0.289 ug/l
RT: 10.768 min Scan# 1588
Delta R.T. -0.080 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43	Resp: 952
Ion Ratio	Lower Upper
43	100
70	0.0 39.0 58.6#
55	9.1 21.5 32.3#
61	0.0 22.1 33.1#

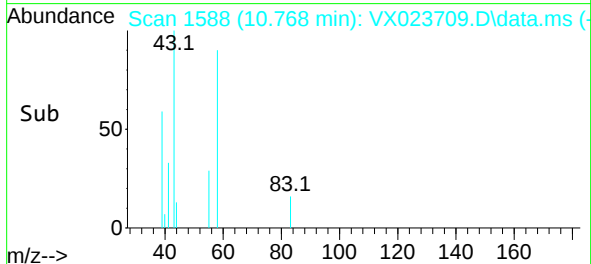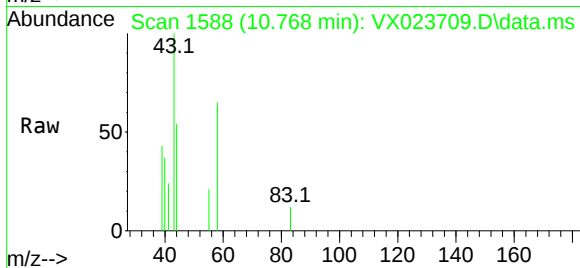

#76
1,2,3-Trichloropropane
Concen: 27.885 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Tgt Ion: 75	Resp: 58617
Ion Ratio	Lower Upper
75	100
77	1.1 19.1 57.5#


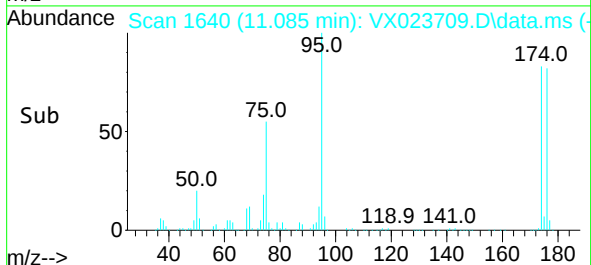

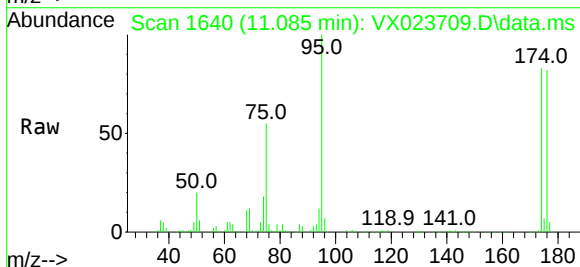




#80
1,3,5-Trimethylbenzene
Concen: 0.224 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:105 Resp: 1316
Ion Ratio Lower Upper
105 100
120 50.1 23.8 71.5

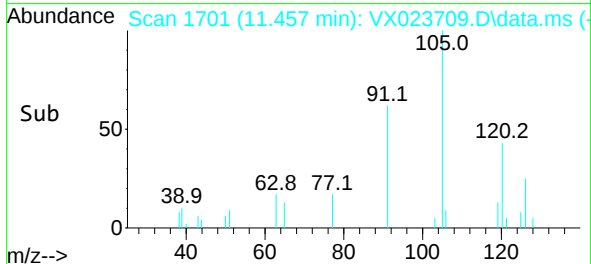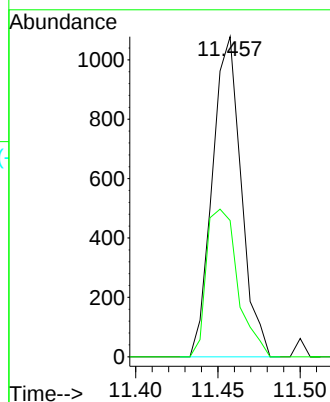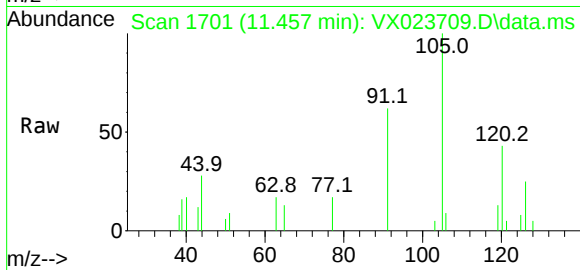

#81
trans-1,4-Dichloro-2-butene
Concen: 74.979 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41

Tgt Ion: 75 Resp: 58617
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.1 37.9 56.9#


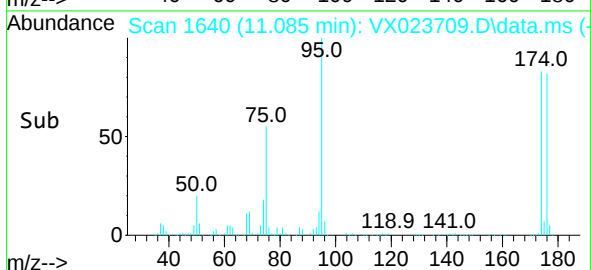
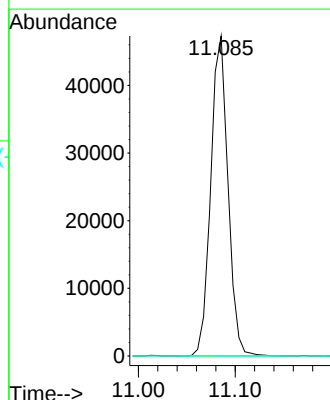
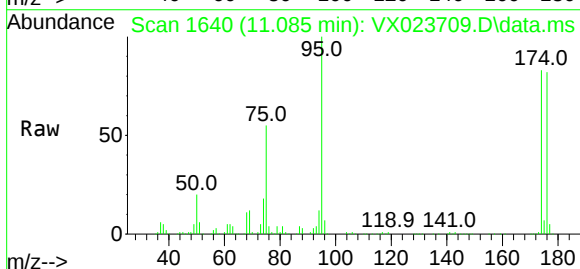


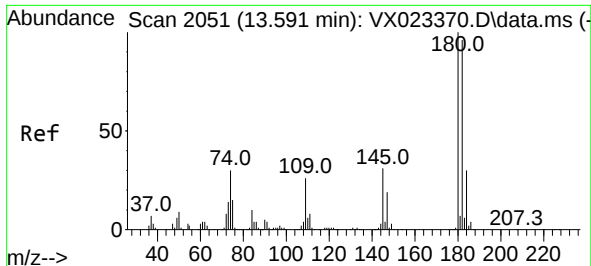

#93
1,2,4-Trichlorobenzene
Concen: 0.270 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.000 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:180 Resp: 528
Ion Ratio Lower Upper
180 100
182 105.9 47.7 143.1
145 45.3 15.0 45.0#

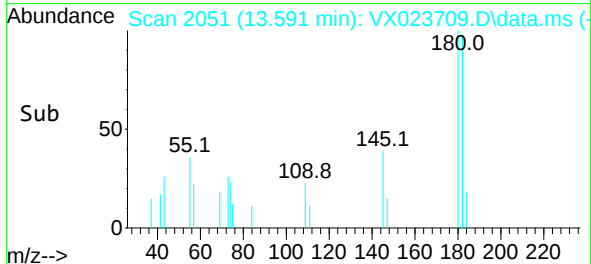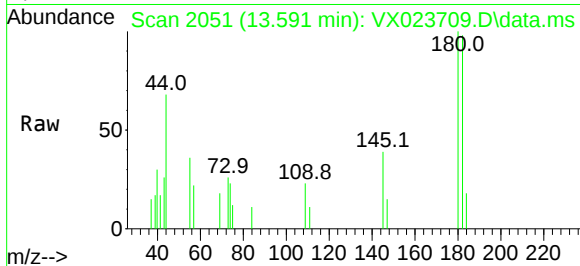

#94
Hexachlorobutadiene
Concen: 0.219 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. -0.006 min
Lab File: VX023709.D
Acq: 13 Aug 2021 23:41


Tgt Ion:225 Resp: 192
Ion Ratio Lower Upper
225 100
223 42.7 31.1 93.2
227 66.7 31.6 95.0

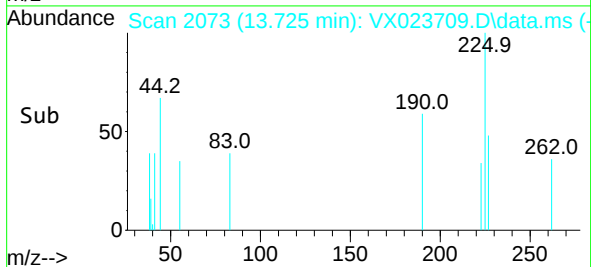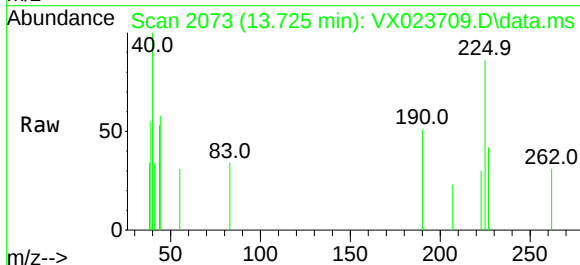

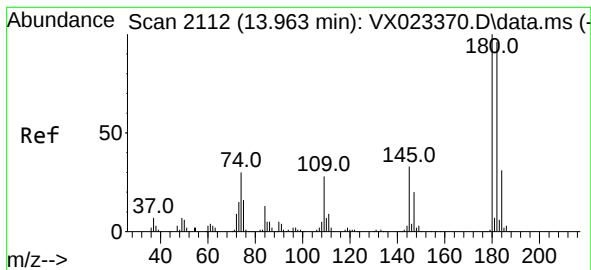

#96
 1,2,3-Trichlorobenzene
 Concen: 0.253 ug/l
 RT: 13.963 min Scan# 2112
 Delta R.T. 0.000 min
 Lab File: VX023709.D
 Acq: 13 Aug 2021 23:41

Instrument :
 MSVOA_X
 ClientSampleId :

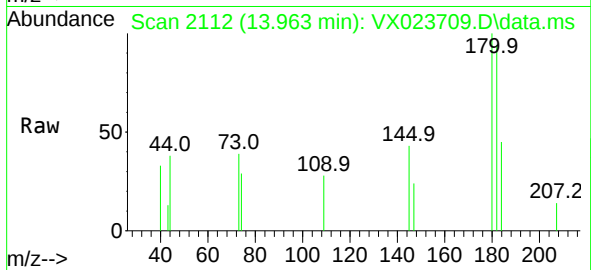

Tgt Ion:	180	Resp:	499
Ion	Ratio	Lower	Upper
180	100		
182	77.6	47.6	142.9
145	29.1	16.1	48.3

