

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081321\
 Data File : VX023712.D
 Acq On : 14 Aug 2021 00:52
 Operator : JC/MD
 Sample : M3394-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SWCS-01-0205

Quant Time: Aug 14 05:34:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 23 06:05:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.568	168	153231	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	263337	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	241797	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	93669	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	108888	56.967	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 113.940%			
35) Dibromofluoromethane	5.397	113	84936	51.586	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 103.180%			
50) Toluene-d8	8.653	98	325750	53.849	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 107.700%			
62) 4-Bromofluorobenzene	11.085	95	106185	51.621	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 103.240%			
Target Compounds					Qvalue	
16) Acetone	2.386	43	28851	30.770	ug/l	91
20) Methylene Chloride	2.794	84	14340	7.863	ug/l	94
43) Isopropyl Acetate	6.348	43	22058	4.739	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081321\
Data File : VX023712.D
Acq On : 14 Aug 2021 00:52
Operator : JC/MD
Sample : M3394-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SWCS-01-0205

Quant Time: Aug 14 05:34:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 23 06:05:38 2021
Response via : Initial Calibration




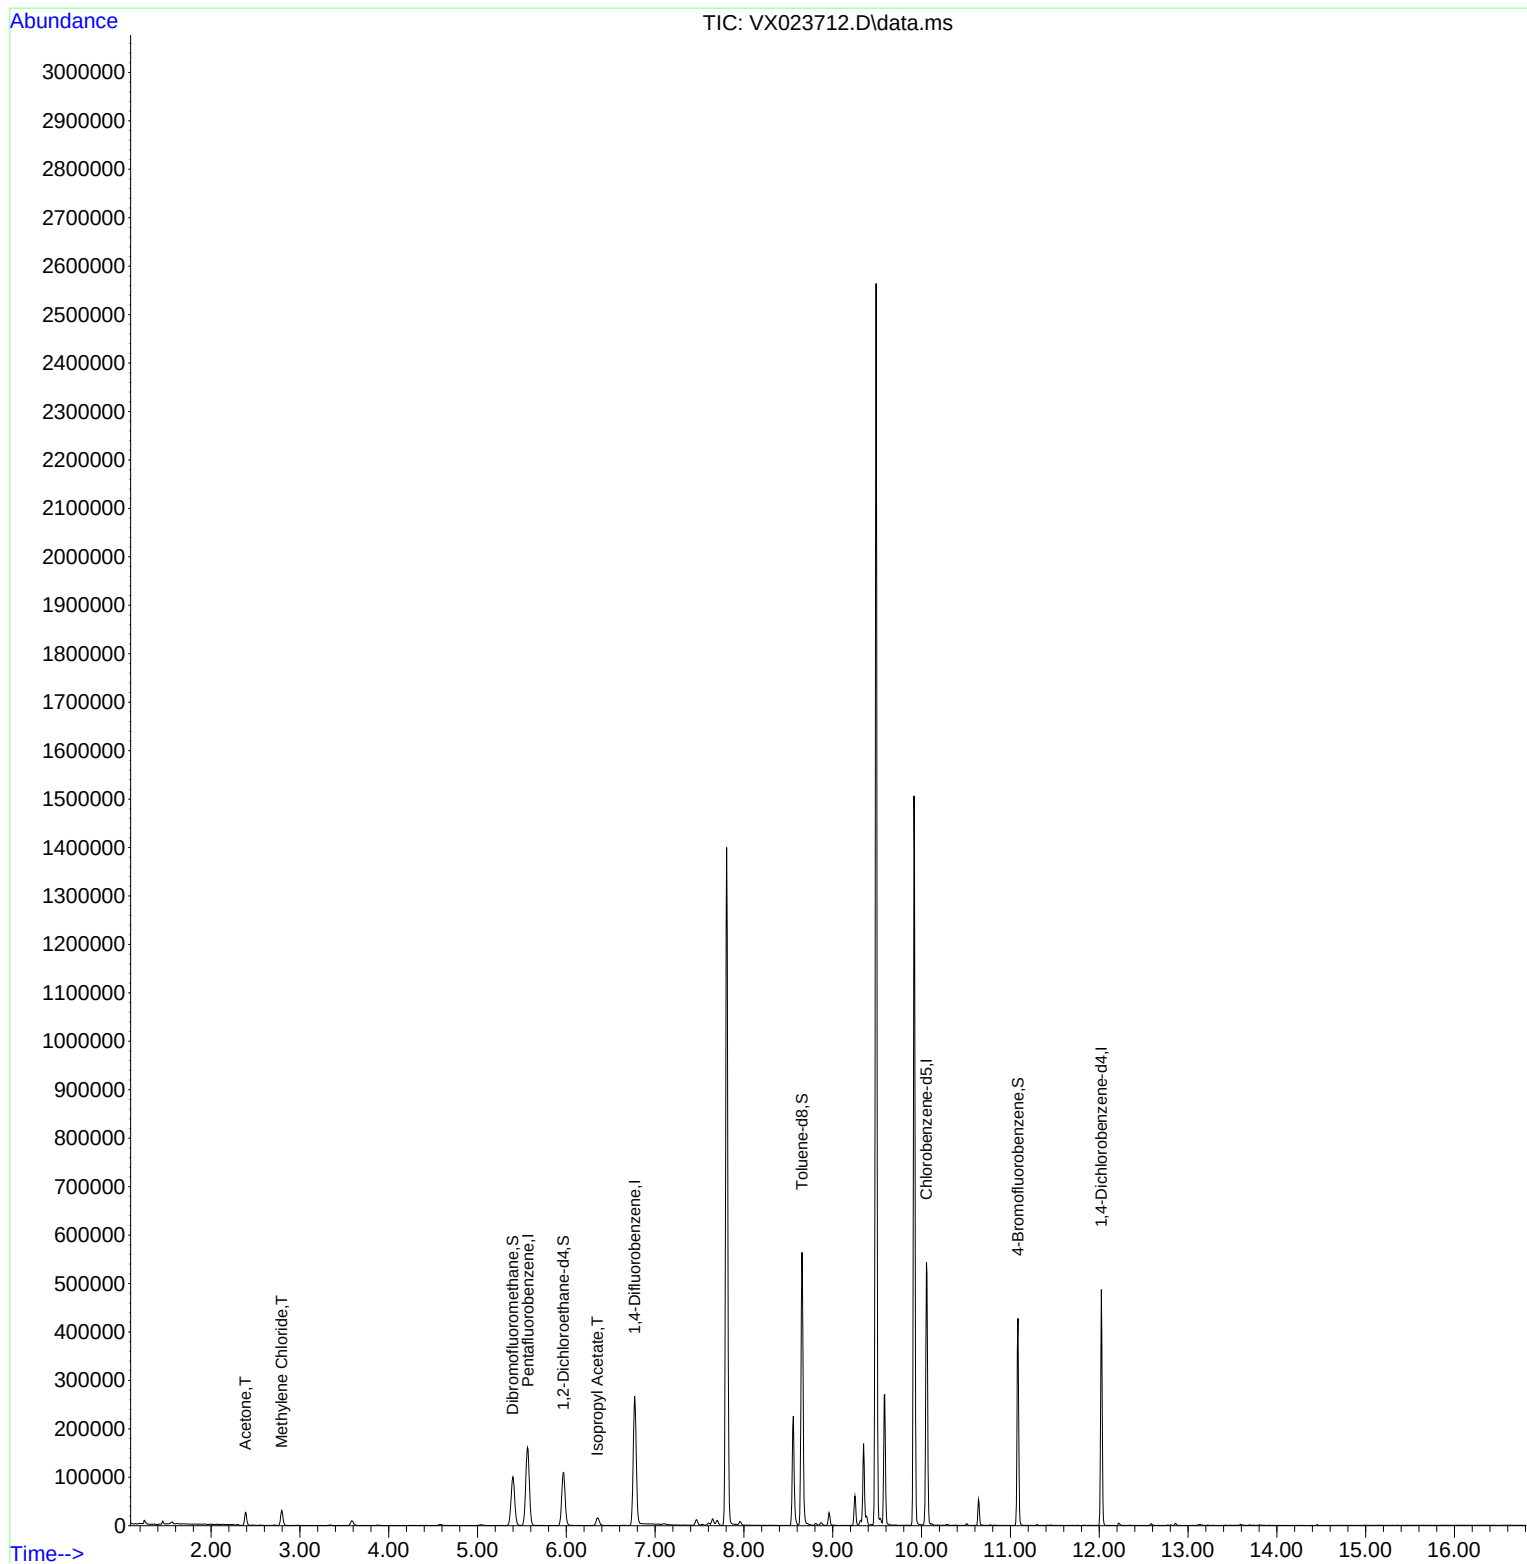


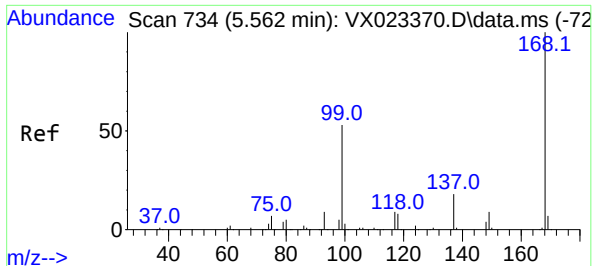

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.568 min Scan# 735
Delta R.T. 0.006 min
Lab File: VX023712.D
Acq: 14 Aug 2021 00:52




Instrument :
MSVOA_X
ClientSampleId :
SWCS-01-0205


Tgt Ion:168 Resp: 153231
Ion Ratio Lower Upper
168 100
99 56.4 45.8 68.6

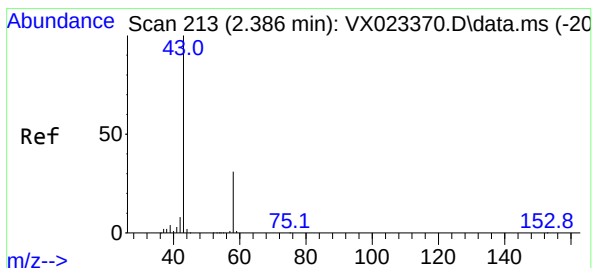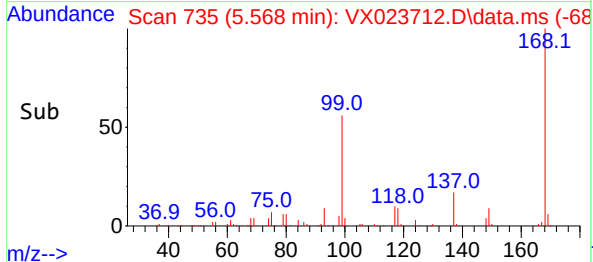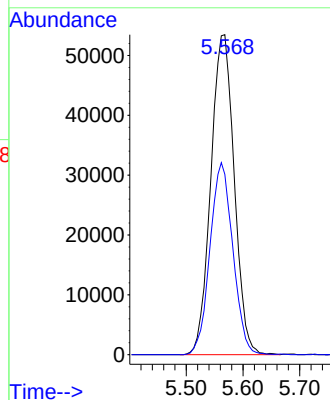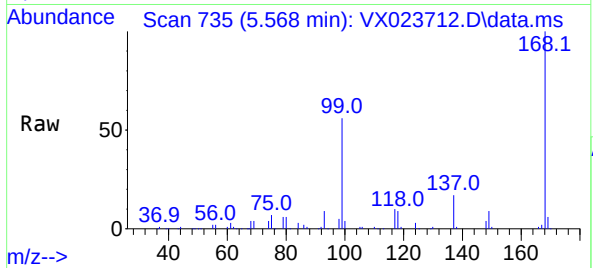

#16
Acetone
Concen: 30.770 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX023712.D
Acq: 14 Aug 2021 00:52

Tgt Ion: 43 Resp: 28851
Ion Ratio Lower Upper
43 100
58 29.3 27.8 41.8

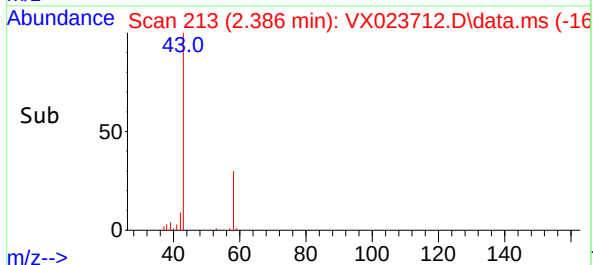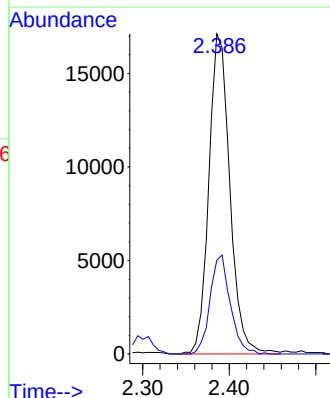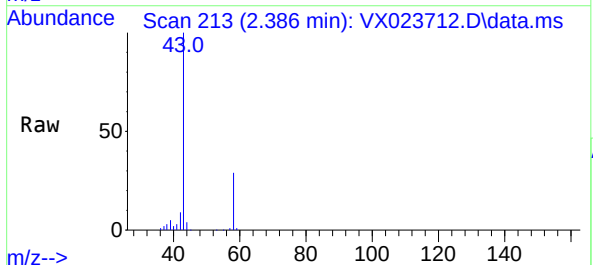




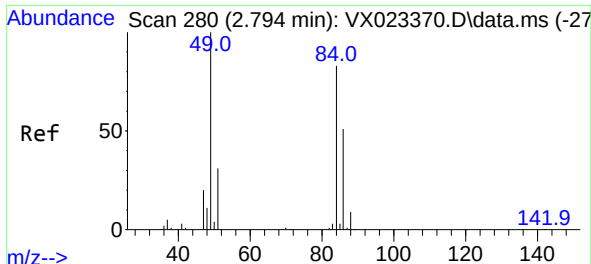


#20
Methylene Chloride
Concen: 7.863 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX023712.D
Acq: 14 Aug 2021 00:52

Instrument :
MSVOA_X
ClientSampleId :
SWCS-01-0205

Tgt Ion: 84 Resp: 14340




Ion	Ratio	Lower	Upper
84	100		
49	117.0	88.6	132.8
51	40.1	27.0	40.6
86	65.1	50.3	75.5

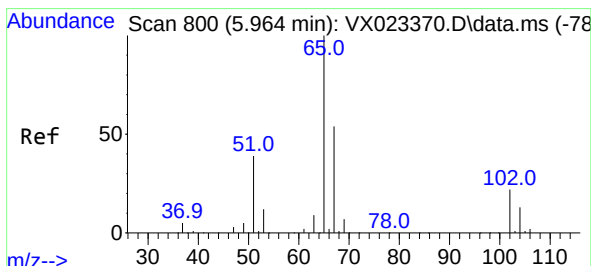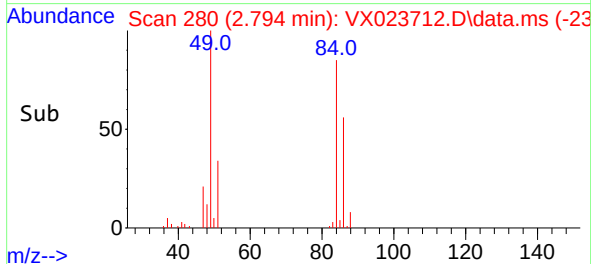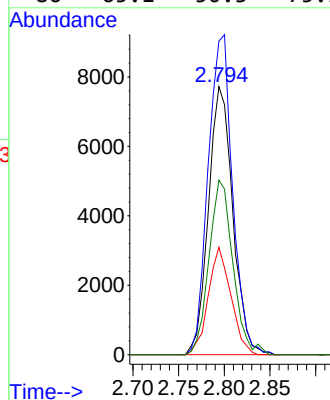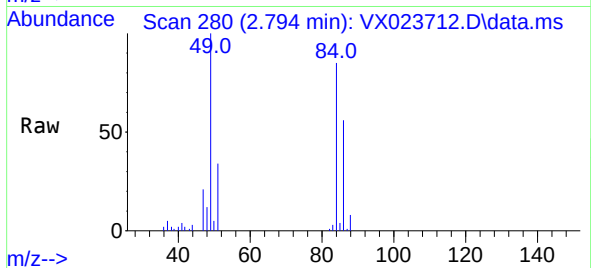


#33
1,2-Dichloroethane-d4
Concen: 56.967 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023712.D
Acq: 14 Aug 2021 00:52

Tgt Ion: 65 Resp: 108888

Ion	Ratio	Lower	Upper
65	100		
67	50.9	0.0	105.4


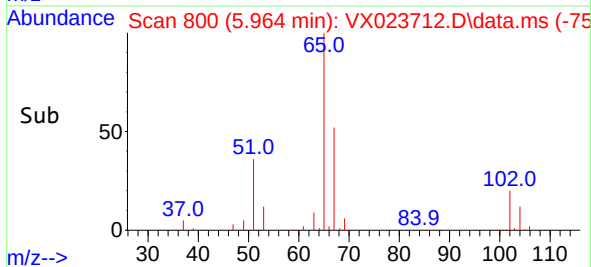
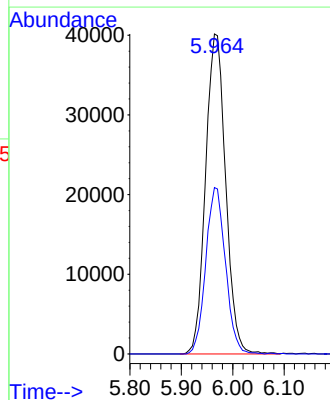
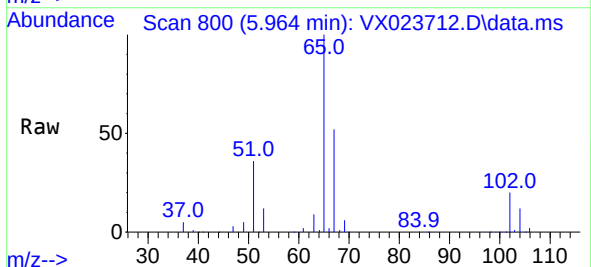


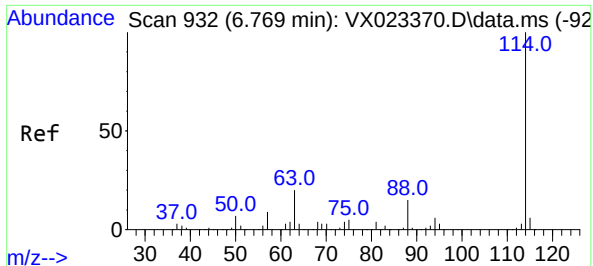

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX023712.D
Acq: 14 Aug 2021 00:52




Instrument :
MSVOA_X
ClientSampleId :
SWCS-01-0205


Tgt Ion:114 Resp: 263337
Ion Ratio Lower Upper
114 100
63 20.5 0.0 40.8
88 15.4 0.0 32.8

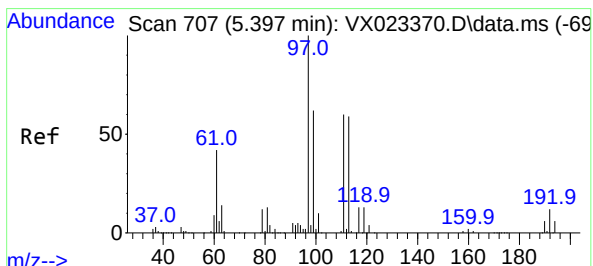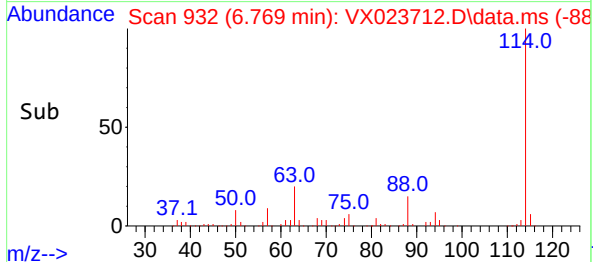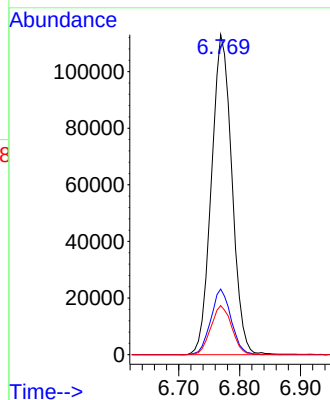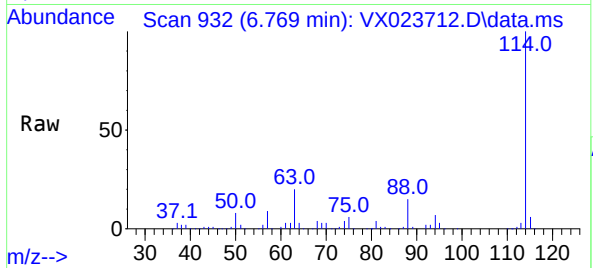

#35
Dibromofluoromethane
Concen: 51.586 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX023712.D
Acq: 14 Aug 2021 00:52

Tgt Ion:113 Resp: 84936
Ion Ratio Lower Upper
113 100
111 103.4 81.9 122.9
192 19.4 16.7 25.1


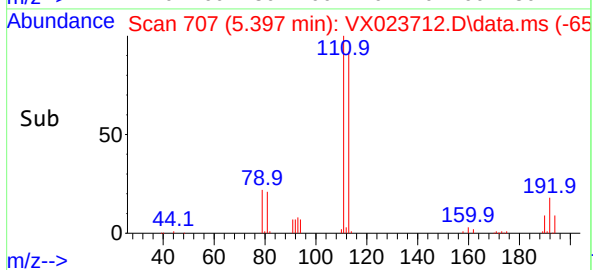
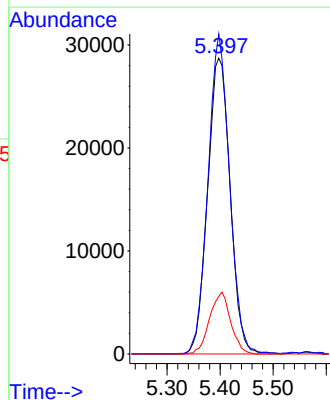
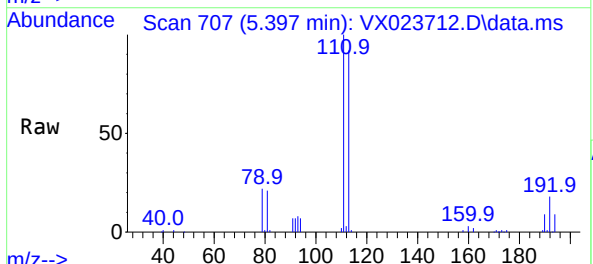


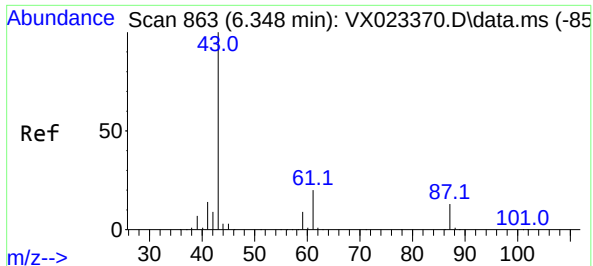

#43
Isopropyl Acetate
Concen: 4.739 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.000 min
Lab File: VX023712.D
Acq: 14 Aug 2021 00:52




Instrument :
MSVOA_X
ClientSampleId :
SWCS-01-0205


Tgt Ion:	43	Resp:	22058
Ion	Ratio	Lower	Upper
43	100		
61	19.6	18.2	27.4
87	12.5	12.5	18.7

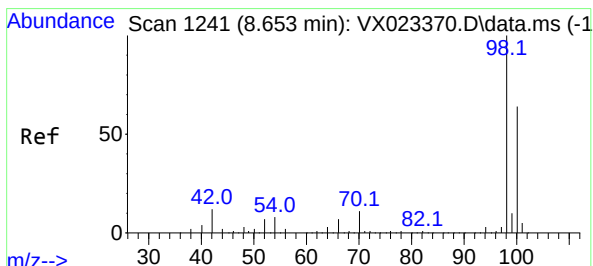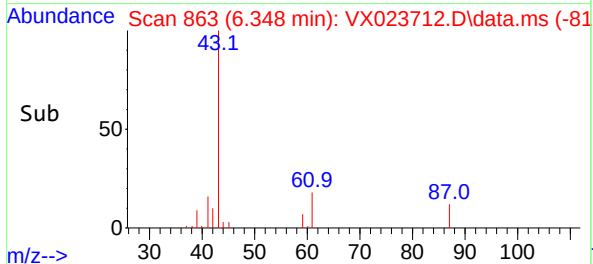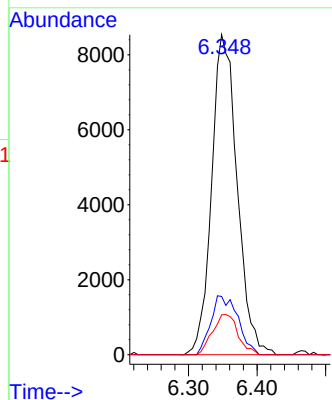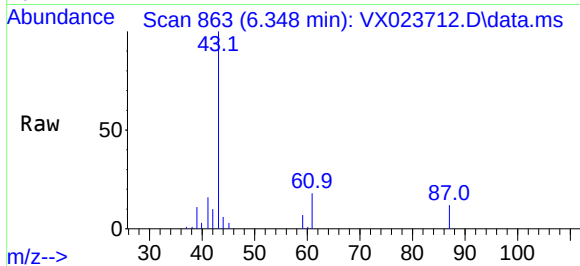

#50
Toluene-d8
Concen: 53.849 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023712.D
Acq: 14 Aug 2021 00:52

Tgt Ion:	98	Resp:	325750
Ion	Ratio	Lower	Upper
98	100		
100	64.4	51.9	77.9


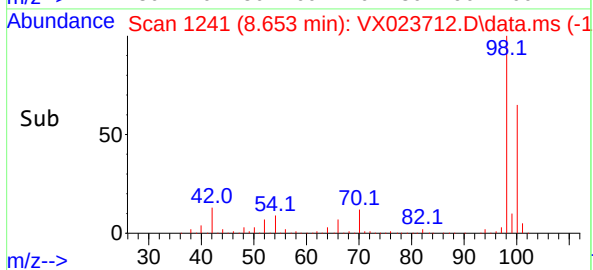
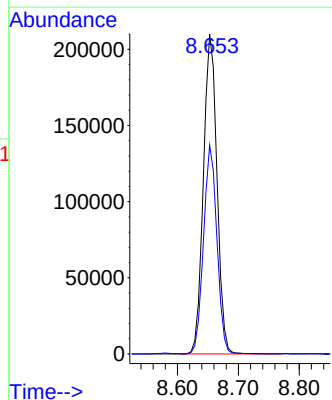
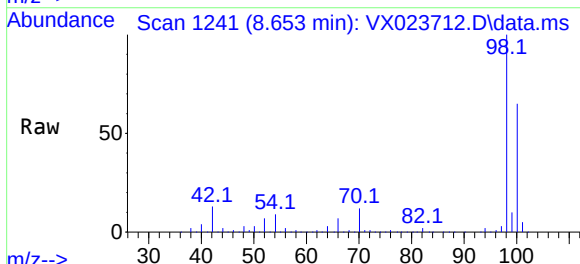


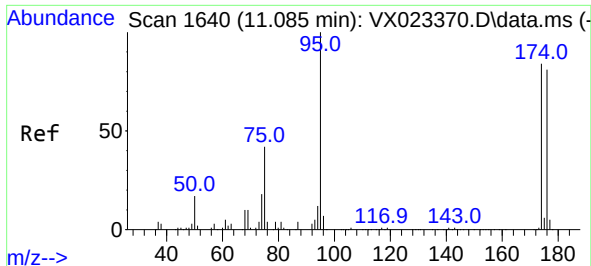

#62
4-Bromofluorobenzene
Concen: 51.621 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023712.D
Acq: 14 Aug 2021 00:52




Instrument :
MSVOA_X
ClientSampleId :
SWCS-01-0205


Tgt Ion: 95 Resp: 106185
Ion Ratio Lower Upper
95 100
174 80.9 0.0 154.6
176 75.9 0.0 155.8

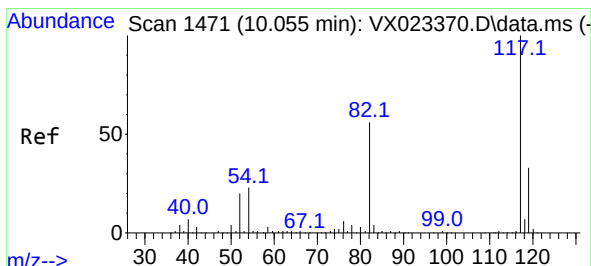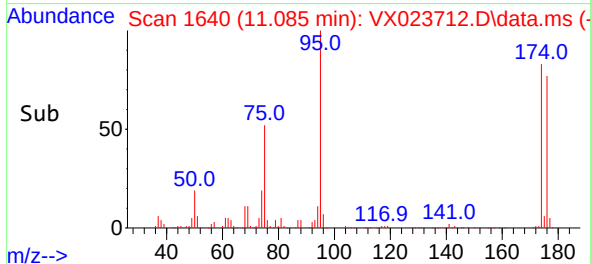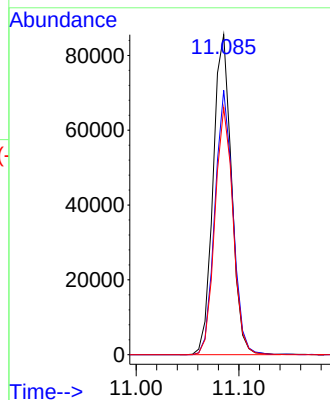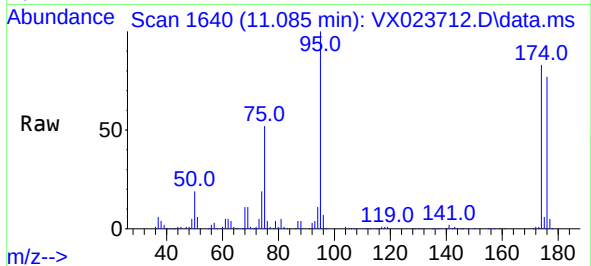

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX023712.D
Acq: 14 Aug 2021 00:52

Tgt Ion: 117 Resp: 241797
Ion Ratio Lower Upper
117 100
82 58.5 47.4 71.2
119 31.9 26.6 39.8

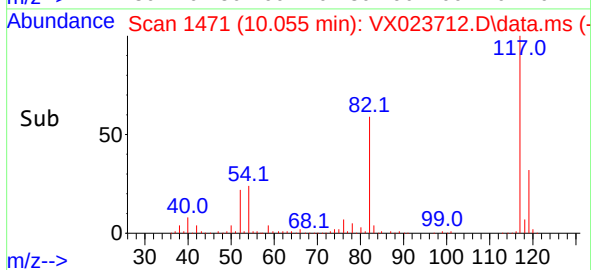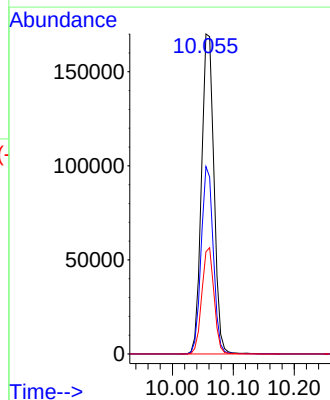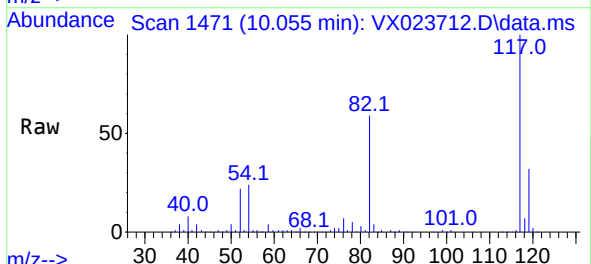

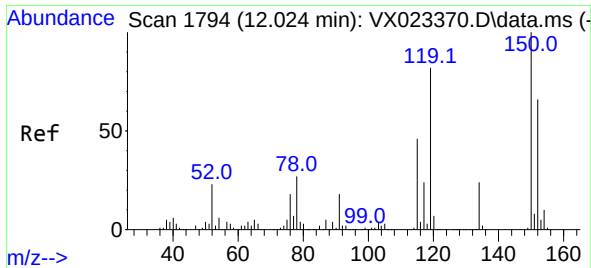

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1794
 Delta R.T. 0.000 min
 Lab File: VX023712.D
 Acq: 14 Aug 2021 00:52

Instrument :
 MSVOA_X
 ClientSampleId :
 SWCS-01-0205

Tgt Ion:152 Resp: 93669
 Ion Ratio Lower Upper
 152 100
 115 59.5 41.1 123.3
 150 157.1 0.0 349.0

