

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030608.D
 Acq On : 13 Aug 2022 09:18
 Operator : JC/MD
 Sample : VX0813MBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Aug 13 21:15:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 13 21:15:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	265227	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	241510	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	110484	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	65995	38.747	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.500%
7) Chloroethane-d5	1.672	69	57471	47.865	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.720%
11) 1,1-Dichloroethene-d2	2.306	63	115563	35.869	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.740%
21) 2-Butanone-d5	4.465	46	177406	112.415	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	112.410%
24) Chloroform-d	5.056	84	176395	50.310	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.620%
26) 1,2-Dichloroethane-d4	5.958	65	125438	52.689	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.380%
32) Benzene-d6	5.976	84	320089	46.269	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.540%
36) 1,2-Dichloropropane-d6	7.305	67	112497	50.121	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.240%
41) Toluene-d8	8.647	98	283888	43.535	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.060%
43) trans-1,3-Dichloroprop...	8.952	79	50542	45.264	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.520%
47) 2-Hexanone-d5	9.384	63	113639	99.329	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.330%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	154539	52.412	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	104.820%
66) 1,2-Dichlorobenzene-d4	12.323	152	103612	48.350	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.700%
Target Compounds						Qvalue
37) 1,2-Dichloropropane	7.305	63	13363	6.491	ug/L	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030608.D
Acq On : 13 Aug 2022 09:18
Operator : JC/MD
Sample : VX0813MBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Aug 13 21:15:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 13 21:15:11 2022
Response via : Initial Calibration

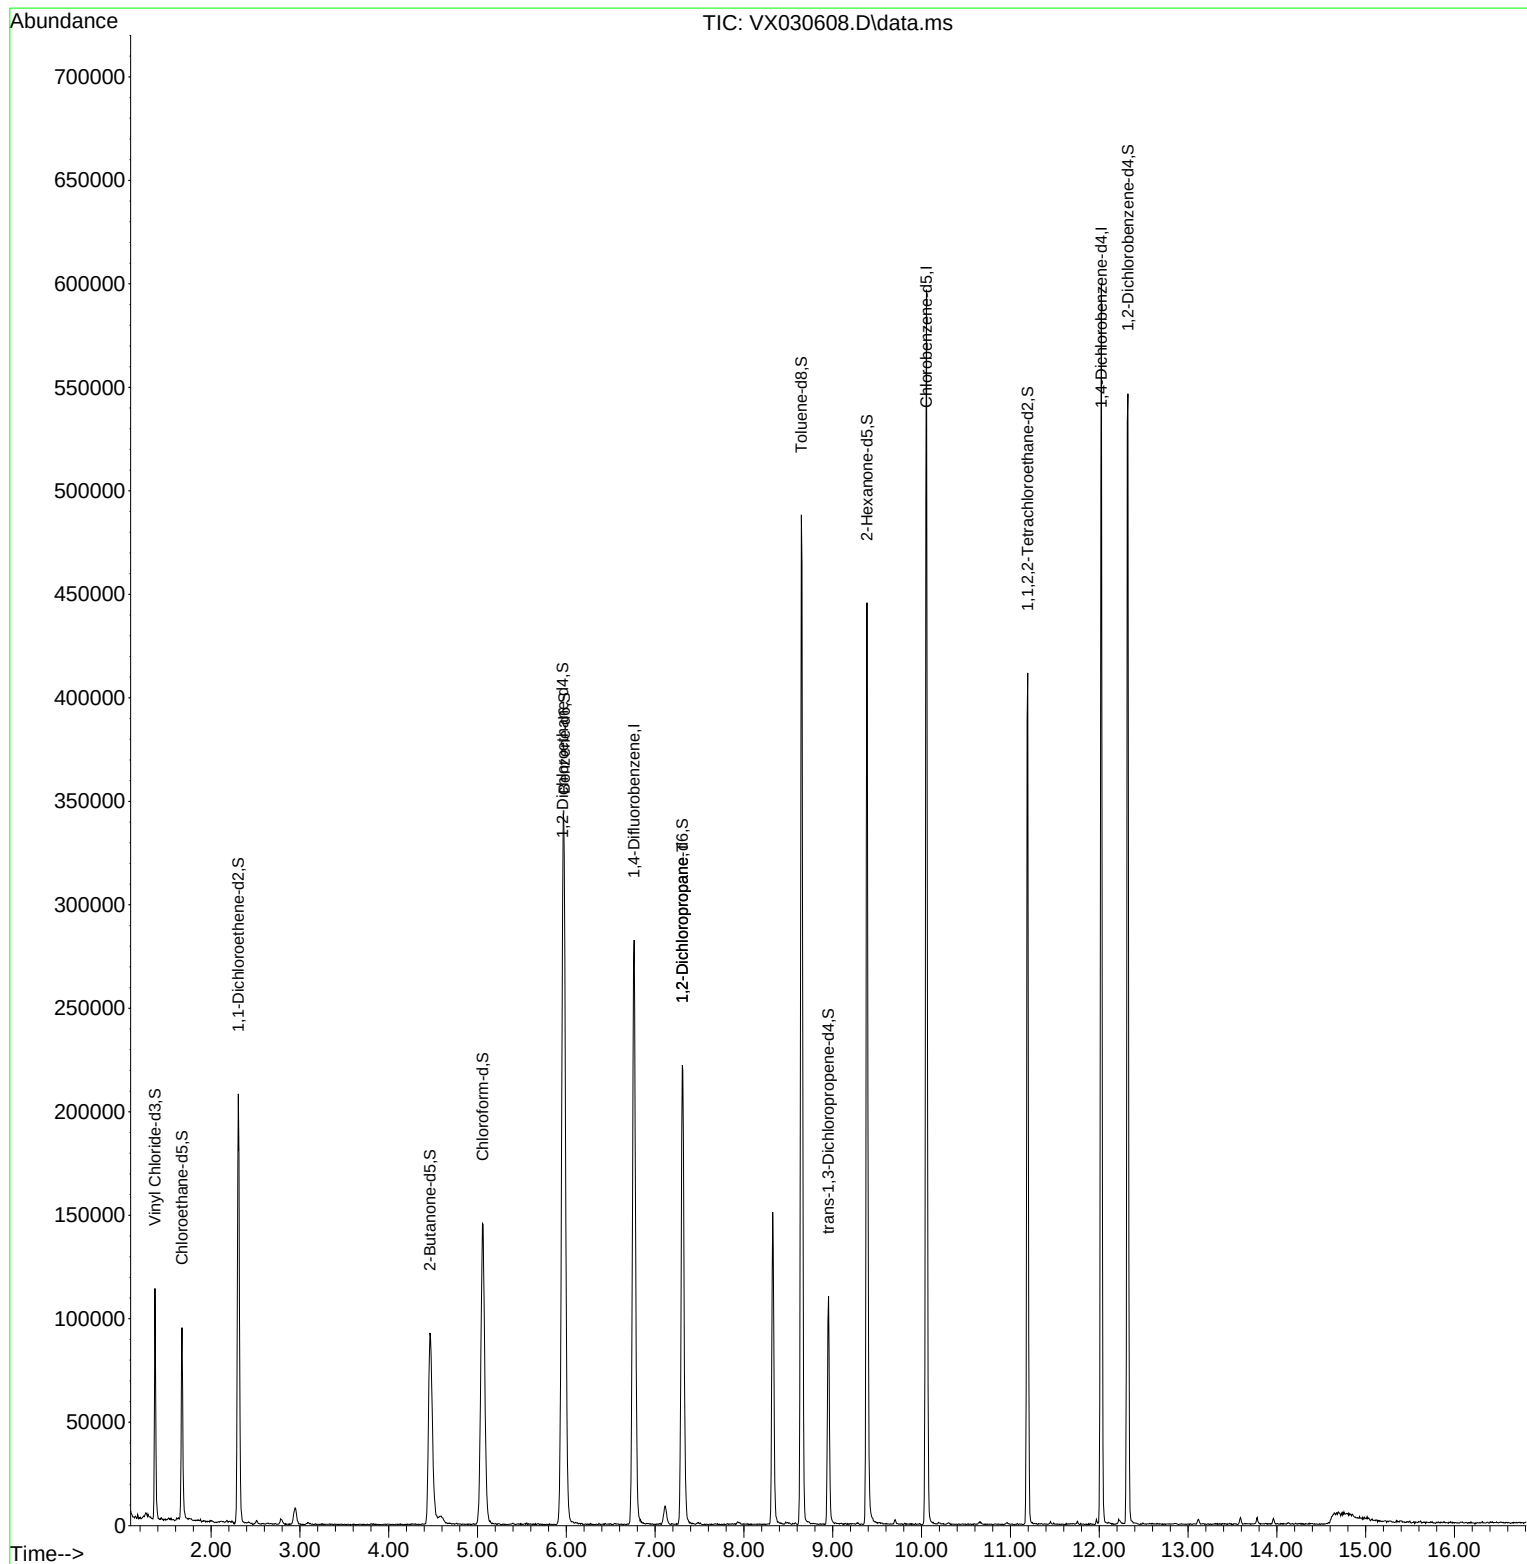

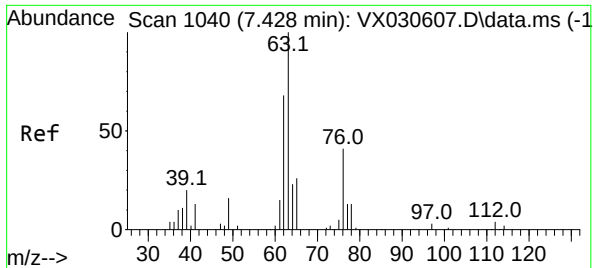

#37
 1,2-Dichloropropane
 Concen: 6.491 ug/L
 RT: 7.305 min Scan# 10
 Delta R.T. -0.122 min
 Lab File: VX030608.D
 Acq: 13 Aug 2022 09:18

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 63 Resp: 13363
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.0 4.4#

