

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030608.D
 Acq On : 13 Aug 2022 09:18
 Operator : JC/MD
 Sample : VX0813MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK682

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030608.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	55	rVB	111638	111982	10.82%	1.367%
2	1.672	91	96	107	rVB	92695	117168	11.32%	1.430%
3	2.306	193	200	212	rBV	207794	325565	31.45%	3.973%
4	2.514	228	234	241	rBV	1873	3217	0.31%	0.039%
5	2.721	266	268	272	rBV	364	335	0.03%	0.004%
6	2.782	274	278	286	rVV5	2711	5375	0.52%	0.066%
7	2.947	297	305	312	rBV2	7895	18486	1.79%	0.226%
8	3.087	322	328	331	rBV3	1073	2085	0.20%	0.025%
9	3.172	339	342	344	rVB2	443	412	0.04%	0.005%
10	3.257	353	356	358	rVB2	407	376	0.04%	0.005%
11	3.392	376	378	380	rBV2	425	420	0.04%	0.005%
12	3.501	394	396	400	rVB2	395	458	0.04%	0.006%
13	3.538	400	402	405	rBV2	347	448	0.04%	0.005%
14	3.800	443	445	448	rVV2	555	562	0.05%	0.007%
15	3.965	466	472	473	rBV2	344	620	0.06%	0.008%
16	3.989	473	476	477	rBV2	296	334	0.03%	0.004%
17	4.080	489	491	494	rBV2	371	420	0.04%	0.005%
18	4.465	545	554	568	rBV	92218	284120	27.44%	3.467%
19	4.763	601	603	605	rVB2	489	391	0.04%	0.005%
20	4.910	625	627	630	rVB2	420	481	0.05%	0.006%
21	4.952	630	634	636	rBV2	586	832	0.08%	0.010%
22	5.056	639	651	664	rBV2	145333	443657	42.85%	5.414%
23	5.227	678	679	686	rVB2	564	998	0.10%	0.012%
24	5.288	686	689	691	rBV2	417	468	0.05%	0.006%
25	5.458	712	717	718	rBV2	425	672	0.06%	0.008%
26	5.550	731	732	734	rVB	790	574	0.06%	0.007%
27	5.678	750	753	756	rBV2	532	688	0.07%	0.008%
28	5.964	787	800	815	rBV2	343395	1035291	100.00%	12.635%
29	6.172	832	834	836	rVB3	507	472	0.05%	0.006%
30	6.367	864	866	869	rVB2	477	367	0.04%	0.004%
31	6.440	876	878	880	rBV2	524	510	0.05%	0.006%
32	6.550	892	896	897	rBV2	587	722	0.07%	0.009%
33	6.653	911	913	917	rBV	464	664	0.06%	0.008%
34	6.684	917	918	921	rBV2	374	379	0.04%	0.005%
35	6.763	921	931	947	rBV	282243	673337	65.04%	8.218%
36	7.013	971	972	975	rVV	376	388	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030608.D
 Acq On : 13 Aug 2022 09:18
 Operator : JC/MD
 Sample : VX0813MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK682

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.056	977	979	981	rVB2	596	460	0.04%	0.006%
38	7.110	981	988	999	rBV4	8978	21758	2.10%	0.266%
39	7.305	1012	1020	1033	rBV	221714	493842	47.70%	6.027%
40	7.488	1044	1050	1052	rBV3	841	1354	0.13%	0.017%
41	7.507	1052	1053	1060	rVB2	826	635	0.06%	0.008%
42	7.580	1063	1065	1068	rVB2	377	442	0.04%	0.005%
43	7.610	1068	1070	1073	rBV	366	494	0.05%	0.006%
44	7.775	1094	1097	1100	rBV	390	384	0.04%	0.005%
45	7.927	1118	1122	1125	rBV3	1224	2063	0.20%	0.025%
46	8.324	1181	1187	1196	rBV	150745	250586	24.20%	3.058%
47	8.470	1208	1211	1213	rBV3	1053	1172	0.11%	0.014%
48	8.549	1222	1224	1227	rBV	536	559	0.05%	0.007%
49	8.580	1227	1229	1233	rVB4	816	876	0.08%	0.011%
50	8.647	1234	1240	1251	rBV	487565	771875	74.56%	9.420%
51	8.878	1276	1278	1281	rBV	313	344	0.03%	0.004%
52	8.952	1284	1290	1301	rBV	110244	168893	16.31%	2.061%
53	9.141	1319	1321	1324	rVB3	499	478	0.05%	0.006%
54	9.165	1324	1325	1328	rVB2	445	339	0.03%	0.004%
55	9.195	1328	1330	1332	rBV	460	353	0.03%	0.004%
56	9.275	1341	1343	1349	rVB3	952	1338	0.13%	0.016%
57	9.323	1349	1351	1353	rBV3	342	346	0.03%	0.004%
58	9.384	1356	1361	1375	rVV	444621	616157	59.52%	7.520%
59	9.701	1410	1413	1416	rBV2	2142	2463	0.24%	0.030%
60	9.811	1428	1431	1433	rVB2	714	539	0.05%	0.007%
61	9.829	1433	1434	1436	rBV2	489	384	0.04%	0.005%
62	9.933	1448	1451	1453	rBV2	462	365	0.04%	0.004%
63	9.982	1457	1459	1461	rVB	635	456	0.04%	0.006%
64	10.055	1463	1471	1482	rBV	596682	790022	76.31%	9.642%
65	10.189	1491	1493	1498	rVB3	854	1076	0.10%	0.013%
66	10.421	1528	1531	1533	rBV2	412	489	0.05%	0.006%
67	10.598	1558	1560	1562	rBV3	405	432	0.04%	0.005%
68	10.652	1564	1569	1570	rBV	1236	1399	0.14%	0.017%
69	10.780	1588	1590	1593	rVB	413	413	0.04%	0.005%
70	10.823	1593	1597	1601	rBV2	382	830	0.08%	0.010%
71	10.963	1613	1620	1622	rBV3	1086	1767	0.17%	0.022%
72	11.079	1637	1639	1641	rVB	521	400	0.04%	0.005%
73	11.110	1641	1644	1645	rBV2	315	345	0.03%	0.004%
74	11.195	1652	1658	1666	rBV	411096	527151	50.92%	6.433%
75	11.317	1677	1678	1681	rBV	467	501	0.05%	0.006%
76	11.347	1681	1683	1688	rVB2	482	485	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030608.D
 Acq On : 13 Aug 2022 09:18
 Operator : JC/MD
 Sample : VX0813MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK682

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.451	1695	1700	1704	rBV3	1300	1383	0.13%	0.017%
78	11.683	1734	1738	1740	rBV2	300	372	0.04%	0.005%
79	11.756	1747	1750	1754	rVB4	1543	1636	0.16%	0.020%
80	11.896	1772	1773	1777	rBV	564	663	0.06%	0.008%
81	11.969	1782	1785	1788	rBV3	2564	2626	0.25%	0.032%
82	12.024	1789	1794	1801	rVB	598711	733305	70.83%	8.949%
83	12.219	1823	1826	1834	rBV4	2295	3714	0.36%	0.045%
84	12.323	1837	1843	1850	rBV	545842	716315	69.19%	8.742%
85	12.494	1869	1871	1875	rVB2	548	454	0.04%	0.006%
86	13.030	1957	1959	1962	rBV	482	421	0.04%	0.005%
87	13.061	1962	1964	1967	rVV	341	469	0.05%	0.006%
88	13.115	1969	1973	1977	rVV5	2357	3558	0.34%	0.043%
89	13.390	2015	2018	2021	rBV	482	533	0.05%	0.007%
90	13.591	2046	2051	2055	rBV5	3356	4491	0.43%	0.055%
91	13.719	2070	2072	2074	rBV	362	339	0.03%	0.004%
92	13.780	2078	2082	2088	rVB3	3355	4483	0.43%	0.055%
93	13.871	2095	2097	2101	rVB	395	418	0.04%	0.005%
94	13.963	2109	2112	2116	rVB4	2775	3511	0.34%	0.043%
95	14.134	2135	2140	2143	rVB2	761	1128	0.11%	0.014%
96	14.213	2151	2153	2156	rVB	588	474	0.05%	0.006%
97	14.323	2170	2171	2174	rBV	459	455	0.04%	0.006%
98	14.579	2212	2213	2215	rBV	529	454	0.04%	0.006%
99	14.646	2215	2224	2227	rBV8	4940	14581	1.41%	0.178%
100	15.798	2411	2413	2415	rBV3	608	567	0.05%	0.007%




Sum of corrected areas: 8193889

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030608.D
Acq On : 13 Aug 2022 09:18
Operator : JC/MD
Sample : VX0813MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK682

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

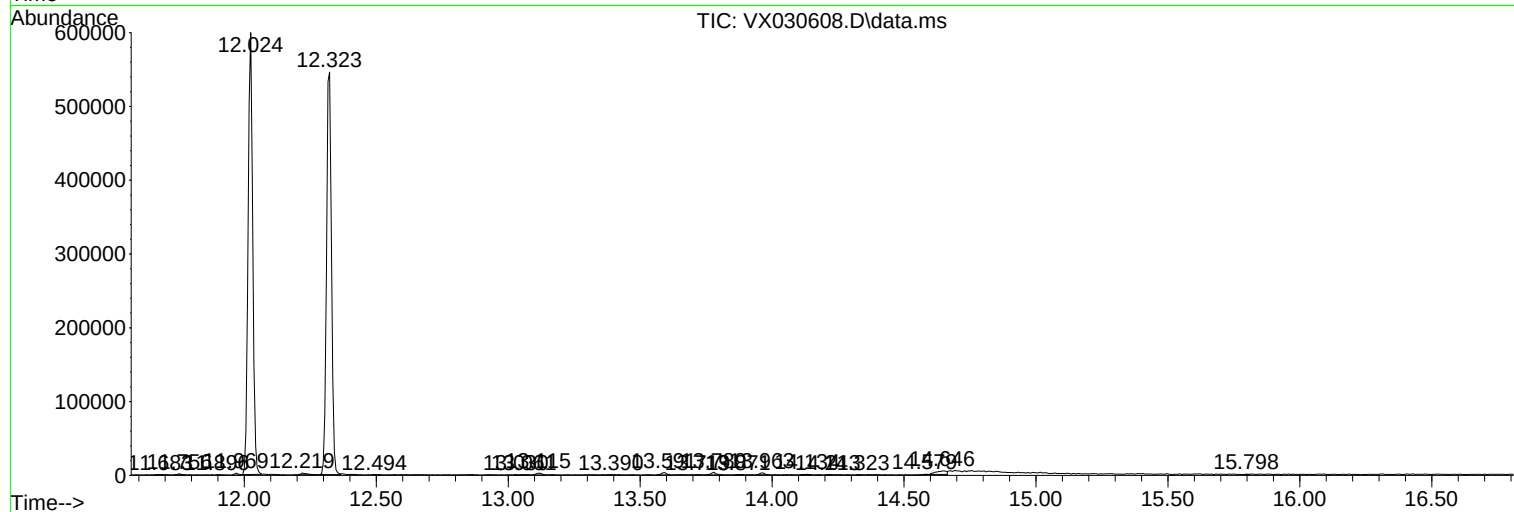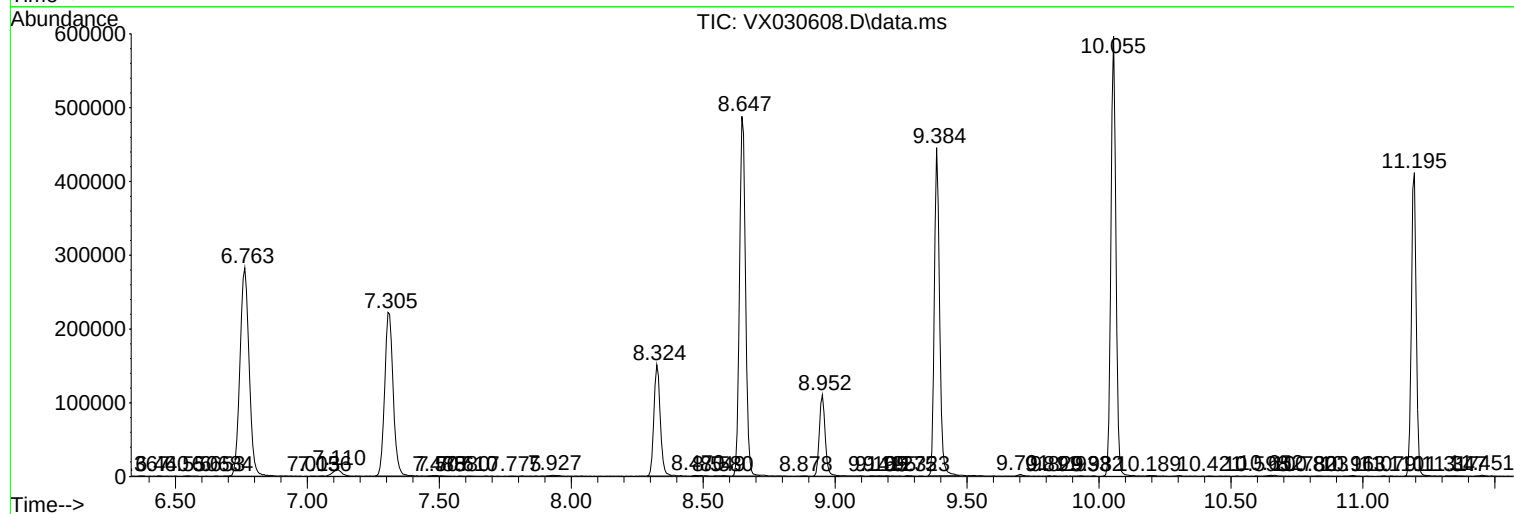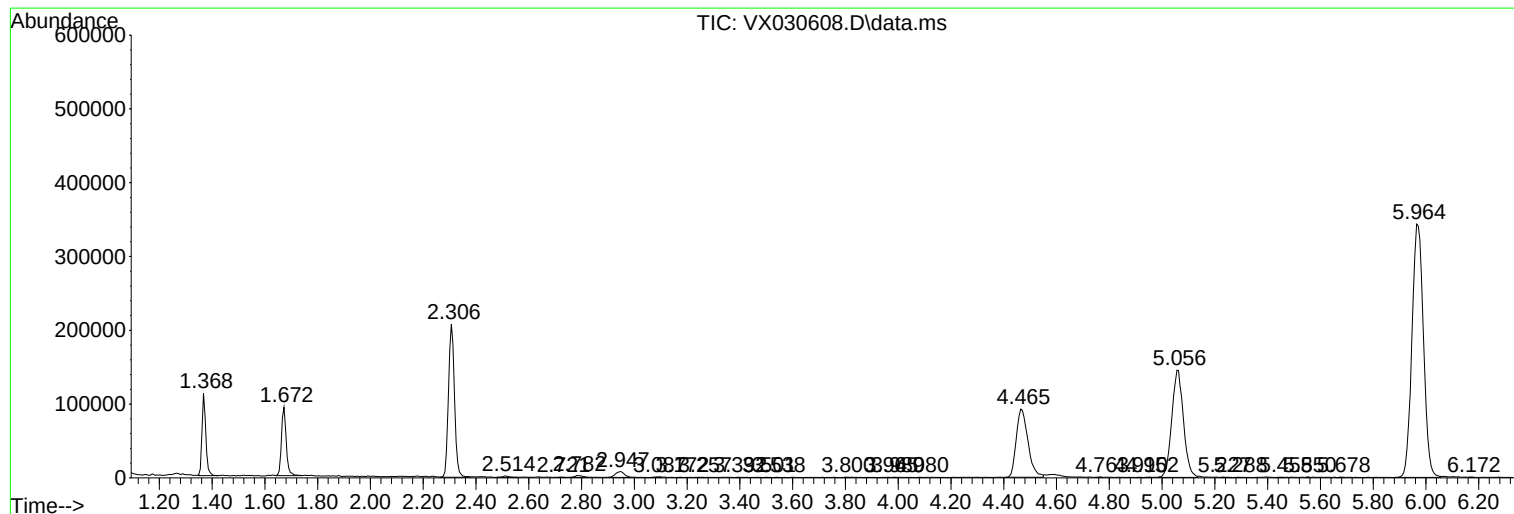

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030608.D
Acq On : 13 Aug 2022 09:18
Operator : JC/MD
Sample : VX0813MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK682

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030608.D
Acq On : 13 Aug 2022 09:18
Operator : JC/MD
Sample : VX0813MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK682

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc