

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030609.D
 Acq On : 13 Aug 2022 09:41
 Operator : JC/MD
 Sample : VX0813WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK683

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	104560	105665	10.66%	1.358%
2	1.672	92	96	102	rVB	85140	102560	10.35%	1.318%
3	1.904	132	134	135	rBV	1101	611	0.06%	0.008%
4	2.306	194	200	211	rVB	190229	299296	30.19%	3.845%
5	2.629	251	253	255	rVB3	574	380	0.04%	0.005%
6	2.648	255	256	258	rBV	497	346	0.03%	0.004%
7	2.794	275	280	285	rVB3	2413	4271	0.43%	0.055%
8	2.947	298	305	315	rBV	7793	17381	1.75%	0.223%
9	3.093	325	329	330	rBV	604	599	0.06%	0.008%
10	3.148	336	338	341	rBV2	452	541	0.05%	0.007%
11	3.209	345	348	350	rBV2	338	488	0.05%	0.006%
12	3.367	372	374	375	rBV	498	391	0.04%	0.005%
13	3.495	392	395	398	rBV2	461	700	0.07%	0.009%
14	3.526	398	400	402	rVV2	440	399	0.04%	0.005%
15	3.727	431	433	436	rVB2	440	444	0.04%	0.006%
16	3.751	436	437	441	rBV2	274	351	0.04%	0.005%
17	3.800	443	445	450	rVV2	280	433	0.04%	0.006%
18	4.117	495	497	500	rVB2	385	367	0.04%	0.005%
19	4.385	537	541	543	rBV	359	420	0.04%	0.005%
20	4.471	545	555	569	rBV	95817	288831	29.14%	3.711%
21	4.733	597	598	604	rBV3	481	588	0.06%	0.008%
22	4.885	621	623	626	rBV	389	356	0.04%	0.005%
23	4.916	626	628	631	rVV2	427	469	0.05%	0.006%
24	5.062	640	652	668	rBV2	135136	425644	42.94%	5.468%
25	5.434	711	713	715	rBV	500	383	0.04%	0.005%
26	5.470	717	719	723	rBV3	327	350	0.04%	0.004%
27	5.641	746	747	750	rBV2	354	346	0.03%	0.004%
28	5.757	762	766	767	rBV2	268	357	0.04%	0.005%
29	5.970	789	801	816	rBV2	331190	991260	100.00%	12.735%
30	6.196	837	838	841	rVV2	400	341	0.03%	0.004%
31	6.318	856	858	861	rBV3	306	398	0.04%	0.005%
32	6.391	868	870	872	rVB2	554	393	0.04%	0.005%
33	6.434	874	877	878	rBV2	397	434	0.04%	0.006%
34	6.495	884	887	888	rVB	535	471	0.05%	0.006%
35	6.598	901	904	907	rBV2	276	400	0.04%	0.005%
36	6.763	921	931	951	rVV	263616	637839	64.35%	8.195%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030609.D
 Acq On : 13 Aug 2022 09:41
 Operator : JC/MD
 Sample : VX0813WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK683

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.001	966	970	972	rBV2	390	444	0.04%	0.006%
38	7.116	980	989	996	rBV6	9041	21066	2.13%	0.271%
39	7.312	1012	1021	1039	rVB	216282	473980	47.82%	6.089%
40	7.549	1056	1060	1062	rBV2	387	546	0.06%	0.007%
41	7.690	1080	1083	1086	rBV2	533	717	0.07%	0.009%
42	7.720	1086	1088	1089	rVV	372	387	0.04%	0.005%
43	7.751	1091	1093	1096	rVB2	696	458	0.05%	0.006%
44	7.940	1119	1124	1131	rVB5	1218	2558	0.26%	0.033%
45	8.122	1152	1154	1157	rVB	562	396	0.04%	0.005%
46	8.269	1176	1178	1181	rBV2	547	483	0.05%	0.006%
47	8.330	1181	1188	1198	rBV	141359	240654	24.28%	3.092%
48	8.446	1205	1207	1209	rVB	564	394	0.04%	0.005%
49	8.482	1209	1213	1219	rBV4	1511	2337	0.24%	0.030%
50	8.561	1225	1226	1229	rVB3	565	416	0.04%	0.005%
51	8.653	1234	1241	1256	rVV	467266	739404	74.59%	9.499%
52	8.909	1281	1283	1284	rVV2	435	347	0.04%	0.004%
53	8.952	1284	1290	1305	rVV	105969	159467	16.09%	2.049%
54	9.055	1305	1307	1312	rVB3	820	1214	0.12%	0.016%
55	9.275	1341	1343	1347	rVB2	1331	1339	0.14%	0.017%
56	9.384	1354	1361	1378	rBV	436512	625257	63.08%	8.033%
57	9.610	1395	1398	1402	rBV2	620	886	0.09%	0.011%
58	9.701	1409	1413	1418	rBV2	3126	4872	0.49%	0.063%
59	9.939	1447	1452	1453	rBV	415	485	0.05%	0.006%
60	9.988	1457	1460	1462	rBV	555	556	0.06%	0.007%
61	10.055	1465	1471	1481	rBV	563163	740337	74.69%	9.511%
62	10.195	1491	1494	1498	rVB2	716	1014	0.10%	0.013%
63	10.299	1507	1511	1514	rVB3	535	737	0.07%	0.009%
64	10.640	1566	1567	1569	rBV	436	395	0.04%	0.005%
65	11.049	1632	1634	1637	rBV2	453	396	0.04%	0.005%
66	11.079	1637	1639	1641	rVV2	509	489	0.05%	0.006%
67	11.195	1652	1658	1668	rVV	406487	507965	51.24%	6.526%
68	11.457	1697	1701	1702	rBV3	628	674	0.07%	0.009%
69	11.890	1770	1772	1774	rVB2	528	456	0.05%	0.006%
70	11.914	1774	1776	1778	rVB	466	353	0.04%	0.005%
71	11.969	1781	1785	1788	rBV2	826	1213	0.12%	0.016%
72	12.024	1789	1794	1804	rVB	565757	679974	68.60%	8.736%
73	12.225	1823	1827	1833	rVB3	1690	3154	0.32%	0.041%
74	12.268	1833	1834	1836	rBV	585	432	0.04%	0.006%
75	12.323	1837	1843	1852	rVV	522787	668597	67.45%	8.590%
76	12.865	1929	1932	1934	rBV2	601	728	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030609.D
 Acq On : 13 Aug 2022 09:41
 Operator : JC/MD
 Sample : VX0813WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK683

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.908	1938	1939	1942	rVV2	530	403	0.04%	0.005%
78	12.945	1944	1945	1948	rBV2	498	497	0.05%	0.006%
79	13.030	1957	1959	1961	rBV	475	477	0.05%	0.006%
80	13.085	1966	1968	1970	rBV2	323	354	0.04%	0.005%
81	13.115	1971	1973	1976	rVV2	732	609	0.06%	0.008%
82	13.189	1983	1985	1986	rBV	359	342	0.03%	0.004%
83	13.268	1997	1998	2001	rVB	802	357	0.04%	0.005%
84	13.445	2025	2027	2030	rBV2	414	456	0.05%	0.006%
85	13.597	2048	2052	2054	rVB4	826	984	0.10%	0.013%
86	13.652	2059	2061	2063	rBV2	334	340	0.03%	0.004%
87	13.780	2081	2082	2086	rVB	582	524	0.05%	0.007%
88	14.127	2138	2139	2144	rVB2	787	950	0.10%	0.012%
89	14.438	2188	2190	2192	rBV2	579	467	0.05%	0.006%
90	14.597	2214	2216	2219	rVB2	591	548	0.06%	0.007%
91	14.798	2246	2249	2250	rBV	835	760	0.08%	0.010%
92	14.920	2266	2269	2270	rBV3	775	752	0.08%	0.010%
93	15.048	2288	2290	2291	rBV	644	397	0.04%	0.005%
94	15.066	2291	2293	2298	rBV4	535	808	0.08%	0.010%
95	15.237	2319	2321	2324	rBV3	666	762	0.08%	0.010%
96	15.328	2334	2336	2338	rBV3	648	479	0.05%	0.006%
97	15.389	2344	2346	2349	rBV2	681	785	0.08%	0.010%
98	15.743	2403	2404	2407	rBV2	735	448	0.05%	0.006%
99	16.194	2476	2478	2479	rBV2	373	337	0.03%	0.004%
100	16.212	2479	2481	2484	rVV3	588	776	0.08%	0.010%




Sum of corrected areas: 7783692

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030609.D
Acq On : 13 Aug 2022 09:41
Operator : JC/MD
Sample : VX0813WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK683

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

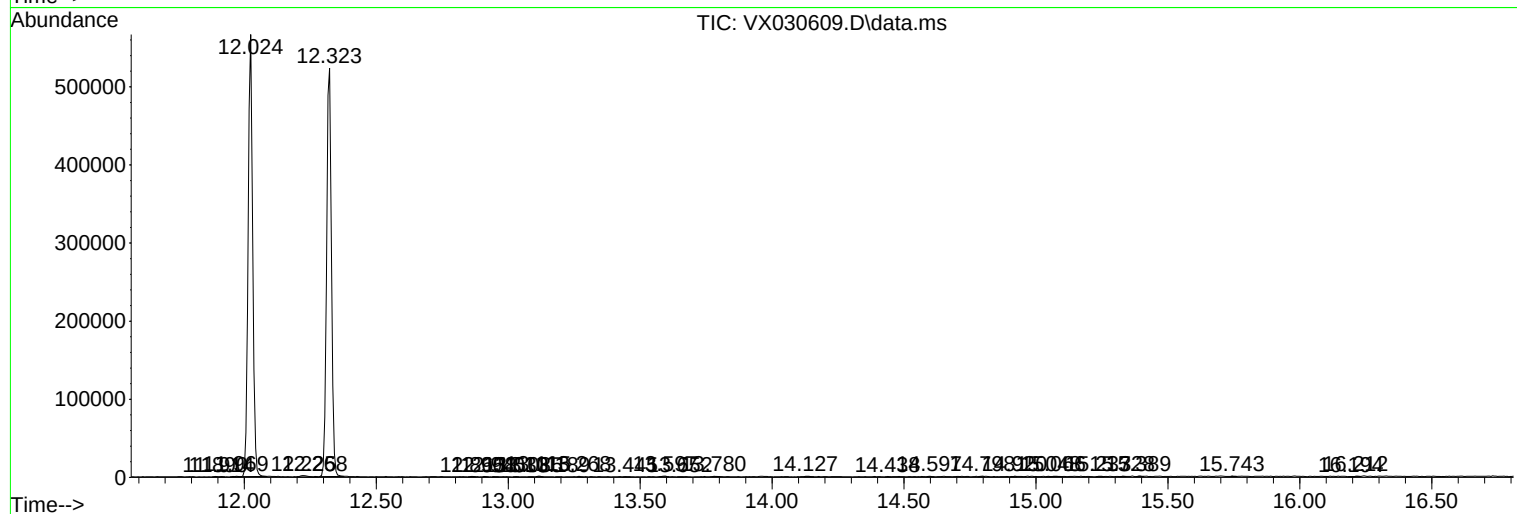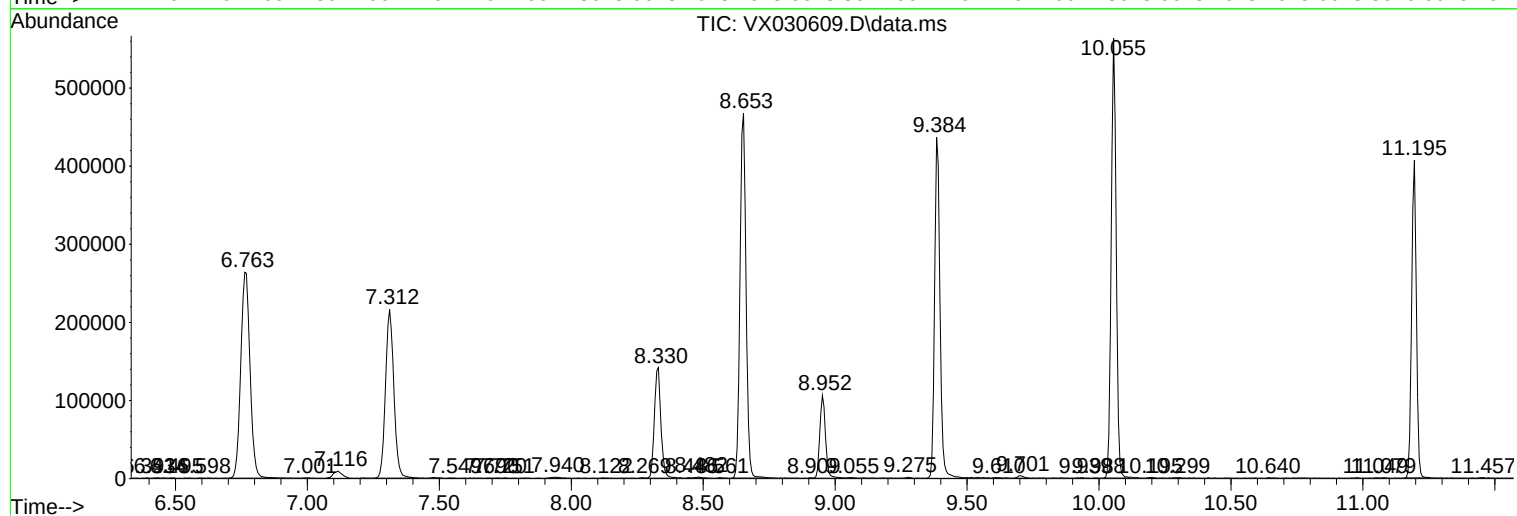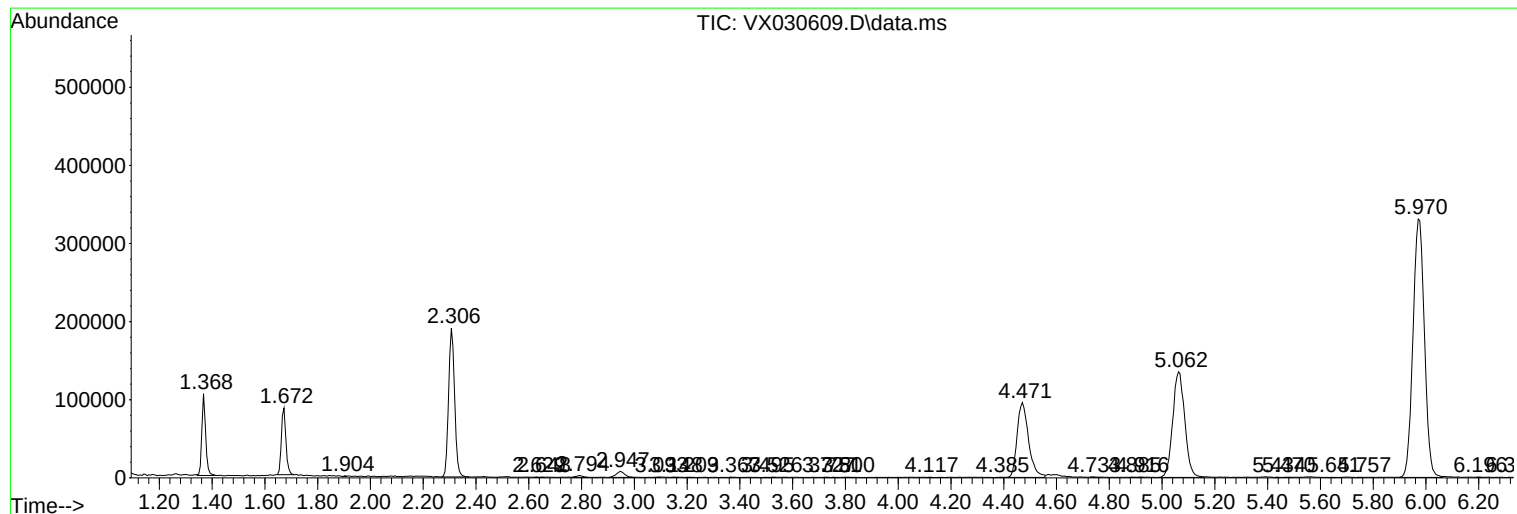

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030609.D
Acq On : 13 Aug 2022 09:41
Operator : JC/MD
Sample : VX0813WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK683

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030609.D
Acq On : 13 Aug 2022 09:41
Operator : JC/MD
Sample : VX0813WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK683

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc