

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030610.D
 Acq On : 13 Aug 2022 10:16
 Operator : JC/MD
 Sample : N4005-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030610.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB	109359	109891	10.77%	1.388%
2	1.666	91	95	102	rVB	85512	108337	10.61%	1.368%
3	2.307	193	200	212	rBV	198791	306638	30.04%	3.873%
4	2.587	244	246	247	rBV2	568	382	0.04%	0.005%
5	2.636	252	254	257	rVB2	574	617	0.06%	0.008%
6	2.788	273	279	286	rBV3	2311	4681	0.46%	0.059%
7	2.947	296	305	314	rBV	10108	23370	2.29%	0.295%
8	3.227	350	351	353	rBV	464	296	0.03%	0.004%
9	3.794	442	444	447	rVB2	453	488	0.05%	0.006%
10	3.819	447	448	450	rBV2	340	295	0.03%	0.004%
11	3.873	455	457	460	rVB	324	354	0.03%	0.004%
12	3.898	460	461	463	rBV	540	395	0.04%	0.005%
13	3.922	463	465	467	rVB	433	344	0.03%	0.004%
14	3.959	467	471	474	rBV2	563	771	0.08%	0.010%
15	4.318	527	530	531	rBV2	348	389	0.04%	0.005%
16	4.349	534	535	540	rVB2	447	546	0.05%	0.007%
17	4.465	542	554	567	rBV	95759	290072	28.42%	3.663%
18	4.751	599	601	605	rVB3	724	660	0.06%	0.008%
19	5.062	637	652	666	rBV	139698	431663	42.29%	5.452%
20	5.324	693	695	697	rBV	429	342	0.03%	0.004%
21	5.349	697	699	700	rBV	469	286	0.03%	0.004%
22	5.733	760	762	764	rBV	401	432	0.04%	0.005%
23	5.830	777	778	781	rVB2	350	323	0.03%	0.004%
24	5.971	788	801	817	rVV2	342808	1020790	100.00%	12.892%
25	6.129	826	827	830	rVV2	738	565	0.06%	0.007%
26	6.166	831	833	834	rVB	748	381	0.04%	0.005%
27	6.422	874	875	878	rBV2	386	374	0.04%	0.005%
28	6.574	899	900	903	rVV	353	297	0.03%	0.004%
29	6.763	921	931	943	rBV2	262913	623812	61.11%	7.878%
30	6.940	959	960	963	rVB2	572	463	0.05%	0.006%
31	7.062	979	980	981	rBV	629	398	0.04%	0.005%
32	7.111	982	988	996	rVB2	9180	20245	1.98%	0.256%
33	7.208	1001	1004	1006	rVB2	361	336	0.03%	0.004%
34	7.306	1012	1020	1032	rBV2	215840	485333	47.54%	6.129%
35	7.415	1036	1038	1041	rVB3	750	728	0.07%	0.009%
36	7.458	1041	1045	1047	rBV3	736	1085	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030610.D
 Acq On : 13 Aug 2022 10:16
 Operator : JC/MD
 Sample : N4005-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.482	1047	1049	1051	rBV2	660	440	0.04%	0.006%
38	7.635	1073	1074	1077	rVB2	461	351	0.03%	0.004%
39	7.897	1114	1117	1118	rBV	337	355	0.03%	0.004%
40	7.934	1118	1123	1132	rVB4	1664	3539	0.35%	0.045%
41	8.025	1137	1138	1141	rVB2	485	409	0.04%	0.005%
42	8.196	1163	1166	1167	rBV	428	289	0.03%	0.004%
43	8.324	1181	1187	1197	rBV	144380	243692	23.87%	3.078%
44	8.482	1209	1213	1216	rBV5	1085	1542	0.15%	0.019%
45	8.568	1226	1227	1229	rBV	431	322	0.03%	0.004%
46	8.647	1234	1240	1249	rBV	473732	759096	74.36%	9.587%
47	8.952	1284	1290	1303	rBV	112848	164895	16.15%	2.083%
48	9.263	1336	1341	1342	rBV2	524	731	0.07%	0.009%
49	9.385	1356	1361	1373	rBV	438018	625510	61.28%	7.900%
50	9.702	1409	1413	1419	rVB4	3895	6245	0.61%	0.079%
51	9.970	1455	1457	1462	rVB2	522	735	0.07%	0.009%
52	10.006	1462	1463	1465	rBV	596	493	0.05%	0.006%
53	10.055	1465	1471	1484	rVV	551927	736768	72.18%	9.305%
54	10.275	1506	1507	1509	rBV2	376	293	0.03%	0.004%
55	10.427	1531	1532	1534	rBV2	492	294	0.03%	0.004%
56	10.476	1538	1540	1543	rVV2	413	368	0.04%	0.005%
57	10.506	1543	1545	1546	rVV	415	323	0.03%	0.004%
58	10.525	1546	1548	1553	rVB2	527	642	0.06%	0.008%
59	10.561	1553	1554	1557	rBV	380	362	0.04%	0.005%
60	10.592	1557	1559	1560	rBV	361	306	0.03%	0.004%
61	10.610	1560	1562	1564	rVV2	463	346	0.03%	0.004%
62	10.653	1566	1569	1570	rVV	431	481	0.05%	0.006%
63	10.775	1585	1589	1590	rBV2	281	384	0.04%	0.005%
64	11.049	1631	1634	1636	rBV	523	443	0.04%	0.006%
65	11.195	1652	1658	1670	rVV	410193	530662	51.99%	6.702%
66	11.299	1673	1675	1679	rVB4	439	538	0.05%	0.007%
67	11.403	1690	1692	1693	rBV	383	325	0.03%	0.004%
68	11.439	1696	1698	1703	rVV2	574	793	0.08%	0.010%
69	11.506	1707	1709	1711	rVB2	417	364	0.04%	0.005%
70	11.573	1718	1720	1721	rBV	405	285	0.03%	0.004%
71	11.610	1724	1726	1729	rVV2	425	402	0.04%	0.005%
72	11.848	1761	1765	1767	rBV2	342	356	0.03%	0.004%
73	11.969	1782	1785	1788	rBV2	412	542	0.05%	0.007%
74	12.024	1788	1794	1805	rBV	568445	687433	67.34%	8.682%
75	12.219	1823	1826	1834	rVB5	2839	5521	0.54%	0.070%
76	12.323	1837	1843	1850	rBV	549676	692670	67.86%	8.748%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030610.D
 Acq On : 13 Aug 2022 10:16
 Operator : JC/MD
 Sample : N4005-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.579	1883	1885	1890	rVB3	337	441	0.04%	0.006%
78	12.725	1906	1909	1913	rVB	338	470	0.05%	0.006%
79	12.774	1915	1917	1919	rVB	734	478	0.05%	0.006%
80	12.805	1919	1922	1925	rBV	414	499	0.05%	0.006%
81	12.963	1945	1948	1950	rBV2	346	411	0.04%	0.005%
82	13.042	1958	1961	1962	rBV2	534	540	0.05%	0.007%
83	13.122	1972	1974	1975	rVB2	536	308	0.03%	0.004%
84	13.158	1978	1980	1985	rVB2	481	626	0.06%	0.008%
85	13.378	2014	2016	2018	rBV2	377	301	0.03%	0.004%
86	13.427	2022	2024	2027	rVV2	457	390	0.04%	0.005%
87	13.463	2029	2030	2034	rVV2	464	415	0.04%	0.005%
88	13.506	2034	2037	2038	rVV2	491	339	0.03%	0.004%
89	13.652	2060	2061	2063	rBV	556	416	0.04%	0.005%
90	13.780	2081	2082	2084	rBV	846	516	0.05%	0.007%
91	13.963	2110	2112	2114	rBV	490	494	0.05%	0.006%
92	14.067	2127	2129	2133	rBV3	389	369	0.04%	0.005%
93	14.182	2146	2148	2151	rVB	477	440	0.04%	0.006%
94	14.304	2166	2168	2171	rVB2	656	702	0.07%	0.009%
95	14.609	2215	2218	2219	rBV	436	455	0.04%	0.006%
96	14.981	2277	2279	2281	rBV2	668	320	0.03%	0.004%
97	15.444	2351	2355	2360	rBV3	625	1490	0.15%	0.019%
98	16.042	2451	2453	2456	rBV3	603	647	0.06%	0.008%
99	16.597	2542	2544	2547	rVV2	804	538	0.05%	0.007%
100	16.645	2550	2552	2554	rBV2	791	547	0.05%	0.007%




Sum of corrected areas: 7918076

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030610.D
Acq On : 13 Aug 2022 10:16
Operator : JC/MD
Sample : N4005-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

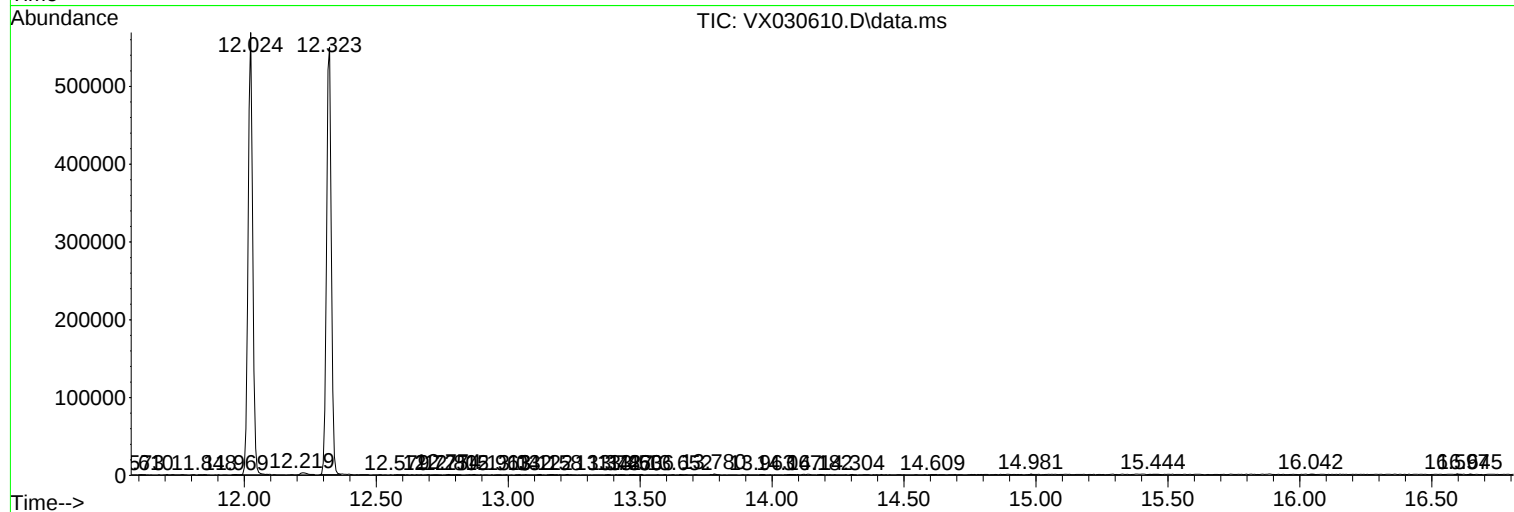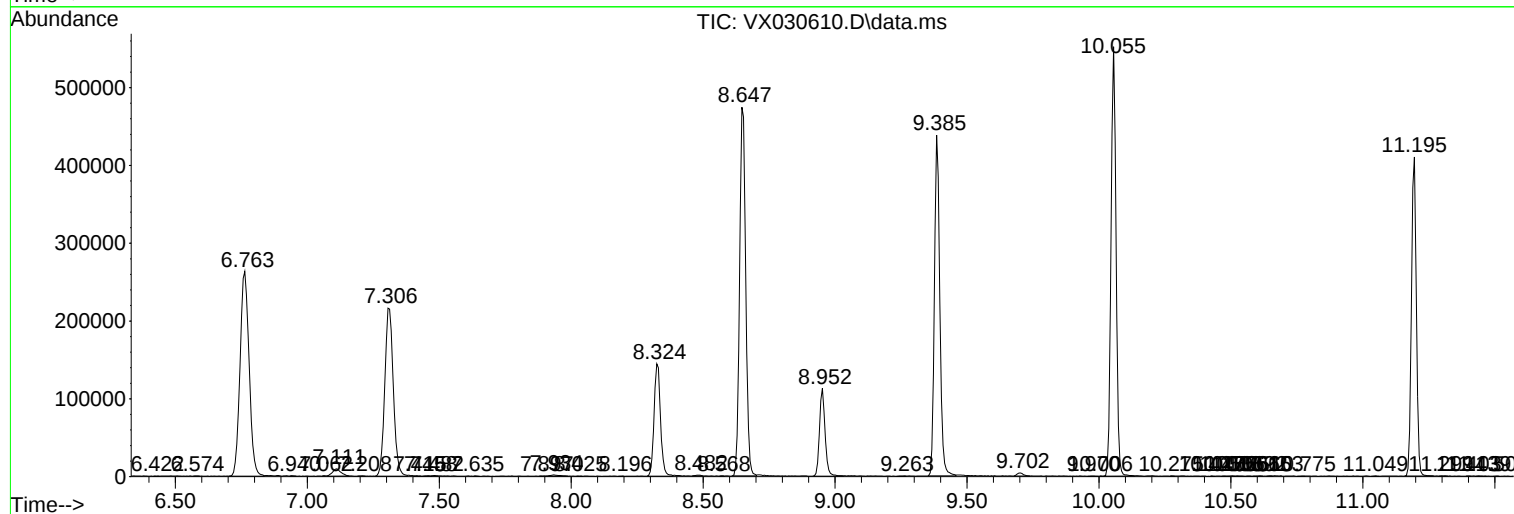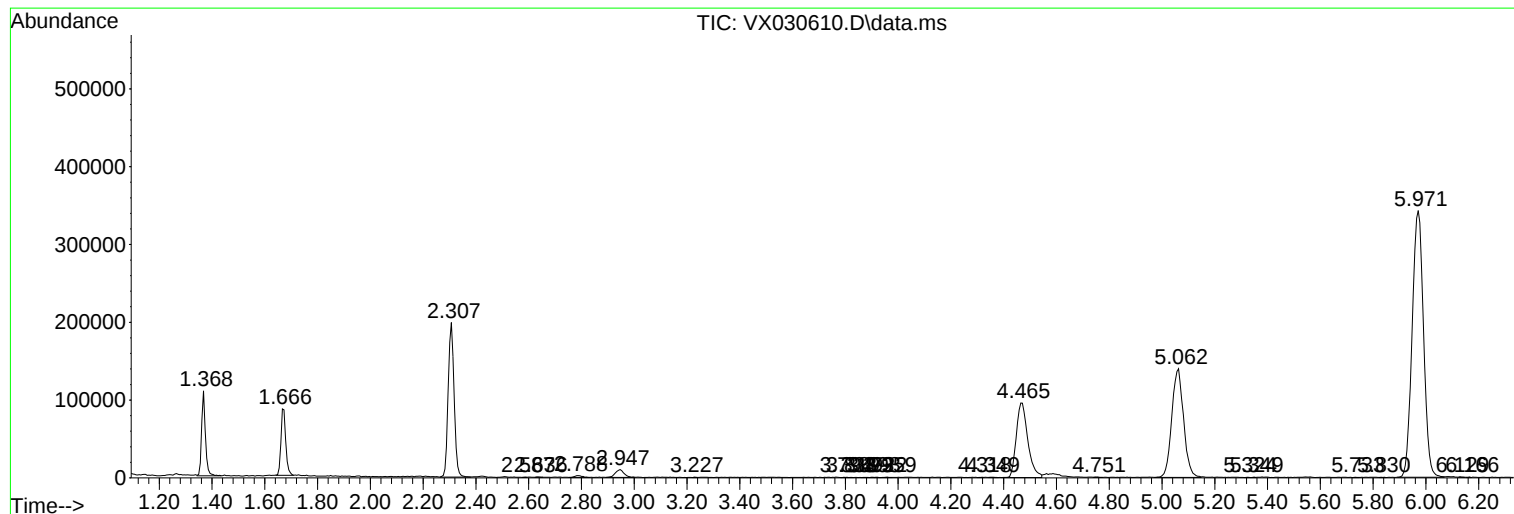

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030610.D
Acq On : 13 Aug 2022 10:16
Operator : JC/MD
Sample : N4005-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030610.D
Acq On : 13 Aug 2022 10:16
Operator : JC/MD
Sample : N4005-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
