

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030611.D
 Acq On : 13 Aug 2022 11:16
 Operator : JC/MD
 Sample : N4131-12DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E15DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030611.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.373	43	47	58	rVB2	273574	323457	30.40%	3.891%
2	1.672	91	96	104	rVB	91740	112711	10.59%	1.356%
3	2.306	194	200	210	rVB	193670	297568	27.97%	3.580%
4	2.587	244	246	250	rVV3	587	742	0.07%	0.009%
5	2.635	252	254	259	rVV2	376	425	0.04%	0.005%
6	2.708	263	266	267	rVV2	637	641	0.06%	0.008%
7	2.794	275	280	286	rVB3	1879	3692	0.35%	0.044%
8	2.861	289	291	294	rVB2	448	339	0.03%	0.004%
9	2.940	296	304	313	rBV2	3449	8661	0.81%	0.104%
10	3.001	313	314	316	rBV	393	351	0.03%	0.004%
11	3.093	322	329	338	rVB2	12321	24271	2.28%	0.292%
12	3.160	338	340	344	rBV2	282	374	0.04%	0.004%
13	3.336	366	369	371	rBV	399	472	0.04%	0.006%
14	3.410	379	381	384	rBV2	371	370	0.03%	0.004%
15	3.434	384	385	389	rVB2	372	383	0.04%	0.005%
16	3.483	389	393	395	rBV2	516	578	0.05%	0.007%
17	3.538	398	402	403	rBV2	315	433	0.04%	0.005%
18	3.818	444	448	449	rBV2	674	839	0.08%	0.010%
19	4.031	478	483	484	rBV	273	402	0.04%	0.005%
20	4.111	494	496	500	rVB2	441	571	0.05%	0.007%
21	4.281	523	524	526	rBV	412	368	0.03%	0.004%
22	4.312	526	529	530	rVB	444	428	0.04%	0.005%
23	4.330	530	532	536	rVB2	344	405	0.04%	0.005%
24	4.373	536	539	541	rBV	420	417	0.04%	0.005%
25	4.464	544	554	573	rBV	102824	312005	29.33%	3.753%
26	4.891	622	624	627	rBV2	357	396	0.04%	0.005%
27	4.915	627	628	634	rVB	518	329	0.03%	0.004%
28	5.056	638	651	667	rBV2	150716	459381	43.18%	5.526%
29	5.165	667	669	671	rBV2	596	423	0.04%	0.005%
30	5.318	692	694	698	rBV	282	383	0.04%	0.005%
31	5.379	702	704	706	rBV3	439	482	0.05%	0.006%
32	5.470	715	719	720	rBV2	334	438	0.04%	0.005%
33	5.549	729	732	734	rBV3	685	973	0.09%	0.012%
34	5.659	748	750	752	rBV	484	373	0.04%	0.004%
35	5.970	787	801	820	rBV3	357004	1063879	100.00%	12.798%
36	6.336	856	861	862	rBV3	357	435	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030611.D
 Acq On : 13 Aug 2022 11:16
 Operator : JC/MD
 Sample : N4131-12DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E15DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.586	900	902	905	rVB2	400	368	0.03%	0.004%
38	6.763	921	931	948	rBV2	260477	620472	58.32%	7.464%
39	6.927	956	958	960	rVB2	539	336	0.03%	0.004%
40	6.964	962	964	967	rBV2	272	361	0.03%	0.004%
41	7.110	980	988	997	rBV4	8312	20067	1.89%	0.241%
42	7.311	1011	1021	1033	rBV	234615	502527	47.24%	6.045%
43	7.470	1045	1047	1049	rBV2	901	914	0.09%	0.011%
44	7.512	1052	1054	1055	rVV	812	491	0.05%	0.006%
45	7.531	1055	1057	1062	rVB2	703	822	0.08%	0.010%
46	7.616	1068	1071	1073	rVB2	297	346	0.03%	0.004%
47	7.653	1073	1077	1079	rBV	465	786	0.07%	0.009%
48	7.671	1079	1080	1083	rVB	531	414	0.04%	0.005%
49	7.836	1104	1107	1108	rVV	536	469	0.04%	0.006%
50	7.933	1119	1123	1129	rVB4	1527	3148	0.30%	0.038%
51	8.098	1148	1150	1154	rVB2	400	589	0.06%	0.007%
52	8.323	1180	1187	1201	rBV	147573	252619	23.75%	3.039%
53	8.476	1209	1212	1221	rVB5	1646	3224	0.30%	0.039%
54	8.567	1226	1227	1229	rBV	366	342	0.03%	0.004%
55	8.653	1231	1241	1251	rBV	476507	754668	70.94%	9.078%
56	8.774	1259	1261	1263	rVB2	730	430	0.04%	0.005%
57	8.842	1268	1272	1274	rBV2	891	1153	0.11%	0.014%
58	8.884	1277	1279	1281	rBV	433	378	0.04%	0.005%
59	8.951	1285	1290	1303	rVV	116691	167189	15.72%	2.011%
60	9.384	1356	1361	1376	rBV	468747	658983	61.94%	7.927%
61	9.701	1409	1413	1420	rVB4	2283	4000	0.38%	0.048%
62	10.055	1465	1471	1482	rBV	551328	738845	69.45%	8.888%
63	10.164	1487	1489	1491	rVB2	669	493	0.05%	0.006%
64	10.360	1515	1521	1522	rBV3	575	861	0.08%	0.010%
65	10.646	1566	1568	1570	rVB	599	444	0.04%	0.005%
66	10.780	1587	1590	1593	rBV2	327	440	0.04%	0.005%
67	10.939	1614	1616	1618	rVB2	425	374	0.04%	0.004%
68	10.969	1618	1621	1624	rBV	454	655	0.06%	0.008%
69	11.116	1644	1645	1647	rVV	538	333	0.03%	0.004%
70	11.195	1652	1658	1668	rVV	428680	548012	51.51%	6.592%
71	11.286	1672	1673	1679	rVV2	496	592	0.06%	0.007%
72	11.372	1685	1687	1690	rBV2	342	488	0.05%	0.006%
73	11.713	1740	1743	1747	rVB3	673	902	0.08%	0.011%
74	11.902	1771	1774	1777	rBV2	515	926	0.09%	0.011%
75	12.024	1789	1794	1802	rVB	597888	684139	64.31%	8.230%
76	12.152	1812	1815	1818	rBV2	445	615	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030611.D
 Acq On : 13 Aug 2022 11:16
 Operator : JC/MD
 Sample : N4131-12DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E15DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.225	1823	1827	1828	rBV3	489	618	0.06%	0.007%
78	12.323	1837	1843	1849	rBV	554339	709270	66.67%	8.532%
79	12.548	1879	1880	1882	rBV	597	365	0.03%	0.004%
80	12.664	1895	1899	1900	rBV2	467	421	0.04%	0.005%
81	12.816	1920	1924	1926	rBV	495	605	0.06%	0.007%
82	12.859	1929	1931	1932	rVB	636	355	0.03%	0.004%
83	13.121	1970	1974	1976	rVB3	535	623	0.06%	0.007%
84	13.164	1979	1981	1983	rVB2	574	387	0.04%	0.005%
85	13.182	1983	1984	1987	rBV2	370	368	0.03%	0.004%
86	13.207	1987	1988	1990	rBV	393	339	0.03%	0.004%
87	13.572	2045	2048	2049	rBV	298	351	0.03%	0.004%
88	13.755	2075	2078	2079	rBV	278	330	0.03%	0.004%
89	13.981	2111	2115	2118	rBV2	428	690	0.06%	0.008%
90	14.133	2138	2140	2142	rVB	1058	794	0.07%	0.010%
91	14.206	2150	2152	2154	rBV2	511	505	0.05%	0.006%
92	14.255	2159	2160	2163	rBV	319	379	0.04%	0.005%
93	14.359	2175	2177	2179	rBV	438	391	0.04%	0.005%
94	14.444	2190	2191	2193	rBV2	550	352	0.03%	0.004%
95	14.938	2270	2272	2273	rVB	679	336	0.03%	0.004%
96	15.633	2384	2386	2387	rBV	817	583	0.05%	0.007%
97	15.718	2397	2400	2401	rBV3	890	998	0.09%	0.012%
98	15.761	2405	2407	2409	rVV	599	474	0.04%	0.006%
99	16.352	2502	2504	2507	rBV4	622	740	0.07%	0.009%
100	16.383	2507	2509	2511	rBV2	1035	911	0.09%	0.011%




Sum of corrected areas: 8312795

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030611.D
Acq On : 13 Aug 2022 11:16
Operator : JC/MD
Sample : N4131-12DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E15DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

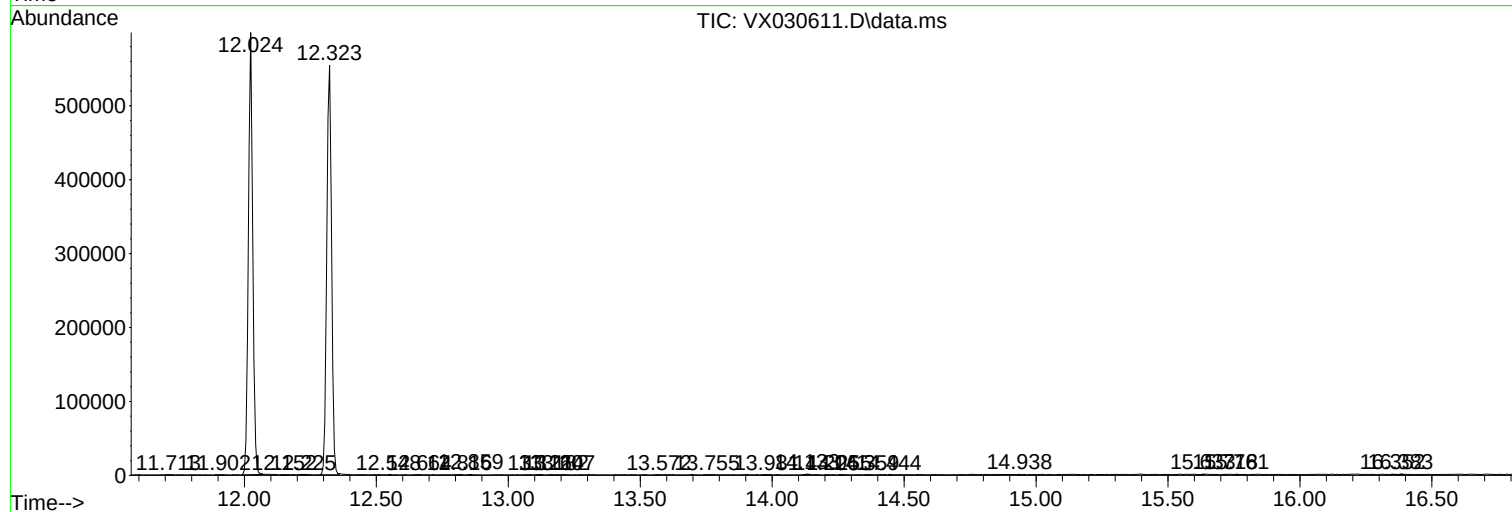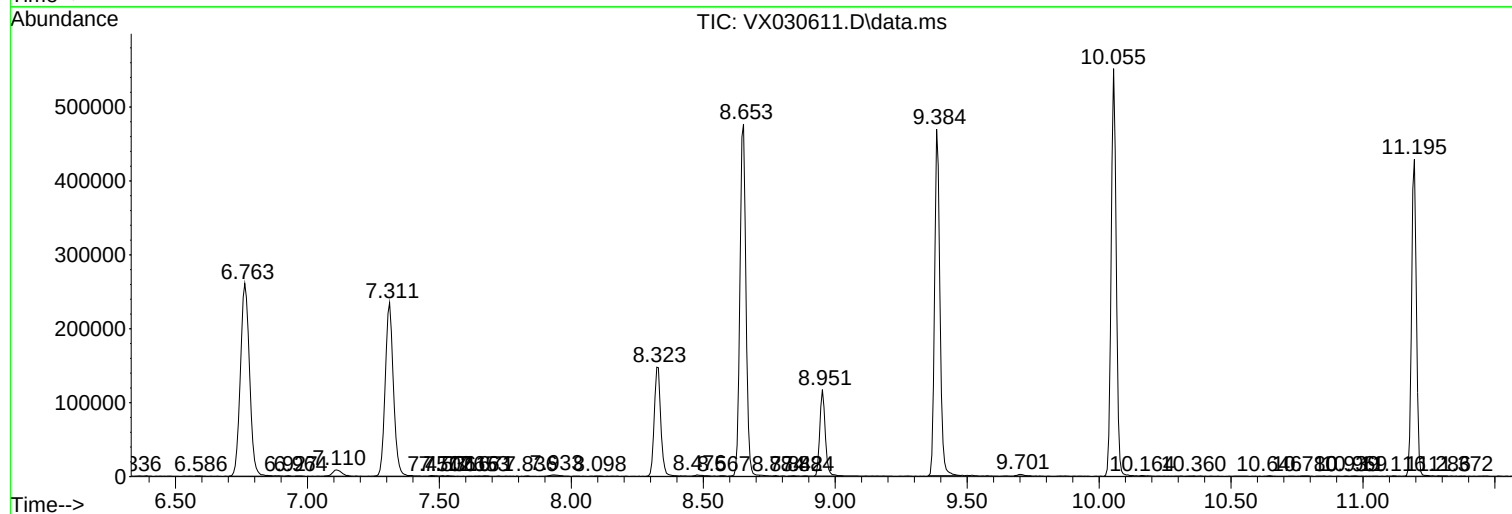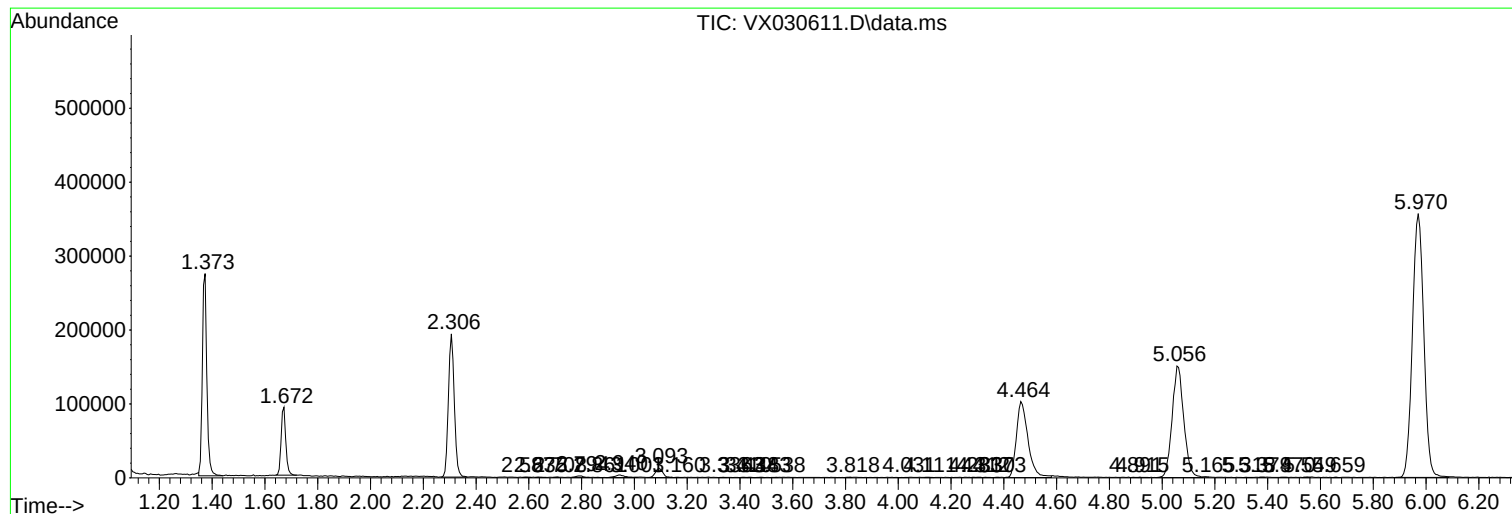

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030611.D
Acq On : 13 Aug 2022 11:16
Operator : JC/MD
Sample : N4131-12DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E15DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030611.D
Acq On : 13 Aug 2022 11:16
Operator : JC/MD
Sample : N4131-12DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E15DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc