

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030613.D
 Acq On : 13 Aug 2022 12:13
 Operator : JC/MD
 Sample : N4131-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030613.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	203518	240290	22.93%	2.911%
2	1.666	91	95	104	rVB	88502	115765	11.05%	1.403%
3	2.307	194	200	209	rBV	193515	293101	27.97%	3.551%
4	2.392	211	214	219	rBV3	888	1587	0.15%	0.019%
5	2.508	230	233	237	rBV2	772	1133	0.11%	0.014%
6	2.654	252	257	258	rBV2	460	500	0.05%	0.006%
7	2.672	258	260	262	rBV2	365	394	0.04%	0.005%
8	2.776	276	277	279	rBV2	442	371	0.04%	0.004%
9	2.995	310	313	319	rVB3	501	953	0.09%	0.012%
10	3.099	321	330	337	rBV	10684	21771	2.08%	0.264%
11	3.258	353	356	358	rBV	284	370	0.04%	0.004%
12	3.471	389	391	394	rBV	485	427	0.04%	0.005%
13	3.599	411	412	414	rBV	569	388	0.04%	0.005%
14	3.825	446	449	452	rVB	471	598	0.06%	0.007%
15	4.014	478	480	483	rVV2	372	426	0.04%	0.005%
16	4.068	486	489	490	rVB2	510	409	0.04%	0.005%
17	4.087	490	492	493	rBV	515	348	0.03%	0.004%
18	4.306	525	528	530	rBV2	503	613	0.06%	0.007%
19	4.477	544	556	573	rBV2	132632	476649	45.49%	5.775%
20	4.782	604	606	610	rBV2	296	459	0.04%	0.006%
21	4.849	612	617	618	rBV3	451	591	0.06%	0.007%
22	4.867	618	620	623	rVB2	442	424	0.04%	0.005%
23	5.068	640	653	670	rBV	144303	453014	43.23%	5.489%
24	5.361	698	701	702	rBV2	462	546	0.05%	0.007%
25	5.385	702	705	706	rBV2	895	879	0.08%	0.011%
26	5.477	717	720	722	rBV2	409	509	0.05%	0.006%
27	5.562	729	734	740	rVB4	1372	2796	0.27%	0.034%
28	5.696	752	756	760	rVB2	474	660	0.06%	0.008%
29	5.751	763	765	769	rVB2	306	395	0.04%	0.005%
30	5.800	769	773	775	rVB2	456	437	0.04%	0.005%
31	5.971	790	801	819	rBV3	355898	1047841	100.00%	12.696%
32	6.184	834	836	839	rVB3	444	360	0.03%	0.004%
33	6.221	839	842	845	rVB2	422	496	0.05%	0.006%
34	6.349	859	863	864	rBV2	525	635	0.06%	0.008%
35	6.373	865	867	868	rVV	634	395	0.04%	0.005%
36	6.763	921	931	943	rBV	253424	599493	57.21%	7.263%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030613.D
 Acq On : 13 Aug 2022 12:13
 Operator : JC/MD
 Sample : N4131-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.031	974	975	979	rVB3	416	352	0.03%	0.004%
38	7.117	981	989	998	rVV7	6914	17289	1.65%	0.209%
39	7.312	1012	1021	1035	rBV	233171	507194	48.40%	6.145%
40	7.824	1104	1105	1108	rVB	482	360	0.03%	0.004%
41	7.860	1108	1111	1114	rVB2	423	578	0.06%	0.007%
42	7.891	1114	1116	1118	rBV2	390	475	0.05%	0.006%
43	7.934	1118	1123	1129	rBV5	1793	3582	0.34%	0.043%
44	8.056	1139	1143	1144	rBV2	361	350	0.03%	0.004%
45	8.074	1144	1146	1149	rBV2	332	345	0.03%	0.004%
46	8.269	1176	1178	1181	rBV2	400	365	0.03%	0.004%
47	8.324	1181	1187	1199	rBV	150162	250035	23.86%	3.029%
48	8.476	1210	1212	1214	rBV2	1296	1532	0.15%	0.019%
49	8.653	1234	1241	1249	rBV	467318	744252	71.03%	9.017%
50	8.848	1271	1273	1276	rBV2	642	684	0.07%	0.008%
51	8.952	1282	1290	1297	rBV2	113068	167293	15.97%	2.027%
52	9.189	1327	1329	1332	rBV3	372	396	0.04%	0.005%
53	9.385	1355	1361	1376	rBV	463481	663367	63.31%	8.037%
54	9.708	1412	1414	1416	rBV	477	504	0.05%	0.006%
55	9.756	1419	1422	1423	rBV2	564	368	0.04%	0.004%
56	9.781	1423	1426	1428	rBV2	385	450	0.04%	0.005%
57	9.842	1435	1436	1439	rBV2	535	473	0.05%	0.006%
58	10.055	1465	1471	1485	rVV	534536	714192	68.16%	8.653%
59	10.403	1526	1528	1532	rVB2	454	581	0.06%	0.007%
60	10.506	1542	1545	1549	rBV2	498	780	0.07%	0.009%
61	10.811	1592	1595	1599	rBV3	470	799	0.08%	0.010%
62	11.018	1627	1629	1631	rBV	549	542	0.05%	0.007%
63	11.195	1652	1658	1668	rVV	447365	556869	53.14%	6.747%
64	11.262	1668	1669	1672	rVB2	607	439	0.04%	0.005%
65	11.403	1689	1692	1693	rBV2	415	398	0.04%	0.005%
66	11.762	1747	1751	1753	rBV2	795	835	0.08%	0.010%
67	11.811	1756	1759	1761	rBV2	325	399	0.04%	0.005%
68	11.896	1771	1773	1775	rVB	376	351	0.03%	0.004%
69	11.927	1775	1778	1779	rBV	363	445	0.04%	0.005%
70	12.024	1789	1794	1806	rVB	522861	642984	61.36%	7.790%
71	12.226	1823	1827	1830	rBV3	1426	1970	0.19%	0.024%
72	12.323	1837	1843	1850	rBV	525577	689407	65.79%	8.353%
73	12.530	1875	1877	1883	rBV3	502	707	0.07%	0.009%
74	12.634	1892	1894	1901	rVB2	506	879	0.08%	0.011%
75	12.707	1903	1906	1908	rBV2	728	662	0.06%	0.008%
76	12.872	1929	1933	1936	rVB3	535	852	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030613.D
 Acq On : 13 Aug 2022 12:13
 Operator : JC/MD
 Sample : N4131-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.902	1936	1938	1941	rBV2	336	367	0.04%	0.004%
78	13.079	1964	1967	1969	rBV2	325	430	0.04%	0.005%
79	13.225	1987	1991	1996	rVB2	457	705	0.07%	0.009%
80	13.500	2034	2036	2037	rVV	557	343	0.03%	0.004%
81	13.542	2041	2043	2045	rVV	514	351	0.03%	0.004%
82	13.768	2078	2080	2084	rVV	575	829	0.08%	0.010%
83	13.823	2086	2089	2092	rBV2	458	579	0.06%	0.007%
84	14.030	2120	2123	2124	rVV	449	457	0.04%	0.006%
85	14.128	2137	2139	2143	rVB	797	816	0.08%	0.010%
86	14.237	2152	2157	2158	rBV2	367	510	0.05%	0.006%
87	14.396	2181	2183	2187	rBV2	328	447	0.04%	0.005%
88	14.609	2212	2218	2222	rVB3	558	1071	0.10%	0.013%
89	14.695	2229	2232	2234	rBV2	551	650	0.06%	0.008%
90	14.743	2237	2240	2242	rBV2	496	613	0.06%	0.007%
91	15.079	2293	2295	2298	rVB2	530	534	0.05%	0.006%
92	15.109	2298	2300	2303	rBV2	413	536	0.05%	0.006%
93	15.219	2317	2318	2319	rBV	726	350	0.03%	0.004%
94	15.438	2352	2354	2356	rBV	779	349	0.03%	0.004%
95	15.780	2406	2410	2412	rBV2	754	890	0.08%	0.011%
96	16.146	2468	2470	2472	rBV2	527	614	0.06%	0.007%
97	16.280	2491	2492	2495	rVB2	654	537	0.05%	0.007%
98	16.456	2519	2521	2523	rBV2	562	361	0.03%	0.004%
99	16.615	2545	2547	2549	rBV	548	419	0.04%	0.005%
100	16.713	2561	2563	2565	rVB	877	411	0.04%	0.005%




Sum of corrected areas: 8253527

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030613.D
Acq On : 13 Aug 2022 12:13
Operator : JC/MD
Sample : N4131-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

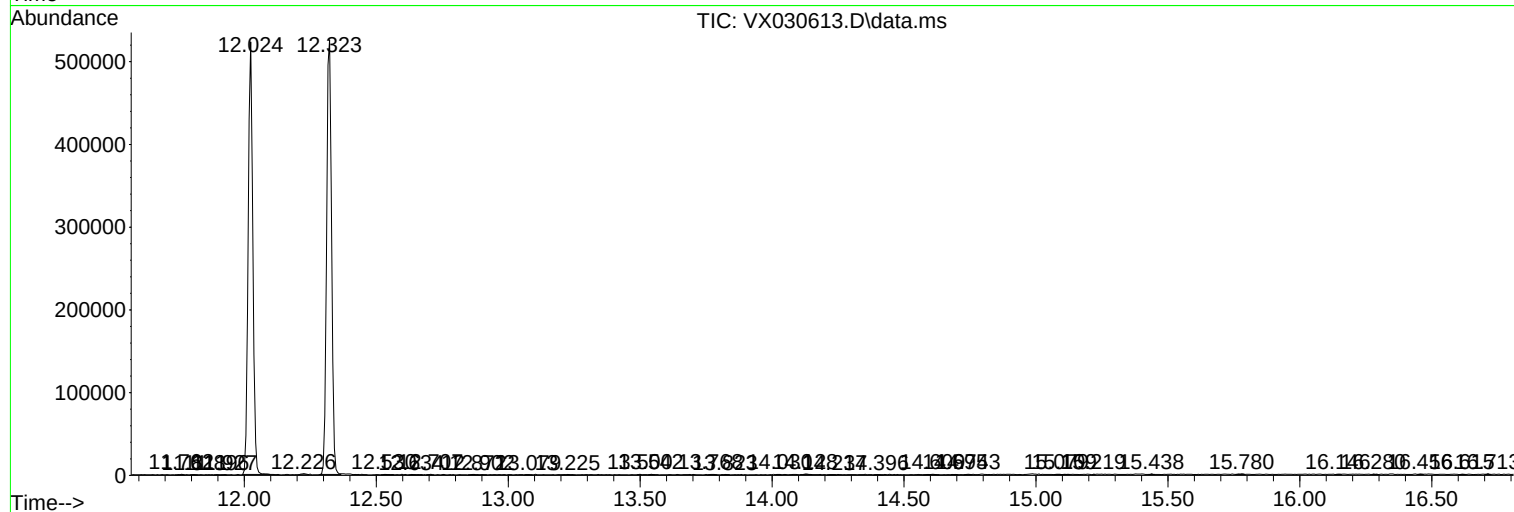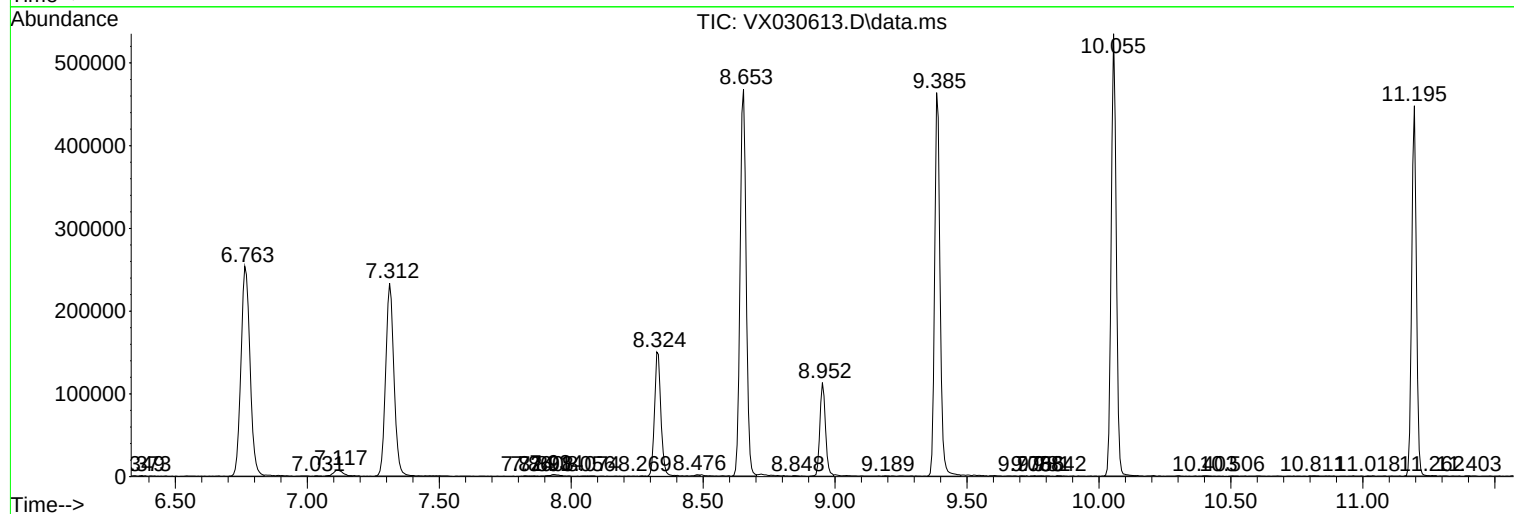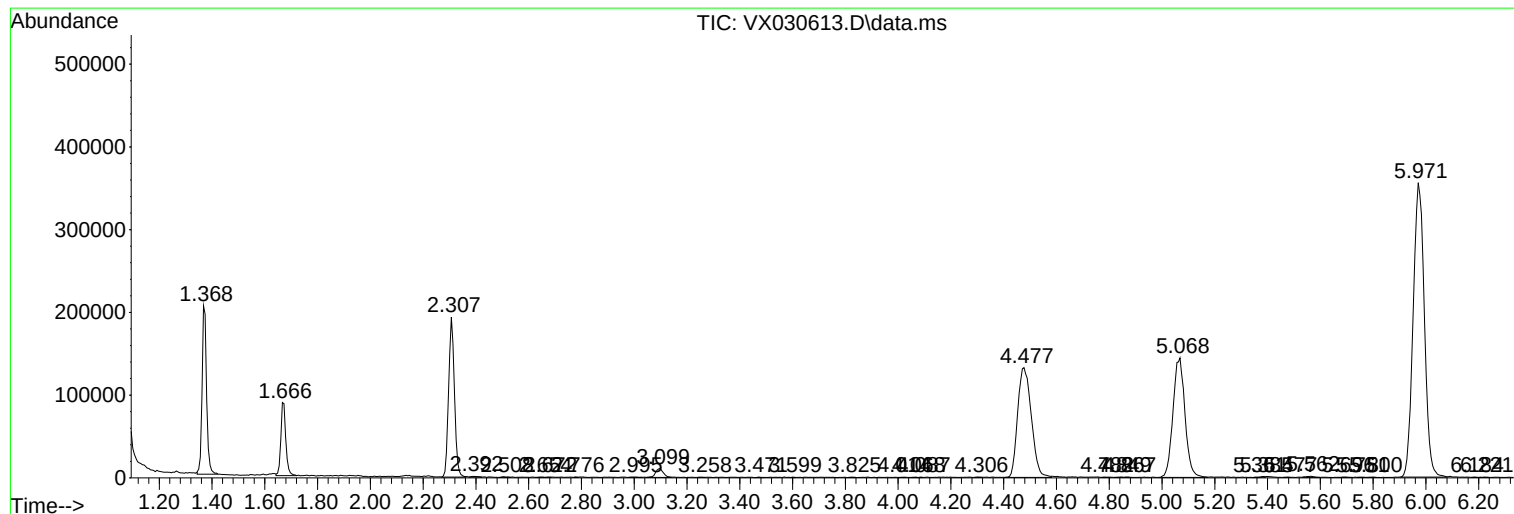

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030613.D
Acq On : 13 Aug 2022 12:13
Operator : JC/MD
Sample : N4131-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030613.D
Acq On : 13 Aug 2022 12:13
Operator : JC/MD
Sample : N4131-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc