

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030614.D
 Acq On : 13 Aug 2022 12:36
 Operator : JC/MD
 Sample : N4131-15DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E42DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	196179	234134	21.87%	2.824%
2	1.666	91	95	105	rVB	90533	116489	10.88%	1.405%
3	2.306	194	200	211	rVB	187395	292709	27.35%	3.531%
4	2.623	250	252	254	rVB2	528	361	0.03%	0.004%
5	2.733	268	270	273	rVV2	287	345	0.03%	0.004%
6	2.788	275	279	286	rVB6	2457	5391	0.50%	0.065%
7	2.886	291	295	296	rBV2	366	337	0.03%	0.004%
8	2.947	299	305	313	rVB	6779	15052	1.41%	0.182%
9	3.099	326	330	336	rVB4	1082	2192	0.20%	0.026%
10	3.160	338	340	343	rVB3	561	496	0.05%	0.006%
11	3.337	367	369	372	rBV2	431	403	0.04%	0.005%
12	3.379	374	376	379	rVB2	360	349	0.03%	0.004%
13	3.581	407	409	413	rBV	283	318	0.03%	0.004%
14	3.721	429	432	434	rVB2	411	484	0.05%	0.006%
15	3.739	434	435	440	rBV	569	610	0.06%	0.007%
16	3.916	462	464	466	rBV	382	359	0.03%	0.004%
17	3.959	466	471	474	rVV2	525	785	0.07%	0.009%
18	3.989	474	476	479	rVV2	435	438	0.04%	0.005%
19	4.105	492	495	498	rBV	344	440	0.04%	0.005%
20	4.148	500	502	505	rVB2	354	356	0.03%	0.004%
21	4.178	505	507	510	rBV2	287	325	0.03%	0.004%
22	4.471	544	555	568	rBV	114294	379540	35.46%	4.578%
23	4.849	616	617	619	rBV2	572	378	0.04%	0.005%
24	4.910	625	627	630	rBV2	391	360	0.03%	0.004%
25	5.062	640	652	667	rBV	149433	460639	43.03%	5.556%
26	5.233	678	680	684	rVB3	773	668	0.06%	0.008%
27	5.269	684	686	688	rVV3	505	343	0.03%	0.004%
28	5.361	699	701	702	rBV2	518	425	0.04%	0.005%
29	5.391	702	706	715	rVB5	1308	3152	0.29%	0.038%
30	5.464	715	718	719	rBV2	417	436	0.04%	0.005%
31	5.550	729	732	734	rBV2	1198	1503	0.14%	0.018%
32	5.611	741	742	745	rBV	317	311	0.03%	0.004%
33	5.641	745	747	750	rVB	611	518	0.05%	0.006%
34	5.781	769	770	772	rBV	454	354	0.03%	0.004%
35	5.806	772	774	776	rVB2	332	330	0.03%	0.004%
36	5.879	784	786	789	rBV	276	389	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030614.D
 Acq On : 13 Aug 2022 12:36
 Operator : JC/MD
 Sample : N4131-15DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E42DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	5.976	789	802	819	rBV2	360459	1070395	100.00%	12.912%
38	6.464	879	882	883	rVB2	379	324	0.03%	0.004%
39	6.550	893	896	898	rBV	485	547	0.05%	0.007%
40	6.568	898	899	902	rVB2	518	523	0.05%	0.006%
41	6.653	912	913	916	rBV2	458	435	0.04%	0.005%
42	6.763	922	931	943	rBV	256375	614104	57.37%	7.408%
43	7.110	982	988	1002	rVB3	10629	23533	2.20%	0.284%
44	7.312	1012	1021	1033	rBV2	237626	518687	48.46%	6.257%
45	7.476	1046	1048	1051	rVB2	670	618	0.06%	0.007%
46	7.769	1095	1096	1098	rBV	516	329	0.03%	0.004%
47	7.812	1100	1103	1105	rVV2	349	474	0.04%	0.006%
48	7.940	1119	1124	1128	rVV5	1700	3666	0.34%	0.044%
49	7.994	1131	1133	1135	rBV2	496	400	0.04%	0.005%
50	8.013	1135	1136	1138	rBV	444	371	0.03%	0.004%
51	8.330	1181	1188	1201	rVB	154964	252915	23.63%	3.051%
52	8.476	1210	1212	1221	rVB5	1511	3082	0.29%	0.037%
53	8.653	1234	1241	1252	rBV	480919	758227	70.84%	9.146%
54	8.952	1285	1290	1299	rBV	115072	170968	15.97%	2.062%
55	9.134	1319	1320	1325	rBV3	281	427	0.04%	0.005%
56	9.177	1325	1327	1328	rVV	499	347	0.03%	0.004%
57	9.384	1356	1361	1376	rVV	475698	687336	64.21%	8.291%
58	9.701	1411	1413	1418	rVB2	2260	2274	0.21%	0.027%
59	9.787	1422	1427	1428	rBV2	445	427	0.04%	0.005%
60	9.836	1433	1435	1436	rBV	424	325	0.03%	0.004%
61	9.927	1449	1450	1452	rBV	370	322	0.03%	0.004%
62	10.055	1465	1471	1484	rVB	550963	730081	68.21%	8.807%
63	10.415	1528	1530	1534	rVB2	443	380	0.04%	0.005%
64	10.659	1568	1570	1573	rVB	503	392	0.04%	0.005%
65	10.689	1573	1575	1578	rVB2	409	488	0.05%	0.006%
66	10.720	1578	1580	1582	rBV2	396	413	0.04%	0.005%
67	10.841	1597	1600	1601	rBV2	430	356	0.03%	0.004%
68	10.896	1607	1609	1610	rBV	439	361	0.03%	0.004%
69	11.091	1639	1641	1645	rVV	482	462	0.04%	0.006%
70	11.195	1652	1658	1670	rVV	437642	560348	52.35%	6.759%
71	11.378	1685	1688	1690	rVV2	369	523	0.05%	0.006%
72	11.494	1705	1707	1711	rVB	487	455	0.04%	0.005%
73	11.744	1745	1748	1750	rVB2	521	605	0.06%	0.007%
74	12.024	1788	1794	1801	rBV	523547	647172	60.46%	7.807%
75	12.231	1823	1828	1832	rBV5	1344	2479	0.23%	0.030%
76	12.323	1837	1843	1851	rBV	535848	698270	65.23%	8.423%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030614.D
 Acq On : 13 Aug 2022 12:36
 Operator : JC/MD
 Sample : N4131-15DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E42DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.500	1870	1872	1873	rBV	523	452	0.04%	0.005%
78	12.524	1874	1876	1880	rVB	727	646	0.06%	0.008%
79	12.555	1880	1881	1883	rBV	701	410	0.04%	0.005%
80	12.646	1895	1896	1898	rVB	811	440	0.04%	0.005%
81	12.676	1898	1901	1903	rBV2	586	796	0.07%	0.010%
82	12.750	1912	1913	1917	rBV	341	431	0.04%	0.005%
83	12.859	1928	1931	1936	rBV3	796	1632	0.15%	0.020%
84	12.975	1948	1950	1951	rBV	470	344	0.03%	0.004%
85	12.994	1951	1953	1955	rVV3	797	659	0.06%	0.008%
86	13.085	1967	1968	1971	rVB	626	409	0.04%	0.005%
87	13.115	1971	1973	1975	rBV	575	441	0.04%	0.005%
88	13.146	1977	1978	1981	rBV2	455	369	0.03%	0.004%
89	13.170	1981	1982	1985	rBV2	501	450	0.04%	0.005%
90	13.213	1987	1989	1990	rVB	678	409	0.04%	0.005%
91	13.231	1990	1992	1996	rBV2	347	484	0.05%	0.006%
92	13.365	2012	2014	2017	rBV	486	414	0.04%	0.005%
93	13.432	2021	2025	2027	rBV3	437	503	0.05%	0.006%
94	14.134	2135	2140	2142	rBV4	1123	1566	0.15%	0.019%
95	14.853	2256	2258	2261	rBV2	467	555	0.05%	0.007%
96	15.237	2318	2321	2326	rVB5	720	960	0.09%	0.012%
97	16.267	2488	2490	2491	rBV	625	475	0.04%	0.006%
98	16.481	2524	2525	2526	rBV	664	396	0.04%	0.005%
99	16.572	2539	2540	2543	rVB	600	432	0.04%	0.005%
100	16.694	2559	2560	2563	rBV2	713	895	0.08%	0.011%


Sum of corrected areas: 8290128

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030614.D
Acq On : 13 Aug 2022 12:36
Operator : JC/MD
Sample : N4131-15DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E42DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

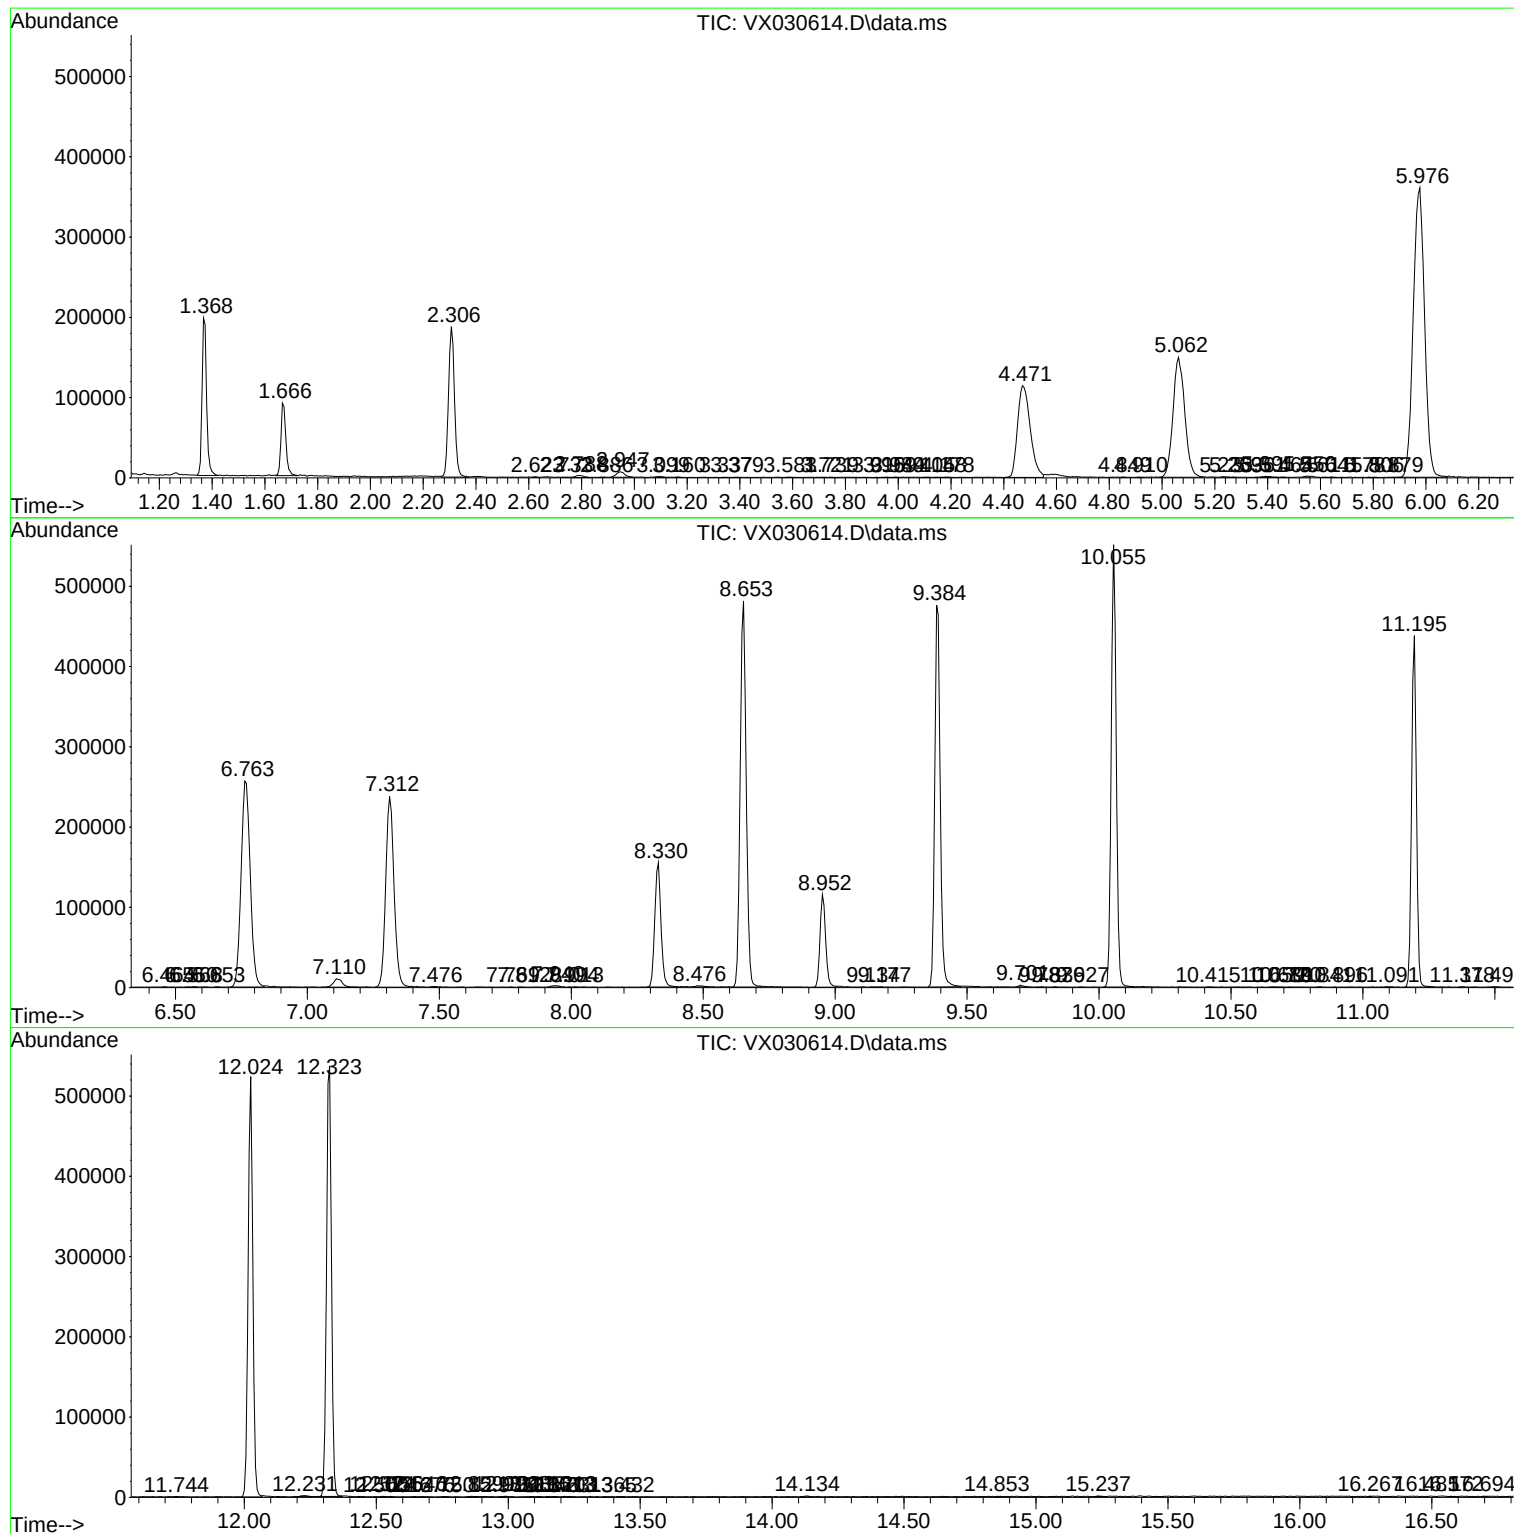

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030614.D
Acq On : 13 Aug 2022 12:36
Operator : JC/MD
Sample : N4131-15DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E42DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030614.D
Acq On : 13 Aug 2022 12:36
Operator : JC/MD
Sample : N4131-15DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E42DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------