

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030615.D
 Acq On : 13 Aug 2022 13:46
 Operator : JC/MD
 Sample : N4131-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	53	rVB	95718	99728	9.87%	1.256%
2	1.666	91	95	106	rVB	86851	108883	10.77%	1.372%
3	2.111	166	168	171	rBV2	726	521	0.05%	0.007%
4	2.306	194	200	211	rVB	180365	271383	26.86%	3.419%
5	2.501	228	232	234	rBV3	537	758	0.08%	0.010%
6	2.593	245	247	250	rVB3	381	363	0.04%	0.005%
7	2.654	255	257	259	rBV2	429	389	0.04%	0.005%
8	2.794	274	280	285	rVB5	2078	3755	0.37%	0.047%
9	2.843	285	288	289	rVB	519	385	0.04%	0.005%
10	2.946	297	305	312	rVV2	6421	14555	1.44%	0.183%
11	3.038	315	320	323	rVB2	462	648	0.06%	0.008%
12	3.300	361	363	365	rVB	468	331	0.03%	0.004%
13	3.318	365	366	369	rBV2	425	334	0.03%	0.004%
14	3.379	373	376	378	rBV2	569	544	0.05%	0.007%
15	3.477	390	392	393	rBV	384	310	0.03%	0.004%
16	3.635	416	418	421	rVV	565	451	0.04%	0.006%
17	3.903	459	462	465	rBV	205	340	0.03%	0.004%
18	4.263	517	521	523	rBV2	401	419	0.04%	0.005%
19	4.318	527	530	531	rVV	370	327	0.03%	0.004%
20	4.470	545	555	569	rBV	101575	307787	30.46%	3.878%
21	4.787	606	607	611	rVB2	642	643	0.06%	0.008%
22	4.836	613	615	618	rVB2	506	556	0.06%	0.007%
23	4.952	630	634	637	rBB	472	417	0.04%	0.005%
24	5.056	638	651	666	rBV	139322	438945	43.44%	5.530%
25	5.196	673	674	679	rBV2	444	568	0.06%	0.007%
26	5.354	698	700	701	rBV	482	477	0.05%	0.006%
27	5.427	710	712	715	rBV2	325	340	0.03%	0.004%
28	5.452	715	716	719	rVB	416	355	0.04%	0.004%
29	5.482	719	721	724	rBV	267	302	0.03%	0.004%
30	5.543	727	731	734	rBV3	1025	2083	0.21%	0.026%
31	5.610	741	742	744	rBV	370	331	0.03%	0.004%
32	5.653	748	749	754	rVB2	459	504	0.05%	0.006%
33	5.696	754	756	760	rBV2	338	593	0.06%	0.007%
34	5.818	772	776	778	rBV2	592	560	0.06%	0.007%
35	5.848	779	781	784	rVB2	442	408	0.04%	0.005%
36	5.970	788	801	821	rBV2	343720	1010545	100.00%	12.732%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030615.D
 Acq On : 13 Aug 2022 13:46
 Operator : JC/MD
 Sample : N4131-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.214	838	841	842	rBV	531	471	0.05%	0.006%
38	6.439	874	878	879	rBV	235	307	0.03%	0.004%
39	6.763	920	931	943	rBV	268937	646373	63.96%	8.143%
40	7.025	972	974	975	rVB	580	361	0.04%	0.005%
41	7.037	975	976	978	rBV	388	329	0.03%	0.004%
42	7.110	982	988	997	rVB3	8912	20810	2.06%	0.262%
43	7.311	1011	1021	1034	rVV	222708	490605	48.55%	6.181%
44	7.439	1041	1042	1044	rVB2	661	341	0.03%	0.004%
45	7.482	1044	1049	1055	rBV4	1019	2192	0.22%	0.028%
46	7.714	1085	1087	1090	rVB2	442	330	0.03%	0.004%
47	7.799	1099	1101	1104	rBV2	329	382	0.04%	0.005%
48	7.836	1105	1107	1110	rVB2	360	358	0.04%	0.005%
49	7.927	1118	1122	1132	rBV4	1949	4426	0.44%	0.056%
50	8.018	1135	1137	1140	rVB2	333	318	0.03%	0.004%
51	8.323	1181	1187	1200	rVV	145165	241917	23.94%	3.048%
52	8.482	1209	1213	1216	rBV4	1325	2132	0.21%	0.027%
53	8.646	1233	1240	1249	rBV	450610	715382	70.79%	9.013%
54	8.835	1269	1271	1272	rBV	428	350	0.03%	0.004%
55	8.951	1284	1290	1302	rBV	108186	161193	15.95%	2.031%
56	9.268	1340	1342	1347	rBV4	548	906	0.09%	0.011%
57	9.347	1354	1355	1356	rBV	435	296	0.03%	0.004%
58	9.384	1356	1361	1376	rVV	479501	662933	65.60%	8.352%
59	9.585	1392	1394	1397	rVB2	538	484	0.05%	0.006%
60	9.634	1401	1402	1404	rBV	462	367	0.04%	0.005%
61	9.701	1409	1413	1419	rVB2	2572	4004	0.40%	0.050%
62	9.774	1424	1425	1427	rBV2	564	312	0.03%	0.004%
63	9.817	1430	1432	1434	rBV	290	343	0.03%	0.004%
64	10.055	1465	1471	1482	rBV	575020	765144	75.72%	9.640%
65	10.158	1486	1488	1491	rVV2	499	491	0.05%	0.006%
66	10.439	1532	1534	1538	rVB2	393	422	0.04%	0.005%
67	10.512	1545	1546	1549	rBV	525	480	0.05%	0.006%
68	10.713	1576	1579	1581	rVB2	448	443	0.04%	0.006%
69	10.823	1595	1597	1600	rVB2	397	383	0.04%	0.005%
70	11.195	1652	1658	1667	rBV	419209	539183	53.36%	6.793%
71	11.286	1672	1673	1676	rVB	670	365	0.04%	0.005%
72	11.695	1737	1740	1743	rBV2	349	455	0.05%	0.006%
73	11.731	1745	1746	1749	rVV2	360	298	0.03%	0.004%
74	11.823	1759	1761	1765	rBV2	408	661	0.07%	0.008%
75	11.890	1771	1772	1774	rVV2	517	324	0.03%	0.004%
76	11.926	1776	1778	1781	rVB2	356	305	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030615.D
 Acq On : 13 Aug 2022 13:46
 Operator : JC/MD
 Sample : N4131-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1788	1794	1802	rBV	586236	702587	69.53%	8.852%
78	12.323	1837	1843	1854	rBV	557890	684723	67.76%	8.627%
79	12.469	1865	1867	1871	rBV2	418	545	0.05%	0.007%
80	12.579	1883	1885	1888	rBV	385	431	0.04%	0.005%
81	12.658	1897	1898	1901	rVB	695	356	0.04%	0.004%
82	12.707	1901	1906	1911	rBV2	492	1146	0.11%	0.014%
83	12.835	1925	1927	1928	rBV	503	311	0.03%	0.004%
84	13.024	1956	1958	1961	rVB	483	395	0.04%	0.005%
85	13.066	1961	1965	1967	rVB2	235	312	0.03%	0.004%
86	13.274	1996	1999	2000	rBV	365	301	0.03%	0.004%
87	13.432	2023	2025	2027	rVB	545	422	0.04%	0.005%
88	13.767	2078	2080	2083	rBV2	513	596	0.06%	0.008%
89	13.847	2092	2093	2095	rBV	494	340	0.03%	0.004%
90	13.963	2110	2112	2115	rVV	346	348	0.03%	0.004%
91	14.042	2123	2125	2127	rBV2	574	598	0.06%	0.008%
92	14.133	2136	2140	2142	rBV2	982	1311	0.13%	0.017%
93	14.237	2154	2157	2160	rBV2	614	627	0.06%	0.008%
94	14.365	2177	2178	2181	rVB	509	371	0.04%	0.005%
95	14.395	2181	2183	2187	rBV3	397	551	0.05%	0.007%
96	14.432	2187	2189	2192	rVV2	567	685	0.07%	0.009%
97	14.462	2192	2194	2196	rVV2	464	381	0.04%	0.005%
98	14.700	2231	2233	2235	rBV2	505	438	0.04%	0.006%
99	15.395	2343	2347	2350	rBV4	1153	1533	0.15%	0.019%
100	15.962	2437	2440	2445	rBV3	569	1008	0.10%	0.013%




Sum of corrected areas: 7937330

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030615.D
Acq On : 13 Aug 2022 13:46
Operator : JC/MD
Sample : N4131-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

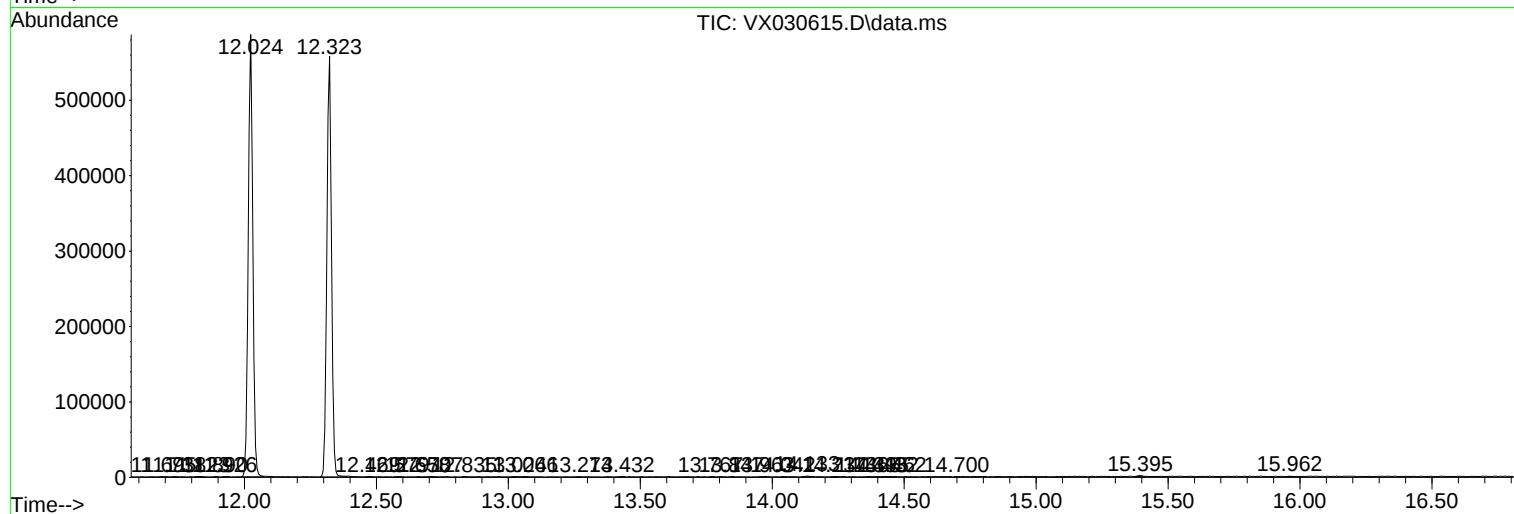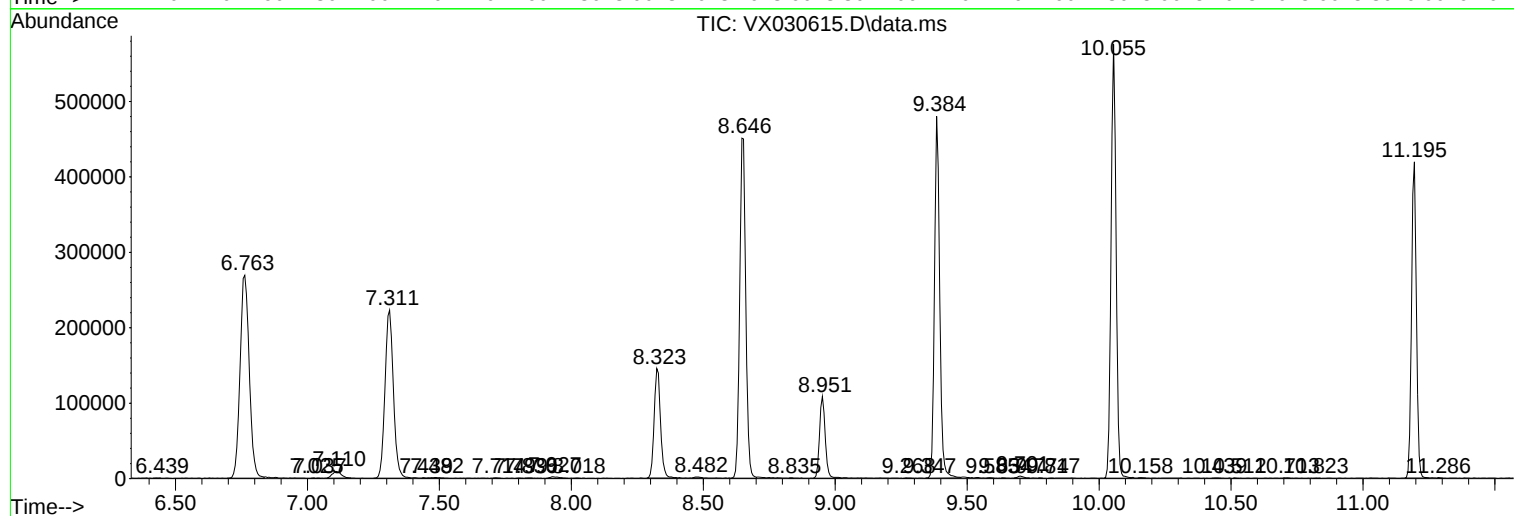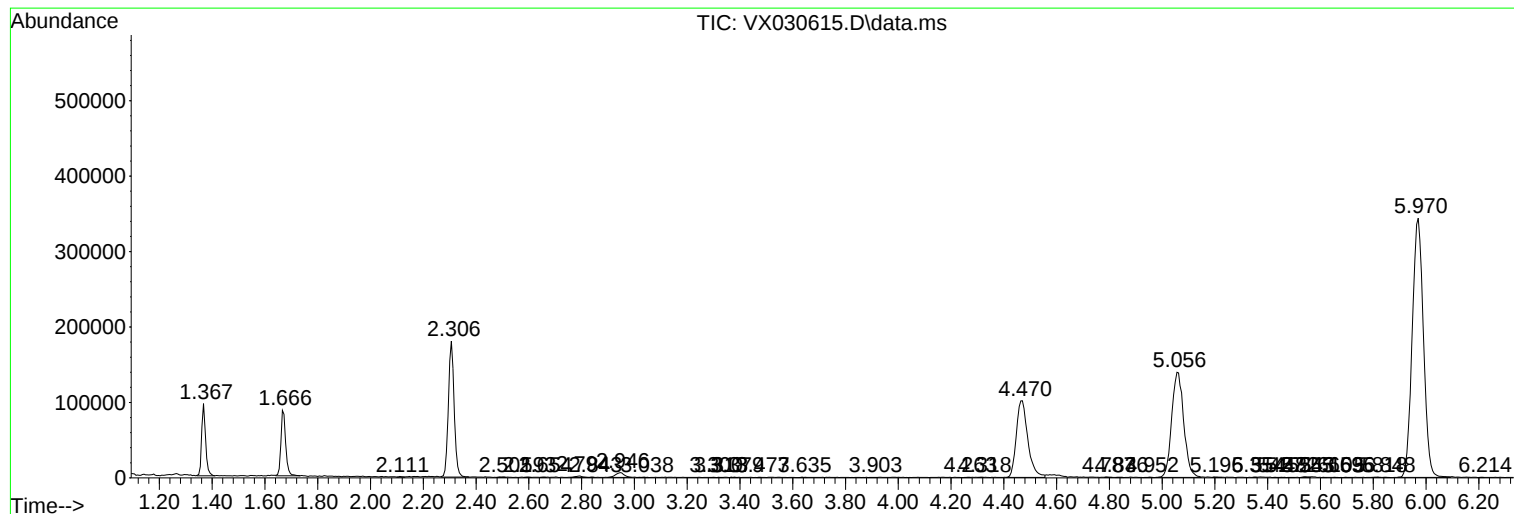

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030615.D
Acq On : 13 Aug 2022 13:46
Operator : JC/MD
Sample : N4131-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
Data File : VX030615.D
Acq On : 13 Aug 2022 13:46
Operator : JC/MD
Sample : N4131-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc