
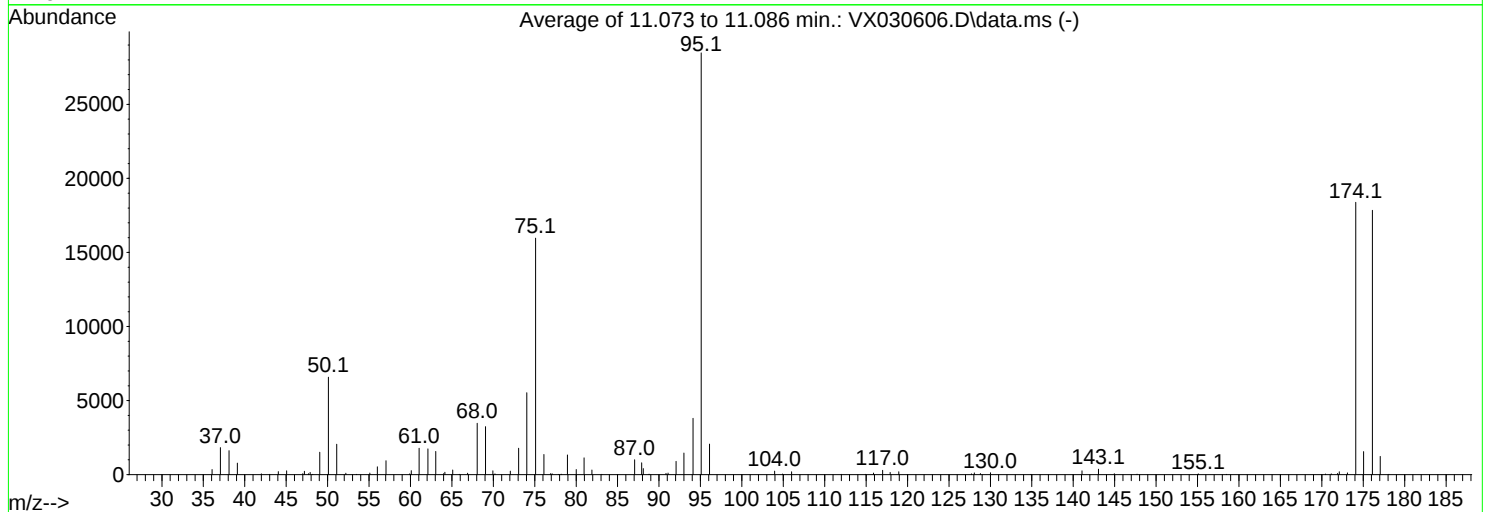


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081322\
 Data File : VX030606.D
 Acq On : 13 Aug 2022 07:58
 Operator : JC/MD
 Sample : BFB678
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB678

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Sat Aug 13 21:15:11 2022

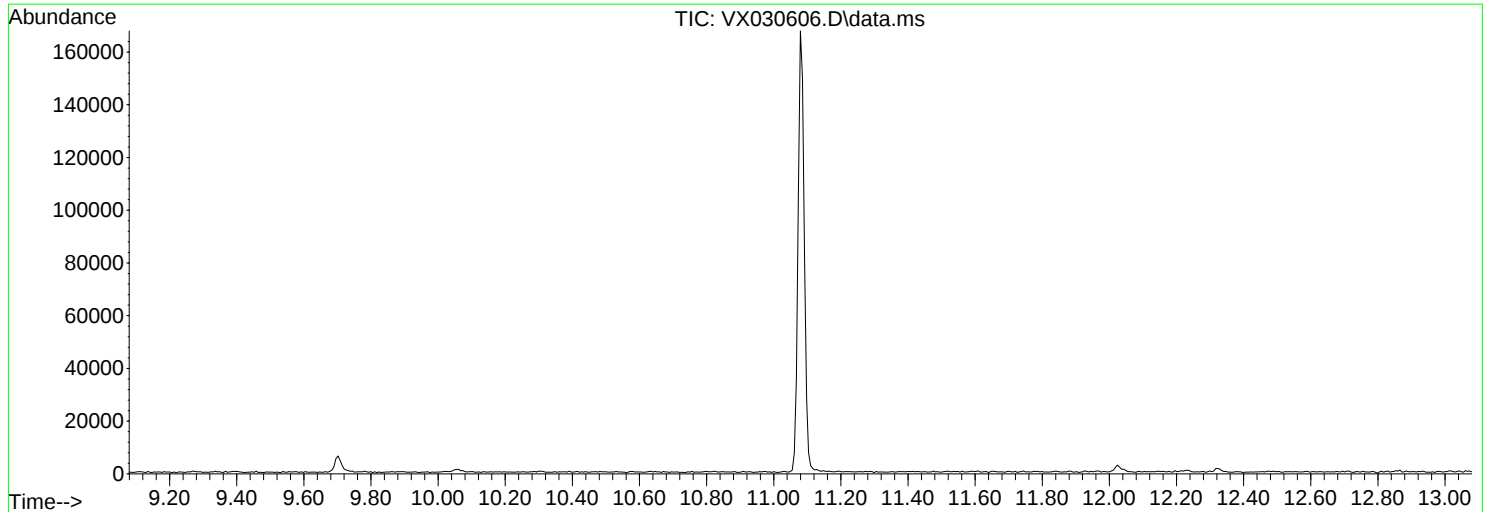

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	6576	PASS
75	95	30	80	56.1	15963	PASS
95	95	100	100	100.0	28475	PASS
96	95	5	9	7.3	2065	PASS
173	174	0.00	2	0.7	122	PASS
174	95	50	120	64.6	18384	PASS
175	174	5	9	8.5	1559	PASS
176	174	95	101	97.1	17848	PASS
177	176	5	9	6.9	1227	PASS

m/z	Abundance
40.00	419.0
44.10	252.0

Instrument :
MSVOA_X
ClientSampleId :
BFB678

m/z	Abundance
36.10	378.0
37.10	1281.0
38.10	1439.0
39.10	669.0
40.00	426.0
42.00	63.0
44.00	397.0
45.10	170.0
47.00	206.0
47.70	188.0
48.20	76.0
49.00	1307.0
50.10	5215.0
51.10	1793.0
52.20	118.0
55.10	184.0
56.10	508.0
57.10	703.0
59.90	178.0
61.00	1375.0
62.10	1398.0
63.00	991.0
64.00	184.0
65.10	187.0
66.90	78.0
68.10	3393.0
69.00	2439.0
70.00	278.0
72.10	119.0
73.10	1295.0
74.00	4235.0
75.10	12889.0
76.10	1030.0
79.00	852.0
80.10	262.0
81.00	942.0
82.00	318.0
83.10	56.0
87.10	871.0
87.90	889.0
91.10	161.0
92.00	571.0
93.00	953.0
94.10	3275.0
95.10	21088.0
96.10	1505.0
103.90	233.0
104.90	51.0
106.00	227.0
115.80	81.0
117.00	355.0
117.80	130.0
118.90	137.0
128.00	70.0
130.00	138.0
141.10	208.0
143.10	254.0
145.00	88.0
158.50	56.0
172.20	141.0
173.10	59.0
174.10	11719.0
175.10	1025.0
176.10	10593.0
177.00	1119.0
178.10	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB678

m/z	Abundance
36.00	448.0
37.10	2426.0
38.10	1954.0
39.10	982.0
40.00	418.0
42.00	89.0
43.00	79.0
44.00	387.0
45.10	291.0
47.20	390.0
47.90	288.0
49.10	1751.0
50.10	7887.0
51.10	2468.0
52.20	133.0
53.50	68.0
55.10	139.0
56.00	532.0
57.00	1270.0
60.10	417.0
61.10	2198.0
62.10	2082.0
63.10	1964.0
64.20	192.0
65.20	330.0
66.90	104.0
68.00	3802.0
69.10	3917.0
69.90	359.0
72.00	298.0
73.00	1913.0
74.10	6640.0
75.10	19336.0
76.10	1867.0
76.90	194.0
77.90	61.0
78.90	1545.0
80.00	477.0
80.90	1317.0
81.80	280.0
87.00	1057.0
87.90	1526.0
90.80	135.0
91.10	147.0
92.10	952.0
93.00	1776.0
94.10	4313.0
95.10	34952.0
96.10	2682.0
103.90	267.0
104.90	93.0
106.00	217.0
112.00	71.0
114.90	78.0
115.90	157.0
117.00	330.0
117.90	166.0
119.00	207.0
128.10	134.0
128.80	66.0
130.10	129.0
134.90	50.0
141.00	360.0
143.00	414.0
144.90	113.0
147.70	51.0
155.10	90.0
170.40	62.0
171.20	79.0
171.90	225.0
173.10	142.0
174.10	21112.0
175.10	1785.0
176.10	21472.0
177.10	1279.0

Instrument :
MSVOA_X
ClientSampleId :
BFB678

m/z	Abundance
36.10	225.0
37.00	1786.0
38.10	1471.0
39.10	675.0
40.00	408.0
44.10	578.0
45.00	311.0
47.20	300.0
47.90	170.0
49.00	1477.0
50.10	6625.0
51.10	1894.0
52.20	50.0
55.90	557.0
57.10	834.0
60.10	398.0
61.10	1764.0
62.10	1728.0
63.10	1738.0
64.10	278.0
65.00	421.0
65.90	68.0
66.90	110.0
68.00	3205.0
69.10	3365.0
69.90	134.0
70.20	154.0
72.10	289.0
73.00	2127.0
74.10	5733.0
75.10	15664.0
76.10	1194.0
77.10	206.0
78.20	104.0
78.90	1594.0
79.90	303.0
81.00	1145.0
81.90	338.0
87.10	1093.0
88.10	1218.0
88.80	91.0
90.90	118.0
92.10	1158.0
93.00	1632.0
94.10	3824.0
95.10	29384.0
96.10	2008.0
104.00	210.0
106.10	128.0
116.00	80.0
117.00	200.0
118.00	165.0
118.90	257.0
127.70	158.0
128.10	163.0
128.80	154.0
129.90	112.0
141.10	214.0
143.10	436.0
147.70	58.0
155.10	70.0
170.50	59.0
171.10	76.0
172.10	435.0
173.10	165.0
174.10	22320.0
175.00	1866.0
176.10	21480.0
177.10	1283.0

Instrument :
MSVOA_X
ClientSampleId :
BFB678