



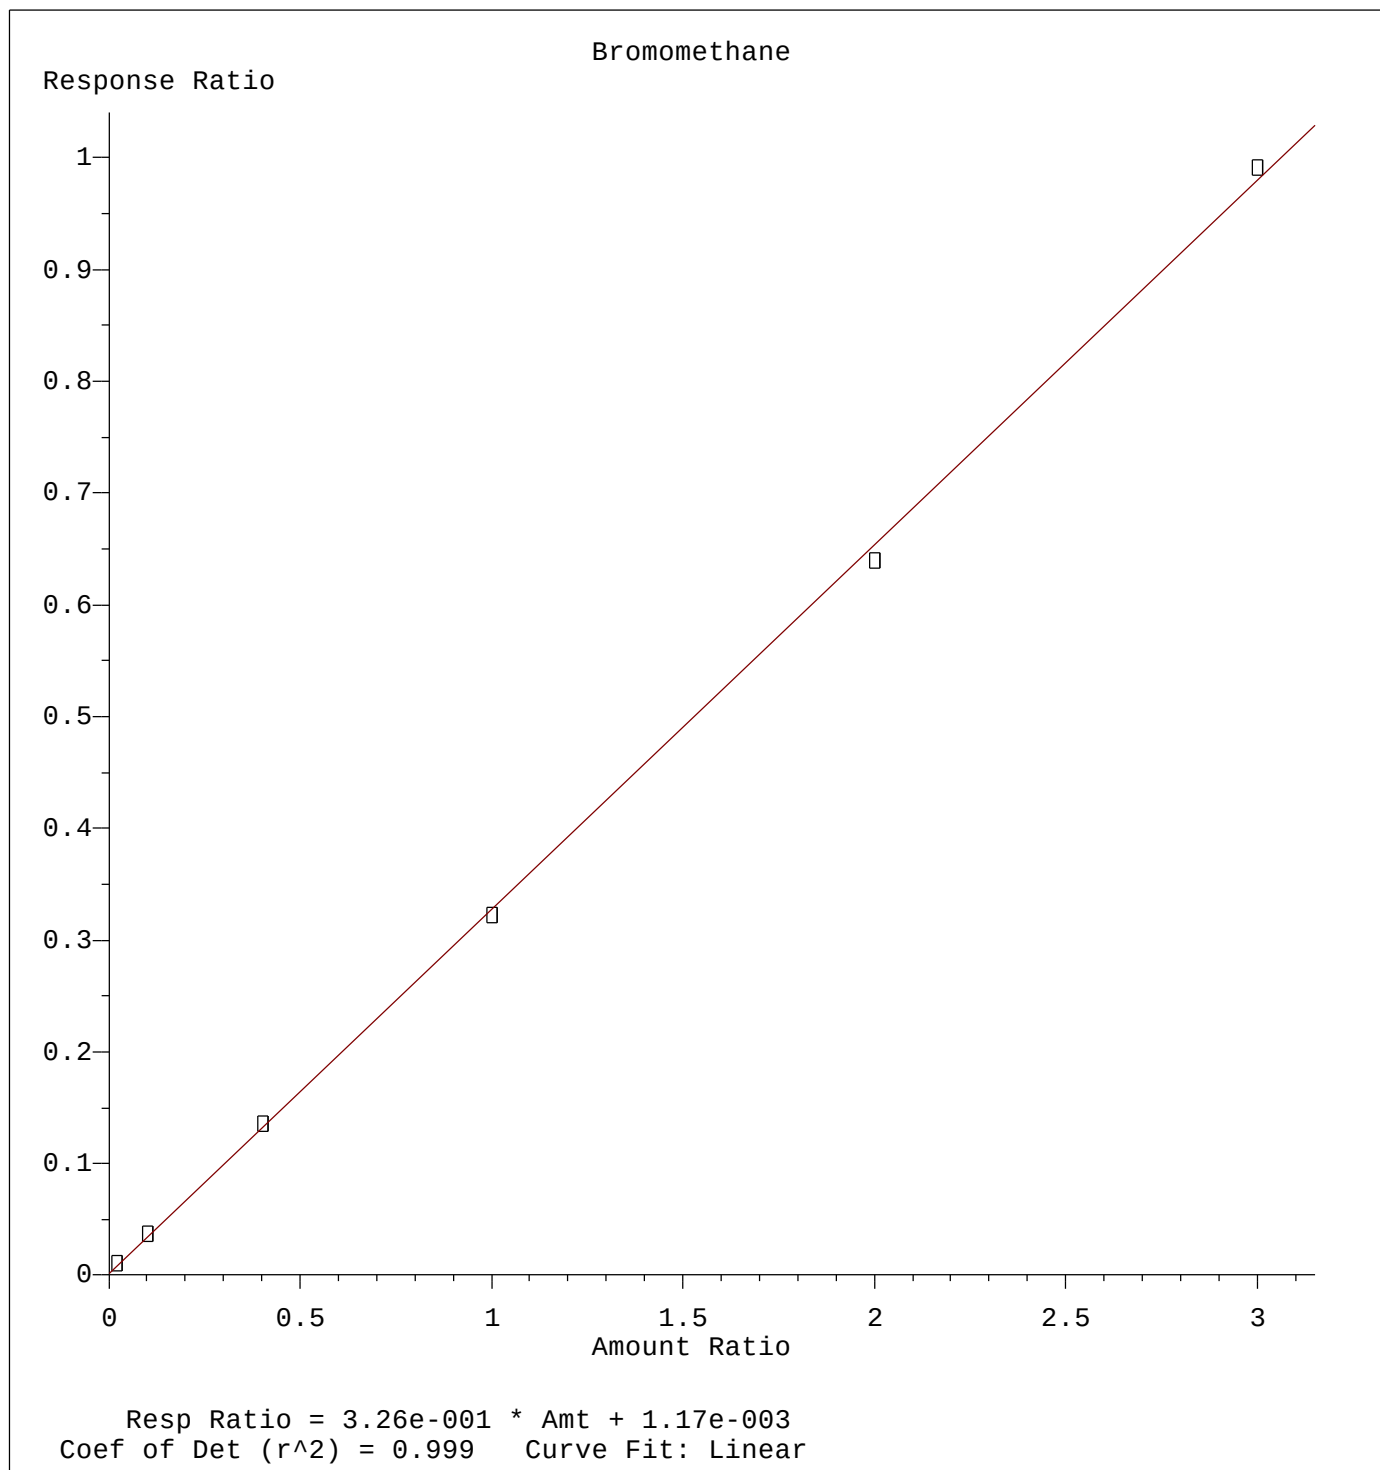

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Calibration Table Last Updated: Wed Aug 15 17:11:27 2018


Chloroethane

Response Ratio

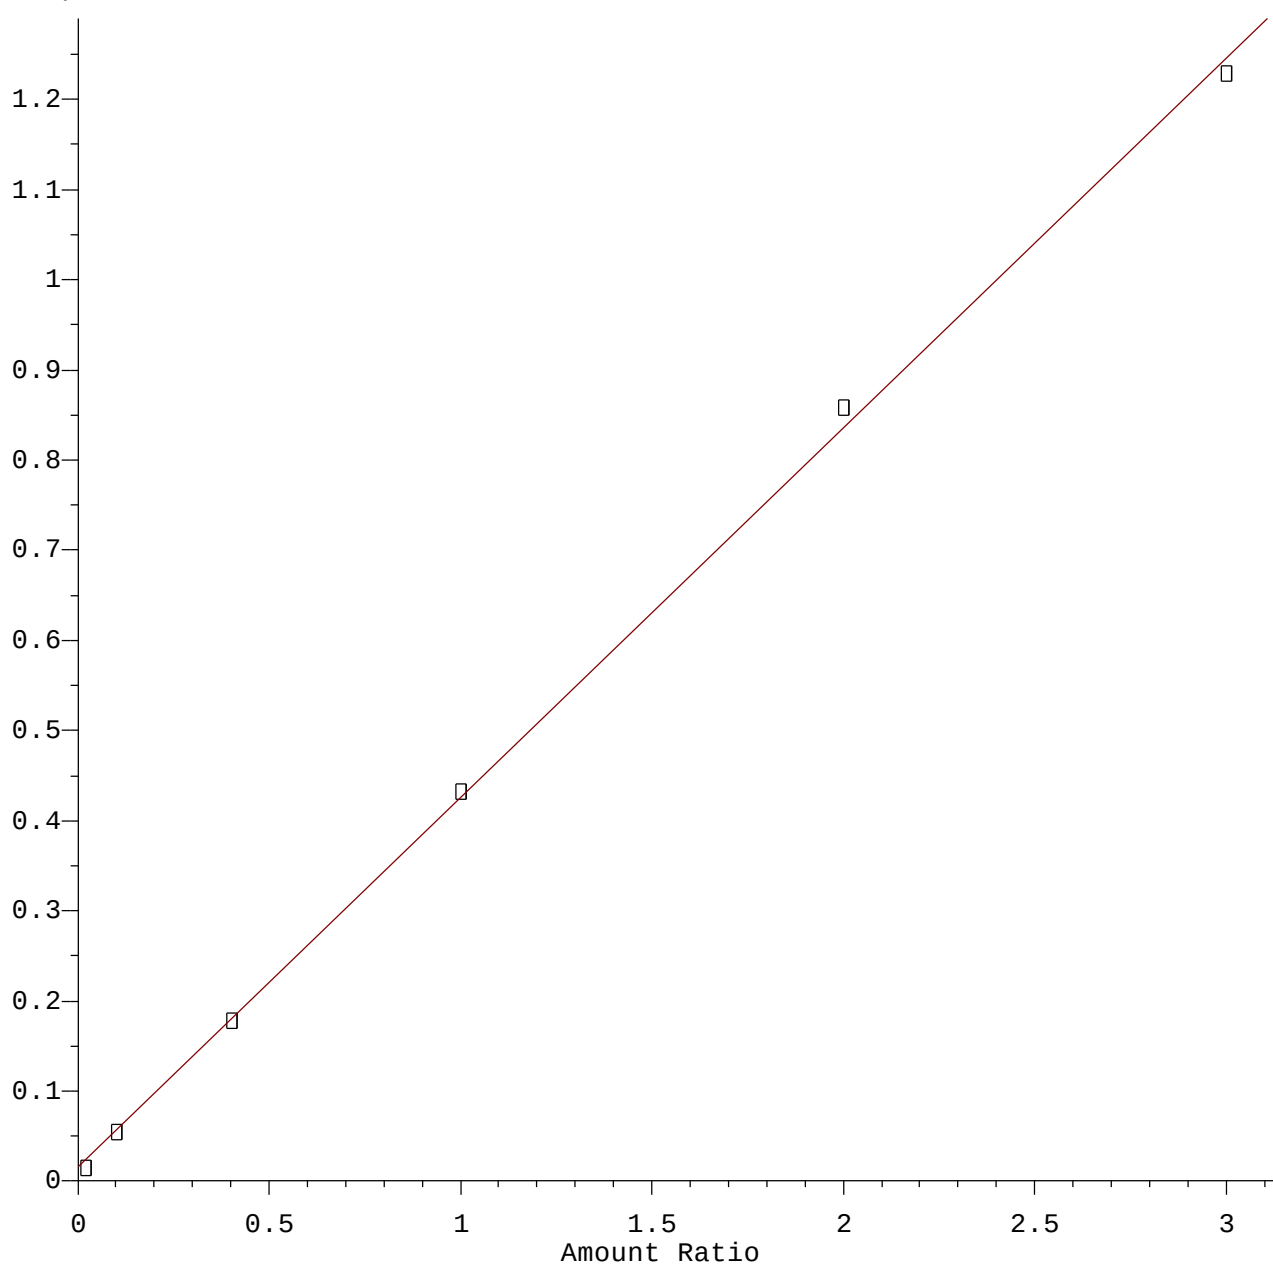

Resp Ratio = $4.10 \times 10^{-1} \times \text{Amt} + 1.51 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Calibration Table Last Updated: Wed Aug 15 17:11:27 2018

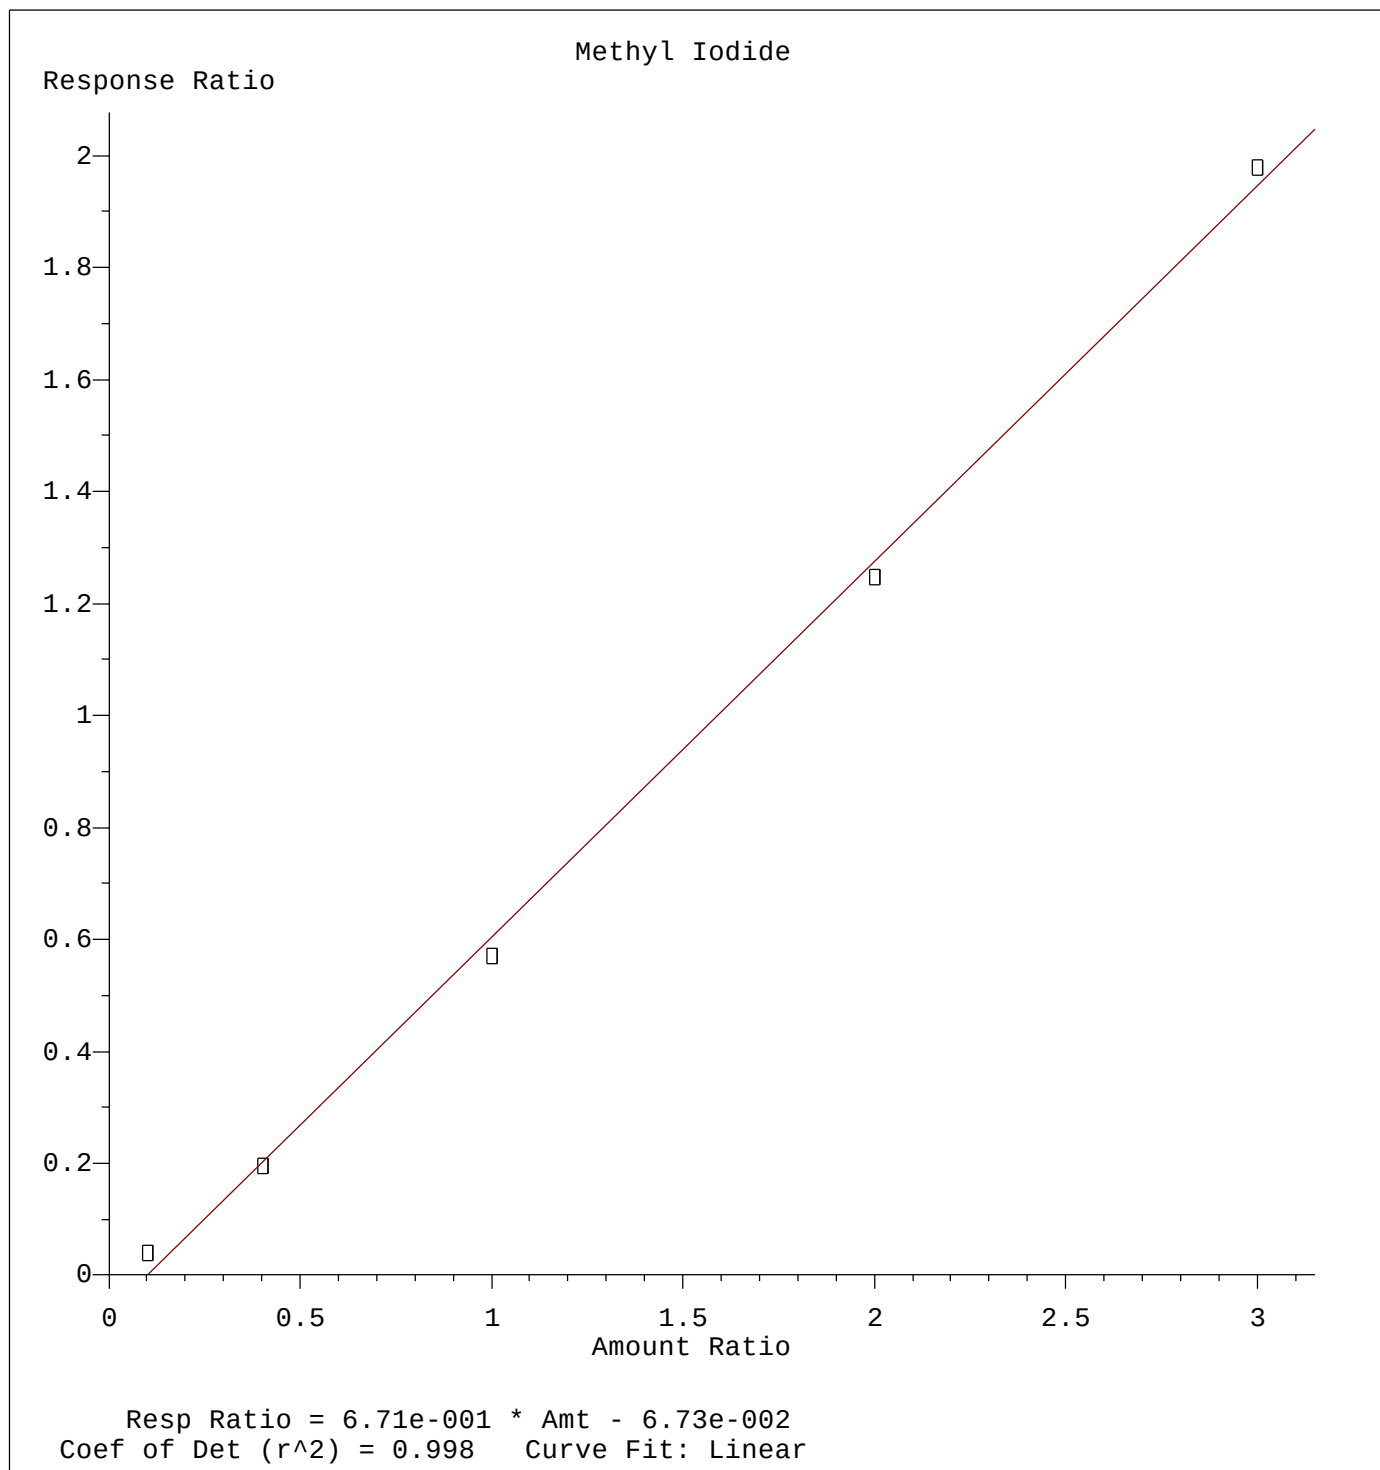

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Calibration Table Last Updated: Wed Aug 15 17:11:27 2018

Acrolein

Response Ratio

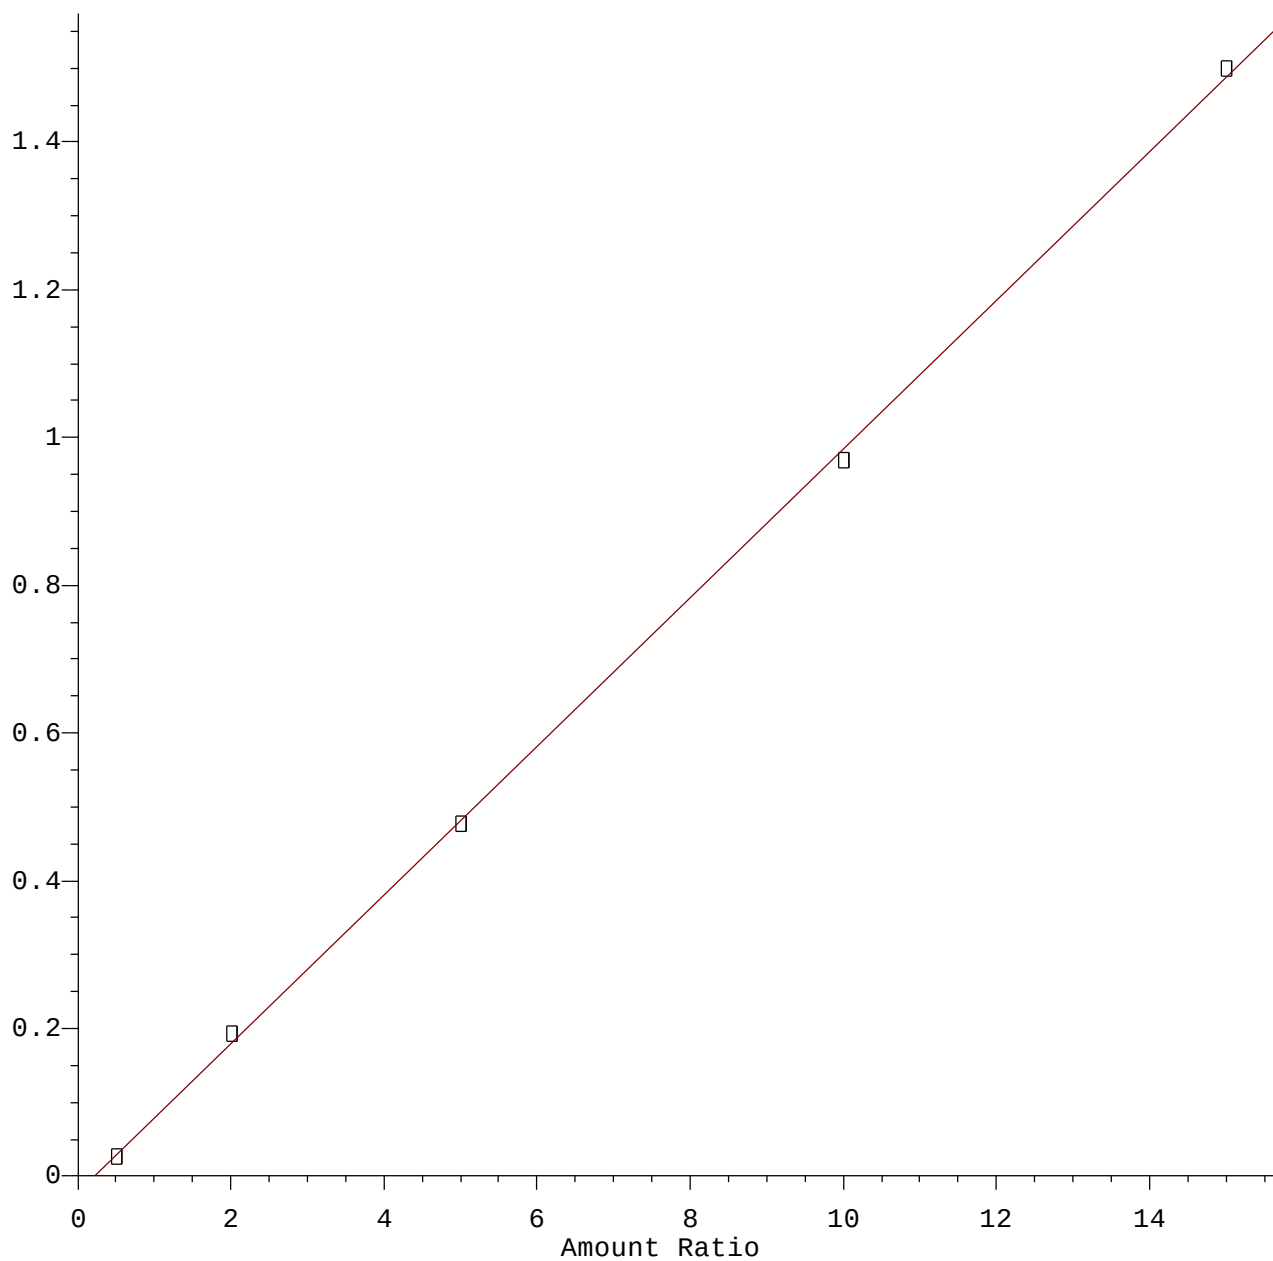


Resp Ratio = 1.01e-001 * Amt - 2.20e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Calibration Table Last Updated: Wed Aug 15 17:11:27 2018

Methylene Chloride

Response Ratio

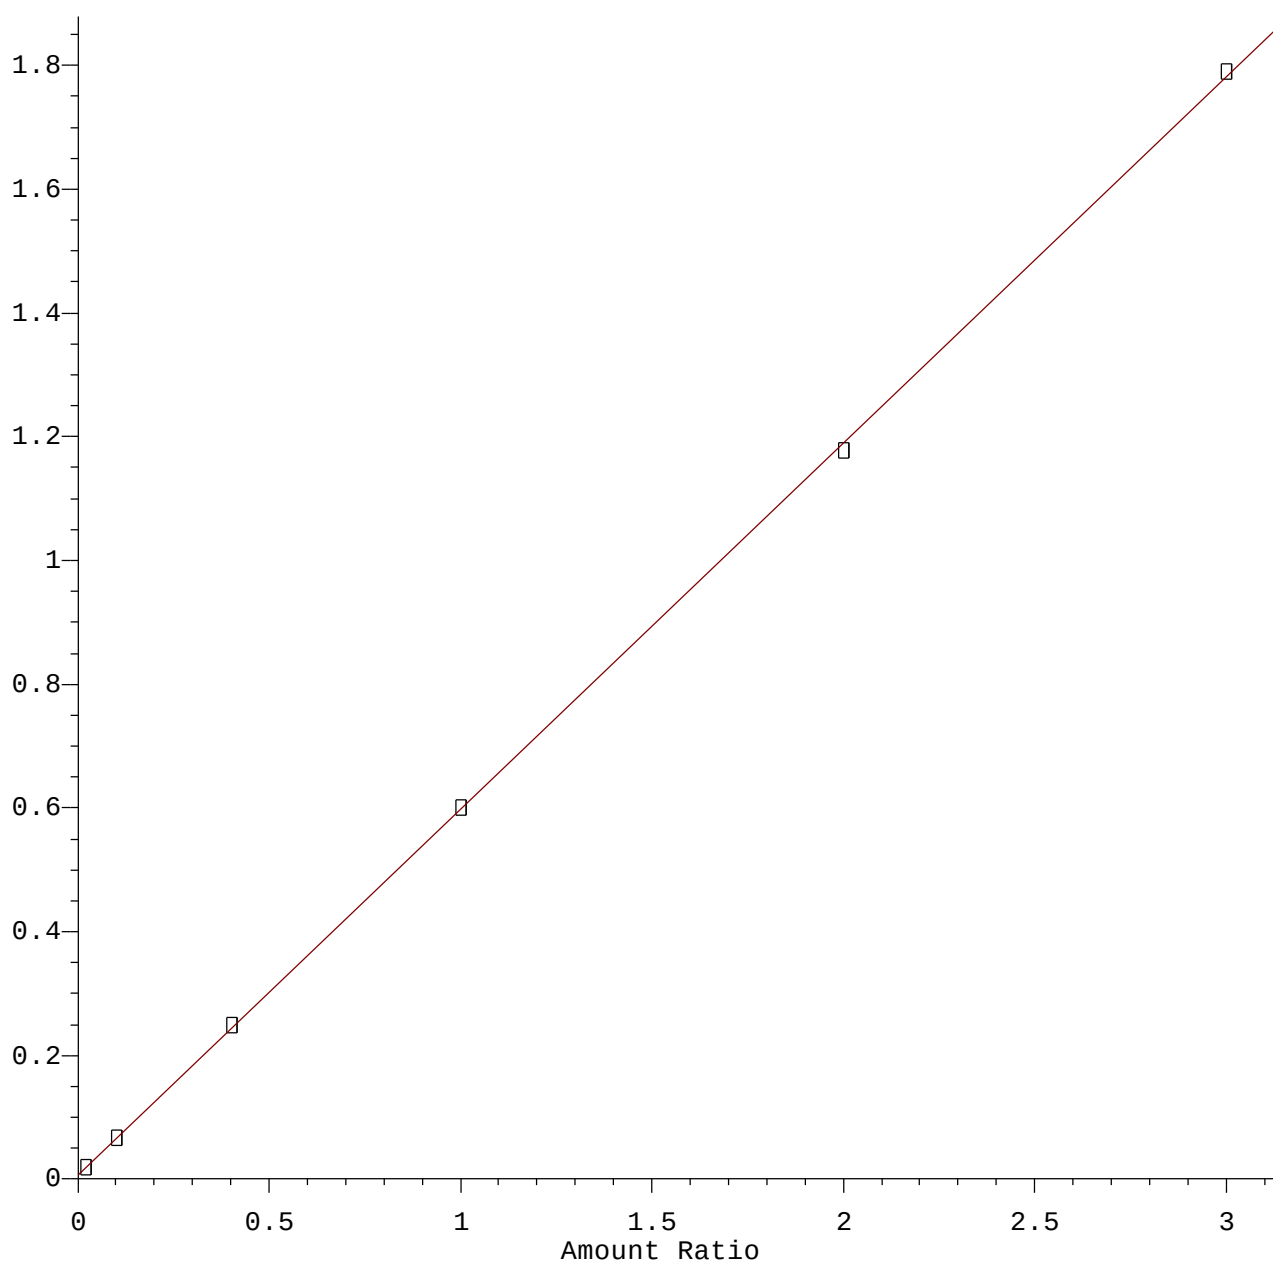


Resp Ratio = $5.91 \times 10^{-1} \times \text{Amt} + 7.27 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Calibration Table Last Updated: Wed Aug 15 17:11:27 2018

Naphthalene

Response Ratio

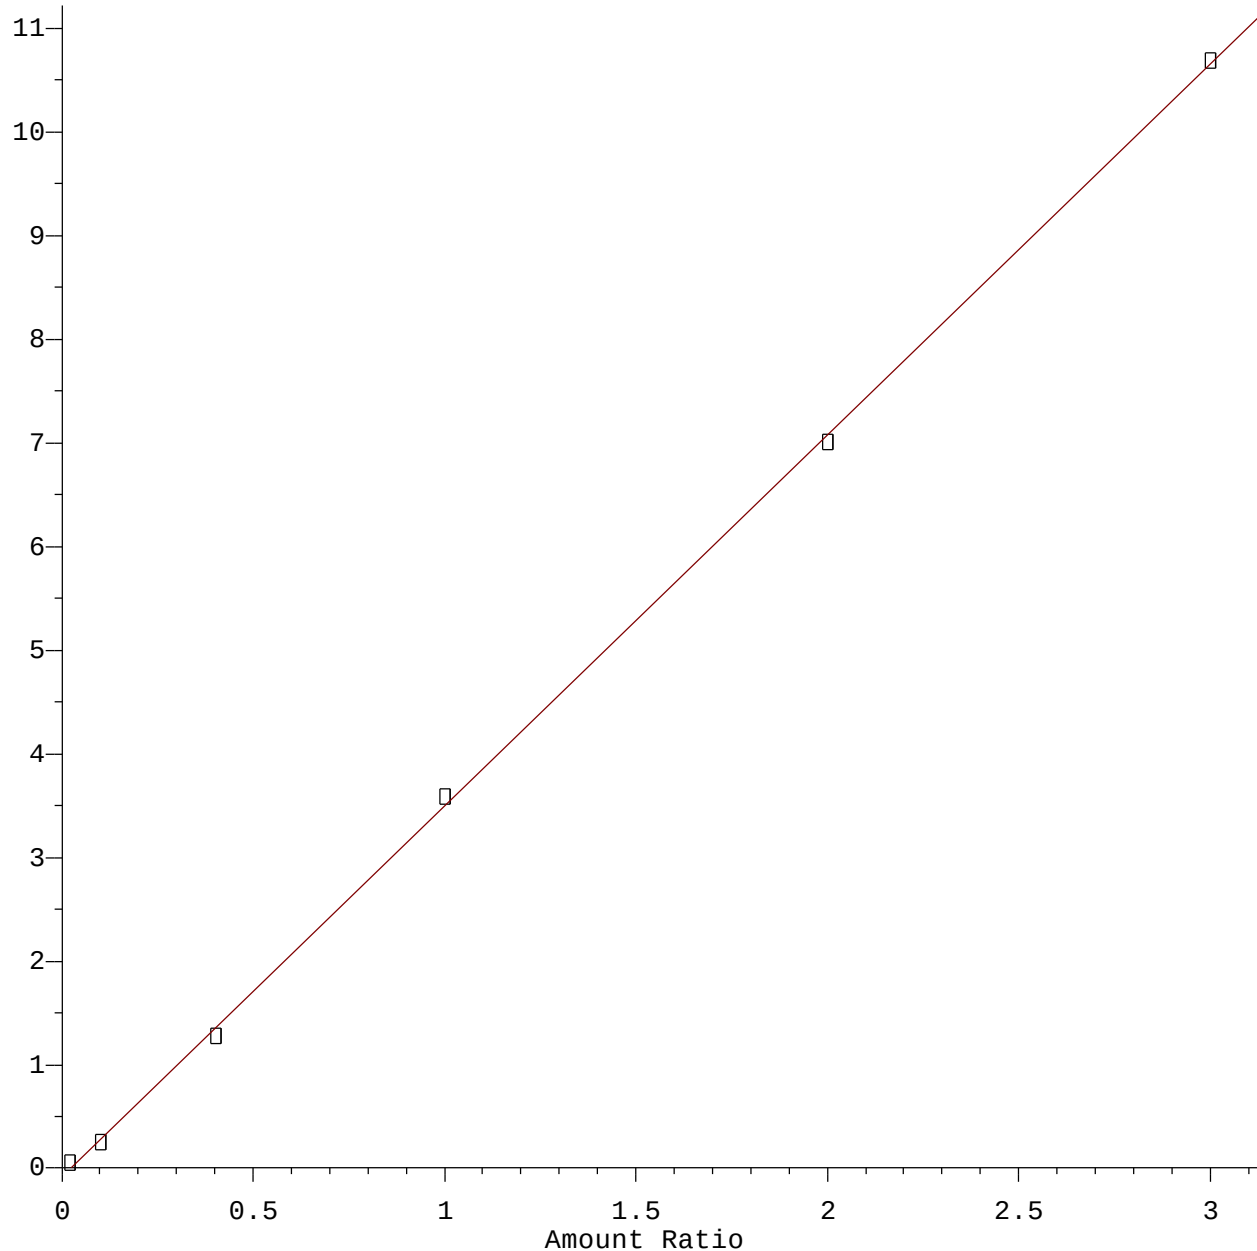

Resp Ratio = 3.58e+000 * Amt - 8.19e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Calibration Table Last Updated: Wed Aug 15 17:11:27 2018