

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081418\
 Data File : VX004062.D
 Acq On : 15 Aug 2018 07:00
 Operator : JC/MD
 Sample : J4439-11
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RB6-SRI3

Quant Time: Aug 15 15:58:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 14 13:27:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	257169	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	401882	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	378135	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	206373	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	192568	53.15	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.30%	
35) Dibromofluoromethane	5.50	113	156543	52.05	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.10%	
50) Toluene-d8	8.72	98	573936	47.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.12%	
62) 4-Bromofluorobenzene	11.14	95	194297	43.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	87.86%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX081418\
Data File : VX004062.D
Acq On : 15 Aug 2018 07:00
Operator : JC/MD
Sample : J4439-11
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RB6-SRI3

Quant Time: Aug 15 15:58:47 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 14 13:27:25 2018
Response via : Initial Calibration

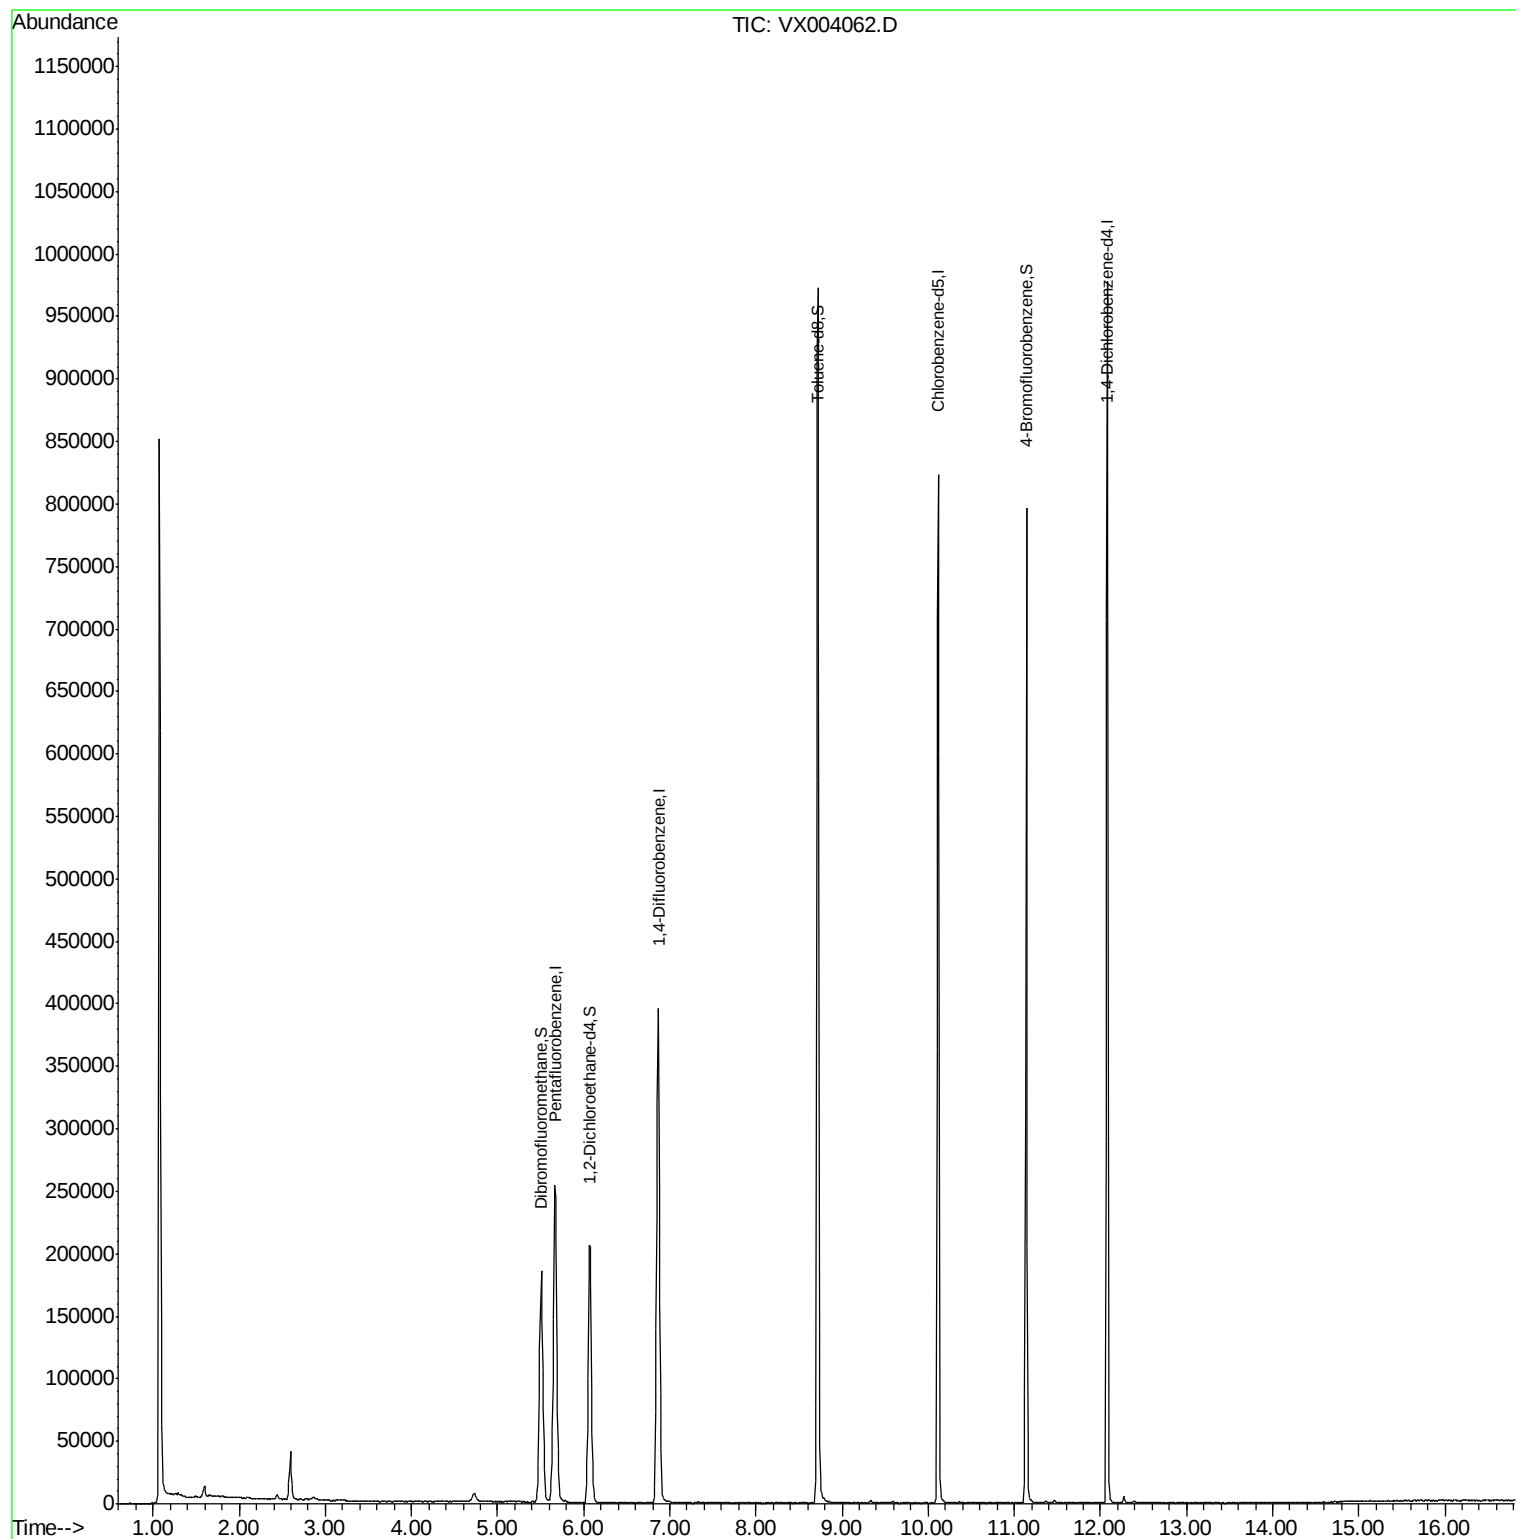



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. 0.01 min

Lab File: VX004062.D

Acq: 15 Aug 2018 07:00

Instrument :

MSVOA_X

ClientSampleId :


RB6-SRI3

Tot Ion:168 Resp: 257169

Ion Ratio Lower Upper

168 100

99 47.9 40.1 60.1

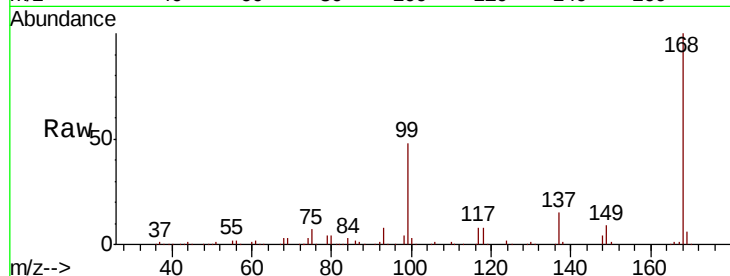

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

100000

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

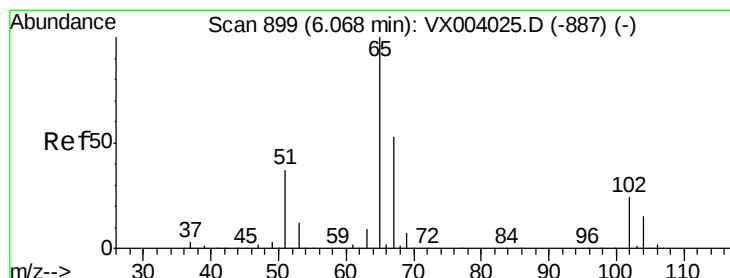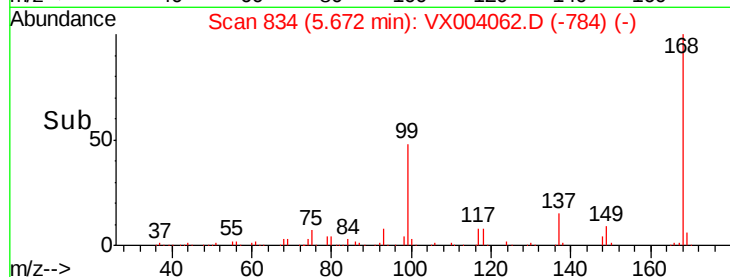

#33

1,2-Dichloroethane-d4

Concen: 53.15 ug/l

RT: 6.07 min Scan# 899

Delta R.T. -0.00 min

Lab File: VX004062.D


Acq: 15 Aug 2018 07:00

Tgt Ion: 65 Resp: 192568

Ion Ratio Lower Upper

65 100

67 52.8 0.0 105.8

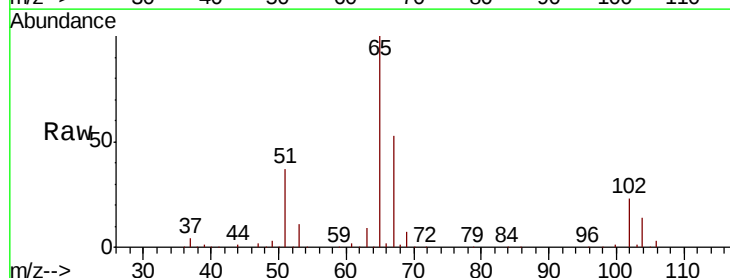

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

80000


60000


40000

20000

0

Time--> 6.00 6.10 6.20

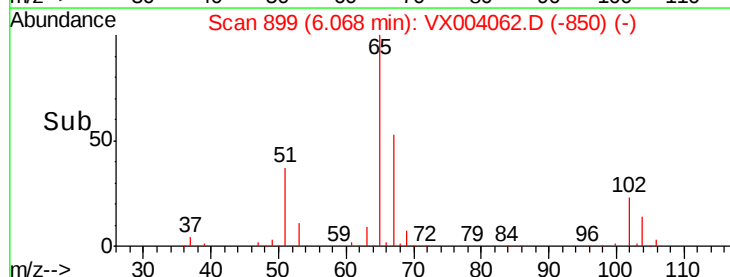


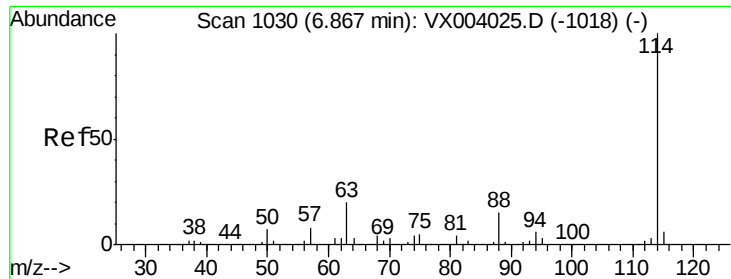




#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. -0.00 min
 Lab File: VX004062.D
 Acq: 15 Aug 2018 07:00

Instrument :
 MSVOA_X
 ClientSampleId :
 RB6-SRI3

Tot Ion:114 Resp: 401882
 Ion Ratio Lower Upper
 114 100
 63 19.0 0.0 39.0
 88 15.5 0.0 32.0

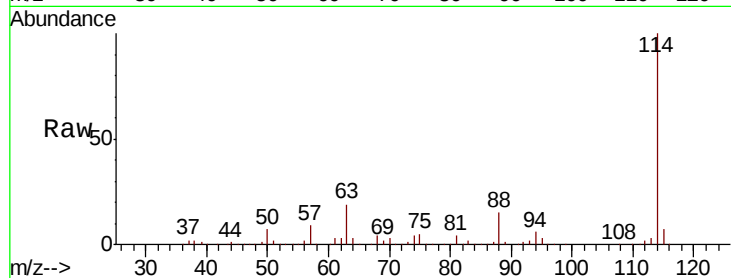


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VX0
 Ion 87.90 (87.60 to 88.60): VX0

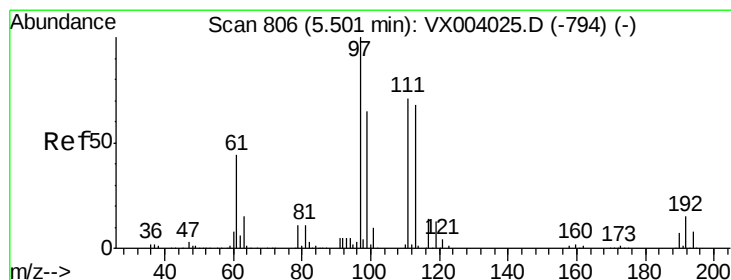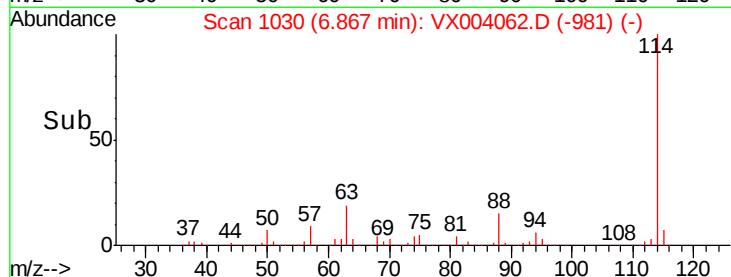
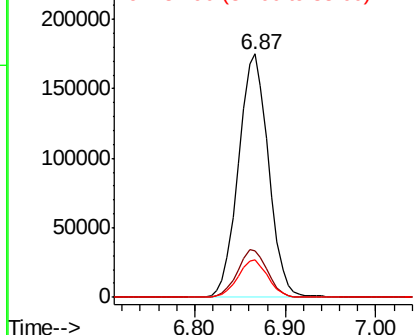



#35
 Dibromofluoromethane
 Concen: 52.05 ug/l
 RT: 5.50 min Scan# 806
 Delta R.T. -0.00 min
 Lab File: VX004062.D
 Acq: 15 Aug 2018 07:00

Tgt Ion:113 Resp: 156543
 Ion Ratio Lower Upper
 113 100
 111 102.6 82.0 123.0
 192 22.6 19.0 28.4

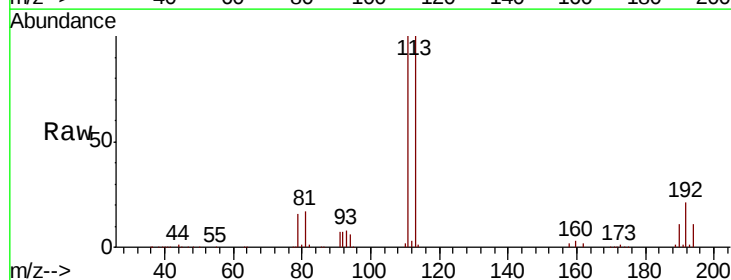

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



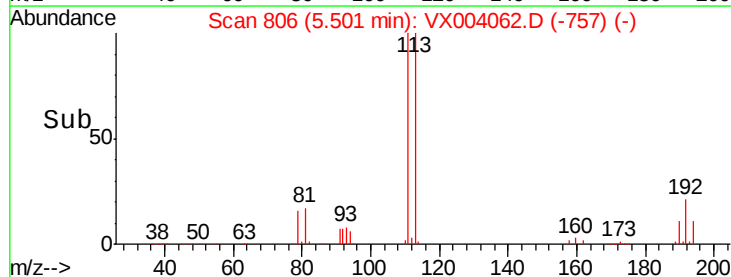
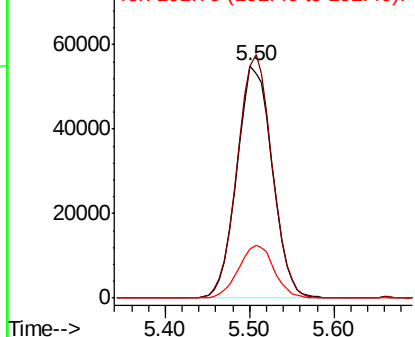


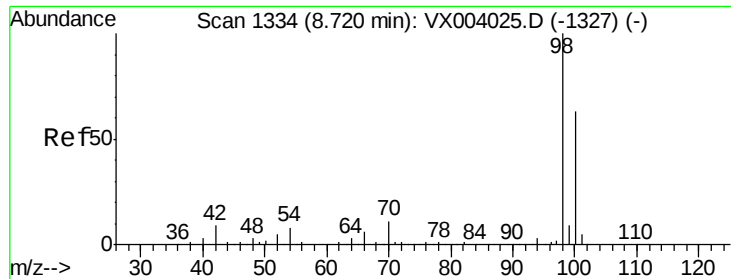

#50
Toluene-d8
Concen: 47.06 ug/l
RT: 8.72 min Scan# 1334
Delta R.T. -0.00 min
Lab File: VX004062.D
Acq: 15 Aug 2018 07:00




Instrument :
MSVOA_X
ClientSampleId :
RB6-SRI3


Tot Ion: 98 Resp: 573936
Ion Ratio Lower Upper
98 100
100 65.6 53.3 79.9

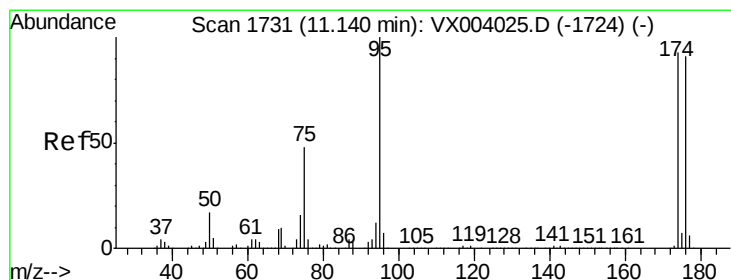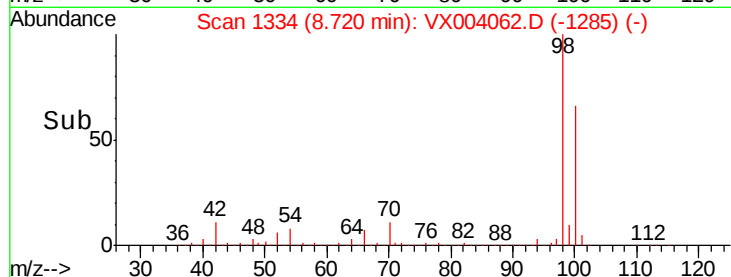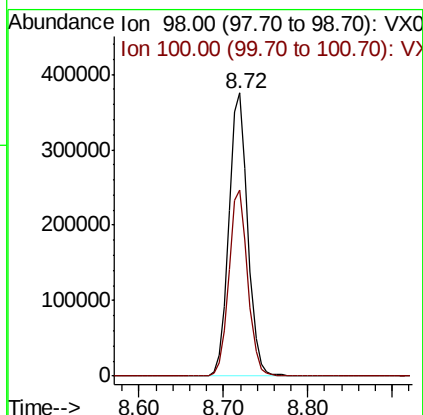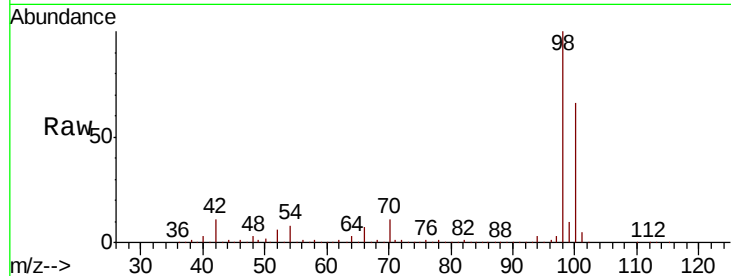

#62
4-Bromofluorobenzene
Concen: 43.93 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. -0.00 min
Lab File: VX004062.D
Acq: 15 Aug 2018 07:00

Tgt Ion: 95 Resp: 194297
Ion Ratio Lower Upper
95 100
174 92.1 0.0 182.8
176 88.5 0.0 179.0

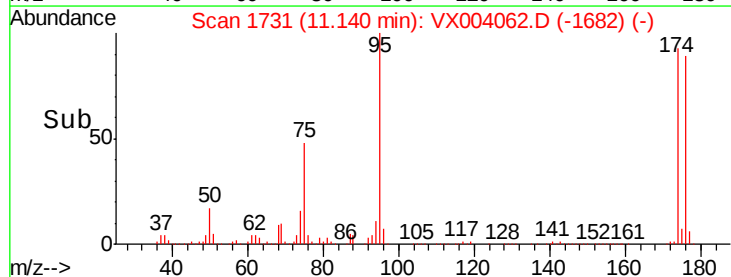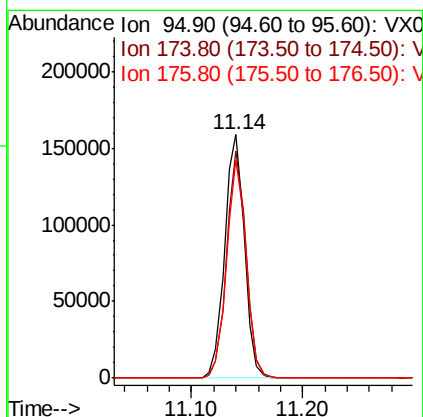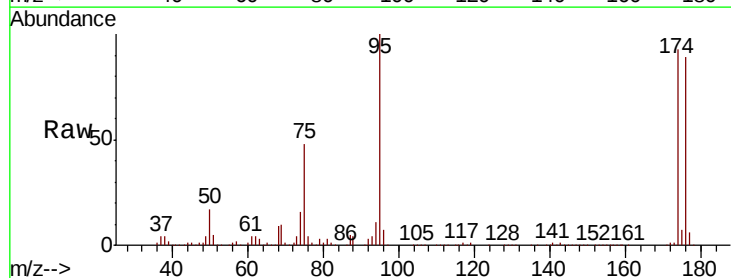


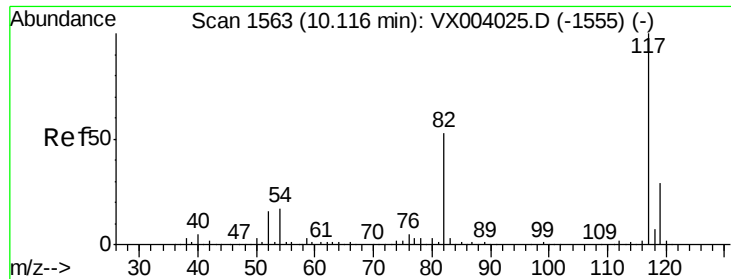




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.00 min
Lab File: VX004062.D
Acq: 15 Aug 2018 07:00

Instrument :
MSVOA_X
ClientSampleId :
RB6-SRI3

Tot Ion:117 Resp: 378135
Ion Ratio Lower Upper
117 100
82 56.0 45.4 68.0
119 31.9 26.6 40.0

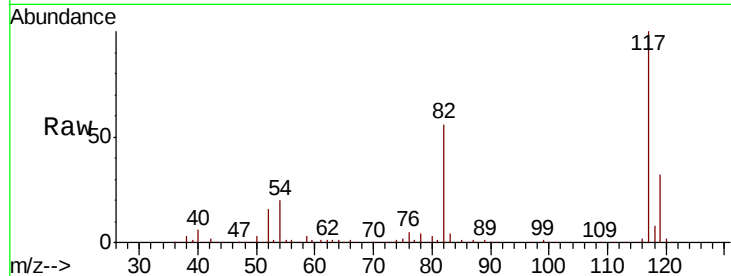


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

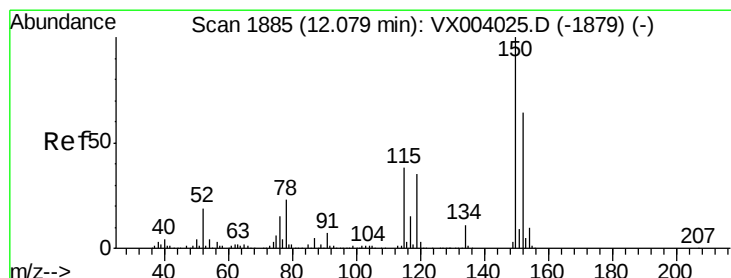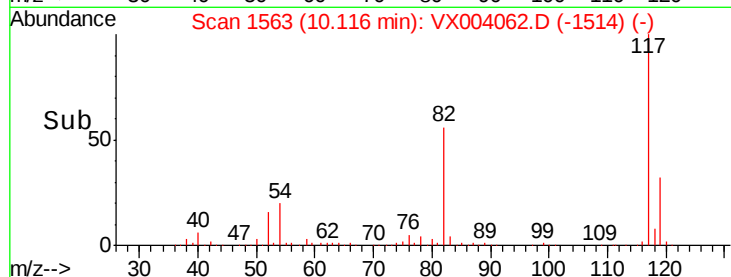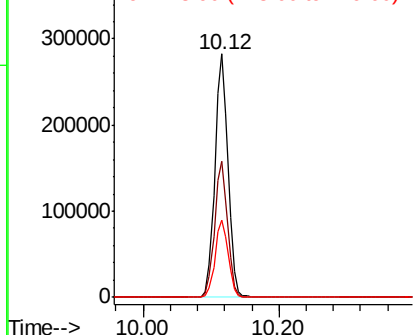

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.08 min Scan# 1885
Delta R.T. -0.00 min
Lab File: VX004062.D
Acq: 15 Aug 2018 07:00

Tgt Ion:152 Resp: 206373
Ion Ratio Lower Upper
152 100
115 54.9 39.1 117.3
150 156.4 0.0 349.2

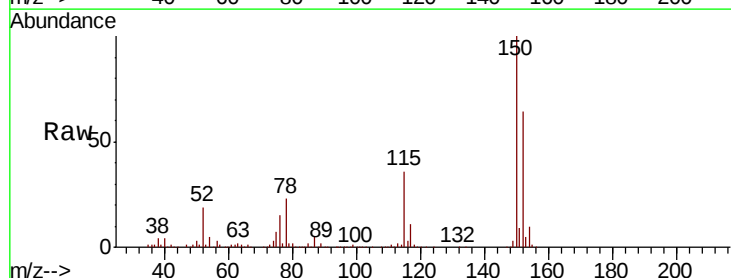

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

