


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081418\
Data File : VX004021.D
Acq On : 14 Aug 2018 10:06
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Title : SW846 8260
Last Update : Tue Aug 14 13:27:25 2018

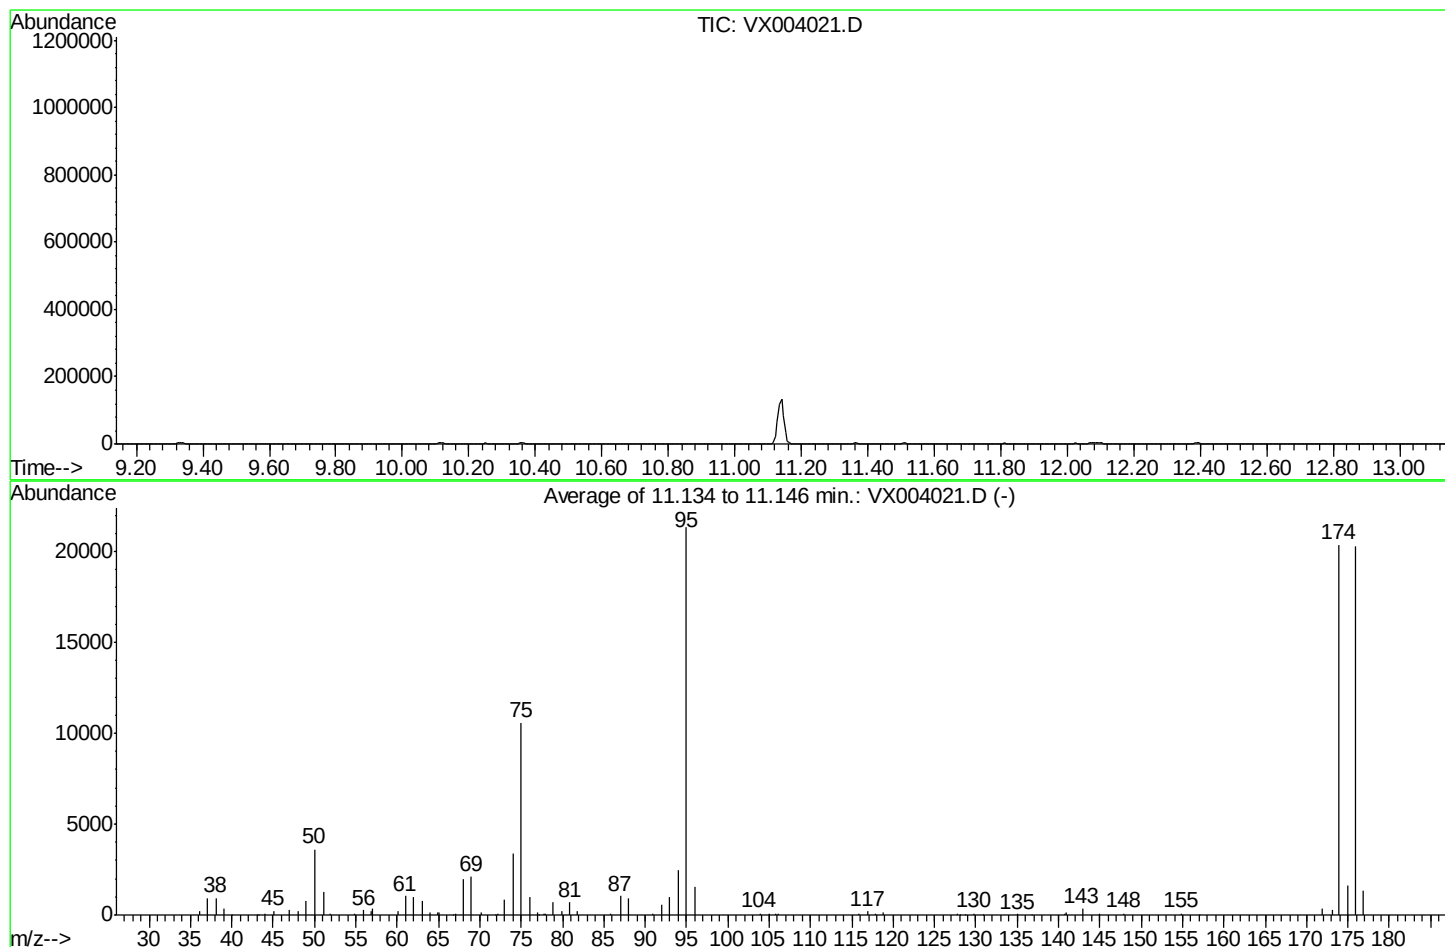

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	3613	PASS
75	95	30	60	49.5	10565	PASS
95	95	100	100	100.0	21330	PASS
96	95	5	9	7.3	1562	PASS
173	174	0.00	2	1.3	262	PASS
174	95	50	100	95.4	20357	PASS
175	174	5	9	7.9	1601	PASS
176	174	95	101	99.8	20309	PASS
177	176	5	9	6.5	1319	PASS