

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081420\
 Data File : VX017896.D
 Acq On : 14 Aug 2020 13:39
 Operator : JC/SP
 Sample : L3697-01
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG0M8

Quant Time: Aug 17 03:02:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 17 01:26:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	275176	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	269305	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	115063	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	90702	4.77	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.40%
7) Chloroethane-d5	1.69	69	75225	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.60%
11) 1,1-Dichloroethene-d2	2.34	63	136811	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	4.53	46	287751	56.98	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.96%
24) Chloroform-d	5.14	84	190436	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	6.03	65	108260	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.20%
32) Benzene-d6	6.05	84	350712	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
36) 1,2-Dichloropropane-d6	7.37	67	114208	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	8.70	98	293306	4.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.40%
45) trans-1,3-Dichloropropene-	8.99	79	46142	4.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.20%
48) 2-Hexanone-d5	9.43	63	212030	51.55	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.10%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	76389	4.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.00%
65) 1,2-Dichlorobenzene-d4	12.36	152	109943	4.96	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.20%


Target Compounds					Ovalue
13) Acetone	2.42	43	15083	4.088 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX081420\
Data File : VX017896.D
Acq On : 14 Aug 2020 13:39
Operator : JC/SP
Sample : L3697-01
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG0M8

Quant Time: Aug 17 03:02:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Aug 17 01:26:51 2020
Response via : Initial Calibration

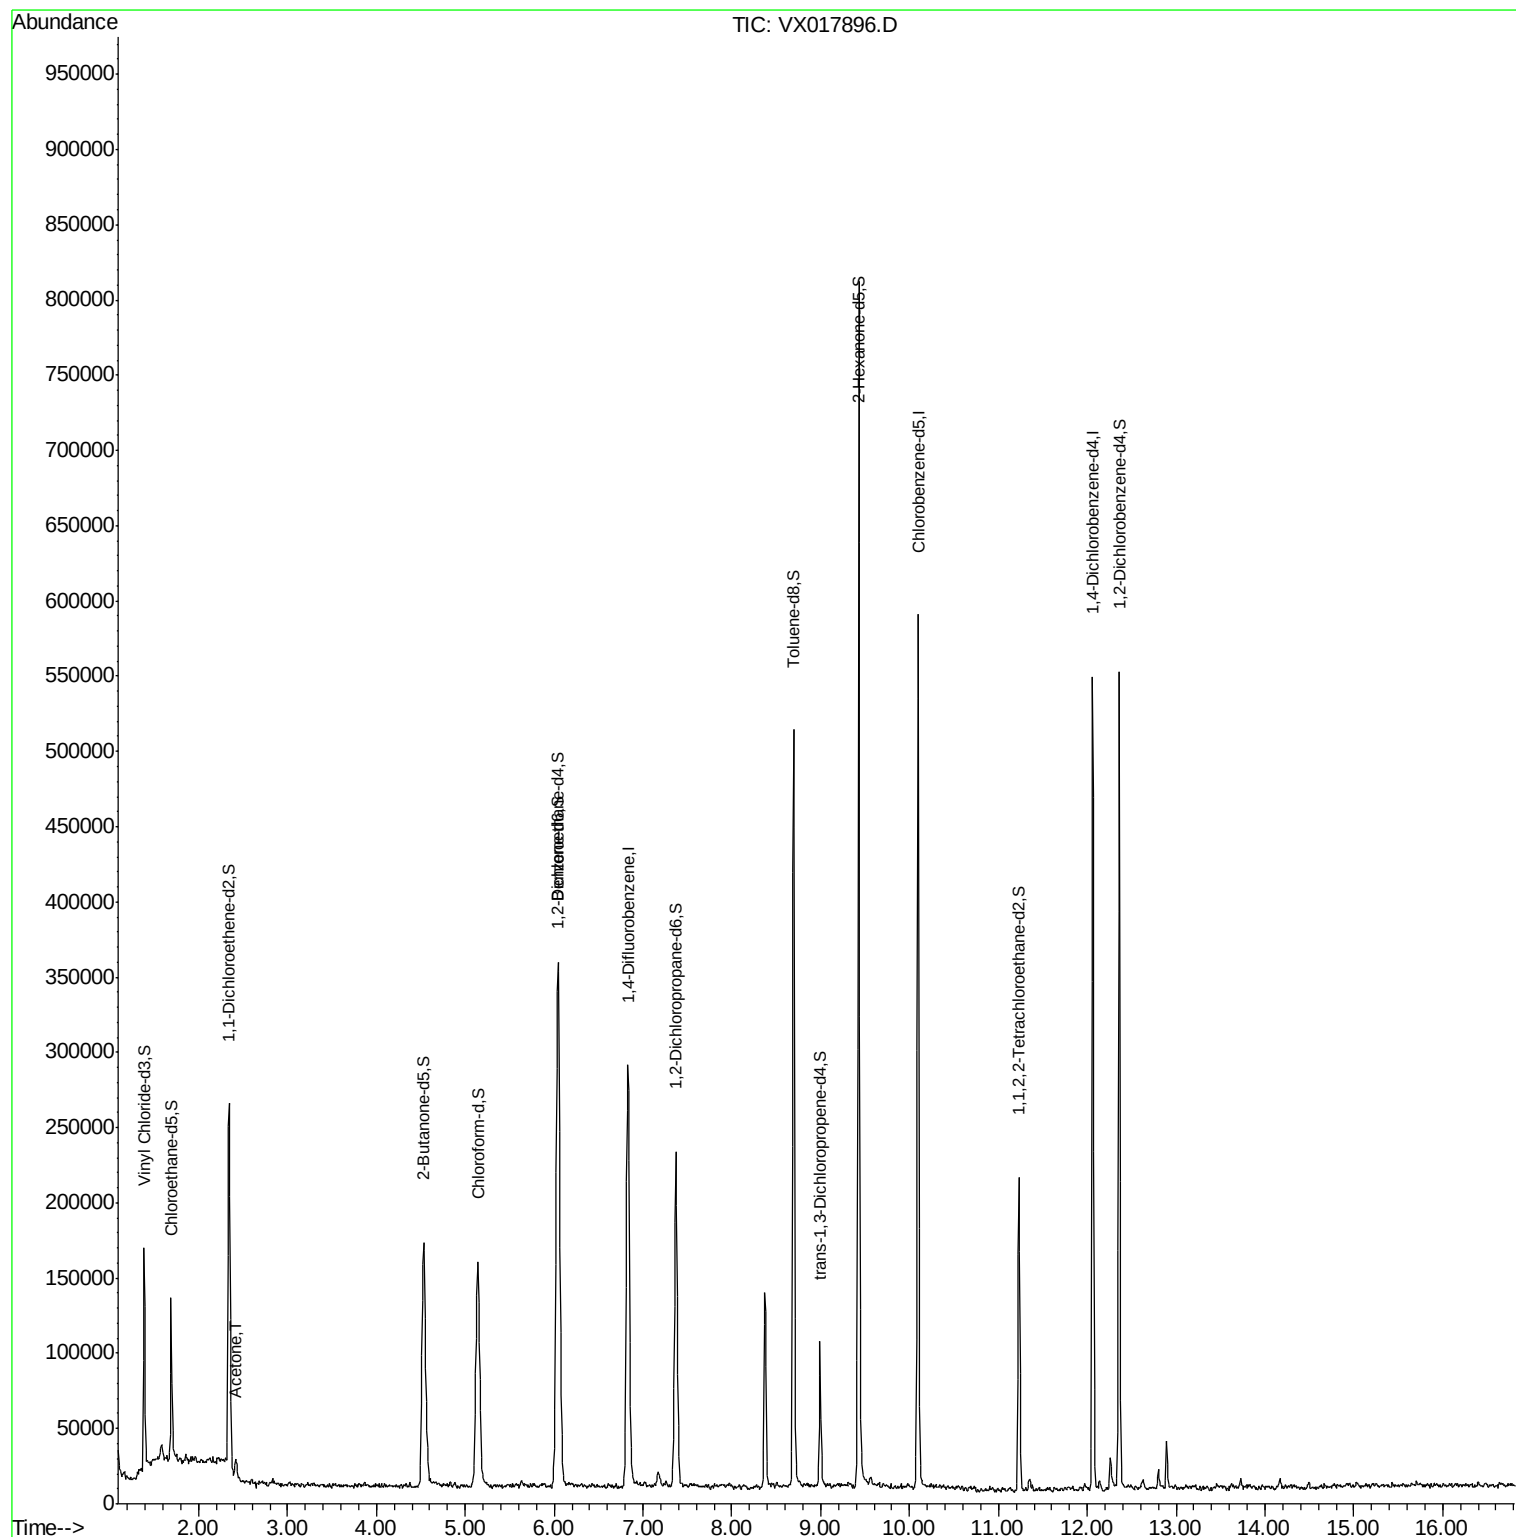

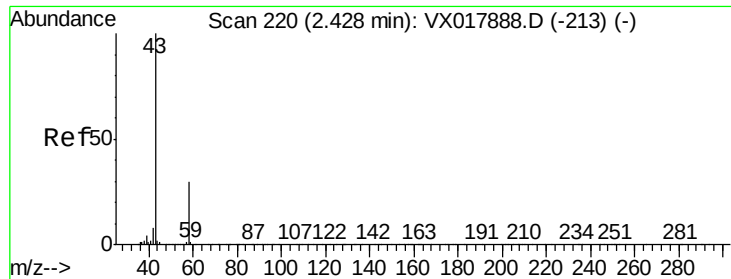

#13
 Acetone
 Concen: 4.088 ug/L
 RT: 2.42 min Scan# 218
 Delta R.T. -0.01 min
 Lab File: VX017896.D
 Acq: 14 Aug 2020 13:39

Instrument :
 MSVOA_X
 ClientSampleId :
 BG0M8

Tot Ion: 43 Resp: 15083
 Ion Ratio Lower Upper
 43 100
 58 35.5 0.0 60.8

