

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081423\
Data File : VX036966.D
Acq On : 14 Aug 2023 15:48
Operator : JC/MD
Sample : 03997-01RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20230811RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M

Title : SW846 8260

Signal : TIC: VX036966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	26	30	35	rBV	7777	8563	1.23%	0.233%
2	1.569	70	79	84	rBV3	3063	7384	1.06%	0.201%
3	2.788	272	279	287	rBV3	3341	6966	1.00%	0.190%
4	5.391	692	706	719	rBV	81570	237990	34.20%	6.480%
5	5.556	722	733	751	rVB	130576	370911	53.30%	10.099%
6	5.958	788	799	820	rBV	86440	229027	32.91%	6.236%
7	6.763	920	931	943	rBV	217999	510322	73.33%	13.895%
8	8.647	1234	1240	1265	rBV	443581	695906	100.00%	18.948%
9	10.055	1465	1471	1485	rBV	456586	616606	88.60%	16.788%
10	11.079	1634	1639	1655	rBV	355797	461961	66.38%	12.578%
11	12.024	1788	1794	1806	rBV	409484	527169	75.75%	14.353%




Sum of corrected areas: 3672805

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081423\
Data File : VX036966.D
Acq On : 14 Aug 2023 15:48
Operator : JC/MD
Sample : 03997-01RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20230811RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

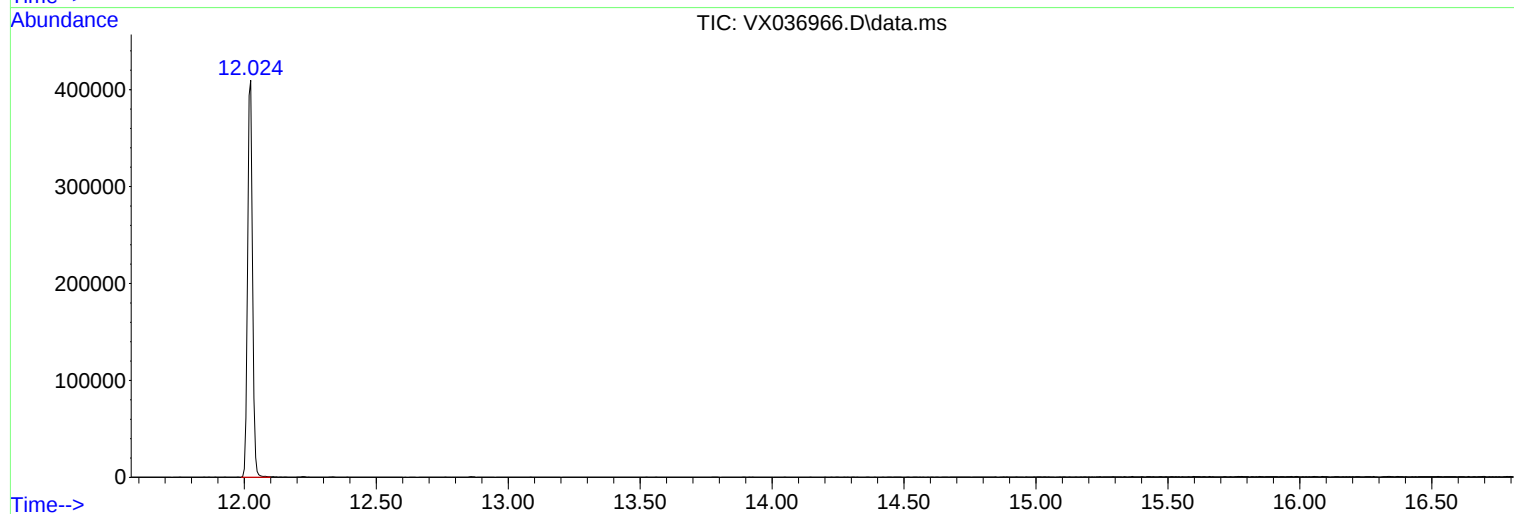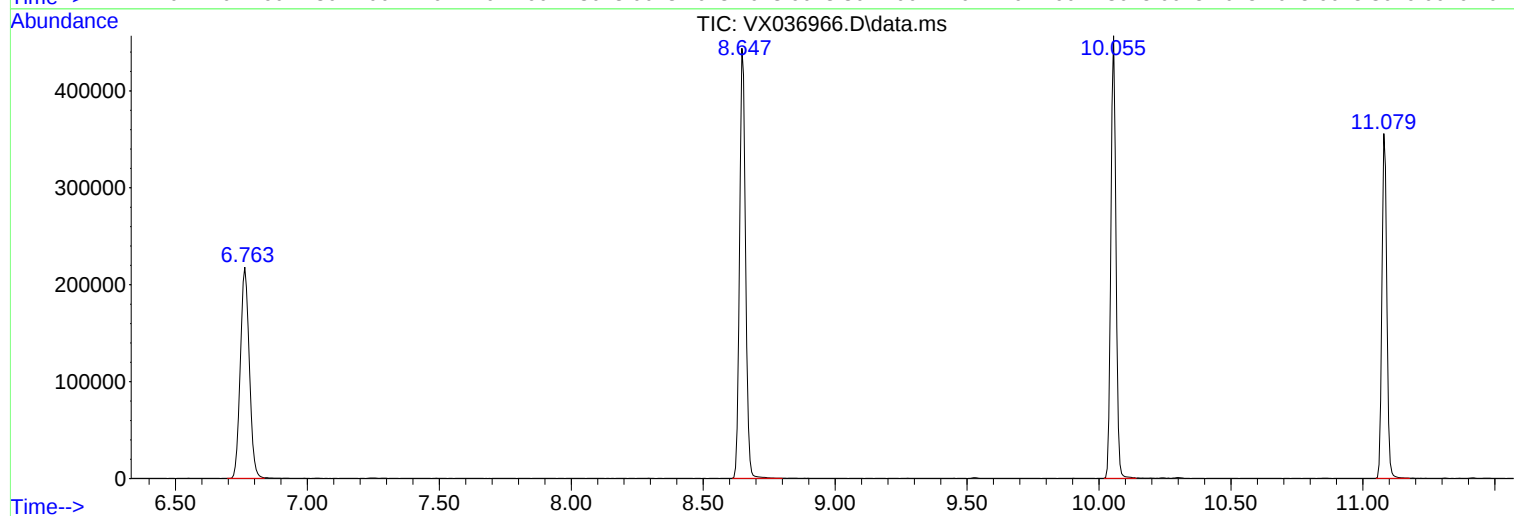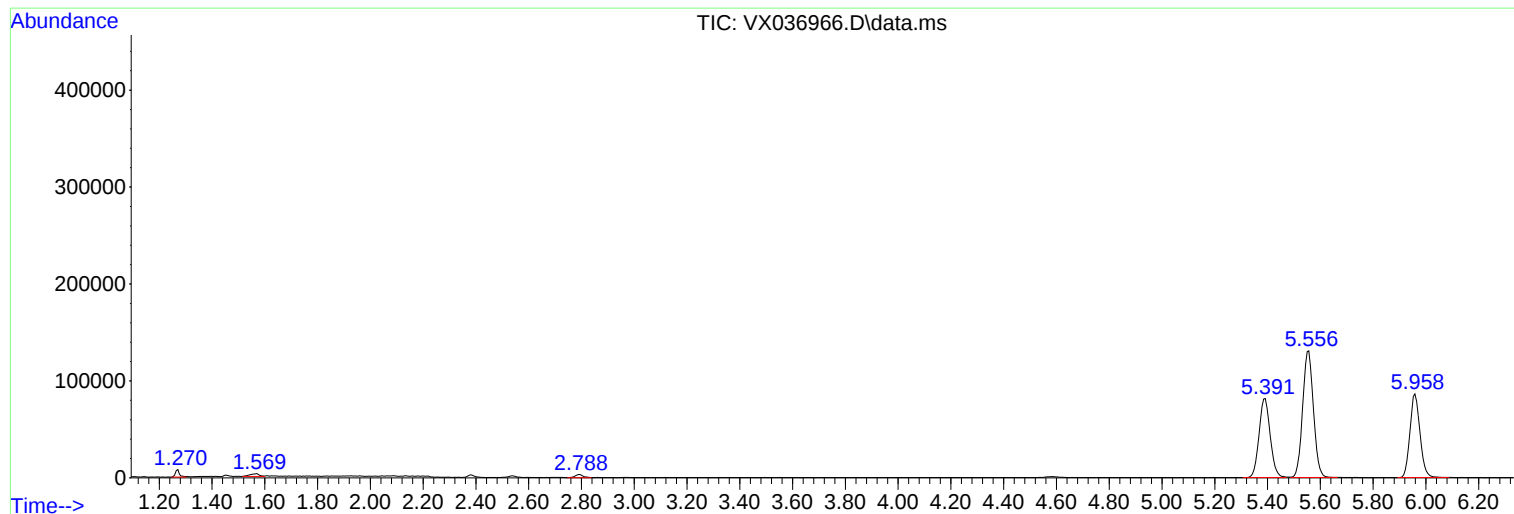

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081423\
Data File : VX036966.D
Acq On : 14 Aug 2023 15:48
Operator : JC/MD
Sample : 03997-01RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20230811RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081423\
Data File : VX036966.D
Acq On : 14 Aug 2023 15:48
Operator : JC/MD
Sample : 03997-01RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20230811RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc