
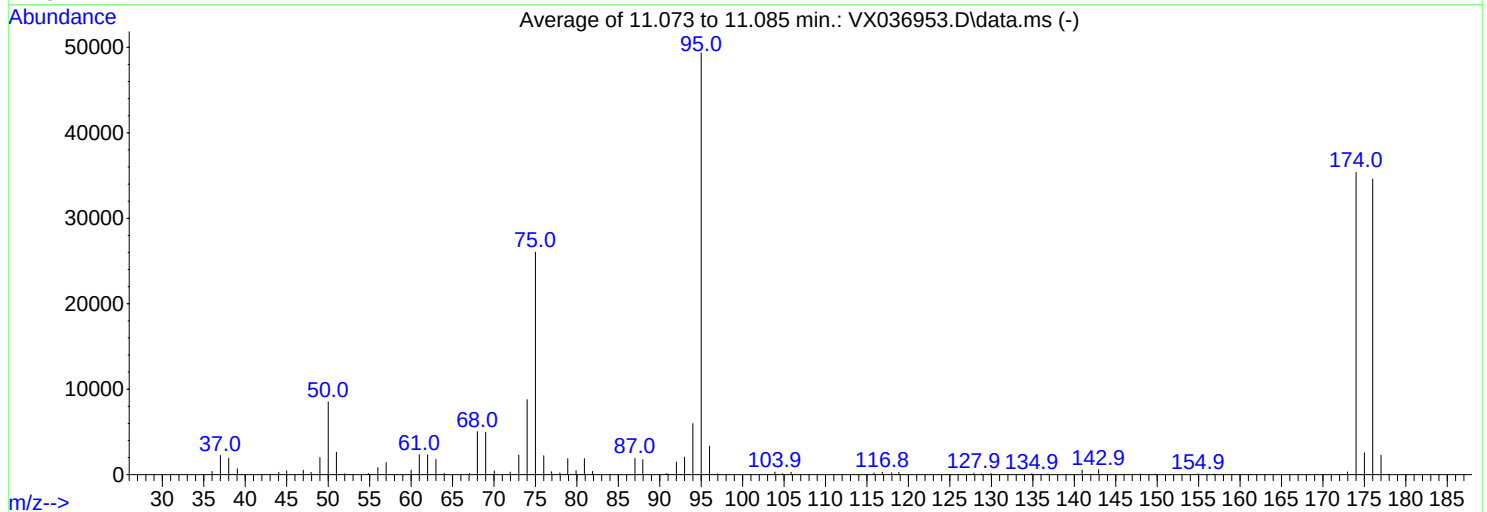


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081423\
 Data File : VX036953.D
 Acq On : 14 Aug 2023 09:35
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Title : SW846 8260
 Last Update : Fri Jul 21 12:14:12 2023

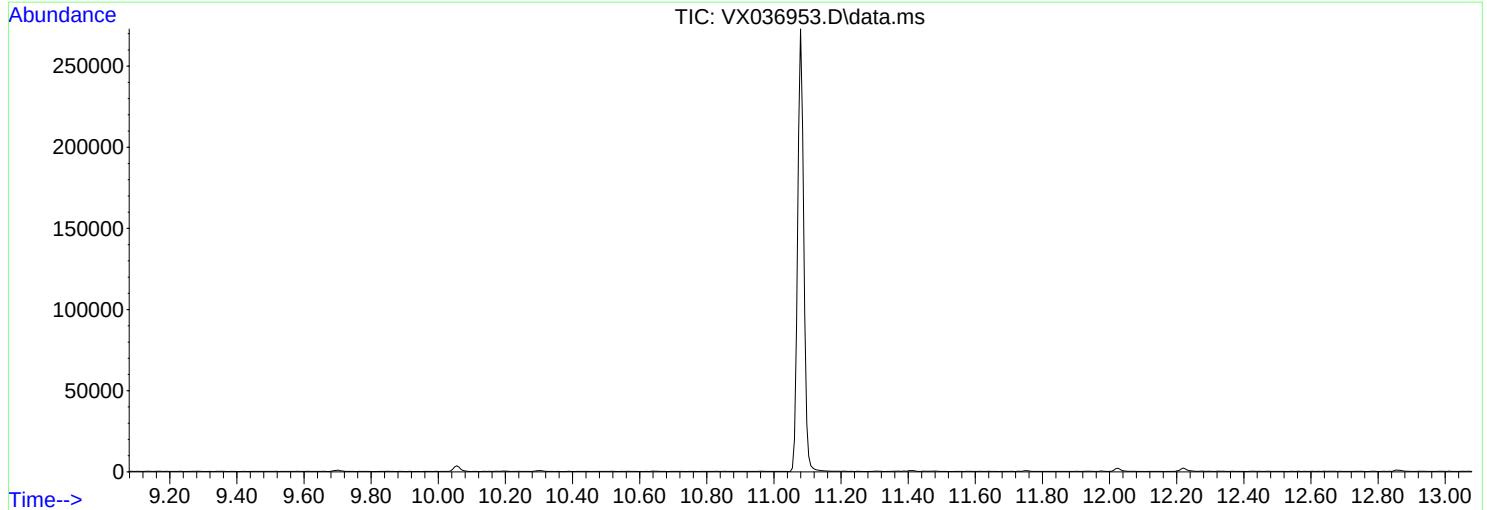

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	8515	PASS
75	95	30	60	52.8	26037	PASS
95	95	100	100	100.0	49357	PASS
96	95	5	9	6.8	3336	PASS
173	174	0.00	2	0.9	317	PASS
174	95	50	100	71.7	35373	PASS
175	174	5	9	7.3	2566	PASS
176	174	95	101	97.8	34597	PASS
177	176	5	9	6.6	2290	PASS