
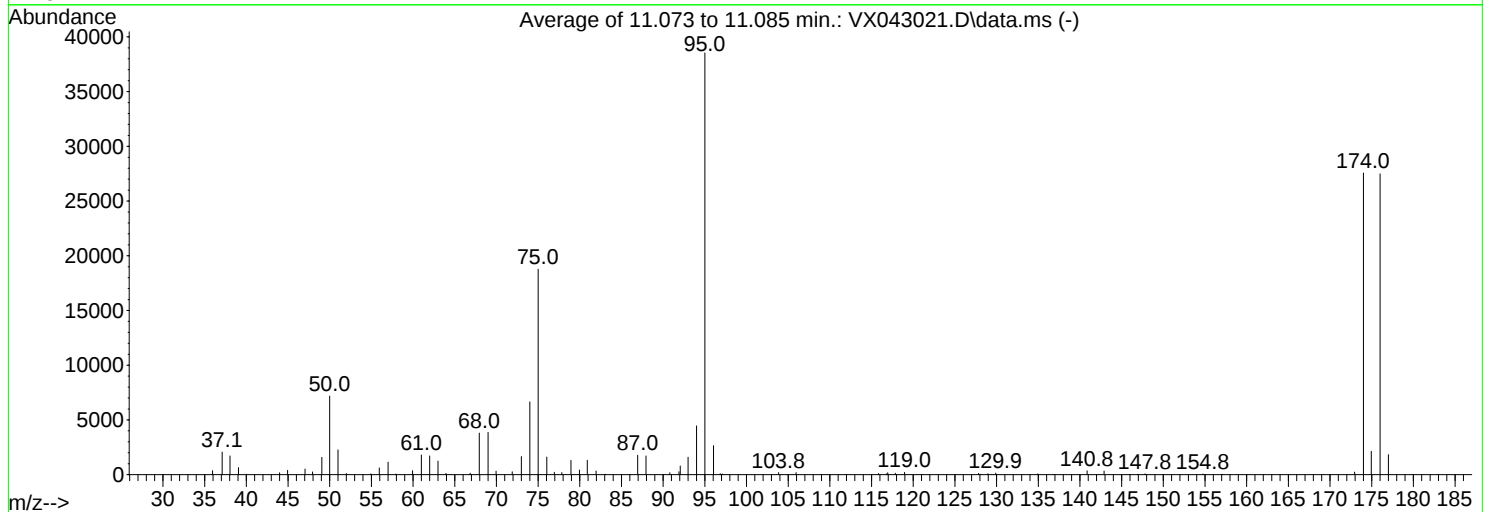


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081424\
Data File : VX043021.D
Acq On : 14 Aug 2024 10:16
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081424W.M
Title : SW846 8260
Last Update : Thu Aug 15 04:22:11 2024

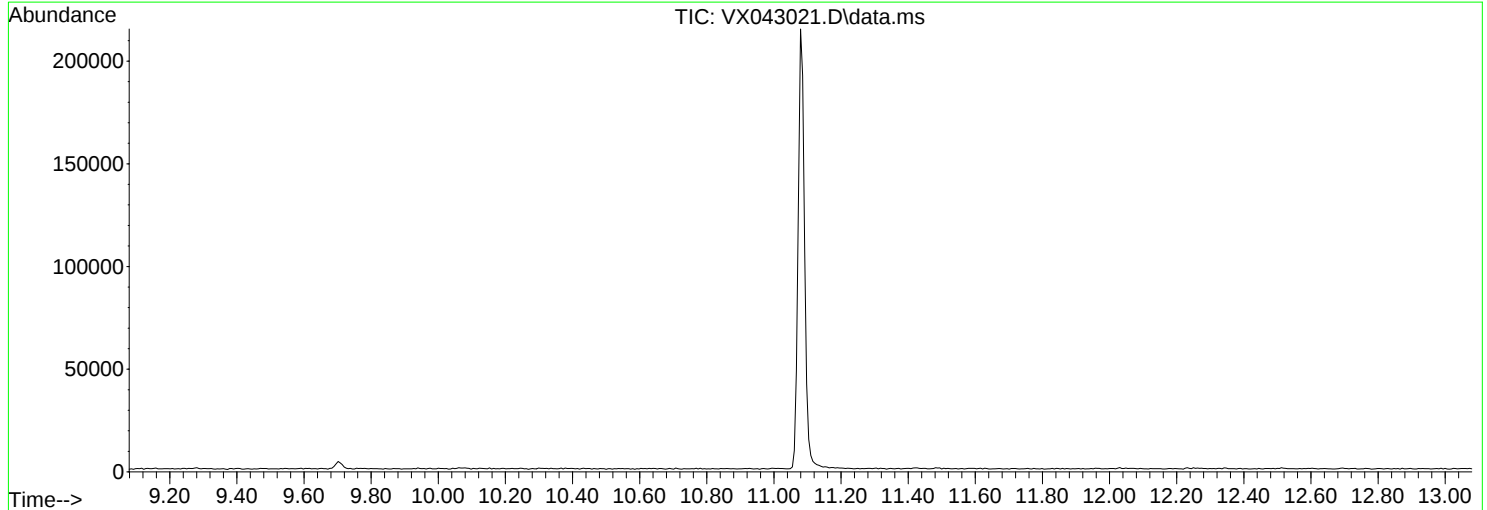

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	7183	PASS
75	95	30	60	48.7	18776	PASS
95	95	100	100	100.0	38544	PASS
96	95	5	9	6.9	2654	PASS
173	174	0.00	2	0.9	235	PASS
174	95	50	100	71.5	27557	PASS
175	174	5	9	7.8	2142	PASS
176	174	95	101	99.8	27493	PASS
177	176	5	9	6.7	1835	PASS