

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081518\  
 Data File : VX004080.D  
 Acq On : 15 Aug 2018 18:41  
 Operator : JC/MD  
 Sample : J4473-02  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 KY038PS027-180813

Quant Time: Aug 16 05:52:32 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X081418W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Aug 14 13:27:25 2018  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 5.67  | 168  | 261792   | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 6.87  | 114  | 399165   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 10.12 | 117  | 381220   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 12.08 | 152  | 195189   | 50.00 | ug/l  | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc  | Units   | Dev(Min) |
|-----------------------------|-------|------|----------|-------|---------|----------|
| 33) 1,2-Dichloroethane-d4   | 6.07  | 65   | 188243   | 51.03 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 102.06% |          |
| 35) Dibromofluoromethane    | 5.51  | 113  | 154009   | 51.55 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 103.10% |          |
| 50) Toluene-d8              | 8.72  | 98   | 574463   | 47.43 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 94.86%  |          |
| 62) 4-Bromofluorobenzene    | 11.14 | 95   | 191065   | 43.49 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 86.98%  |          |


| Target Compounds               | R.T.  | QIon | Response | Conc      | Units | Qvalue |
|--------------------------------|-------|------|----------|-----------|-------|--------|
| 3) Chloromethane               | 1.32  | 50   | 1341     | 0.43      | ug/l  | 96     |
| 4) Vinyl Chloride              | 1.40  | 62   | 1487     | 0.44      | ug/l  | 89     |
| 5) Bromomethane                | 1.65  | 94   | 1105     | 0.47      | ug/l  | 97     |
| 6) Chloroethane                | 1.64  | 64   | 362      | Below Cal | #     | 52     |
| 10) Methyl Iodide              | 2.51  | 142  | 905      | 5.27      | ug/l  | 90     |
| 11) Tert butyl alcohol         | 3.04  | 59   | 1293     | 1.74      | ug/l  | 98     |
| 13) Acrolein                   | 2.29  | 56   | 87       | 11.11     | ug/l  | 44     |
| 16) Acetone                    | 2.44  | 43   | 41611    | 21.70     | ug/l  | 100    |
| 20) Methylene Chloride         | 2.86  | 84   | 735      | Below Cal | #     | 87     |
| 25) 2-Butanone                 | 4.70  | 43   | 6295     | 2.02      | ug/l  | 95     |
| 27) cis-1,2-Dichloroethene     | 4.60  | 96   | 174956   | 49.74     | ug/l  | 90     |
| 29) Tetrahydrofuran            | 5.16  | 42   | 11290    | 7.08      | ug/l  | 94     |
| 31) Cyclohexane                | 5.66  | 56   | 5095     | 1.00      | ug/l  | # 1    |
| 32) 1,1,1-Trichloroethane      | 5.49  | 97   | 965      | 0.20      | ug/l  | # 39   |
| 36) 1,1-Dichloropropene        | 5.66  | 75   | 17822    | 3.92      | ug/l  | # 49   |
| 38) Carbon Tetrachloride       | 5.67  | 117  | 24023    | 5.44      | ug/l  | # 15   |
| 44) Trichloroethene            | 7.21  | 130  | 30462    | 8.23      | ug/l  | 98     |
| 60) Dibromochloromethane       | 9.34  | 129  | 37644    | 10.98     | ug/l  | # 11   |
| 64) Tetrachloroethene          | 9.34  | 164  | 43016    | 11.91     | ug/l  | 94     |
| 76) 1,2,3-Trichloropropane     | 11.14 | 75   | 92748    | 23.69     | ug/l  | # 36   |
| 81) trans-1,4-Dichloro-2-buten | 11.14 | 75   | 92748    | 73.35     | ug/l  | # 10   |
| 95) Naphthalene                | 13.84 | 128  | 396      | 1.17      | ug/l  | # 83   |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX081518\  
Data File : VX004080.D  
Acq On : 15 Aug 2018 18:41  
Operator : JC/MD  
Sample : J4473-02  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
KY038PS027-180813

Quant Time: Aug 16 05:52:32 2018  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X081418W.M  
Quant Title : SW846 8260  
QLast Update : Tue Aug 14 13:27:25 2018  
Response via : Initial Calibration

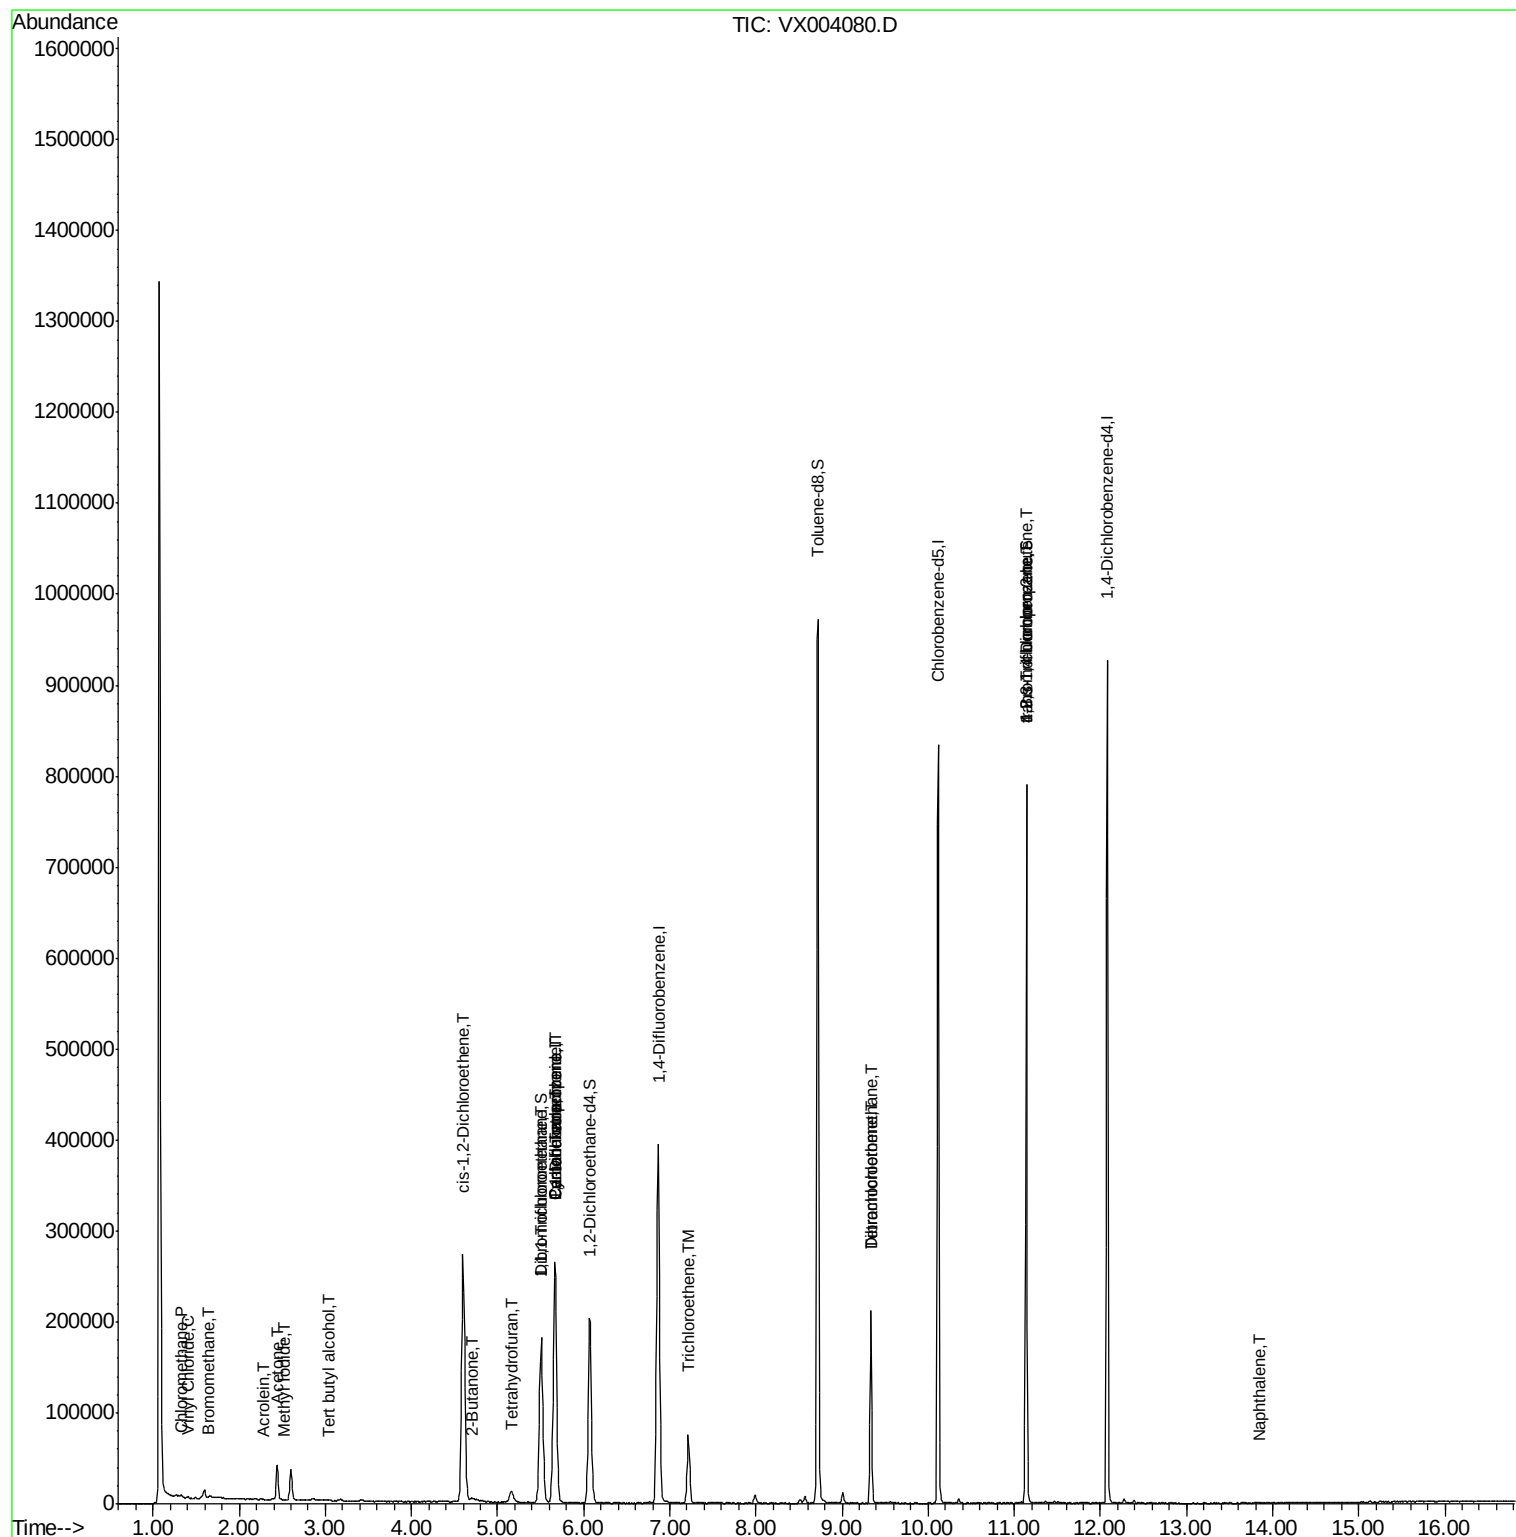



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.00 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41

Instrument :

MSVOA\_X

ClientSampleId :


KY038PS027-180813

Tot Ion:168 Resp: 261792

Ion Ratio Lower Upper




168 100

99 51.3 40.1 60.1

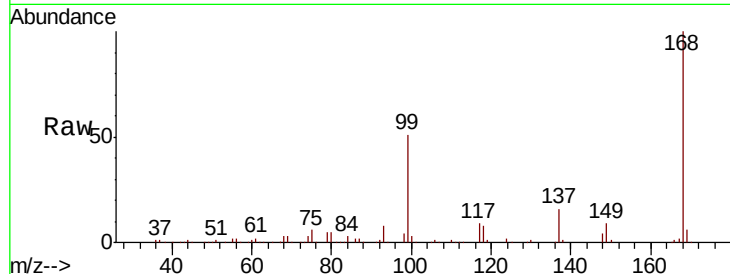

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

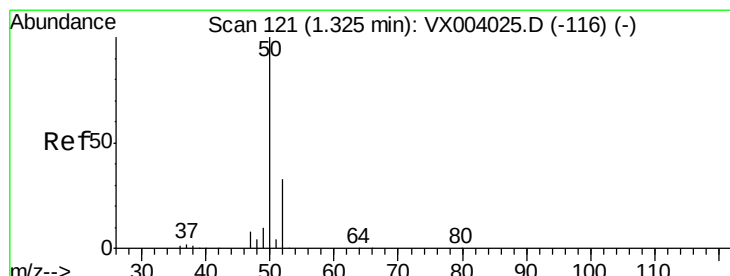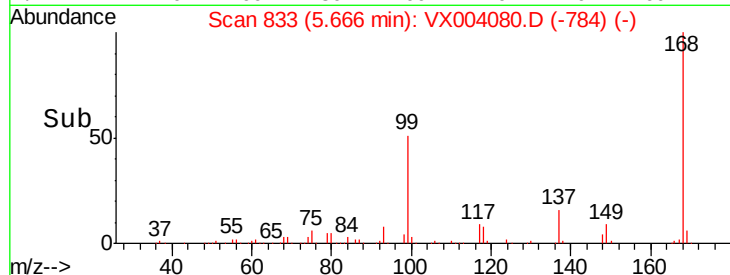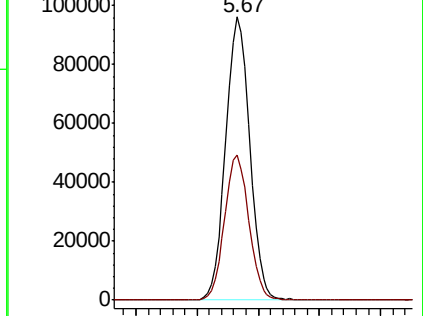

#3

Chloromethane

Concen: 0.43 ug/l

RT: 1.32 min Scan# 121

Delta R.T. -0.00 min

Lab File: VX004080.D


Acq: 15 Aug 2018 18:41

Tgt Ion: 50 Resp: 1341

Ion Ratio Lower Upper



50 100


52 35.7 26.6 39.8

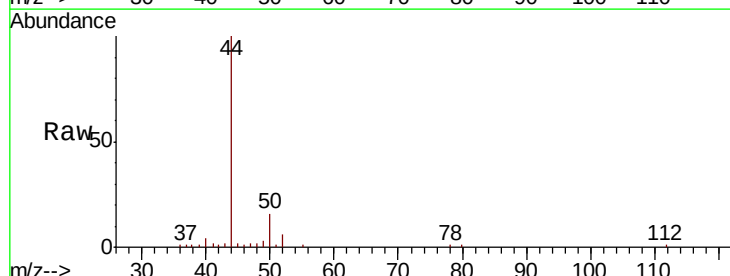

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

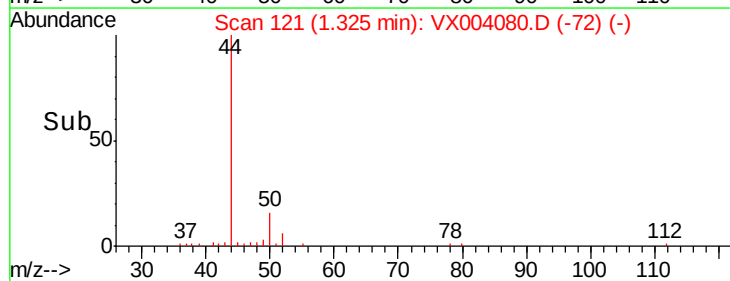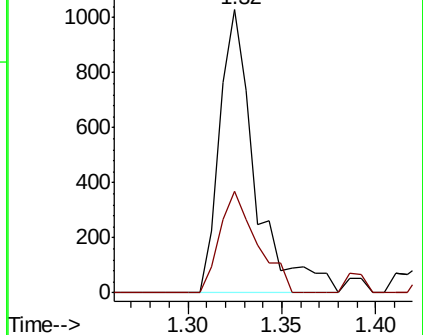

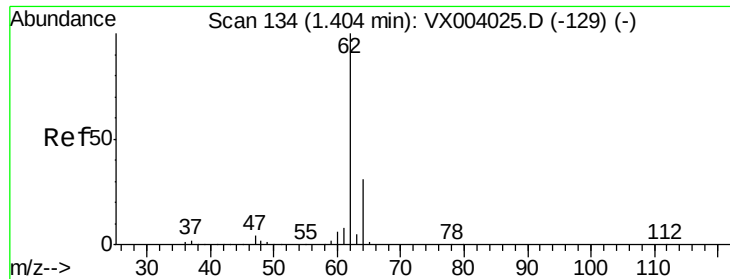

#4

Vinyl Chloride

Concen: 0.44 ug/l

RT: 1.40 min Scan# 134

Delta R.T. -0.00 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41

Instrument :

MSVOA\_X

ClientSampleId :


KY038PS027-180813

Tot Ion: 62 Resp: 1487

Ion Ratio Lower Upper




62 100

64 26.3 26.0 39.0

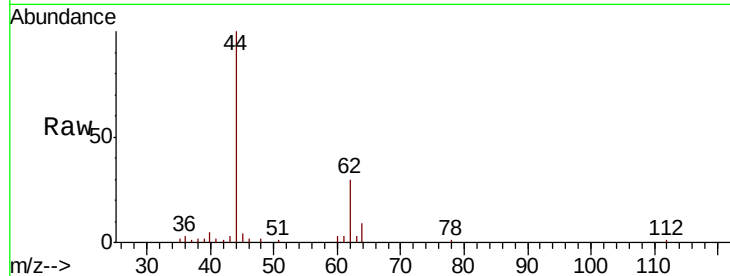

Abundance Ion 61.90 (61.60 to 62.60): VX0

Ion 63.90 (63.60 to 64.60): VX0

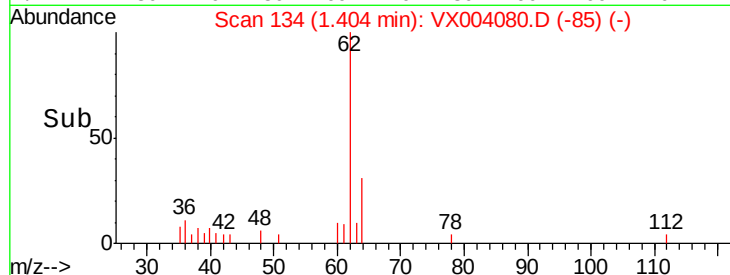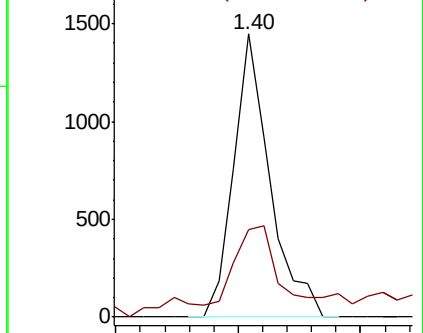

#5

Bromomethane

Concen: 0.47 ug/l

RT: 1.65 min Scan# 174

Delta R.T. 0.01 min

Lab File: VX004080.D


Acq: 15 Aug 2018 18:41

Tgt Ion: 94 Resp: 1105

Ion Ratio Lower Upper



94 100


96 91.3 75.2 112.8



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

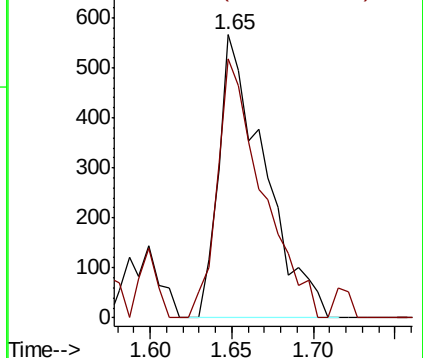

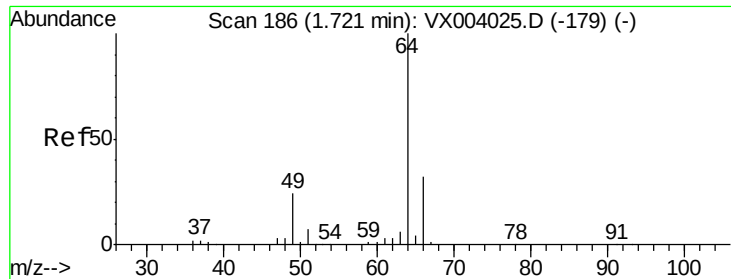

#6

Chloroethane

Concen: Below Cal

RT: 1.64 min Scan# 173

Delta R.T. -0.08 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41

Instrument :

MSVOA\_X

ClientSampleId :





KY038PS027-180813

Tot Ion: 64 Resp: 362

Ion Ratio Lower Upper

64 100

66 5.7 26.5 39.7#

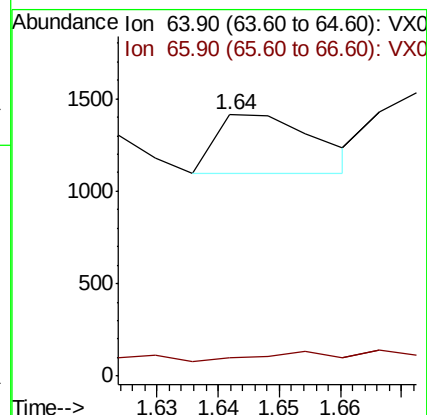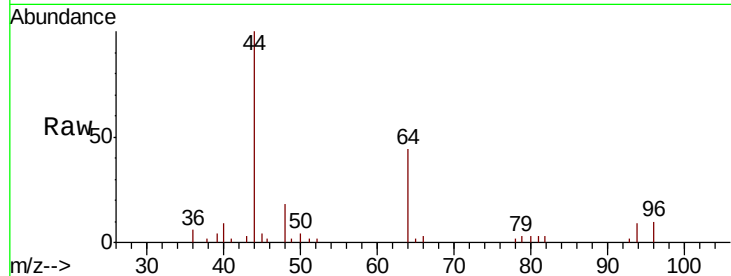

#10

Methyl Iodide

Concen: 5.27 ug/l

RT: 2.51 min Scan# 316

Delta R.T. 0.00 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41




Tgt Ion:142 Resp: 905


Ion Ratio Lower Upper

142 100

127 42.8 33.1 49.7

141 0.0 11.1 16.7#



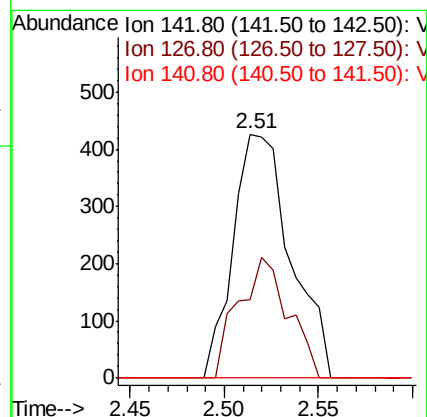





#11  
Tert butyl alcohol  
Concen: 1.74 ug/l  
RT: 3.04 min Scan# 402  
Delta R.T. -0.01 min  
Lab File: VX004080.D  
Acq: 15 Aug 2018 18:41




Instrument :  
MSVOA\_X  
ClientSampleId :  
KY038PS027-180813


Tot Ion: 59 Resp: 1293  
Ion Ratio Lower Upper  
59 100  
57 9.4 8.1 12.1

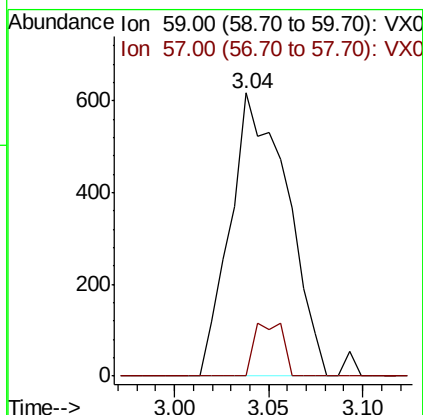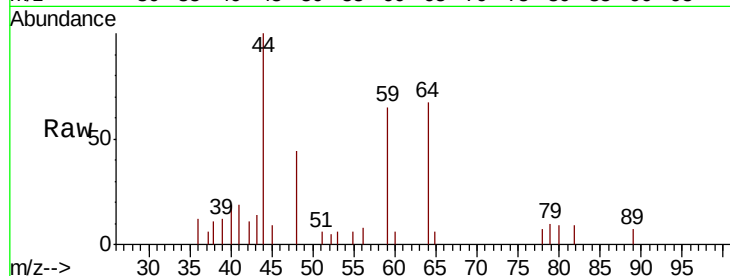

#13  
Acrolein  
Concen: 11.11 ug/l  
RT: 2.29 min Scan# 279  
Delta R.T. 0.00 min  
Lab File: VX004080.D  
Acq: 15 Aug 2018 18:41

Tgt Ion: 56 Resp: 87  
Ion Ratio Lower Upper  
56 100  
55 24.1 56.1 84.1#

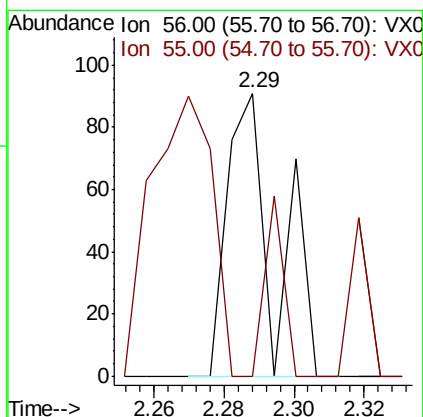

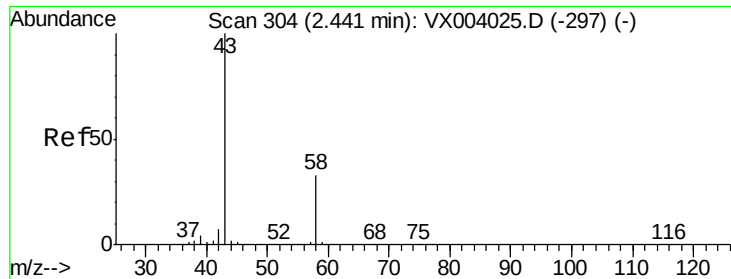

#16

Acetone

Concen: 21.70 ug/l

RT: 2.44 min Scan# 304

Delta R.T. -0.00 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41

Instrument :

MSVOA\_X

ClientSampleId :





KY038PS027-180813

Tot Ion: 43 Resp: 41611

Ion Ratio Lower Upper

43 100

58 32.8 26.4 39.6

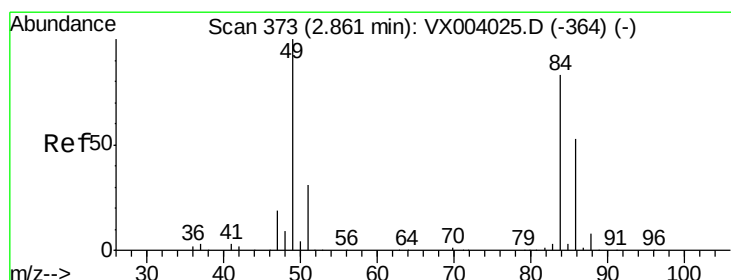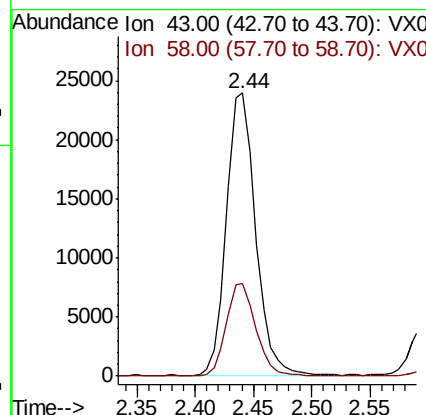

#20

Methylene Chloride

Concen: Below Cal

RT: 2.86 min Scan# 372

Delta R.T. -0.01 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41

Tgt Ion: 84 Resp: 735




Ion Ratio Lower Upper


84 100

49 129.8 98.9 148.3

51 28.1 29.9 44.9#

86 83.6 51.0 76.6#

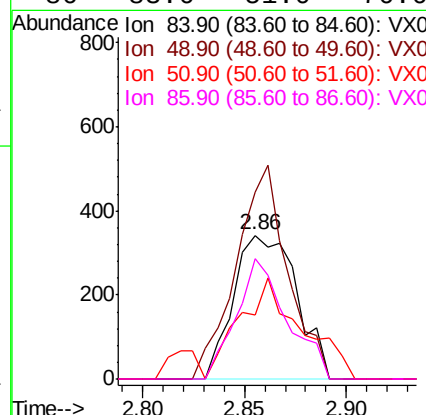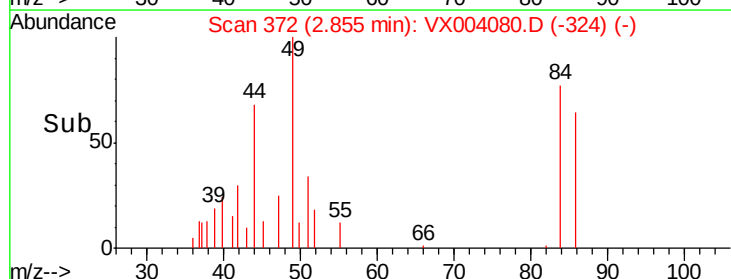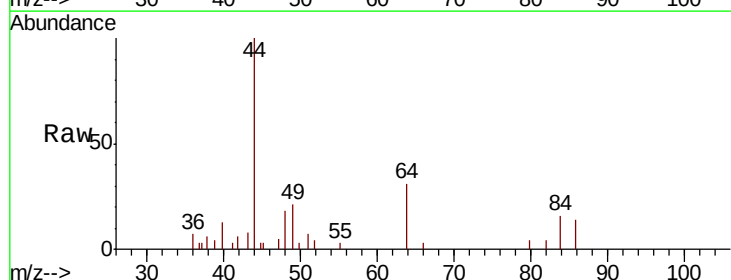

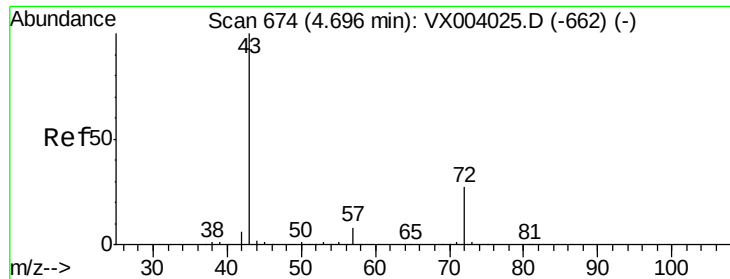

#25

2-Butanone

Concen: 2.02 ug/l

RT: 4.70 min Scan# 675

Delta R.T. 0.01 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41

Instrument :

MSVOA\_X

ClientSampleId :


KY038PS027-180813

Tot Ion: 43 Resp: 6295

Ion Ratio Lower Upper




43 100

72 24.2 21.4 32.0

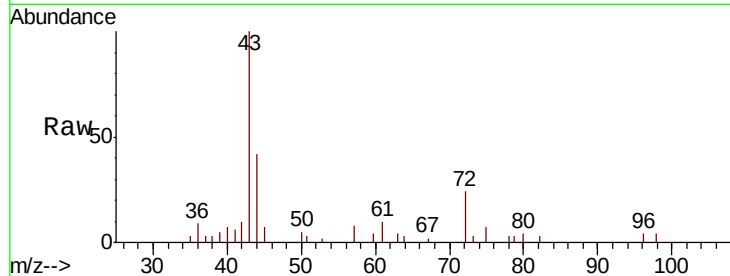

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

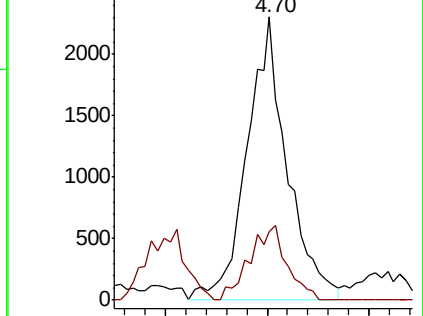

#27

cis-1,2-Dichloroethene

Concen: 49.74 ug/l

RT: 4.60 min Scan# 658

Delta R.T. -0.00 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41


Tgt Ion: 96 Resp: 174956

Ion Ratio Lower Upper

96 100

61 128.8 0.0 293.0



98 64.5 0.0 131.8




Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

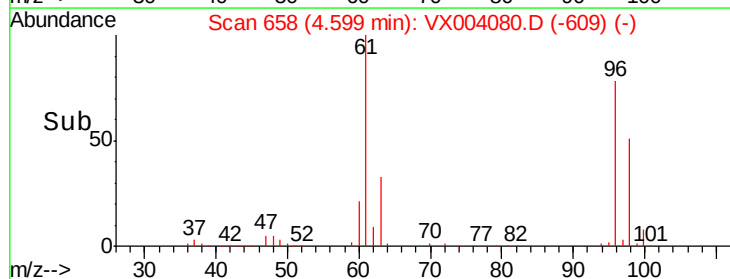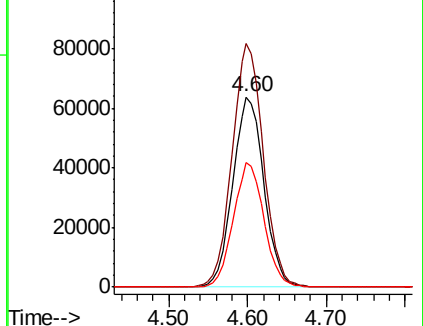





#29

Tetrahydrofuran

Concen: 7.08 ug/l

RT: 5.16 min Scan# 750

Delta R.T. 0.01 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41

Instrument :

MSVOA\_X

ClientSampleId :

KY038PS027-180813


Tot Ion: 42 Resp: 11290

Ion Ratio Lower Upper

42 100

72 43.4 37.7 56.5




71 39.4 35.0 52.6

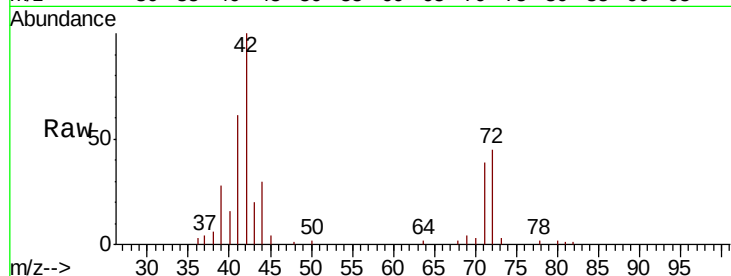

Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

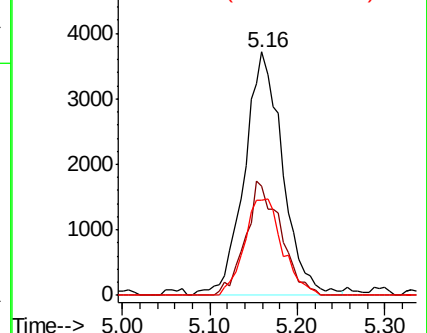

#31

Cyclohexane

Concen: 1.00 ug/l

RT: 5.66 min Scan# 832

Delta R.T. 0.08 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41


Tgt Ion: 56 Resp: 5095

Ion Ratio Lower Upper

56 100

69 192.8 24.9 37.3#



84 138.0 71.7 107.5#




Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

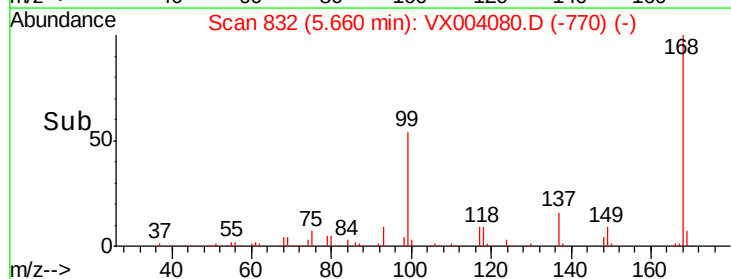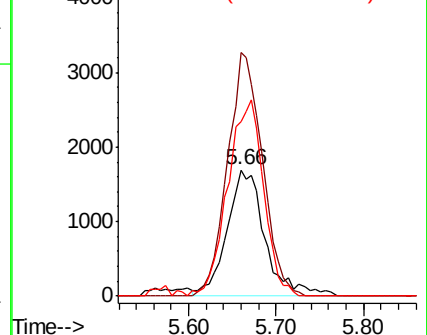

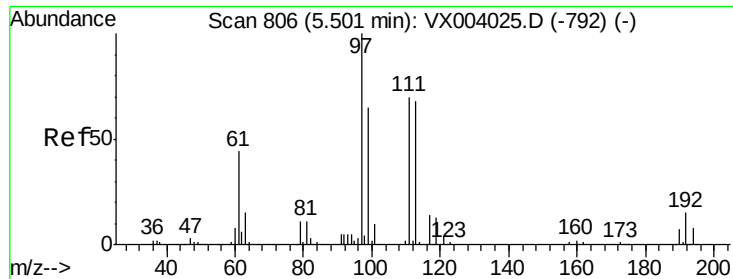

#32

1,1,1-Trichloroethane

Concen: 0.20 ug/l

RT: 5.49 min Scan# 805

Delta R.T. -0.01 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41

Instrument :

MSVOA\_X

ClientSampleId :

KY038PS027-180813


Tot Ion: 97 Resp: 965

Ion Ratio Lower Upper

97 100

99 0.0 51.8 77.8#




61 62.2 34.4 51.6#

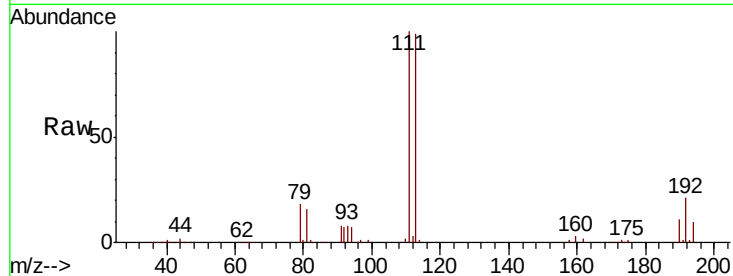

Abundance Ion 96.90 (96.60 to 97.60): VX0

Ion 98.90 (98.60 to 99.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

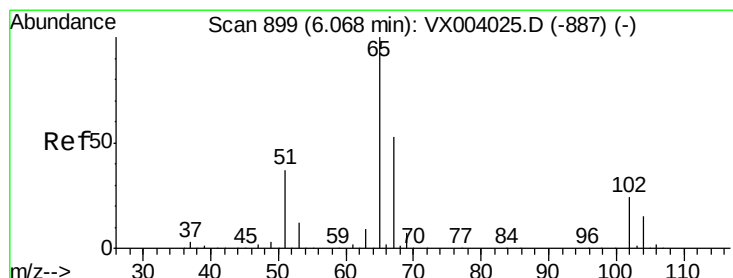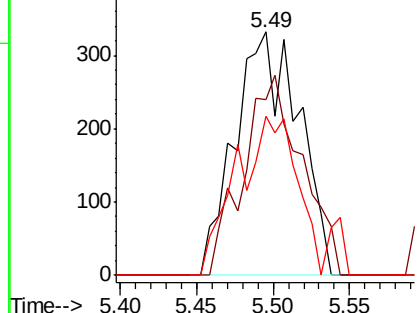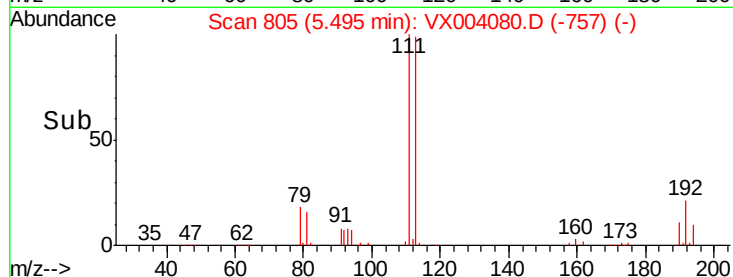

#33

1,2-Dichloroethane-d4

Concen: 51.03 ug/l

RT: 6.07 min Scan# 899

Delta R.T. -0.00 min

Lab File: VX004080.D


Acq: 15 Aug 2018 18:41

Tgt Ion: 65 Resp: 188243

Ion Ratio Lower Upper



65 100


67 52.8 0.0 105.8

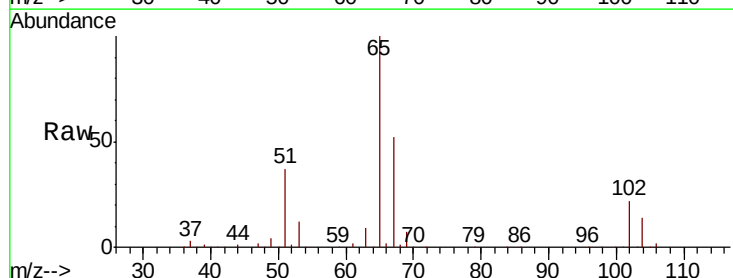

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0



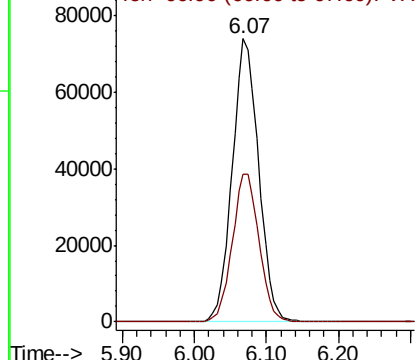
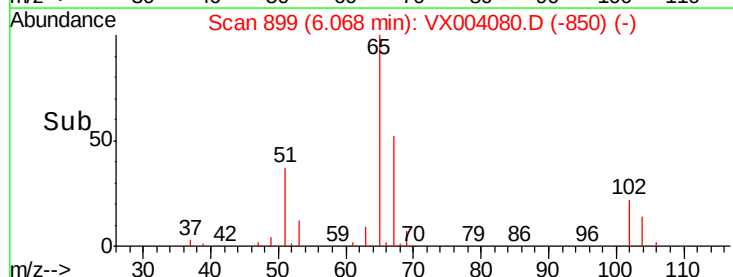


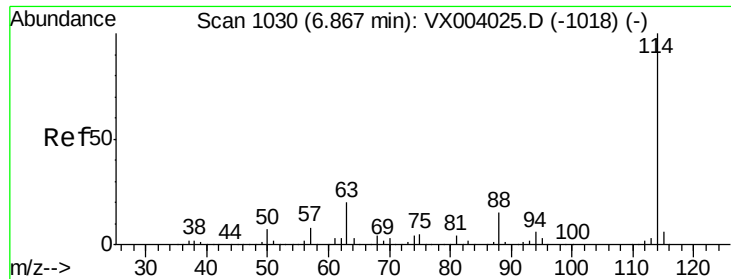

#34  
 1,4-Difluorobenzene  
 Concen: 50.00 ug/l  
 RT: 6.87 min Scan# 1030  
 Delta R.T. -0.00 min  
 Lab File: VX004080.D  
 Acq: 15 Aug 2018 18:41




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 KY038PS027-180813


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 114     | 100   |       |       |
| 63      | 19.9  | 0.0   | 39.0  |
| 88      | 15.2  | 0.0   | 32.0  |

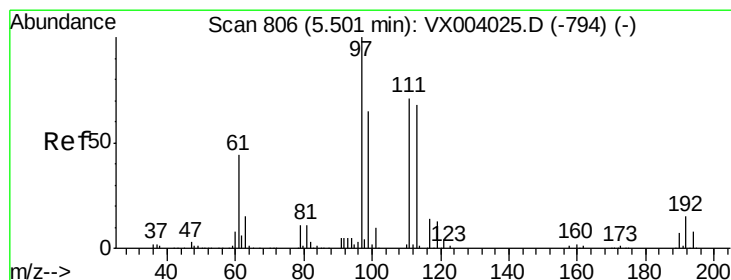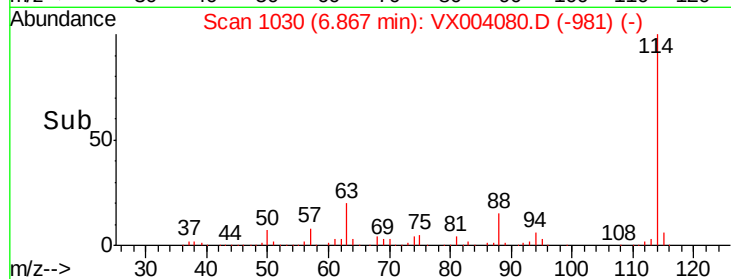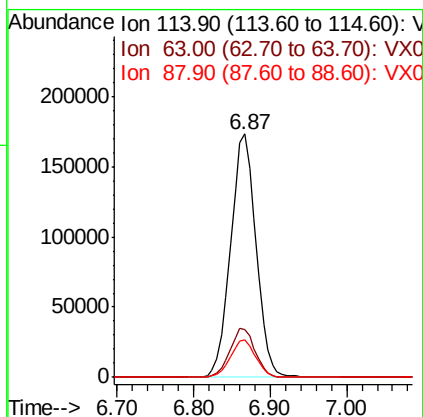

#35  
 Dibromofluoromethane  
 Concen: 51.55 ug/l  
 RT: 5.51 min Scan# 807  
 Delta R.T. 0.01 min  
 Lab File: VX004080.D  
 Acq: 15 Aug 2018 18:41

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 113     | 100   |       |       |
| 111     | 102.6 | 82.0  | 123.0 |
| 192     | 23.0  | 19.0  | 28.4  |

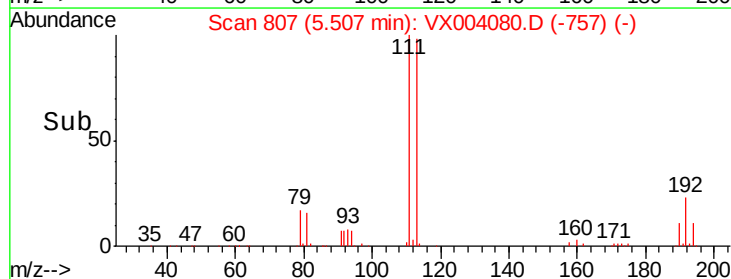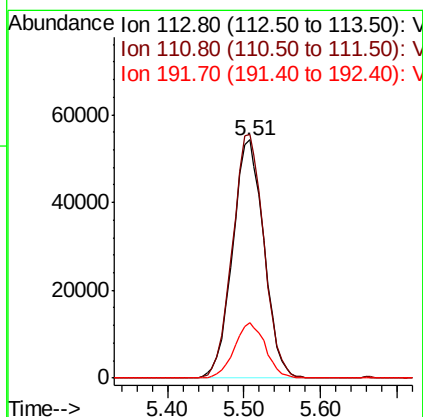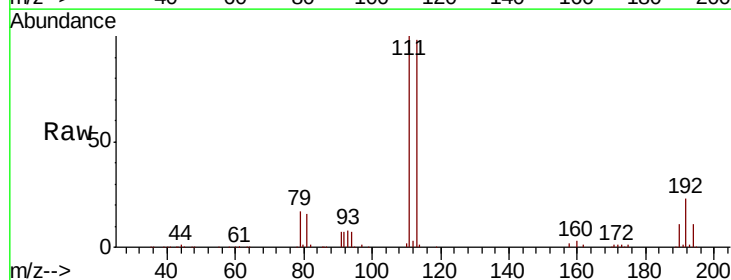


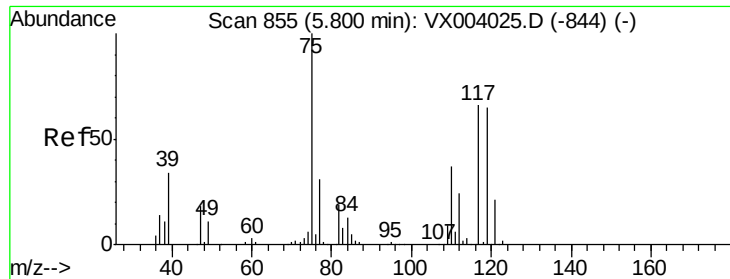




#36  
 1,1-Dichloropropene  
 Concen: 3.92 ug/l  
 RT: 5.66 min Scan# 832  
 Delta R.T. -0.14 min  
 Lab File: VX004080.D  
 Acq: 15 Aug 2018 18:41

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 KY038PS027-180813

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 75      | 100   |       |       |
| 110     | 9.2   | 18.2  | 54.6# |
| 77      | 0.0   | 25.0  | 37.4# |

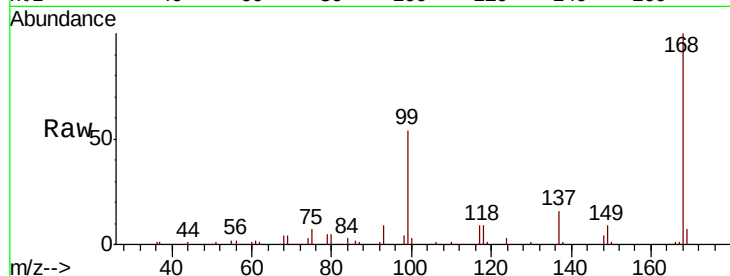


Abundance Ion 74.90 (74.60 to 75.60): VX0  
 Ion 109.90 (109.60 to 110.60): V  
 Ion 76.90 (76.60 to 77.60): VX0


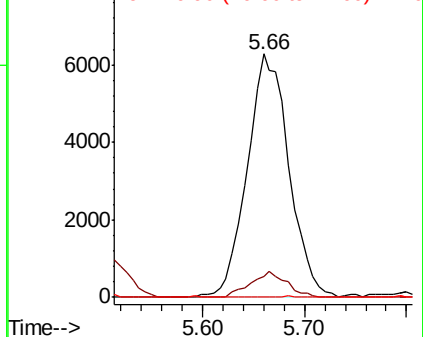



#38  
 Carbon Tetrachloride  
 Concen: 5.44 ug/l  
 RT: 5.67 min Scan# 833  
 Delta R.T. -0.12 min  
 Lab File: VX004080.D  
 Acq: 15 Aug 2018 18:41

| Tgt Ion | Ratio | Lower | Upper  |
|---------|-------|-------|--------|
| 117     | 100   |       |        |
| 119     | 6.0   | 79.5  | 119.3# |
| 121     | 0.0   | 25.0  | 37.4#  |



Abundance Ion 116.80 (116.50 to 117.50): V  
 Ion 118.80 (118.50 to 119.50): V  
 Ion 120.80 (120.50 to 121.50): V

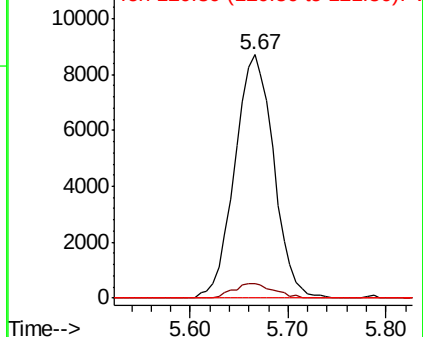


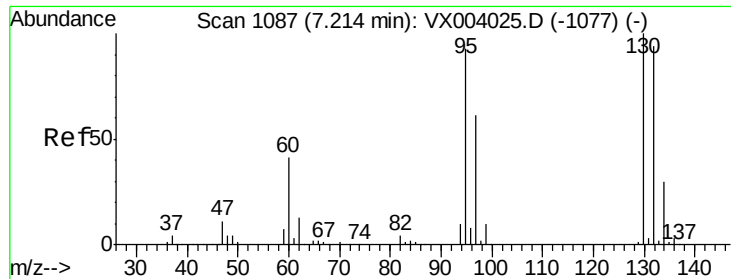




#44  
 Trichloroethene  
 Concen: 8.23 ug/l  
 RT: 7.21 min Scan# 1087  
 Delta R.T. -0.00 min  
 Lab File: VX004080.D  
 Acq: 15 Aug 2018 18:41

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 KY038PS027-180813

Tot Ion:130 Resp: 30462  
 Ion Ratio Lower Upper  
 130 100  
 95 98.1 0.0 199.4

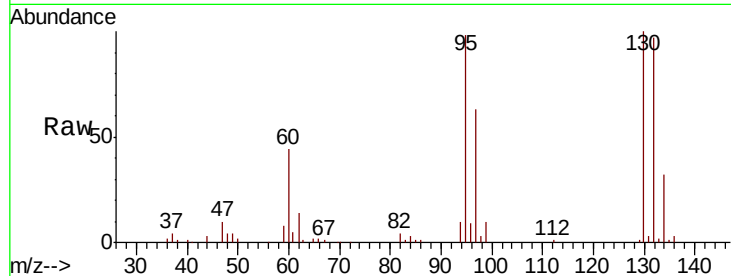


Abundance Ion 129.80 (129.50 to 130.50): V  
 Ion 94.90 (94.60 to 95.60): VX0

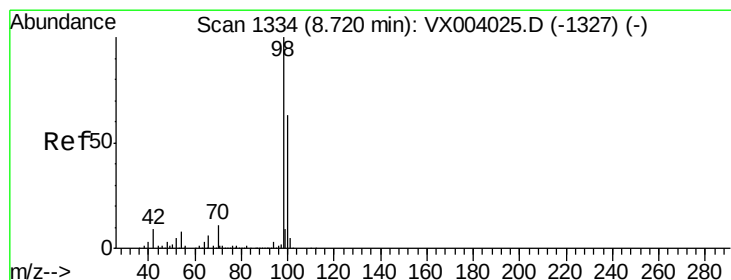
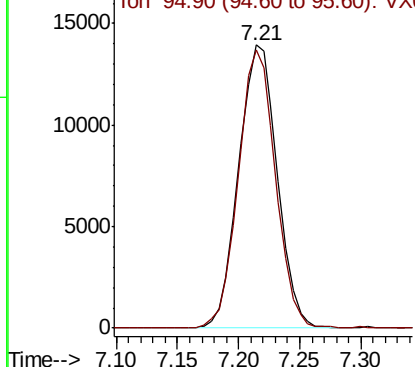



#50  
 Toluene-d8  
 Concen: 47.43 ug/l  
 RT: 8.72 min Scan# 1334  
 Delta R.T. -0.00 min  
 Lab File: VX004080.D  
 Acq: 15 Aug 2018 18:41

Tgt Ion: 98 Resp: 574463  
 Ion Ratio Lower Upper  
 98 100  
 100 65.9 53.3 79.9



Abundance Ion 98.00 (97.70 to 98.70): VX0  
 Ion 100.00 (99.70 to 100.70): V

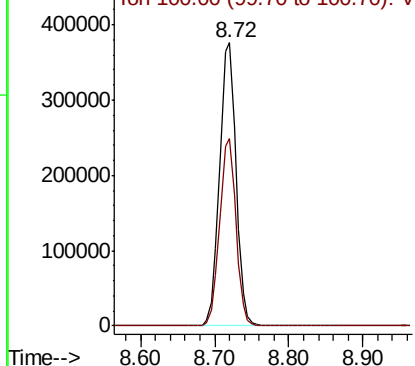



#60

Dibromochloromethane

Concen: 10.98 ug/l

RT: 9.34 min Scan# 1435

Delta R.T. -0.25 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41

Instrument :

MSVOA\_X

ClientSampleId :


KY038PS027-180813

Tot Ion:129 Resp: 37644

Ion Ratio Lower Upper

129 100

127 0.0 38.8 116.3#

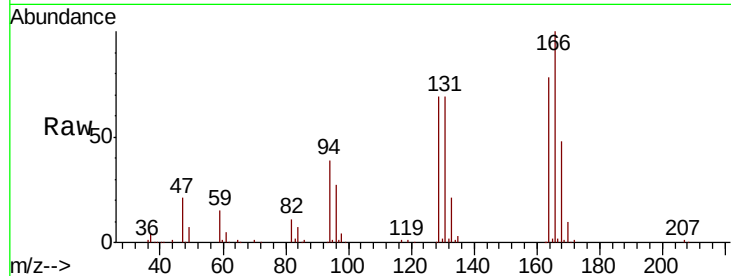

Abundance Ion 128.80 (128.50 to 129.50): V

Ion 126.80 (126.50 to 127.50): V

9.34

25000

20000



15000

10000

5000

0

Time-->

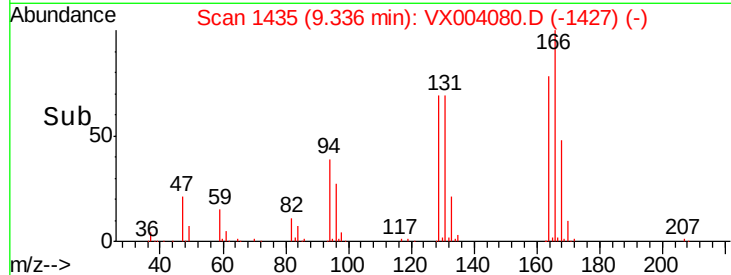

#62

4-Bromofluorobenzene

Concen: 43.49 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.00 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41


Tgt Ion: 95 Resp: 191065

Ion Ratio Lower Upper

95 100

174 91.0 0.0 182.8

176 88.0 0.0 179.0

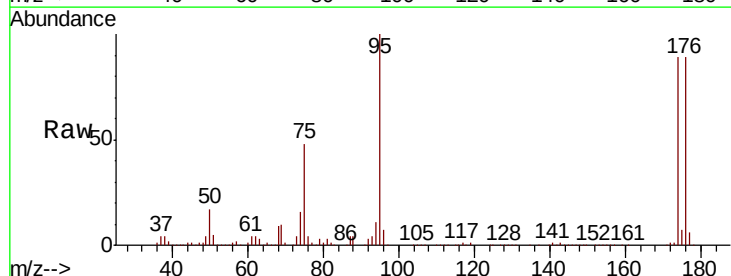

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

11.14

200000


150000


100000

50000

0

Time-->




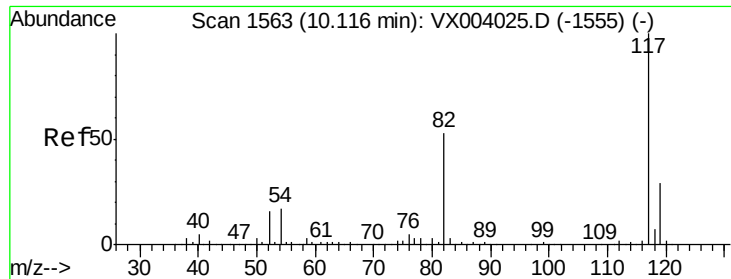




#63  
Chlorobenzene-d5  
Concen: 50.00 ug/l  
RT: 10.12 min Scan# 1563  
Delta R.T. -0.00 min  
Lab File: VX004080.D  
Acq: 15 Aug 2018 18:41

Instrument :  
MSVOA\_X  
ClientSampleId :  
KY038PS027-180813

Tot Ion:117 Resp: 381220  
Ion Ratio Lower Upper  
117 100  
82 50.4 45.4 68.0  
119 32.6 26.6 40.0




Abundance Ion 116.90 (116.60 to 117.60): V  
Ion 82.00 (81.70 to 82.70): VX0  
Ion 118.90 (118.60 to 119.60): V

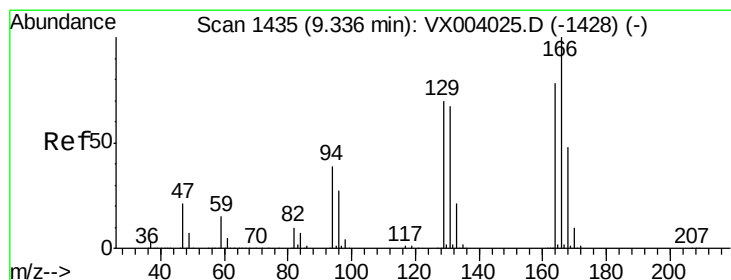
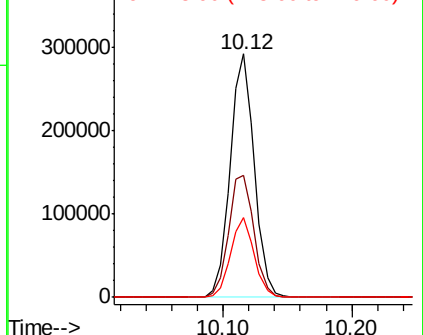



#64  
Tetrachloroethene  
Concen: 11.91 ug/l  
RT: 9.34 min Scan# 1435  
Delta R.T. -0.00 min  
Lab File: VX004080.D  
Acq: 15 Aug 2018 18:41

Tgt Ion:164 Resp: 43016  
Ion Ratio Lower Upper  
164 100  
166 127.6 98.0 147.0  
129 87.5 64.3 96.5  
131 88.5 66.8 100.2



Abundance Ion 163.80 (163.50 to 164.50): V  
Ion 165.80 (165.50 to 166.50): V  
Ion 128.80 (128.50 to 129.50): V  
Ion 130.80 (130.50 to 131.50): V

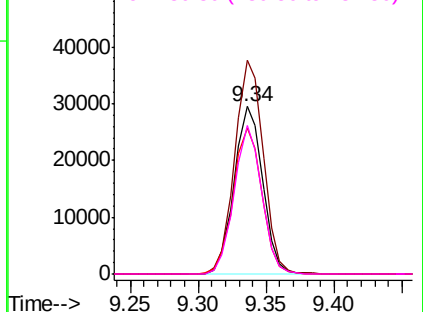



#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.08 min Scan# 1885

Delta R.T. -0.00 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41

Instrument :

MSVOA\_X

ClientSampleId :

KY038PS027-180813


Tot Ion:152 Resp: 195189

Ion Ratio Lower Upper

152 100

115 56.1 39.1 117.3




150 153.1 0.0 349.2

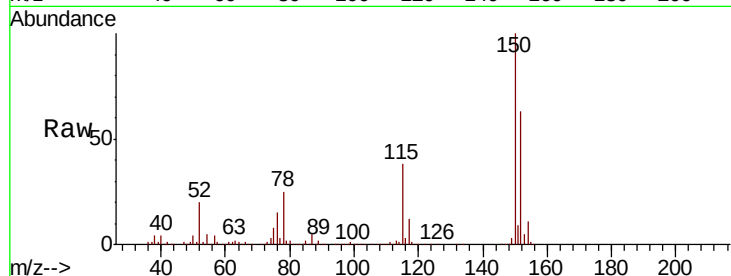

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

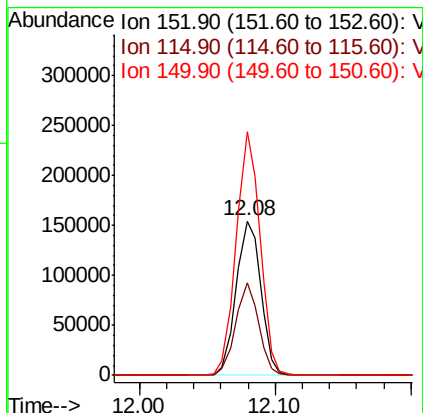

#76

1,2,3-Trichloropropane

Concen: 23.69 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.16 min

Lab File: VX004080.D


Acq: 15 Aug 2018 18:41

Tgt Ion: 75 Resp: 92748

Ion Ratio Lower Upper



75 100

77 1.3 20.8 62.5#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

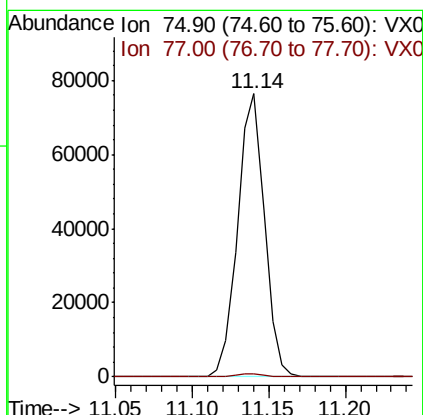





#81

trans-1,4-Dichloro-2-butene

Concen: 73.35 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.06 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41

Instrument :

MSVOA\_X

ClientSampleId :

KY038PS027-180813


Tot Ion: 75 Resp: 92748

Ion Ratio Lower Upper

75 100

53 0.3 80.3 120.5#




89 0.0 37.8 56.8#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

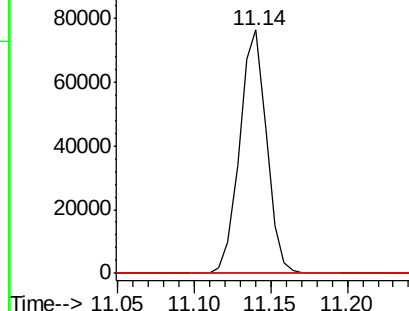

#95

Naphthalene

Concen: 1.17 ug/l

RT: 13.84 min Scan# 2174

Delta R.T. 0.01 min

Lab File: VX004080.D

Acq: 15 Aug 2018 18:41


Tgt Ion: 128 Resp: 396

Ion Ratio Lower Upper

128 100

127 10.4 10.2 15.2

129 0.0 8.8 13.2#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

