


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081518\
Data File : VX004069.D
Acq On : 15 Aug 2018 12:23
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Title : SW846 8260
Last Update : Tue Aug 14 13:27:25 2018

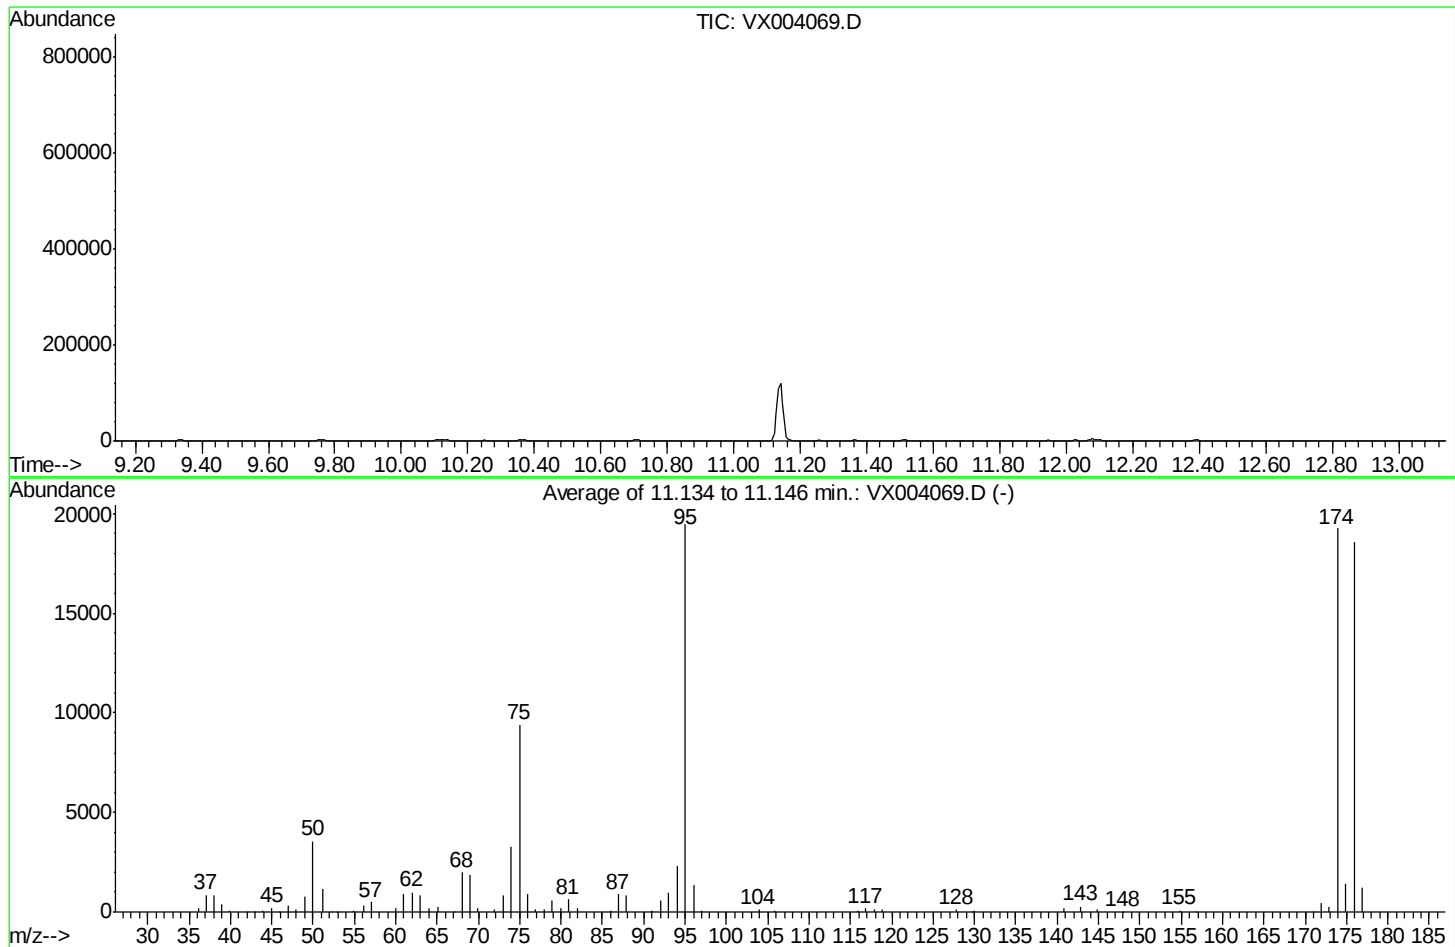

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	3545	PASS
75	95	30	60	48.3	9403	PASS
95	95	100	100	100.0	19466	PASS
96	95	5	9	7.0	1355	PASS
173	174	0.00	2	1.4	270	PASS
174	95	50	100	99.0	19263	PASS
175	174	5	9	7.4	1433	PASS
176	174	95	101	96.3	18552	PASS
177	176	5	9	6.7	1234	PASS