


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081518\
Data File : VX004092.D
Acq On : 16 Aug 2018 00:27
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Title : SW846 8260
Last Update : Tue Aug 14 13:27:25 2018

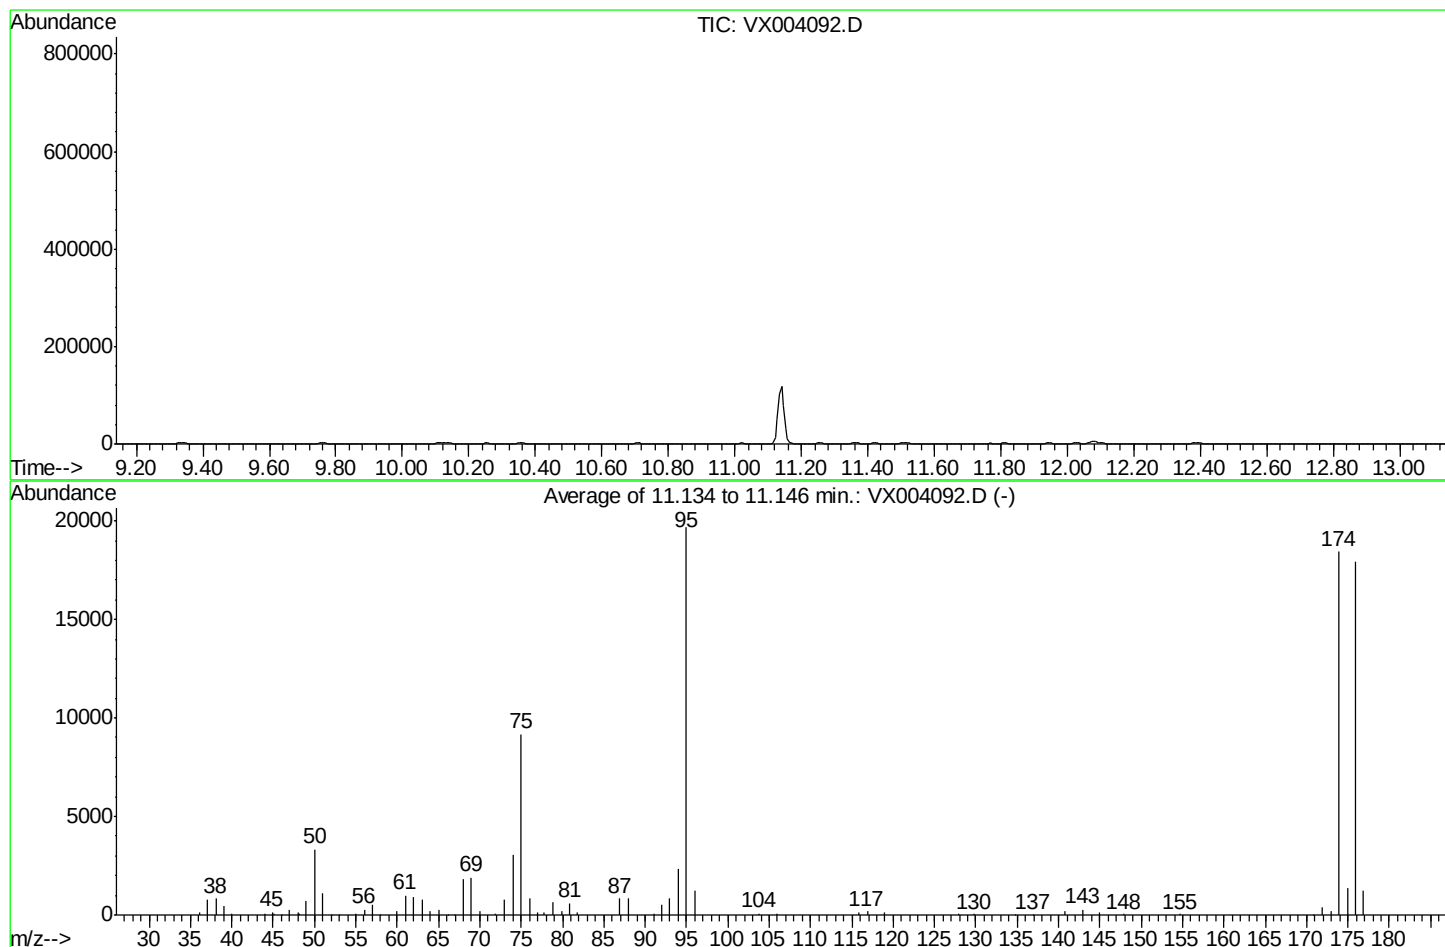

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	3320	PASS
75	95	30	60	46.7	9184	PASS
95	95	100	100	100.0	19672	PASS
96	95	5	9	6.3	1241	PASS
173	174	0.00	2	0.9	174	PASS
174	95	50	100	93.7	18440	PASS
175	174	5	9	7.5	1391	PASS
176	174	95	101	97.3	17945	PASS
177	176	5	9	6.9	1236	PASS