



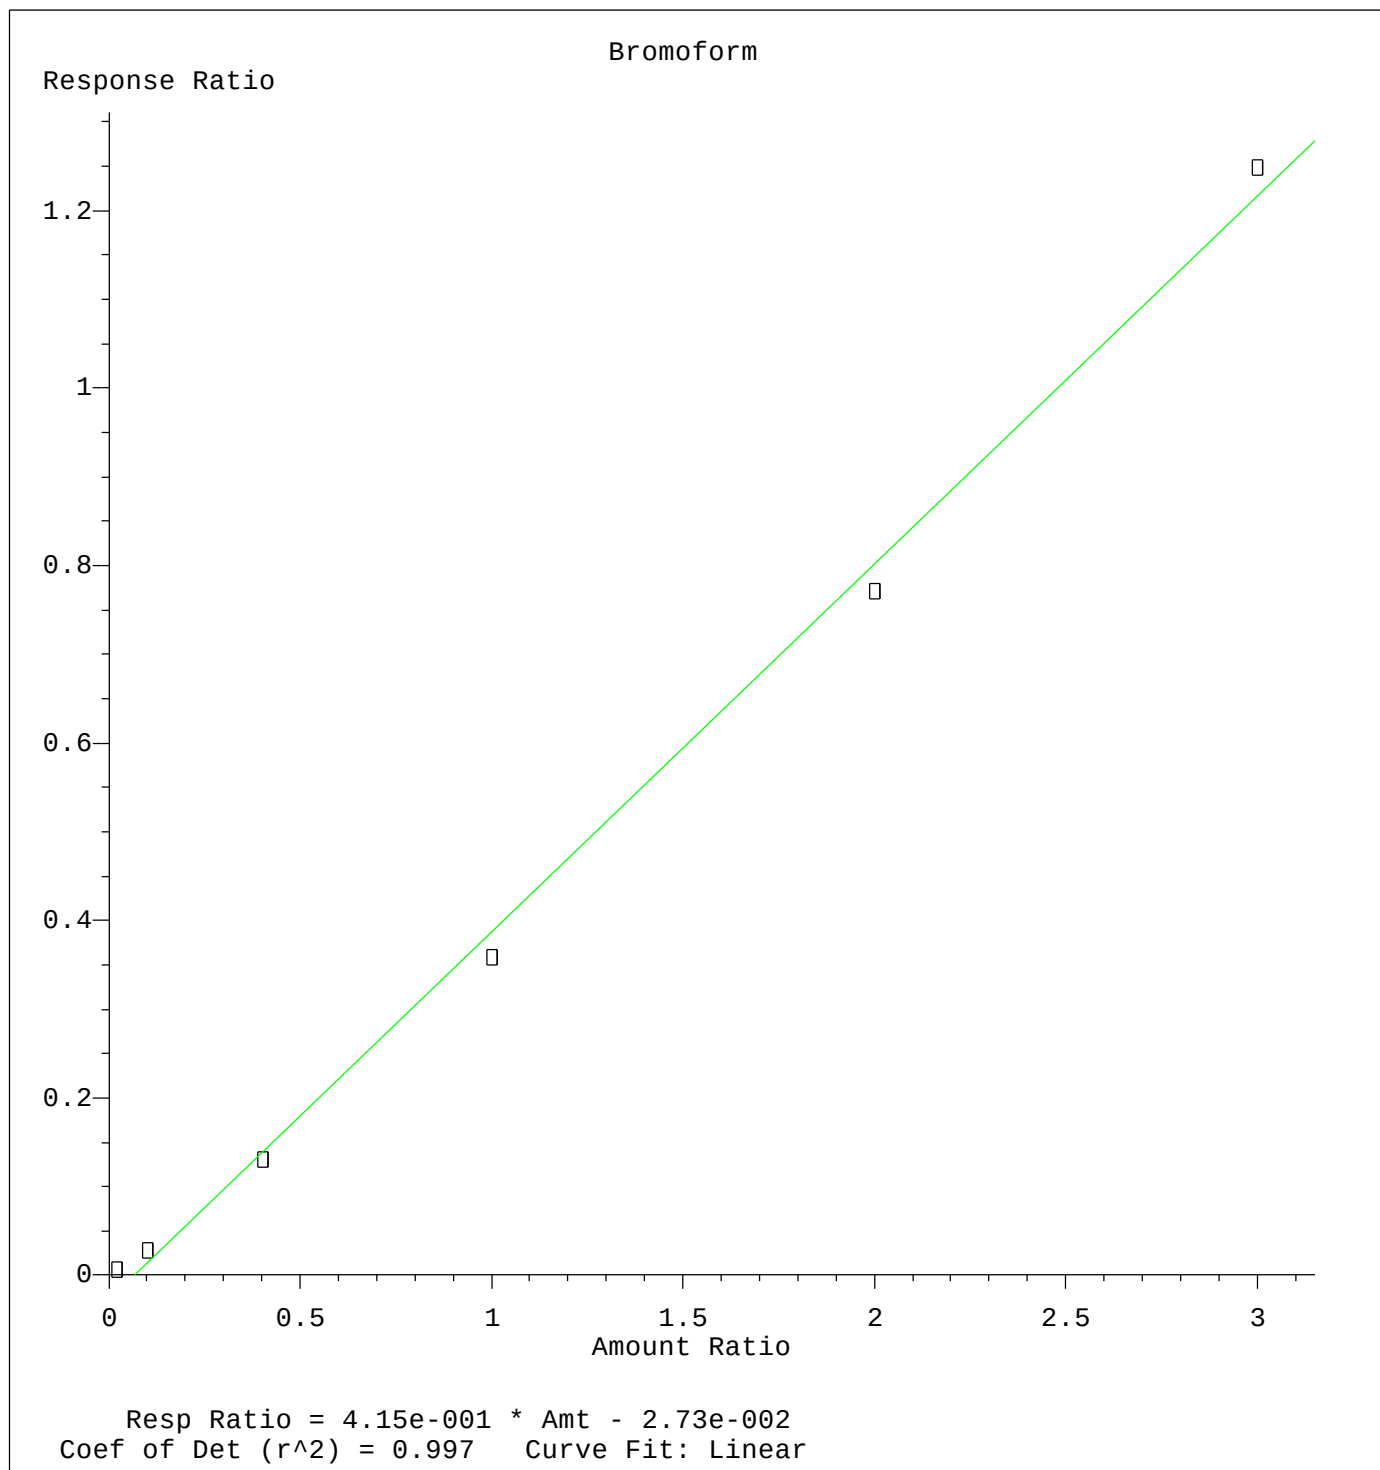

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
Calibration Table Last Updated: Fri Aug 16 04:15:26 2019


trans-1,4-Dichloro-2-butene

Response Ratio

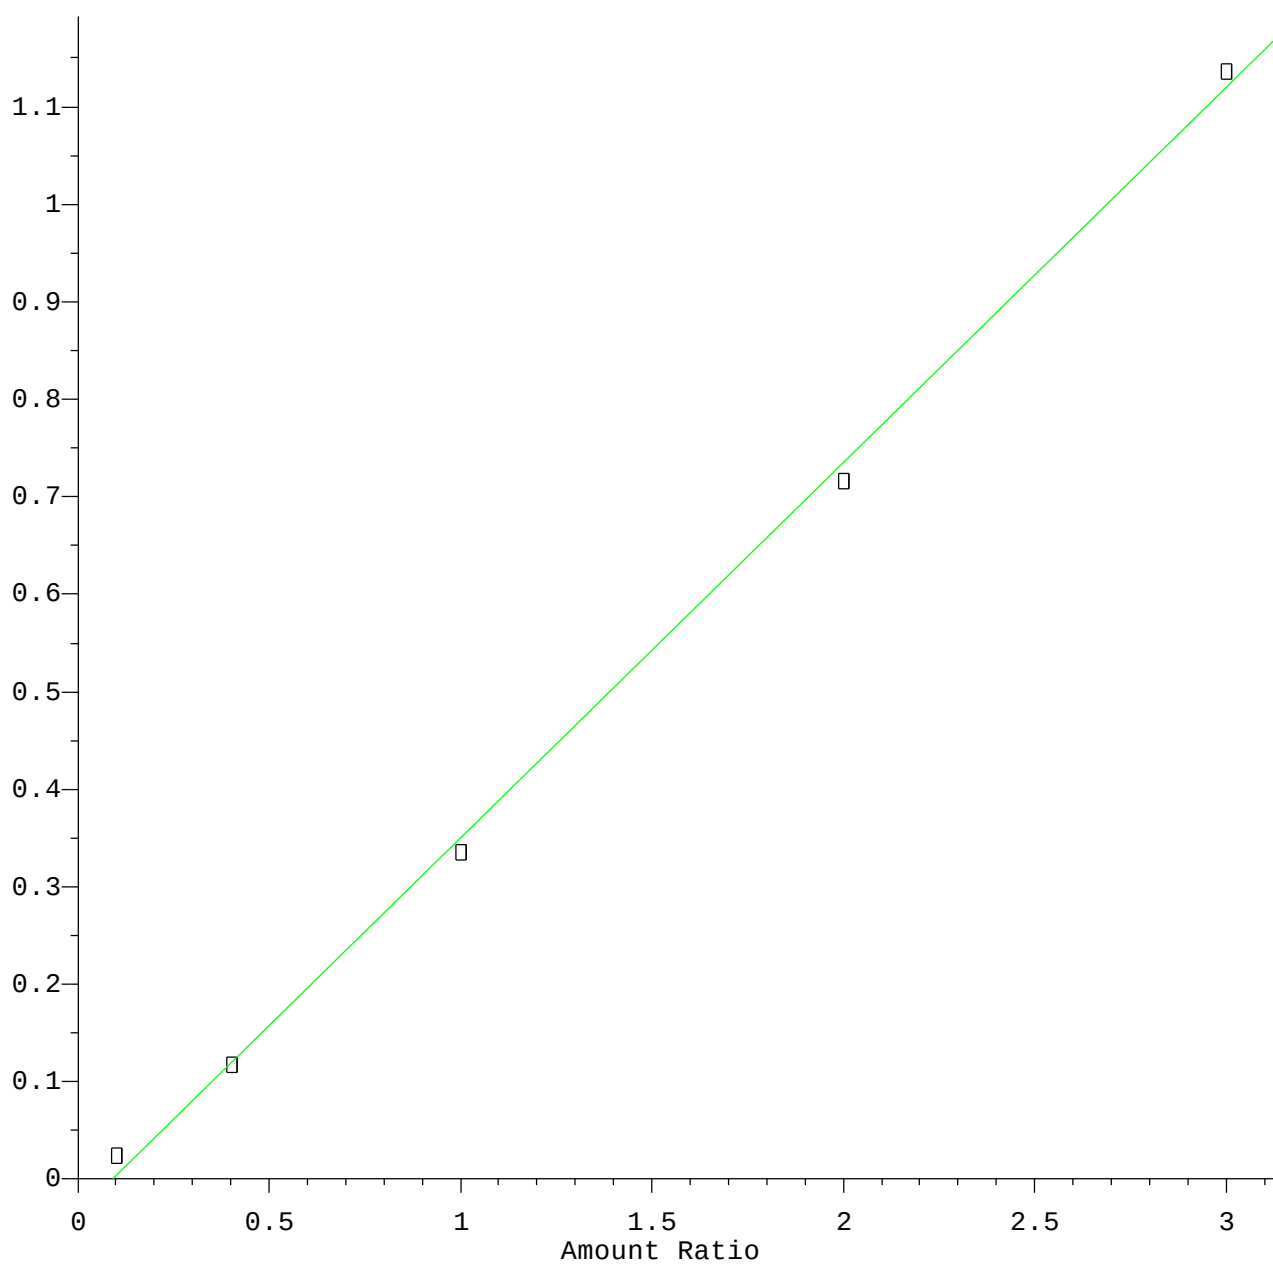

Resp Ratio = $3.84 \times 10^{-1} \times \text{Amt} - 3.45 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
Calibration Table Last Updated: Fri Aug 16 04:15:26 2019

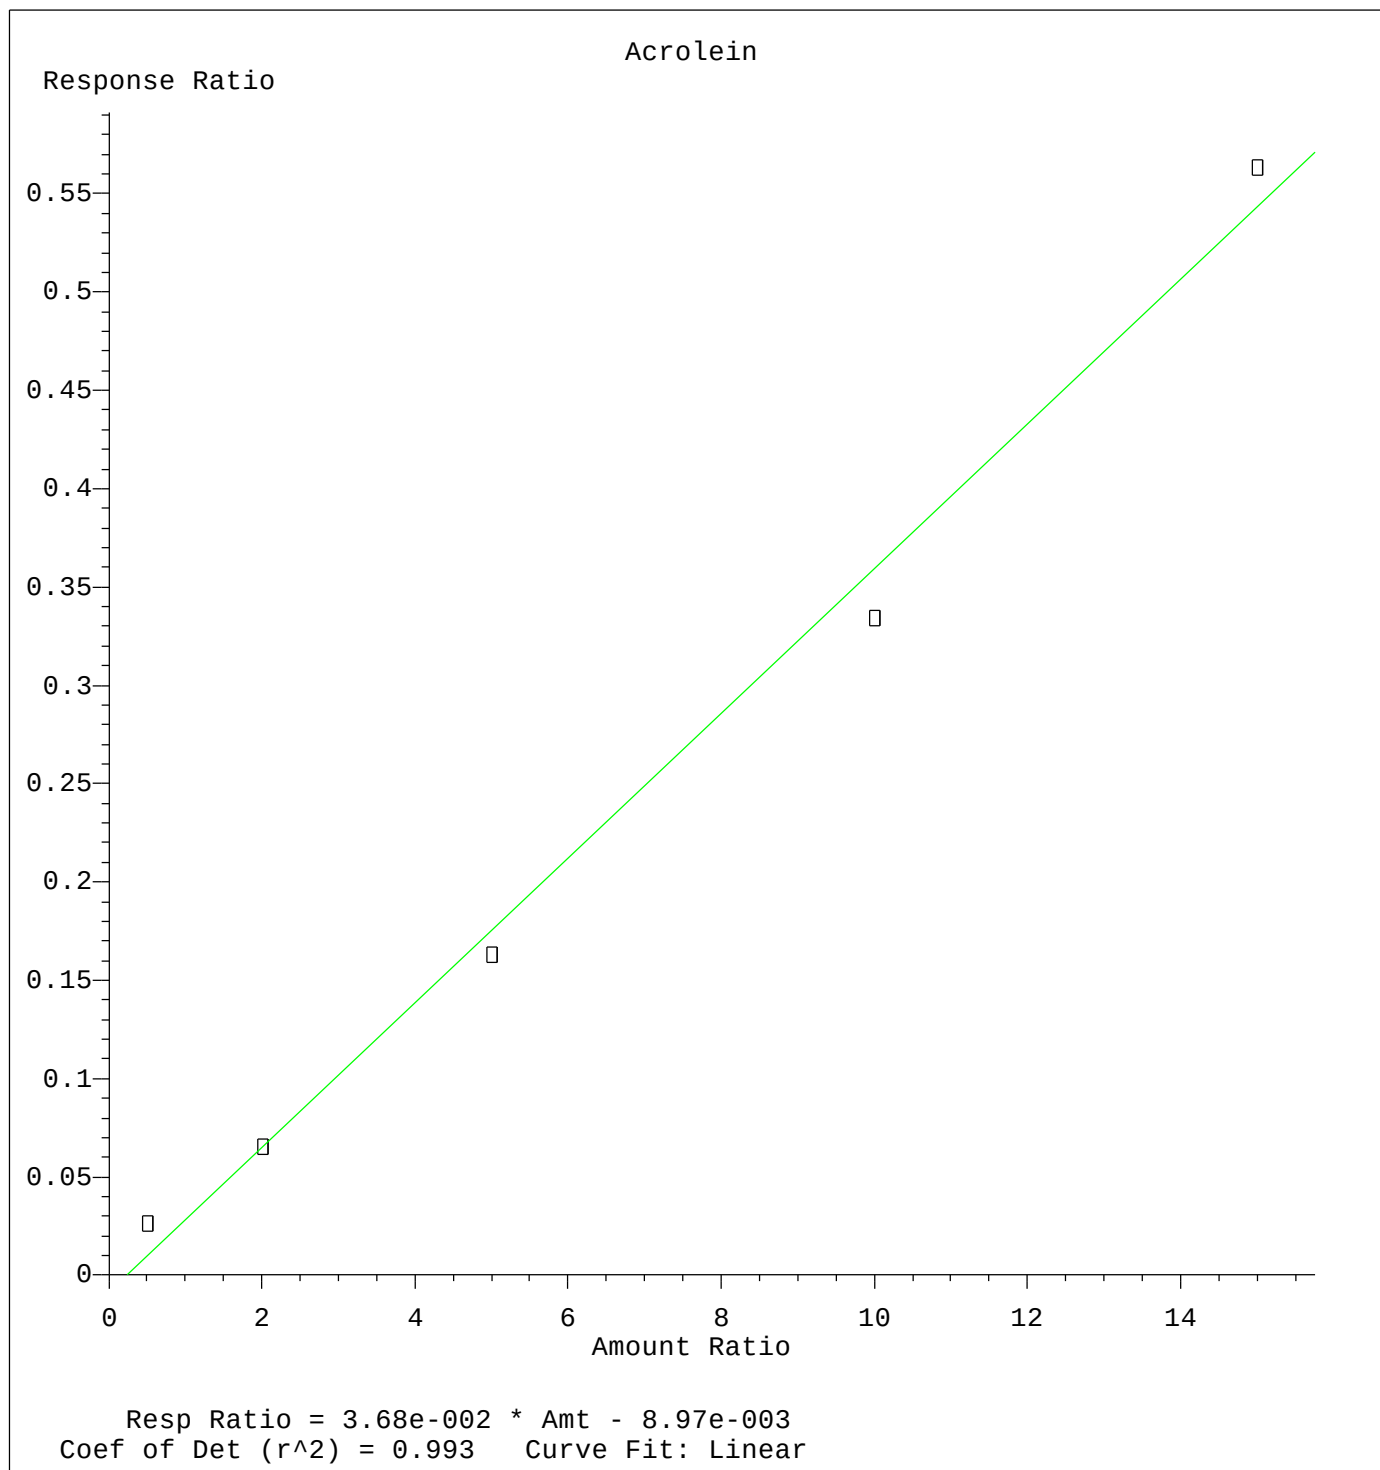

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
Calibration Table Last Updated: Fri Aug 16 04:15:26 2019