


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081519\
Data File : VX011562.D
Acq On : 15 Aug 2019 16:49
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
Title : SW846 8260
Last Update : Fri Aug 16 04:15:26 2019

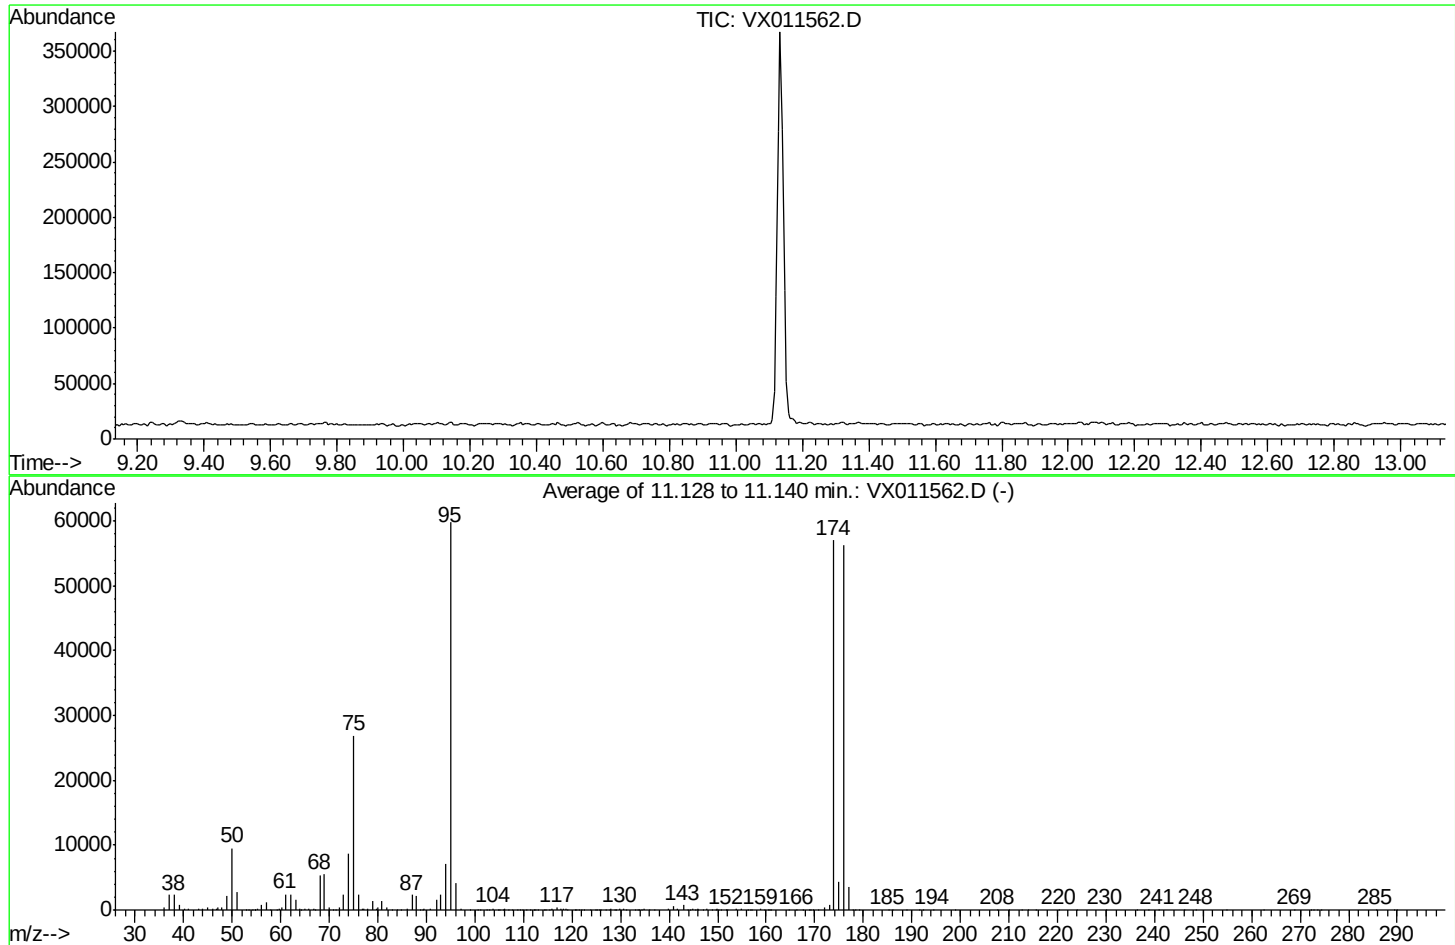

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	9495	PASS
75	95	30	60	45.1	26953	PASS
95	95	100	100	100.0	59814	PASS
96	95	5	9	6.9	4099	PASS
173	174	0.00	2	1.3	742	PASS
174	95	50	100	95.4	57053	PASS
175	174	5	9	7.7	4410	PASS
176	174	95	101	98.6	56233	PASS
177	176	5	9	6.2	3476	PASS