

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030619.D
 Acq On : 15 Aug 2022 10:55
 Operator : JC/MD
 Sample : VX0815MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK684

Quant Time: Aug 16 04:28:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 16 04:27:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	250088	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	220503	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	101301	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	55070	34.290	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	68.580%		
7) Chloroethane-d5	1.673	69	50698	44.780	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	89.560%		
11) 1,1-Dichloroethene-d2	2.307	63	99779	32.844	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.680%		
21) 2-Butanone-d5	4.465	46	183901	123.584	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	123.580%		
24) Chloroform-d	5.056	84	164426	49.735	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.460%		
26) 1,2-Dichloroethane-d4	5.958	65	117563	52.371	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.740%		
32) Benzene-d6	5.977	84	287398	45.502	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.000%		
36) 1,2-Dichloropropane-d6	7.312	67	103103	50.312	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.620%		
41) Toluene-d8	8.647	98	247583	41.584	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.160%		
43) trans-1,3-Dichloroprop...	8.952	79	45705	44.832	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.660%		
47) 2-Hexanone-d5	9.385	63	119124	114.043	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	114.040%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	150984	56.085	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	112.160%		
66) 1,2-Dichlorobenzene-d4	12.323	152	93288	47.479	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.960%		
Target Compounds						Qvalue
37) 1,2-Dichloropropane	7.306	63	12177	6.478	ug/L #	89
39) cis-1,3-Dichloropropene	8.330	75	3481	1.241	ug/L #	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030619.D
Acq On : 15 Aug 2022 10:55
Operator : JC/MD
Sample : VX0815MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK684

Quant Time: Aug 16 04:28:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 16 04:27:08 2022
Response via : Initial Calibration

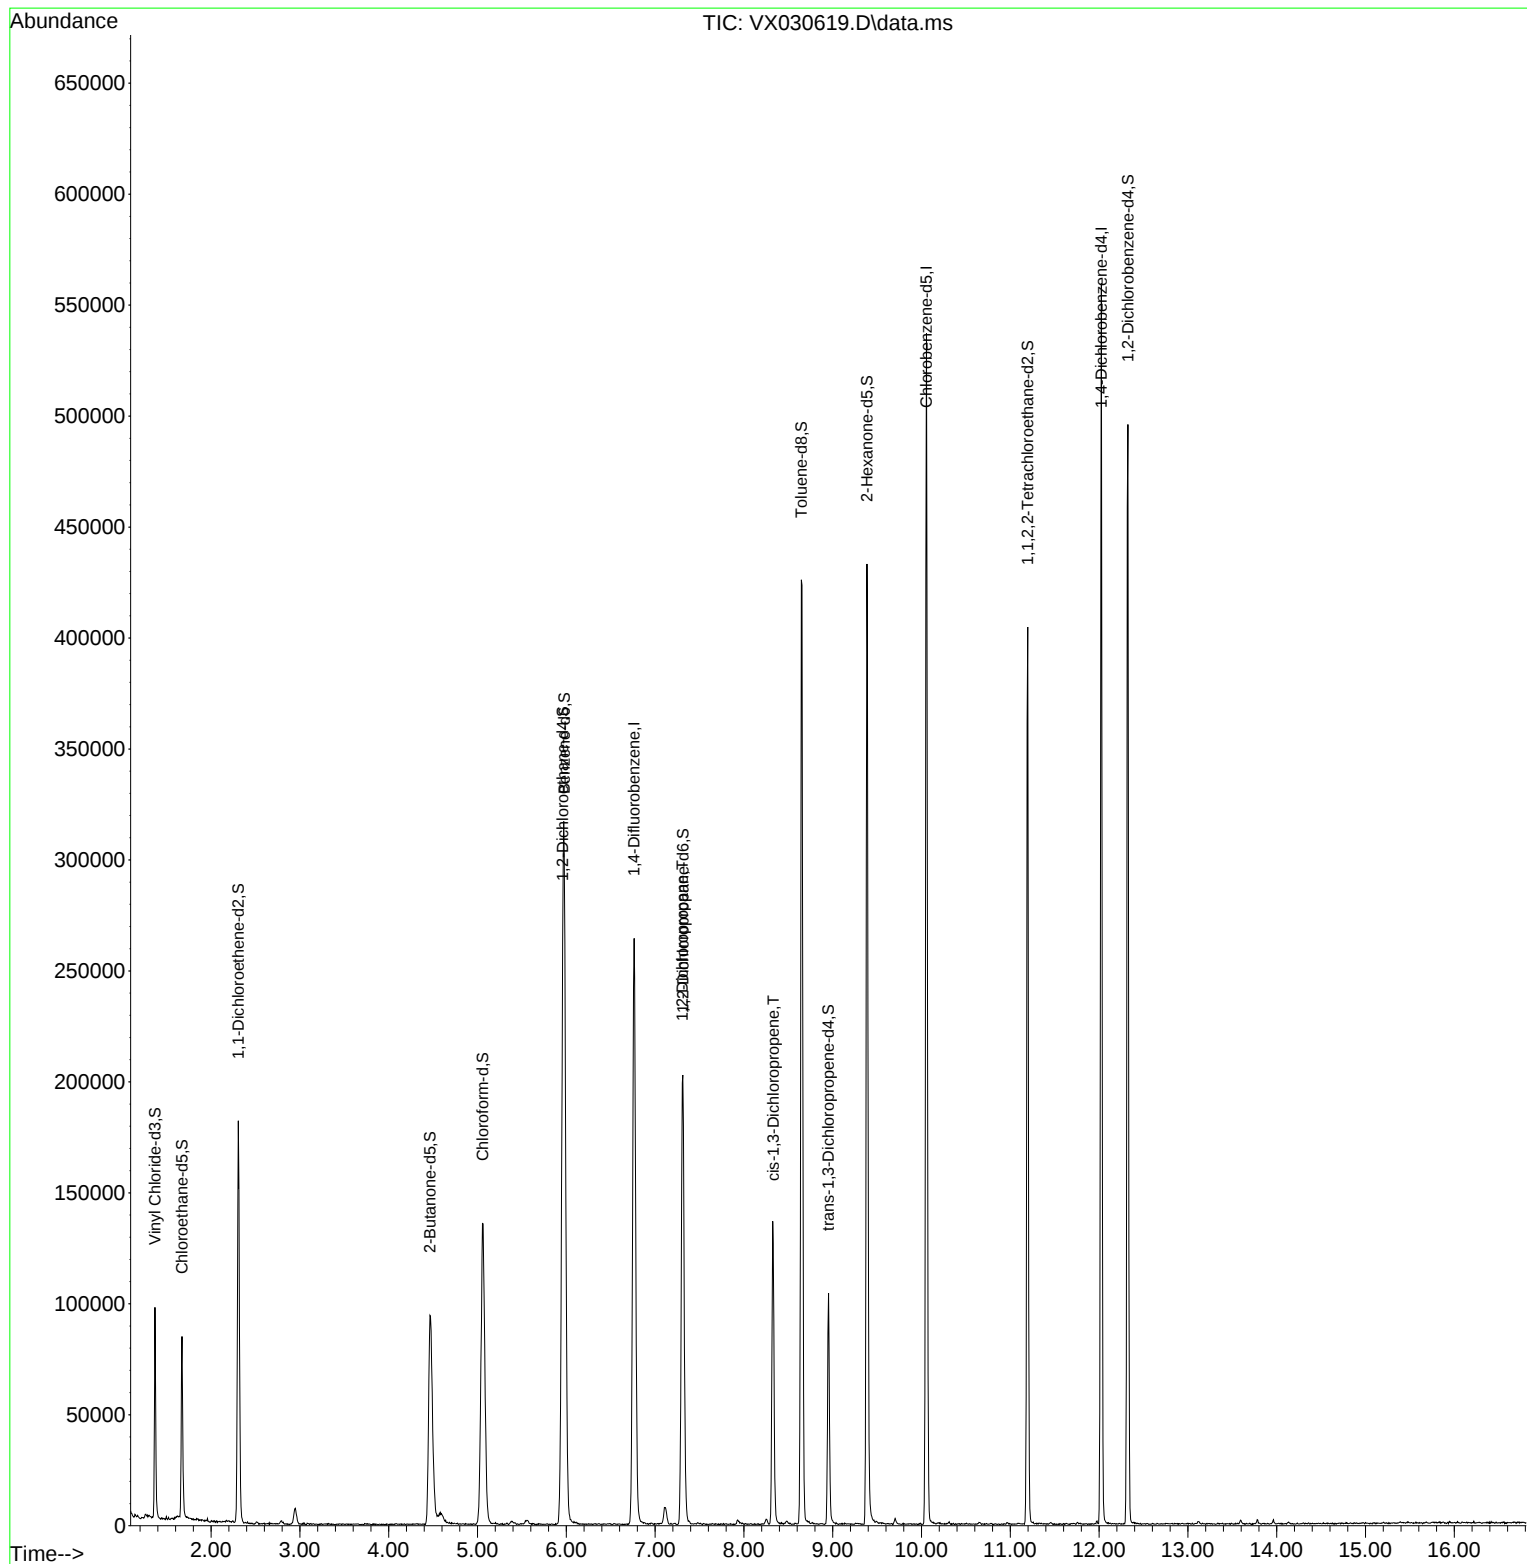

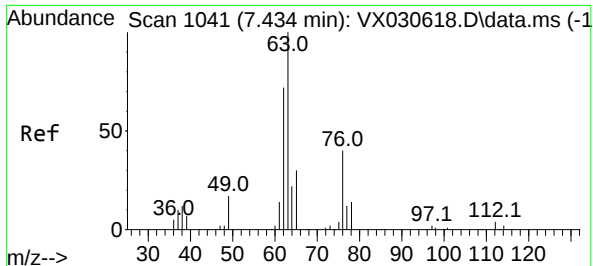

#37

1,2-Dichloropropane

Concen: 6.478 ug/L

RT: 7.306 min Scan# 1187

Delta R.T. -0.128 min

Lab File: VX030619.D

Acq: 15 Aug 2022 10:55

Instrument :

MSVOA_X

ClientSampleId :





VBLK684

Tgt Ion: 63 Resp: 12177

Ion Ratio Lower Upper

63 100

112 0.0 3.0 4.4#

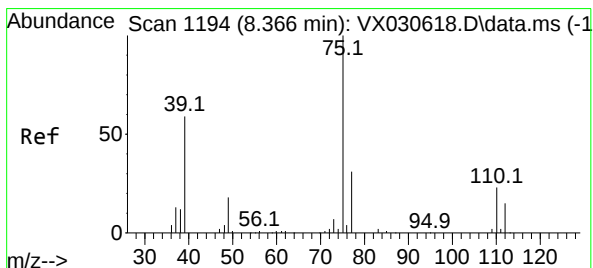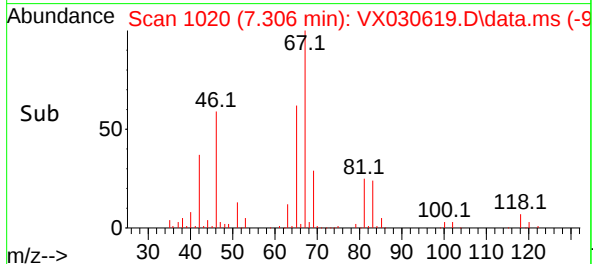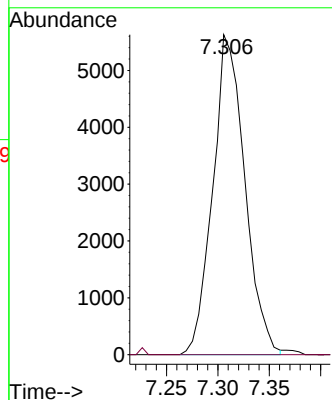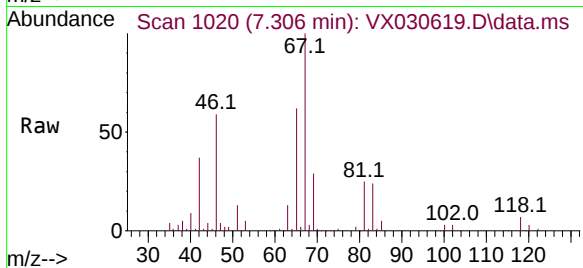

#39

cis-1,3-Dichloropropene

Concen: 1.241 ug/L

RT: 8.330 min Scan# 1188

Delta R.T. -0.036 min

Lab File: VX030619.D

Acq: 15 Aug 2022 10:55

Tgt Ion: 75 Resp: 3481

Ion Ratio Lower Upper

75 100

77 47.0 22.4 41.6#

