

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030624.D
 Acq On : 15 Aug 2022 13:42
 Operator : JC/MD
 Sample : N4193-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Quant Time: Aug 16 04:29:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 16 04:27:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	245478	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	227002	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	99190	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	84063	53.325	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery	= 106.660%		
7) Chloroethane-d5	1.672	69	65548	58.983	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery	= 117.960%		
11) 1,1-Dichloroethene-d2	2.306	63	140098	46.982	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery	= 93.960%		
21) 2-Butanone-d5	4.471	46	167304	114.542	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery	= 114.540%		
24) Chloroform-d	5.056	84	179588	55.341	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	= 110.680%		
26) 1,2-Dichloroethane-d4	5.958	65	131575	59.714	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	= 119.420%		
32) Benzene-d6	5.977	84	350560	53.912	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	= 107.820%		
36) 1,2-Dichloropropane-d6	7.312	67	115062	54.540	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery	= 109.080%		
41) Toluene-d8	8.653	98	316452	51.630	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery	= 103.260%		
43) trans-1,3-Dichloroprop...	8.952	79	52182	49.720	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery	= 99.440%		
47) 2-Hexanone-d5	9.384	63	107544	100.010	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery	= 100.010%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	150960	54.470	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery	= 108.940%		
66) 1,2-Dichlorobenzene-d4	12.323	152	105899	55.044	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery	= 110.080%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	8.952	75	2355	0.833	ug/L #	76
61) 1,2,3-Trichloropropane	12.024	75	12980	6.093	ug/L #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030624.D
Acq On : 15 Aug 2022 13:42
Operator : JC/MD
Sample : N4193-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Time: Aug 16 04:29:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 16 04:27:08 2022
Response via : Initial Calibration




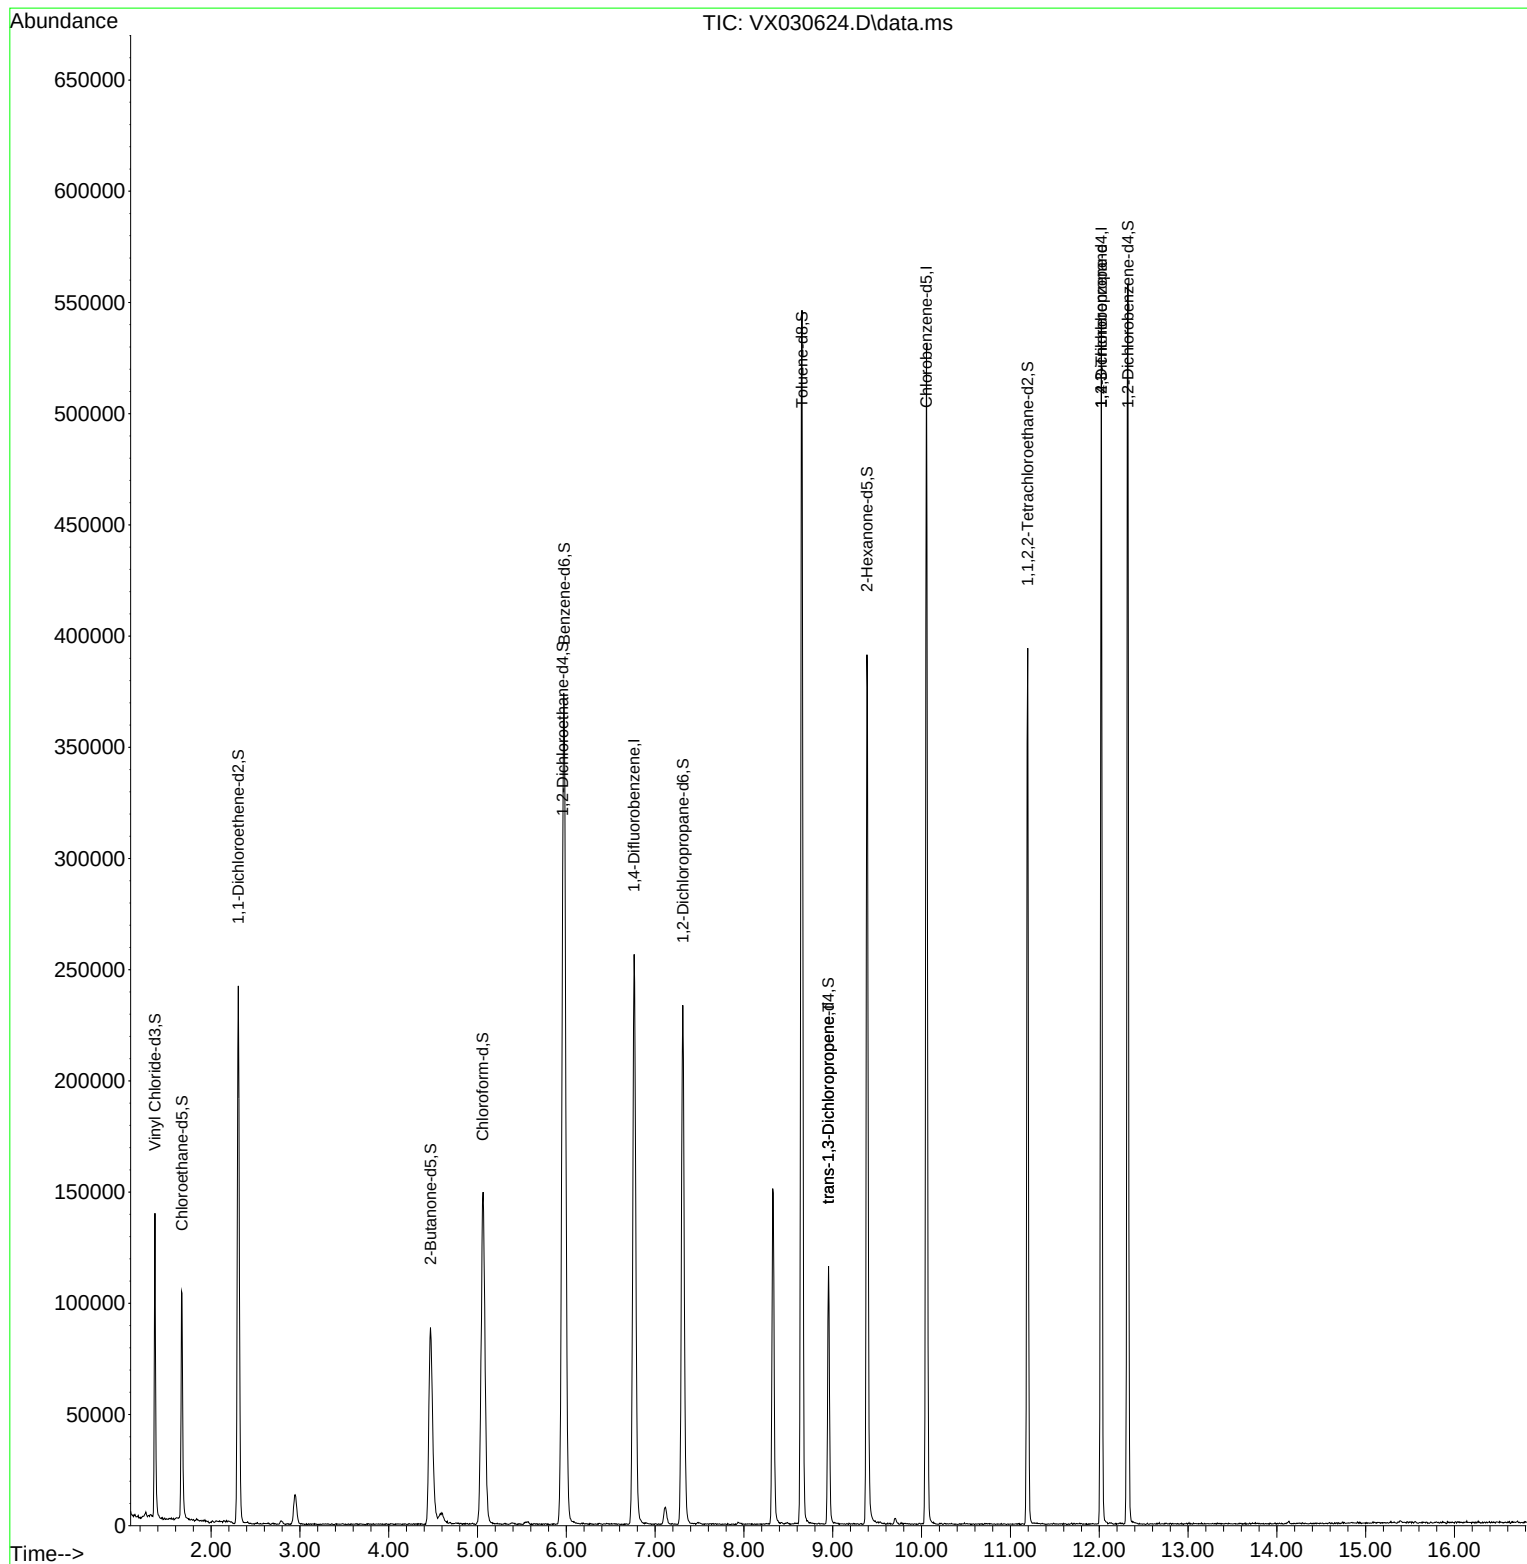


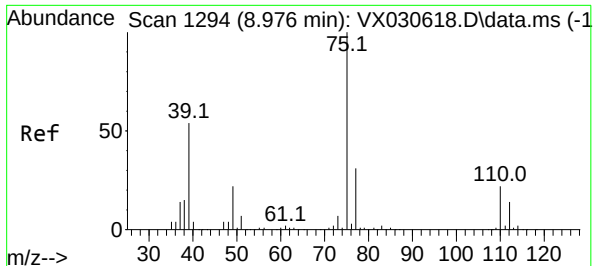

#44
trans-1,3-Dichloropropene
Concen: 0.833 ug/L
RT: 8.952 min Scan# 1794
Delta R.T. -0.024 min
Lab File: VX030624.D
Acq: 15 Aug 2022 13:42

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Tgt Ion: 75 Resp: 2355
Ion Ratio Lower Upper
75 100
77 45.7 22.5 41.7#

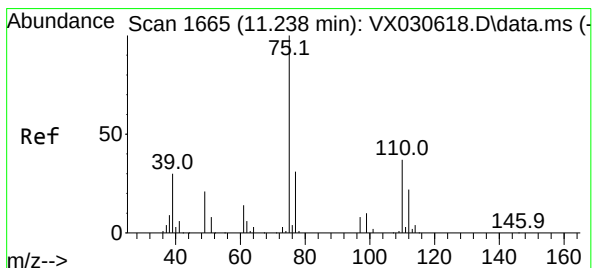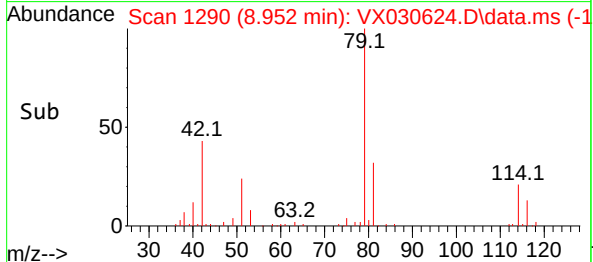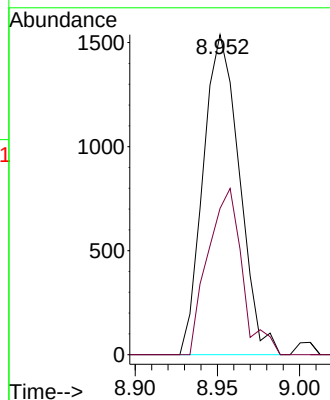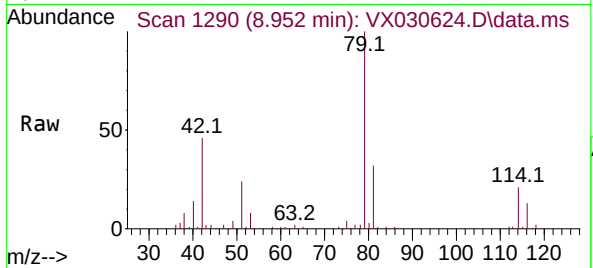

#61
1,2,3-Trichloropropane
Concen: 6.093 ug/L
RT: 12.024 min Scan# 1794
Delta R.T. 0.786 min
Lab File: VX030624.D
Acq: 15 Aug 2022 13:42

Tgt Ion: 75 Resp: 12980
Ion Ratio Lower Upper
75 100
77 33.5 26.1 39.1
110 4.0 30.5 45.7#

