

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030627.D
 Acq On : 15 Aug 2022 15:01
 Operator : JC/MD
 Sample : N4168-02
 Misc : 9.65g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX9B1

Quant Time: Aug 16 04:30:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 16 04:27:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	228008	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	203114	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	85528	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	43409	29.646	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	59.300%#
7) Chloroethane-d5	1.666	69	23688	22.949	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	45.900%#
11) 1,1-Dichloroethene-d2	2.282	63	69624	25.137	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	50.280%#
21) 2-Butanone-d5	4.507	46	71012	52.342	ug/L	0.04
Spiked Amount	100.000	Range	40 - 130	Recovery	=	52.340%
24) Chloroform-d	5.068	84	87100	28.897	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	57.800%#
26) 1,2-Dichloroethane-d4	5.964	65	67065	32.769	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	65.540%#
32) Benzene-d6	5.970	84	181376	31.174	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	62.340%#
36) 1,2-Dichloropropane-d6	7.312	67	59008	31.260	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	62.520%#
41) Toluene-d8	8.653	98	164585	30.011	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	60.020%#
43) trans-1,3-Dichloroprop...	8.958	79	24710	26.313	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	52.620%#
47) 2-Hexanone-d5	9.409	63	47324	49.184	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	49.180%
56) 1,1,2,2-Tetrachloroeth...	11.201	84	67100	27.059	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	54.120%#
66) 1,2-Dichlorobenzene-d4	12.323	152	51349	30.954	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	61.900%#
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.727	43	11169	5.427	ug/L	98
61) 1,2,3-Trichloropropane	12.024	75	11551	6.289	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030627.D
Acq On : 15 Aug 2022 15:01
Operator : JC/MD
Sample : N4168-02
Misc : 9.65g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX9B1

Quant Time: Aug 16 04:30:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 16 04:27:08 2022
Response via : Initial Calibration




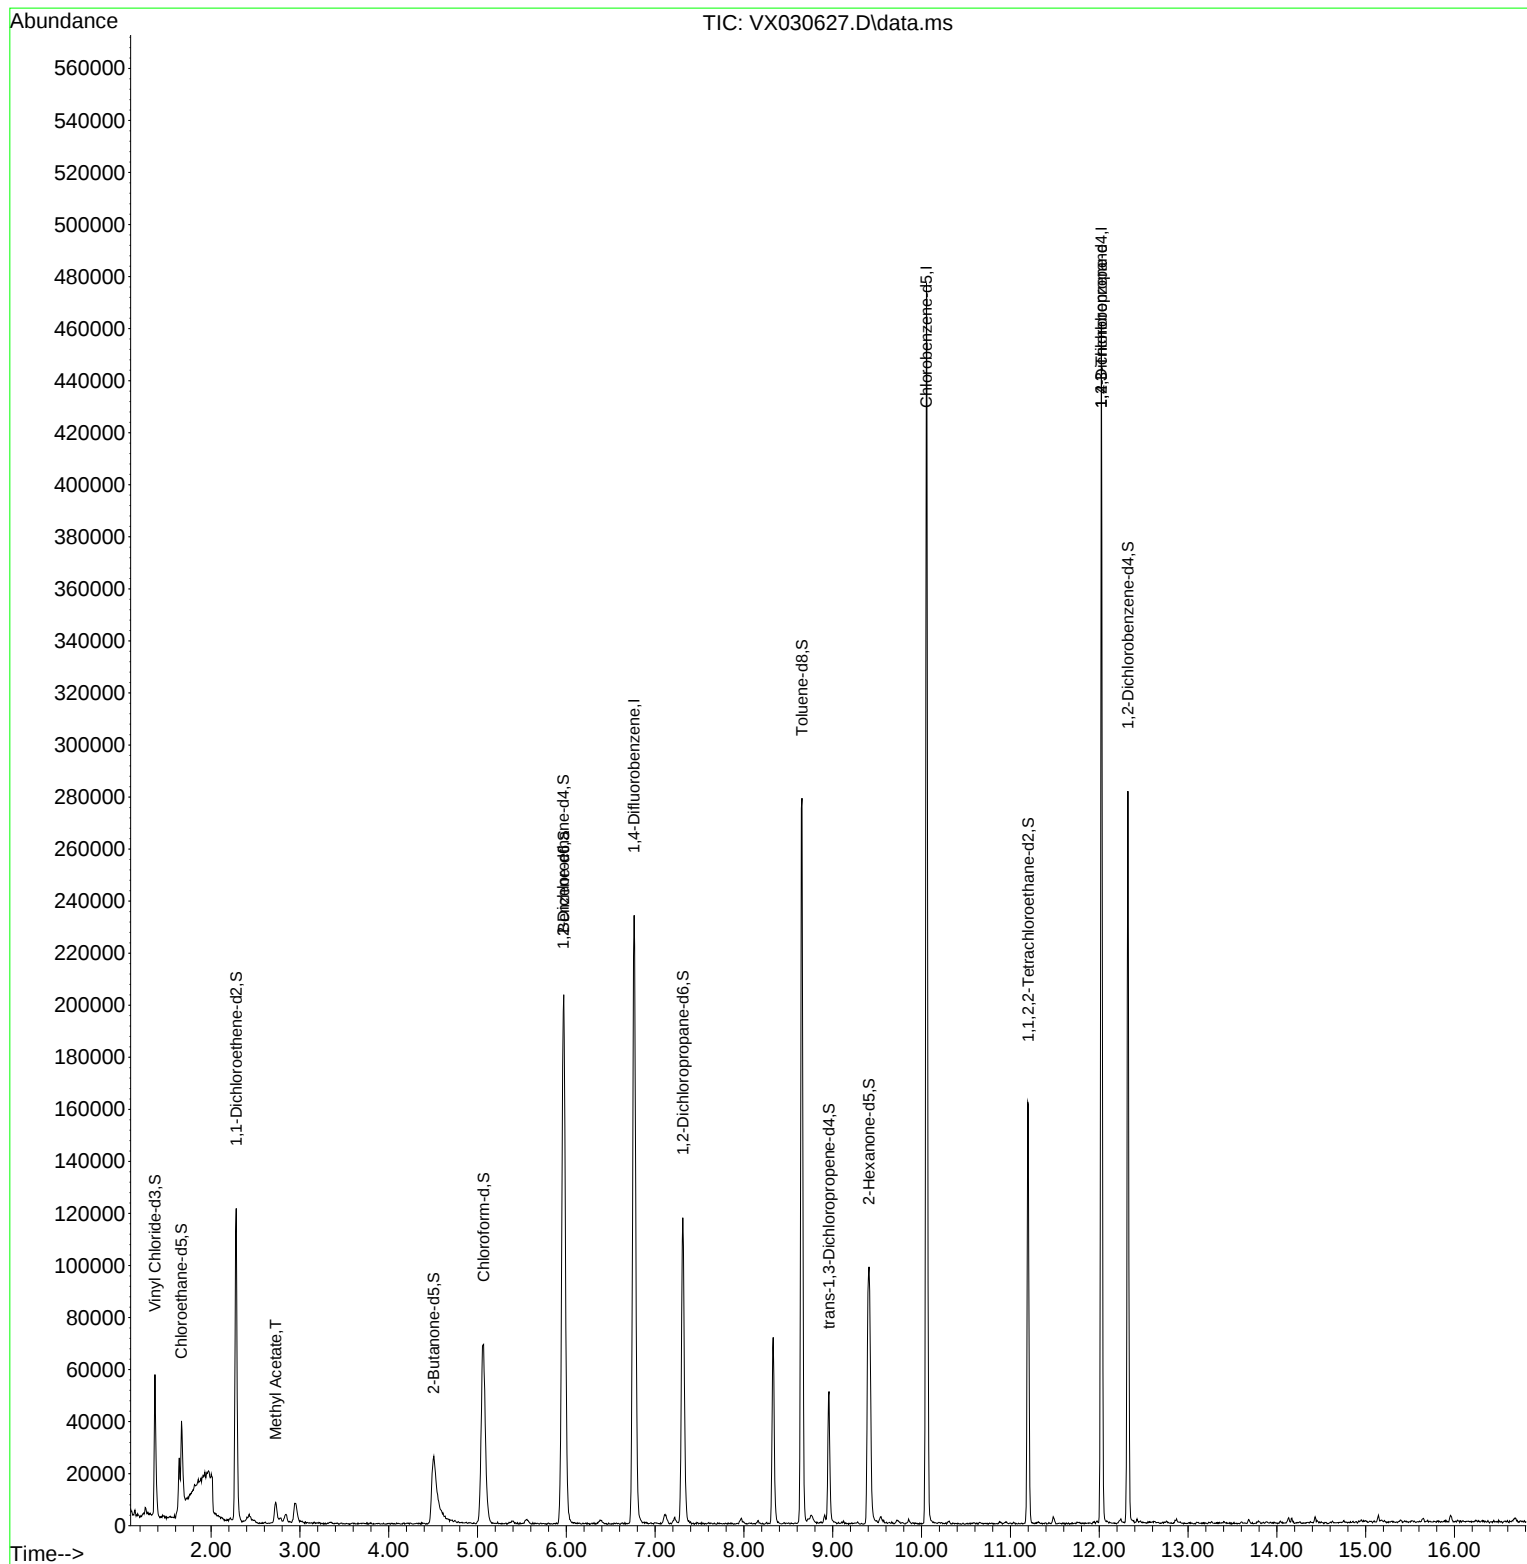


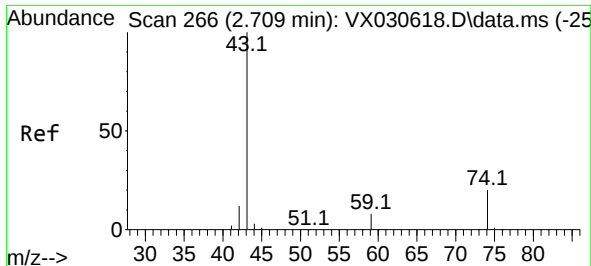

#15
Methyl Acetate
Concen: 5.427 ug/L
RT: 2.727 min Scan# 21
Delta R.T. 0.018 min
Lab File: VX030627.D
Acq: 15 Aug 2022 15:01

Instrument :
MSVOA_X
ClientSampleId :
EX9B1

Tgt Ion: 43 Resp: 11169
Ion Ratio Lower Upper
43 100
74 22.6 17.2 25.8

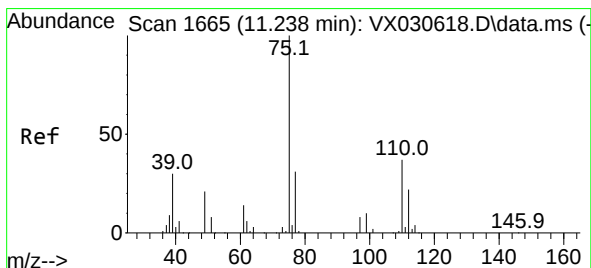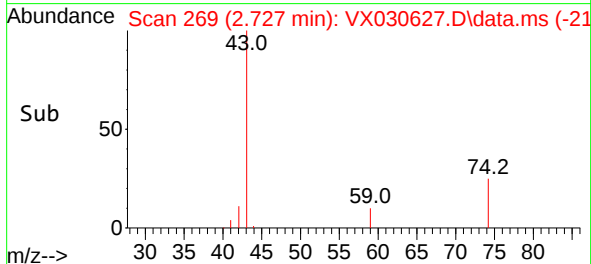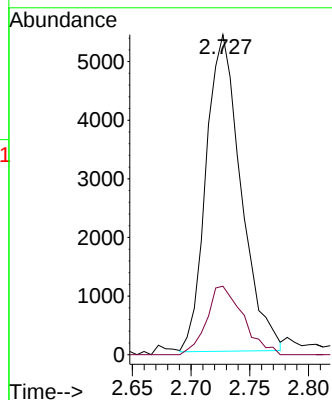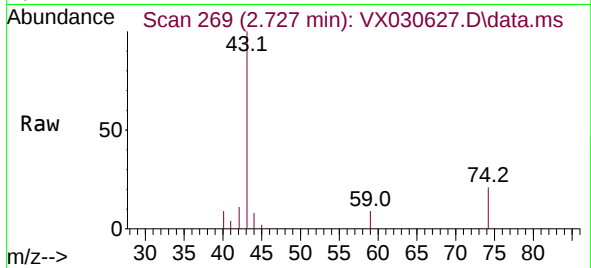

#61
1,2,3-Trichloropropane
Concen: 6.289 ug/L
RT: 12.024 min Scan# 1794
Delta R.T. 0.786 min
Lab File: VX030627.D
Acq: 15 Aug 2022 15:01

Tgt Ion: 75 Resp: 11551
Ion Ratio Lower Upper
75 100
77 34.4 26.1 39.1
110 2.7 30.5 45.7#

