

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030628.D
 Acq On : 15 Aug 2022 15:24
 Operator : JC/MD
 Sample : N4168-03
 Misc : 9.24g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX9B2

Quant Time: Aug 16 04:30:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 16 04:27:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	323829	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	287093	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	123950	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	60509	29.097	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	58.200%#		
7) Chloroethane-d5	1.666	69	32606	22.242	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	44.480%#		
11) 1,1-Dichloroethene-d2	2.276	63	96440	24.516	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	49.040%#		
21) 2-Butanone-d5	4.507	46	96080	49.864	ug/L	0.04
Spiked Amount 100.000	Range 40 - 130		Recovery =	49.860%		
24) Chloroform-d	5.062	84	126825	29.626	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	59.260%#		
26) 1,2-Dichloroethane-d4	5.958	65	94103	32.374	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	64.740%#		
32) Benzene-d6	5.970	84	258144	31.390	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	62.780%#		
36) 1,2-Dichloropropane-d6	7.312	67	83322	31.229	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	62.460%#		
41) Toluene-d8	8.653	98	234840	30.295	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	60.600%#		
43) trans-1,3-Dichloroprop...	8.958	79	35188	26.510	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	53.020%#		
47) 2-Hexanone-d5	9.403	63	62528	45.977	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	45.980%		
56) 1,1,2,2-Tetrachloroeth...	11.201	84	93309	26.621	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	53.240%#		
66) 1,2-Dichlorobenzene-d4	12.323	152	73748	30.675	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	61.360%#		
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	7.312	63	9648	3.942	ug/L #	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030628.D
Acq On : 15 Aug 2022 15:24
Operator : JC/MD
Sample : N4168-03
Misc : 9.24g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX9B2

Quant Time: Aug 16 04:30:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 16 04:27:08 2022
Response via : Initial Calibration

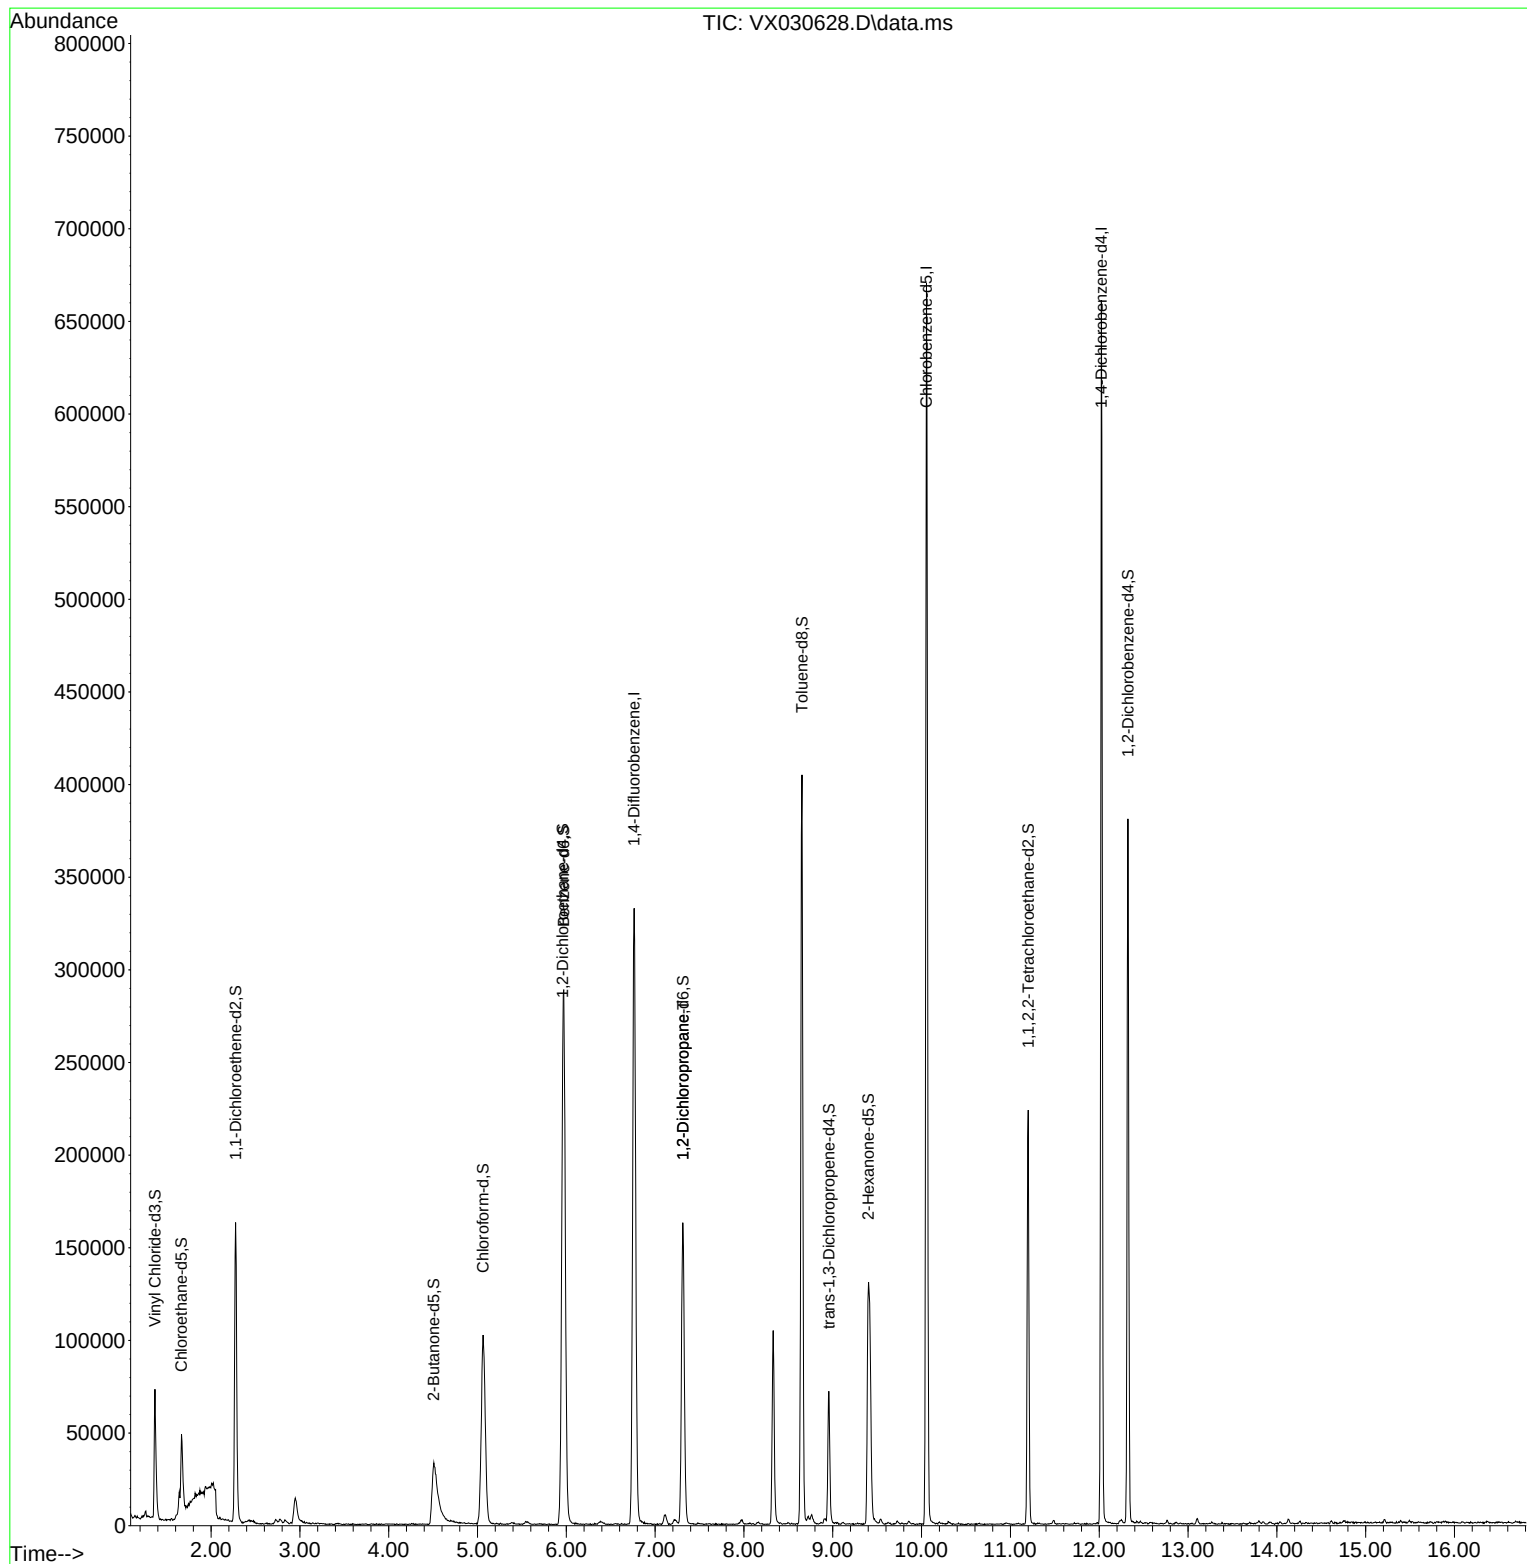

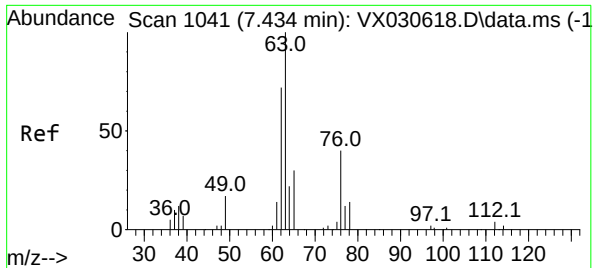

#37
 1,2-Dichloropropane
 Concen: 3.942 ug/L
 RT: 7.312 min Scan# 10
 Delta R.T. -0.122 min
 Lab File: VX030628.D
 Acq: 15 Aug 2022 15:24

Instrument :
 MSVOA_X
 ClientSampleId :
 EX9B2

Tgt Ion: 63 Resp: 9648
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.0 4.4#

